

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060122\
 Data File : BP010654.D
 Acq On : 01 Jun 2022 16:41
 Operator : CG/JU
 Sample : N2984-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P020-SS001-2430-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010654.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	394	401	420	rBV	1247707	1993647	27.87%	6.070%
2	7.034	663	671	690	rBV	1296505	2254745	31.52%	6.865%
3	7.857	804	811	821	rBV	232338	395481	5.53%	1.204%
4	9.022	1000	1009	1028	rBV	790833	1425691	19.93%	4.341%
5	10.663	1279	1288	1299	rBV	320959	604158	8.45%	1.840%
6	13.116	1699	1705	1722	rBV	2061791	3258822	45.56%	9.922%
7	14.498	1932	1940	1952	rBV	573554	882833	12.34%	2.688%
8	15.986	2187	2193	2209	rBV	2117218	3186988	44.56%	9.704%
9	17.251	2402	2408	2419	rBV	752129	1124660	15.72%	3.424%
10	17.921	2518	2522	2527	rBV	83068	102563	1.43%	0.312%
11	19.810	2837	2843	2855	rBV	4874163	6150456	85.99%	18.727%
12	21.051	3049	3054	3064	rBV	644256	912685	12.76%	2.779%
13	21.339	3098	3103	3108	rBV	1134150	1515078	21.18%	4.613%
14	21.456	3117	3123	3145	rBV	4707815	7152796	100.00%	21.779%
15	23.745	3506	3512	3523	rVB2	919161	1882661	26.32%	5.732%




Sum of corrected areas: 32843264

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060122\
Data File : BP010654.D
Acq On : 01 Jun 2022 16:41
Operator : CG/JU
Sample : N2984-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P020-SS001-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

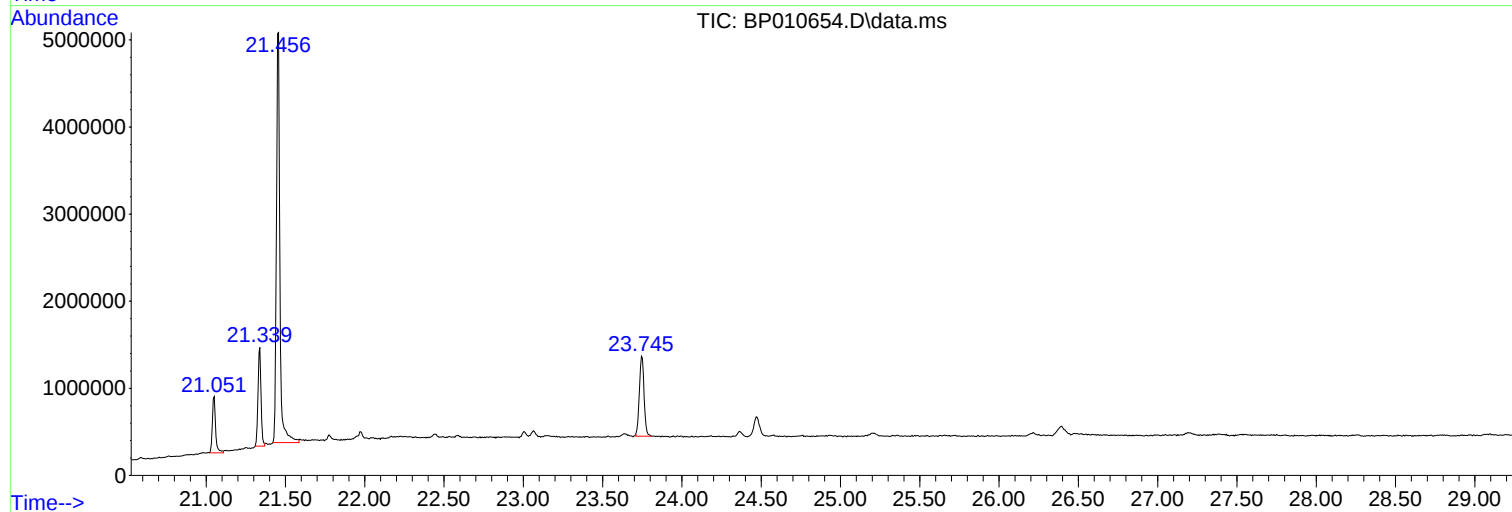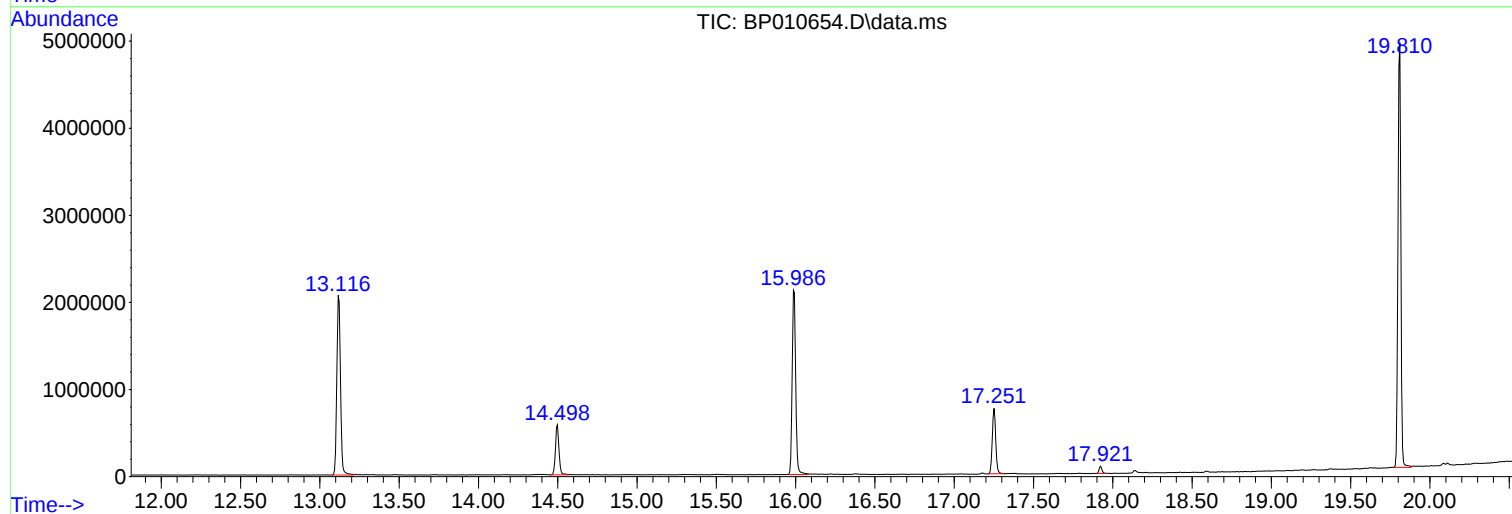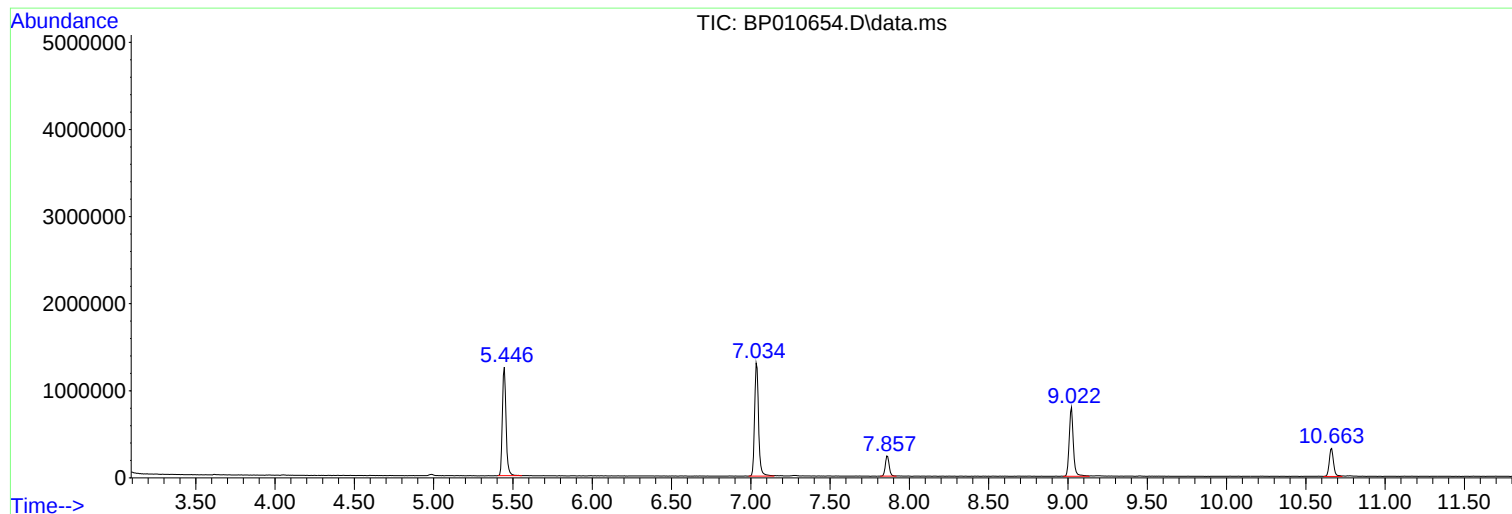

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060122\
Data File : BP010654.D
Acq On : 01 Jun 2022 16:41
Operator : CG/JU
Sample : N2984-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P020-SS001-2430-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclotetracosane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.051	12.05 ng	912685	Chrysene-d12	21.339

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetracosane	336	C24H48	000297-03-0	95
2			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
3			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94
4			1-Tetracosene	336	C24H48	010192-32-2	94
5			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94

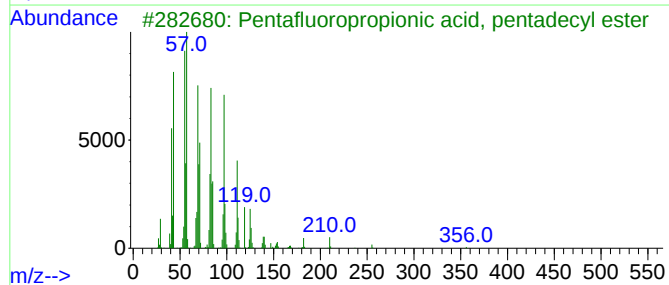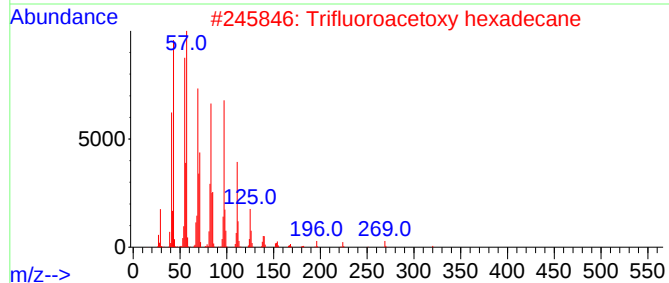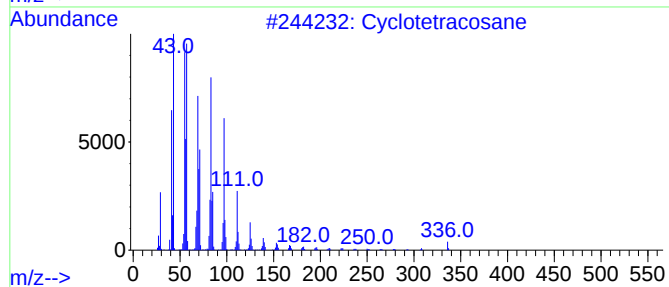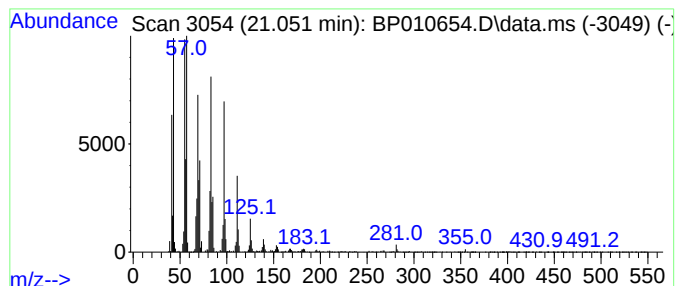

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060122\
Data File : BP010654.D
Acq On : 01 Jun 2022 16:41
Operator : CG/JU
Sample : N2984-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P020-SS001-2430-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.456	94.42 ng	7152800	Chrysene-d12	21.339

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	98
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	64
4			1H-Indole-3-acetic acid, 5-[(tri...]	277	C14H19NO3Si	072101-35-0	25
5			Vanadium, cycloheptatrienyl-(pen...]	277	C17H22V	1000155-20-5	25

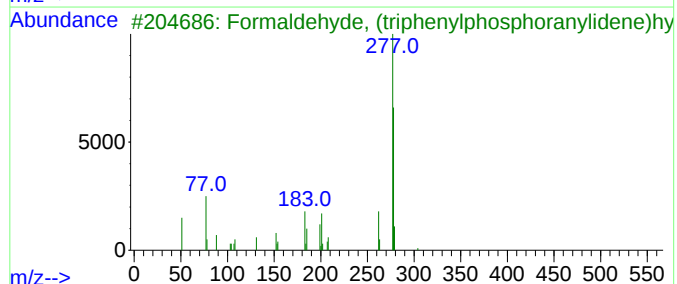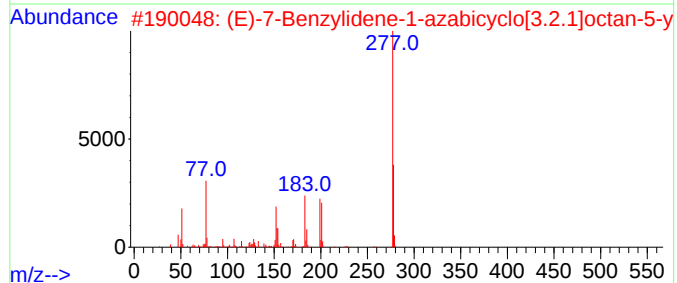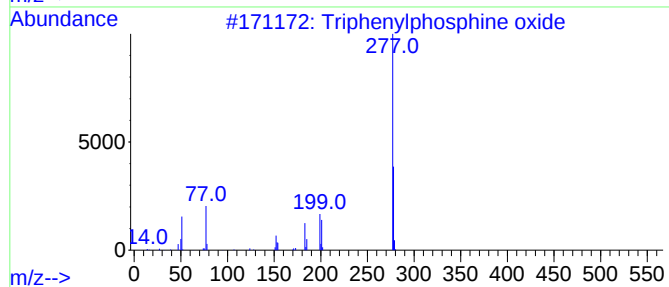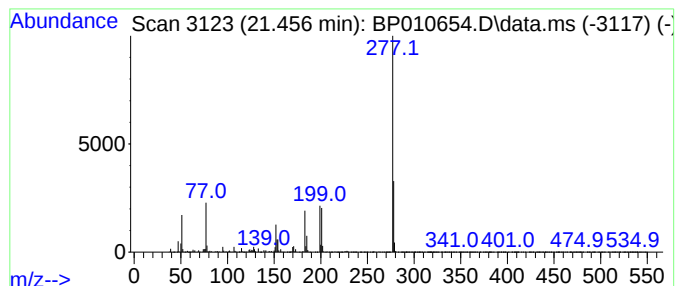

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060122\
Data File : BP010654.D
Acq On : 01 Jun 2022 16:41
Operator : CG/JU
Sample : N2984-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P020-SS001-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclotetracosane	21.051	12.1	ng	912685	5	21.339	1515080	20.0
Triphenylphosph...	21.456	94.4	ng	7152800	5	21.339	1515080	20.0