


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060122\
 Data File : BP010643.D
 Acq On : 01 Jun 2022 09:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 28 02:18:04 2022

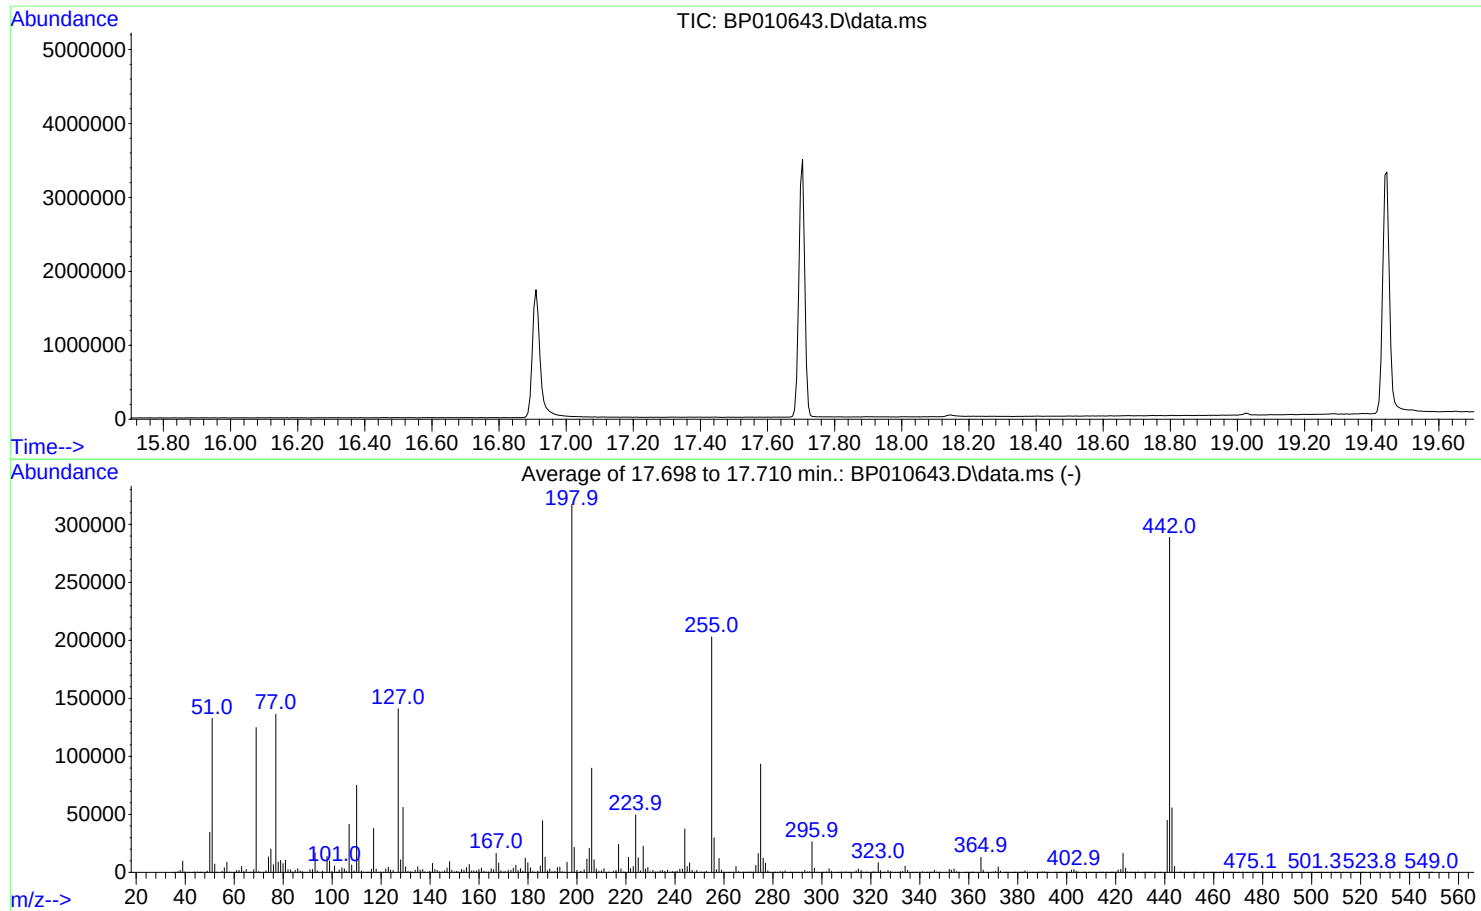




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	132689	PASS
68	69	0.00	2	1.9	2404	PASS
69	198	0.00	100	39.4	124830	PASS
70	69	0.00	2	0.6	781	PASS
127	198	10	80	44.5	140965	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	317120	PASS
199	198	5	9	6.8	21586	PASS
275	198	10	60	29.5	93435	PASS
365	198	1	100	4.1	12981	PASS
441	198	0.01	100	14.1	44852	PASS
442	442	100	100	100.0	288789	PASS
443	442	15	24	19.2	55563	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060122\
Data File : BP010643.D
Acq On : 01 Jun 2022 09:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 02 06:19:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 28 02:18:04 2022
Response via : Initial Calibration

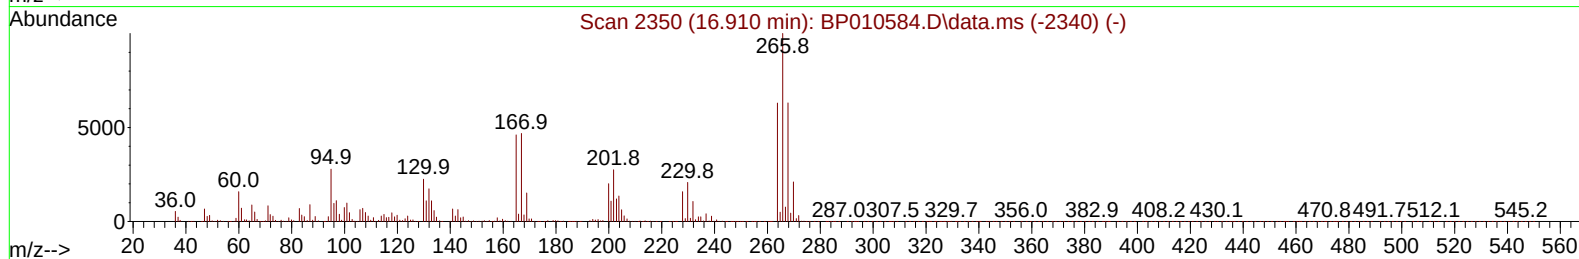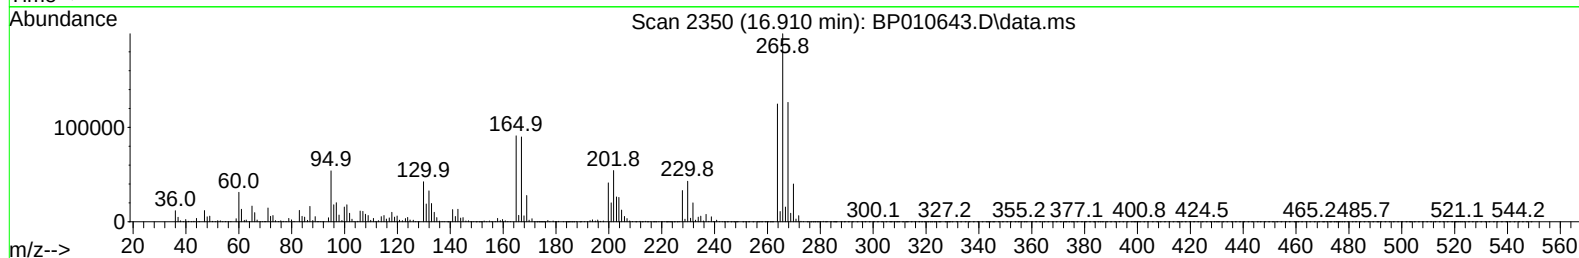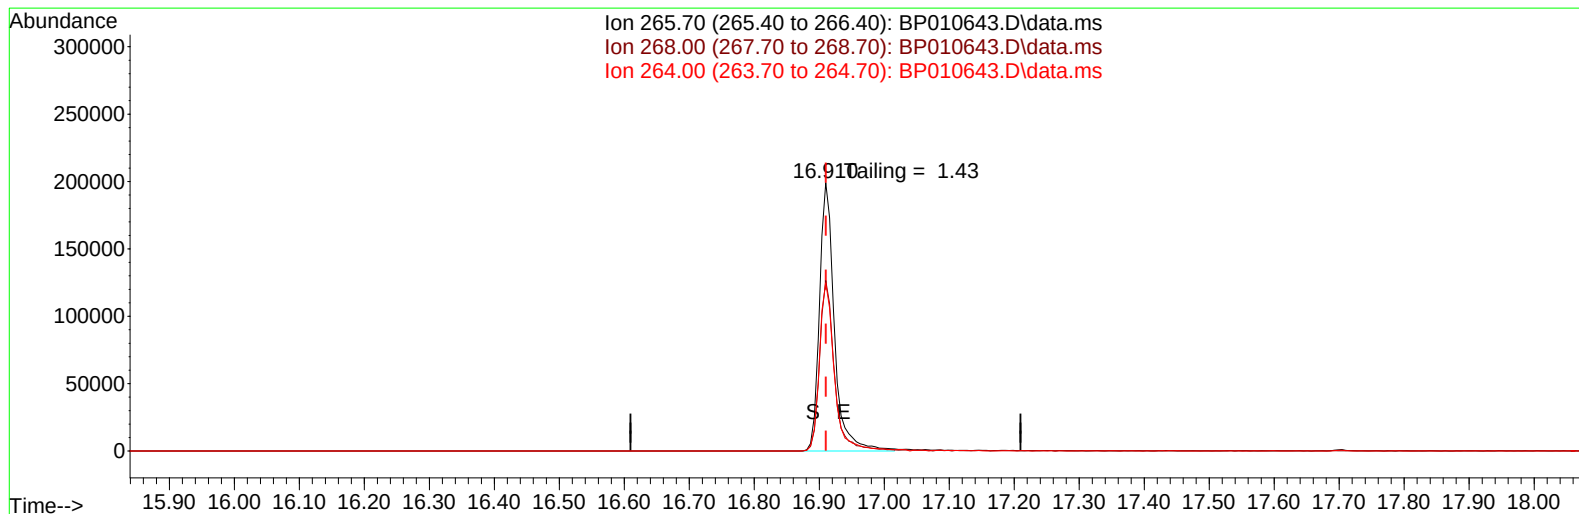

TIC: BP010643.D\data.ms

(70) Pentachlorophenol (C)

16.910min (0.000) 4254116.09 ng




response 322785

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.52
264.00	63.00	62.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060122\
 Data File : BP010643.D
 Acq On : 01 Jun 2022 09:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 02 06:19:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 28 02:18:04 2022
 Response via : Initial Calibration

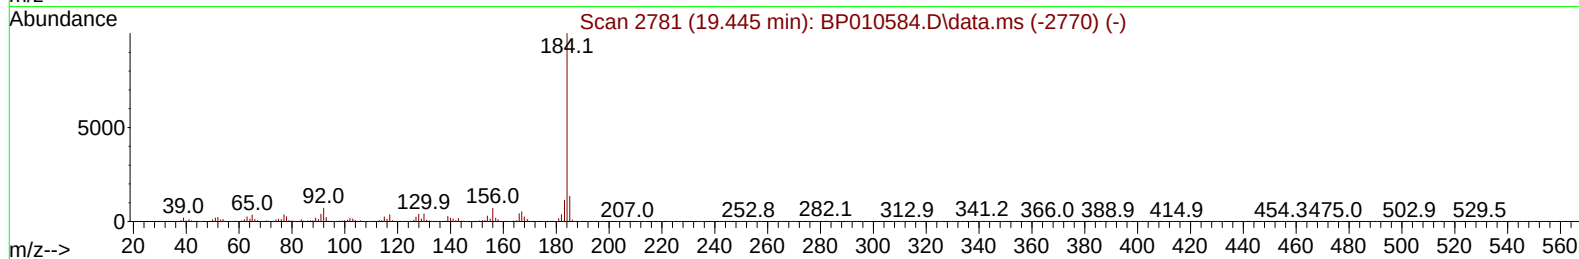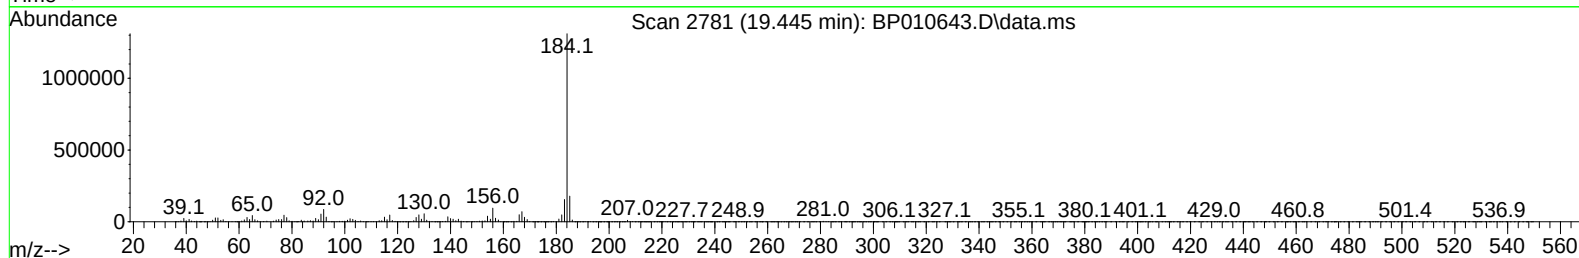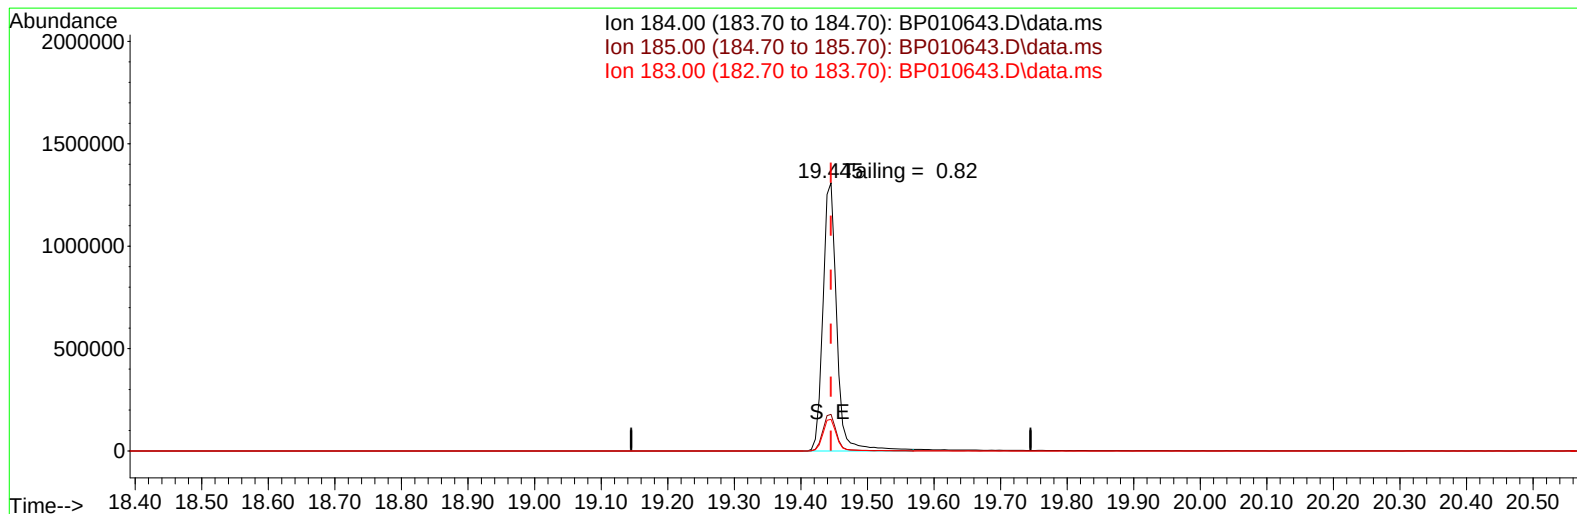

TIC: BP010643.D\data.ms

(77) Benzidine

19.445min (-0.000) 1857670.00 ng

response 1891286

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.64
183.00	11.30	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/1/2022	BNA_P	<u>BP010643.D</u>
Compound Name	Response	Retention Time
DDT	1064850	20.645
DDD	11489	20.222
DDE	2016	19.722
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13505	1078355	1.25

Instrument :
BNA_P
ClientSampleId :
DFTPP