
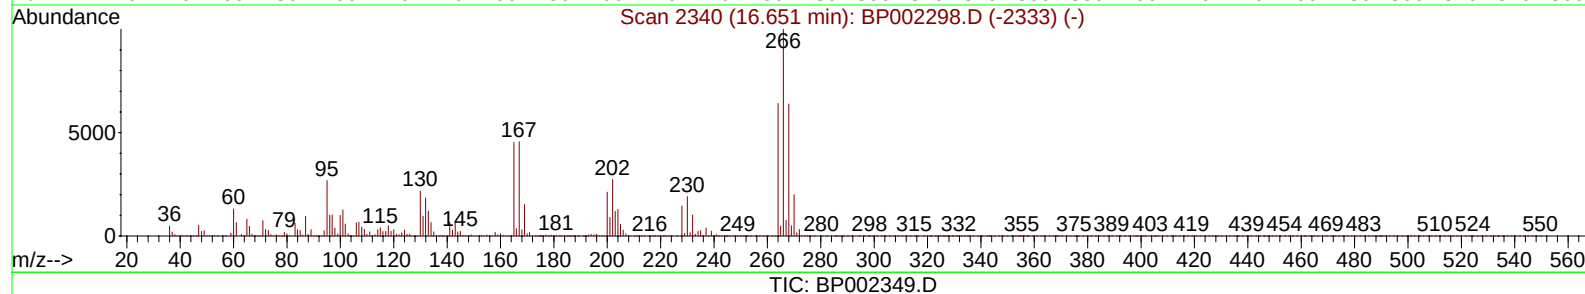
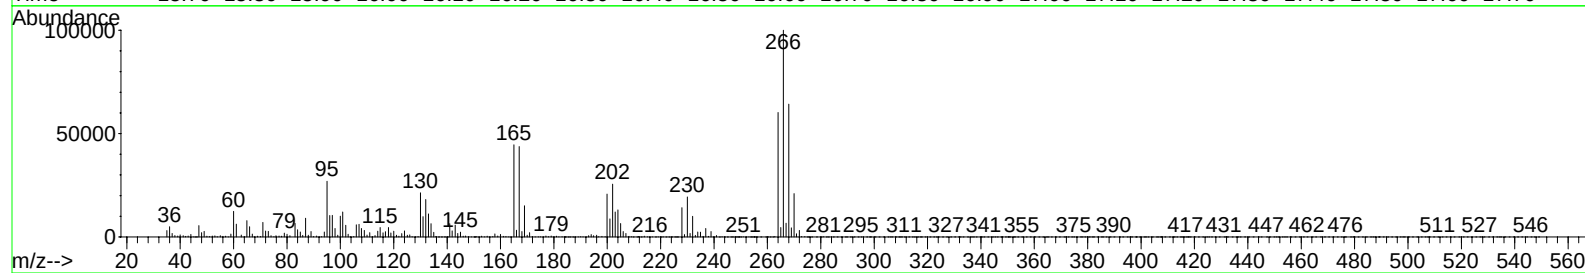


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP060220\
Data File : BP002349.D
Acq On : 02 Jun 2020 10:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 12:26:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP052720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 02 12:11:53 2020
Response via : Initial Calibration

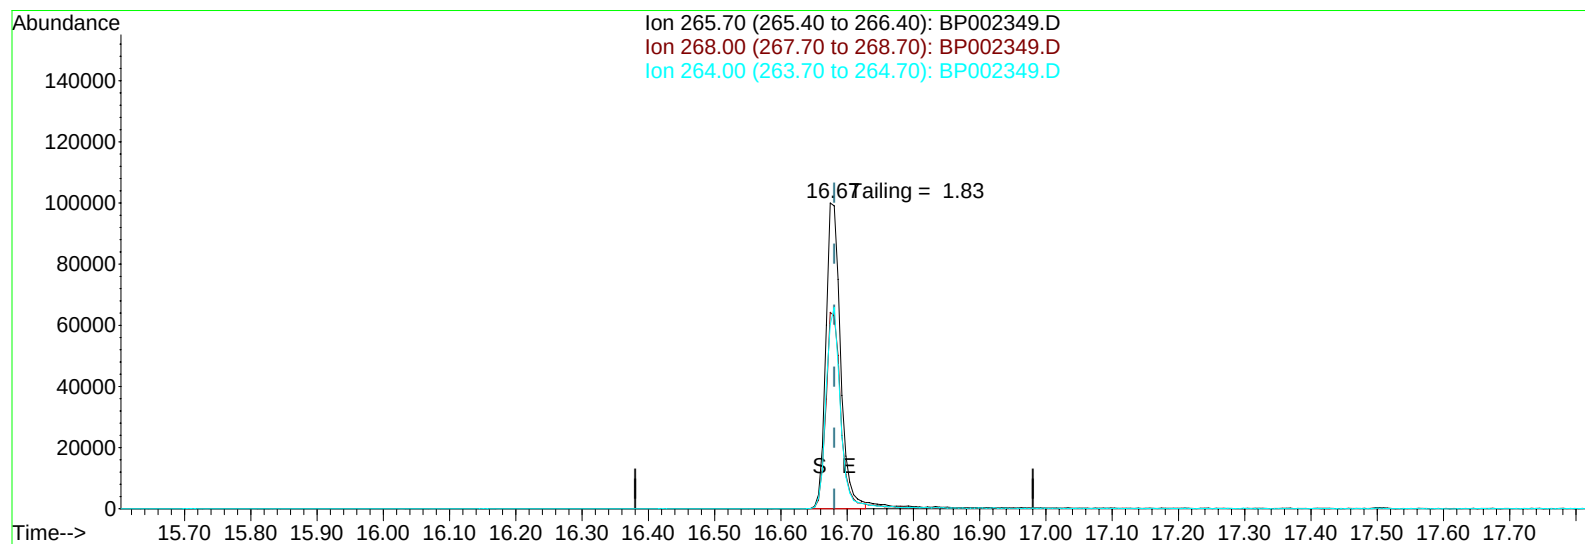

(70) Pentachlorophenol (C)




16.674min (-0.006) 261596.91ng

response 159064

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	64.26
264.00	60.40	60.21
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP060220\
 Data File : BP002349.D
 Acq On : 02 Jun 2020 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 12:26:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP052720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 02 12:11:53 2020
 Response via : Initial Calibration

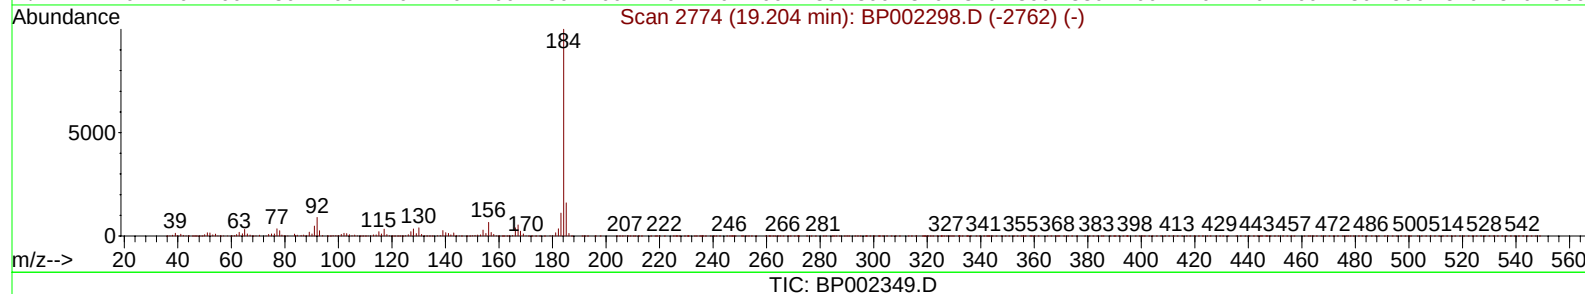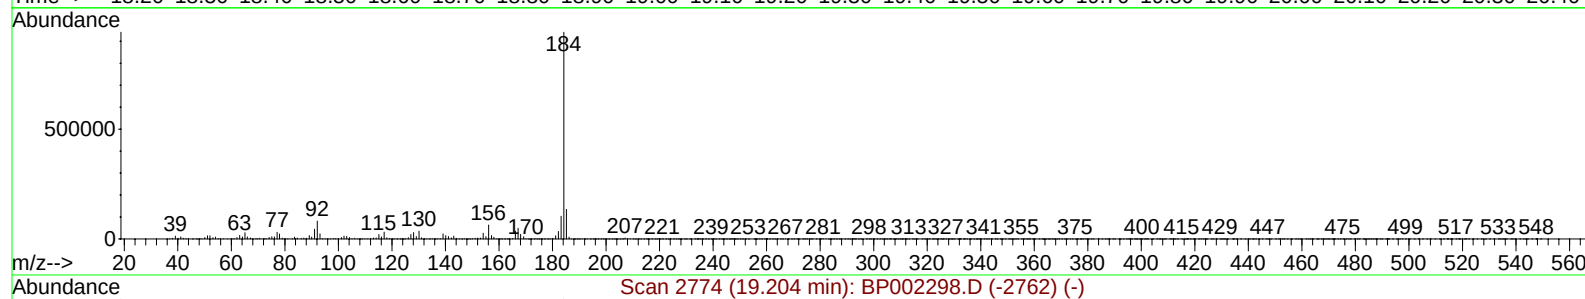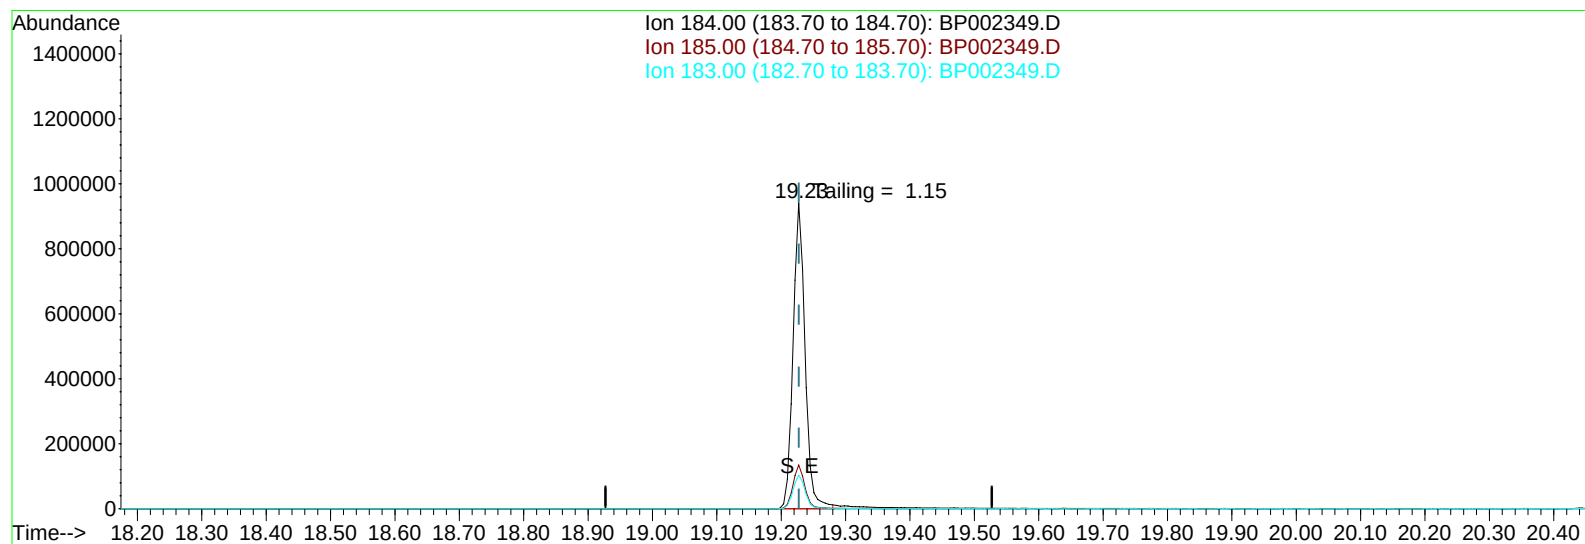

(77) Benzidine

19.227min (+0.000) 560964.17ng

response 1264493

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.32
183.00	11.40	11.00
0.00	0.00	0.00