

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP060220\
 Data File : BP002354.D
 Acq On : 02 Jun 2020 13:11
 Operator : CG/JU
 Sample : L2814-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PL-02-052920

Quant Time: Jun 03 02:18:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP052720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 02 12:11:53 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	234267	20.00	ng	0.00
21) Naphthalene-d8	10.38	136	901229	20.00	ng	0.00
39) Acenaphthene-d10	14.25	164	522829	20.00	ng	-0.01
64) Phenanthrene-d10	17.01	188	1105235	20.00	ng	-0.01
76) Chrysene-d12	21.12	240	1111262	20.00	ng	-0.01
86) Perylene-d12	23.33	264	1186091	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.23	112	1658190	132.94	ng	0.00
7) Phenol-d6	6.80	99	1922044	113.28	ng	0.00
23) Nitrobenzene-d5	8.75	82	1659591	110.71	ng	0.00
42) 2,4,6-Tribromophenol	15.76	330	866001	174.77	ng	0.00
45) 2-Fluorobiphenyl	12.87	172	3394244	114.55	ng	0.00
79) Terphenyl-d14	19.60	244	4800458	104.61	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.72	163	395685	11.181	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP060220\
Data File : BP002354.D
Acq On : 02 Jun 2020 13:11
Operator : CG/JU
Sample : L2814-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PL-02-052920

Quant Time: Jun 03 02:18:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP052720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 02 12:11:53 2020
Response via : Initial Calibration

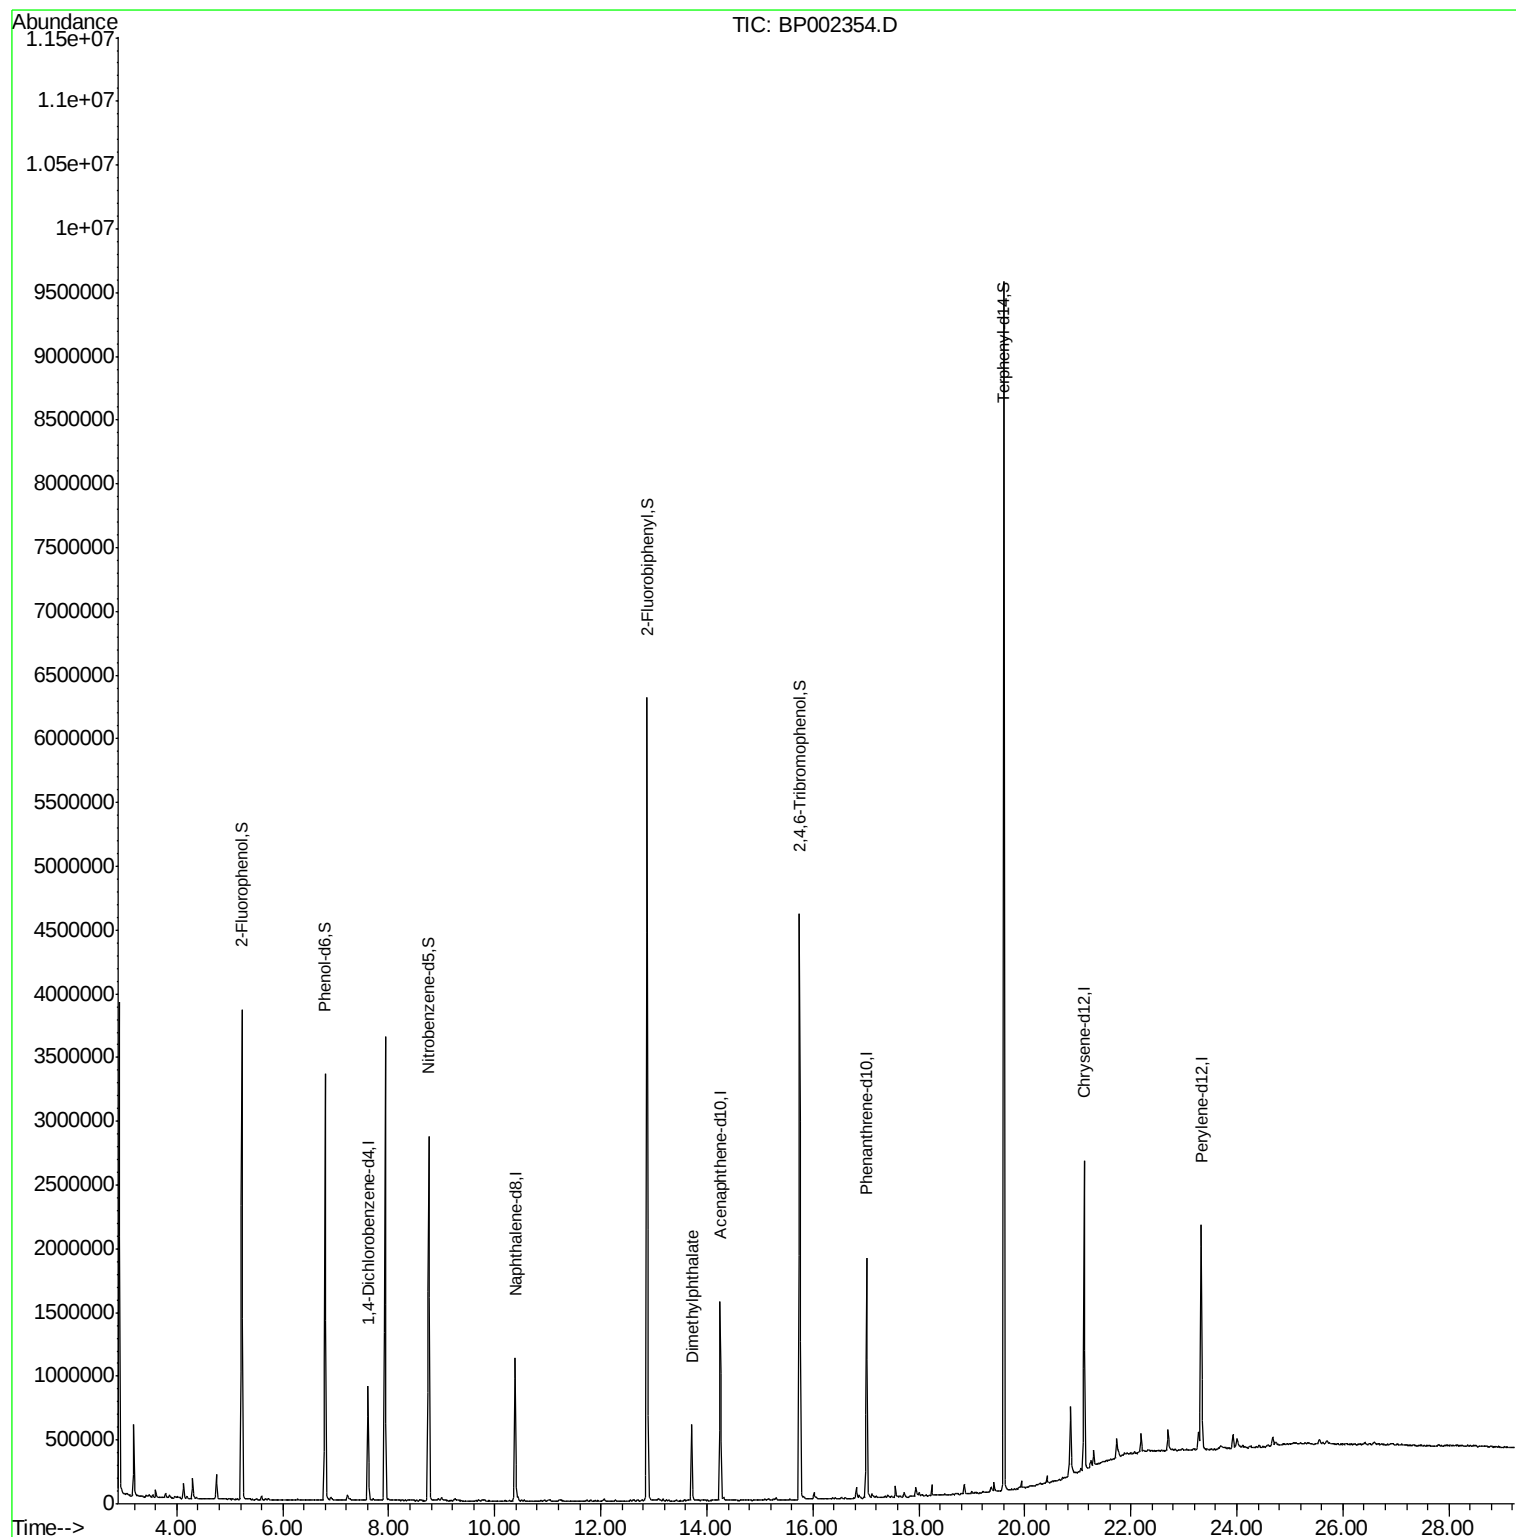







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.60 min Scan# 802
Delta R.T. -0.01 min
Lab File: BP002354.D
Acq: 02 Jun 2020 13:11

Instrument :
BNA_P
ClientSampleId :
PL-02-052920




Tot Ion	152	Resp	234267
Ion	Ratio	Lower	Upper
152	100		
150	158.6	124.7	187.1
115	59.7	49.4	74.2

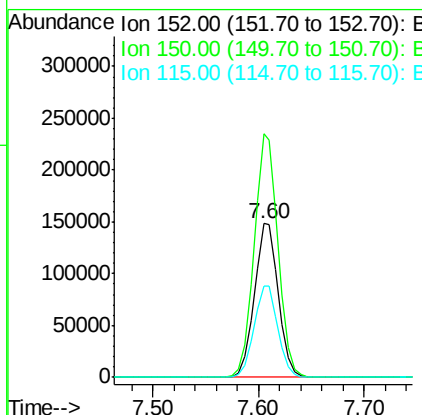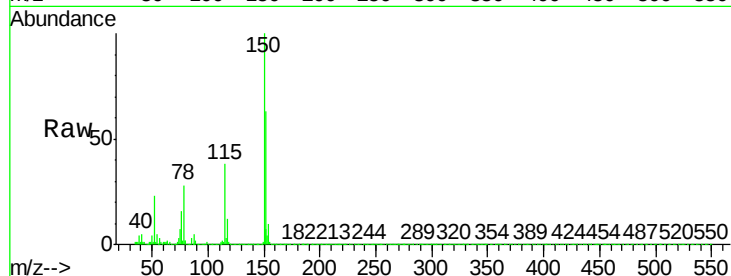


#5

2-Fluorophenol
Concen: 132.938 ng
RT: 5.23 min Scan# 398
Delta R.T. 0.00 min
Lab File: BP002354.D
Acq: 02 Jun 2020 13:11

Tgt Ion	112	Resp	1658190
Ion	Ratio	Lower	Upper
112	100		
64	57.0	47.0	70.4
63	29.8	24.0	36.0

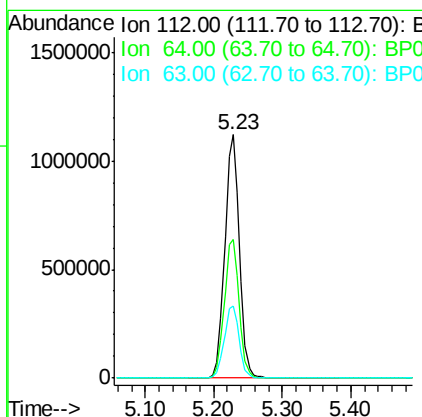



#7

Phenol-d6

Concen: 113.275 ng

RT: 6.80 min Scan# 665

Delta R.T. -0.01 min

Lab File: BP002354.D

Acq: 02 Jun 2020 13:11

Instrument :

BNA_P

ClientSampleId :

PL-02-052920


Tot Ion: 99 Resp: 1922044

Ion Ratio Lower Upper

99 100

42 17.5 13.9 20.9




71 32.9 25.8 38.8



Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

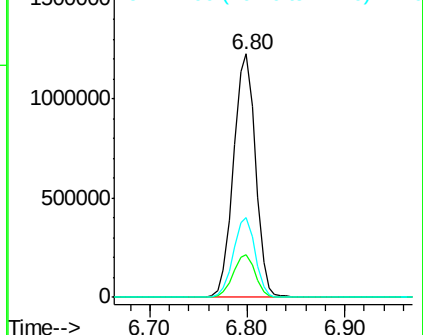

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.38 min Scan# 1274

Delta R.T. -0.01 min

Lab File: BP002354.D

Acq: 02 Jun 2020 13:11

Tgt Ion: 136 Resp: 901229


Ion Ratio Lower Upper

136 100

137 10.5 8.8 13.2

54 8.4 6.9 10.3

68 6.8 5.6 8.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0



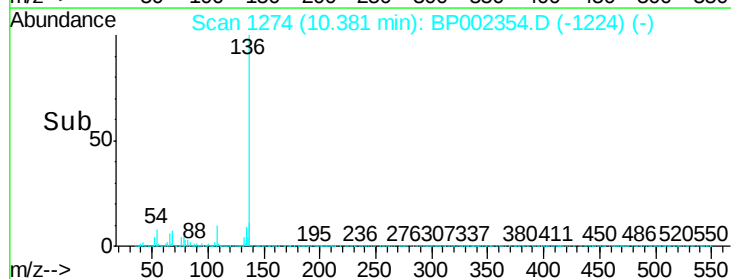
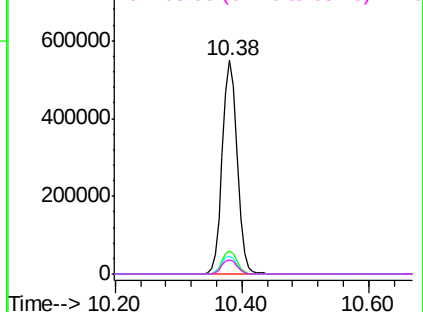


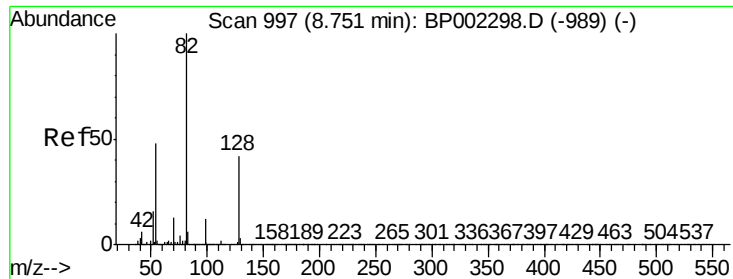

#23
Nitrobenzene-d5
Concen: 110.714 ng
RT: 8.75 min Scan# 997
Delta R.T. -0.01 min
Lab File: BP002354.D
Acq: 02 Jun 2020 13:11




Instrument :
BNA_P
ClientSampleId :
PL-02-052920


Tot Ion: 82 Resp: 1659591
Ion Ratio Lower Upper
82 100
128 42.5 33.4 50.0
54 49.3 38.3 57.5

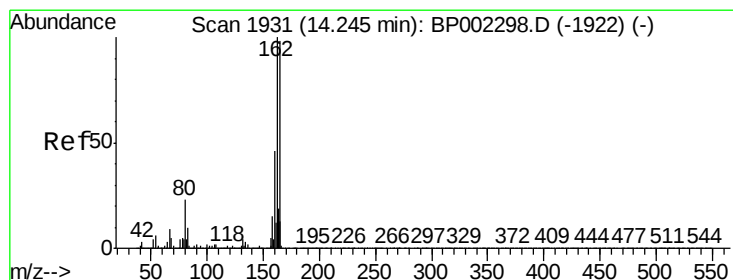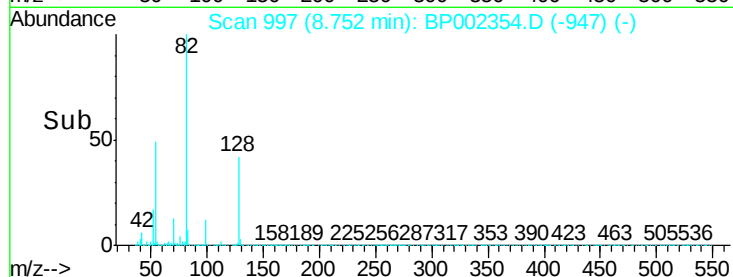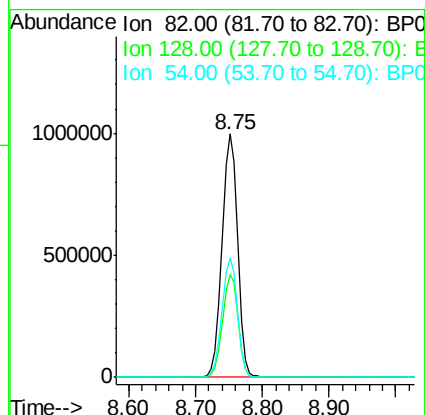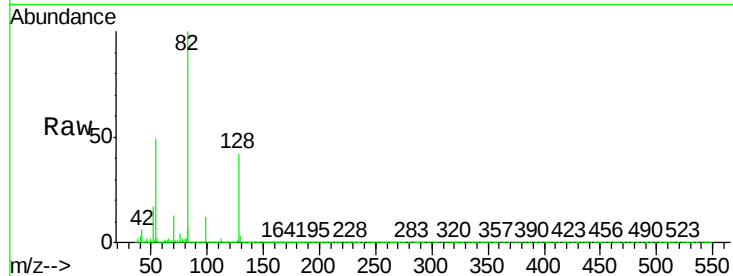

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.25 min Scan# 1932
Delta R.T. -0.01 min
Lab File: BP002354.D
Acq: 02 Jun 2020 13:11

Tgt Ion: 164 Resp: 522829
Ion Ratio Lower Upper
164 100
162 98.8 81.3 121.9
160 46.4 37.2 55.8


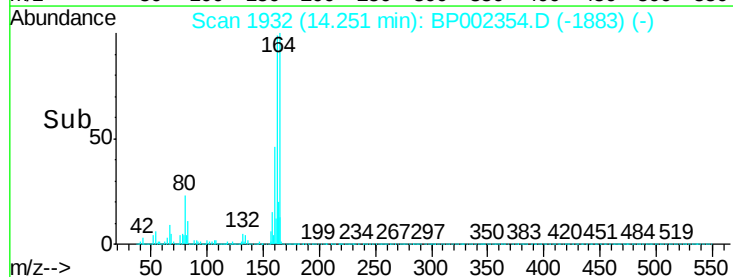
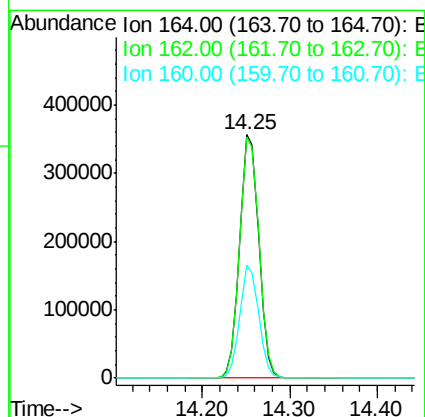
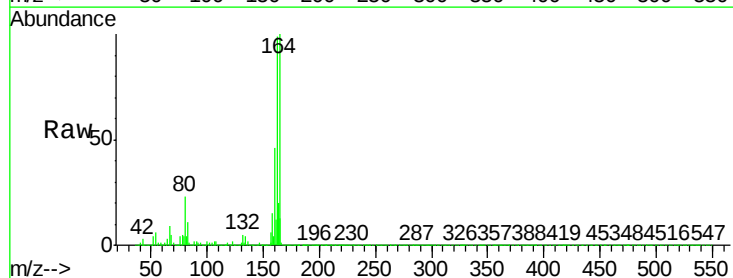


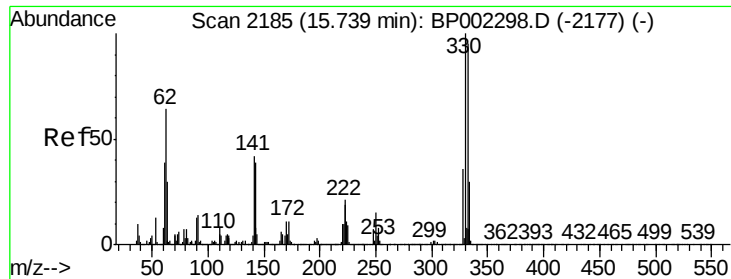

#42
2,4,6-Tribromophenol
Concen: 174.768 ng
RT: 15.76 min Scan# 2188
Delta R.T. -0.01 min
Lab File: BP002354.D
Acq: 02 Jun 2020 13:11




Instrument :
BNA_P
ClientSampleId :
PL-02-052920


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.5	76.9	115.3
141	36.2	31.4	47.2

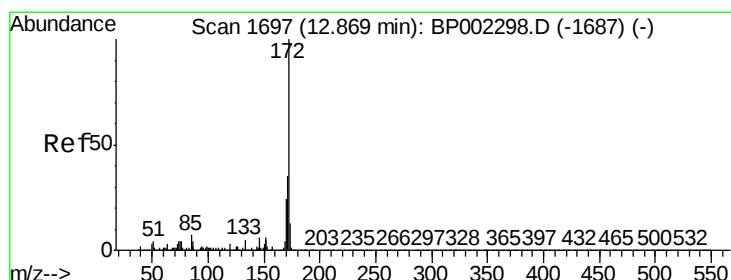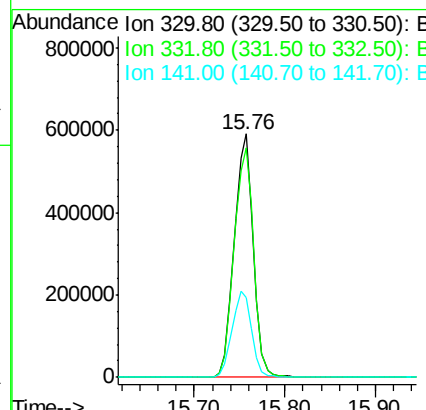

#45
2-Fluorobiphenyl
Concen: 114.555 ng
RT: 12.87 min Scan# 1698
Delta R.T. -0.01 min
Lab File: BP002354.D
Acq: 02 Jun 2020 13:11

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.6	27.6	41.4
170	24.4	18.9	28.3


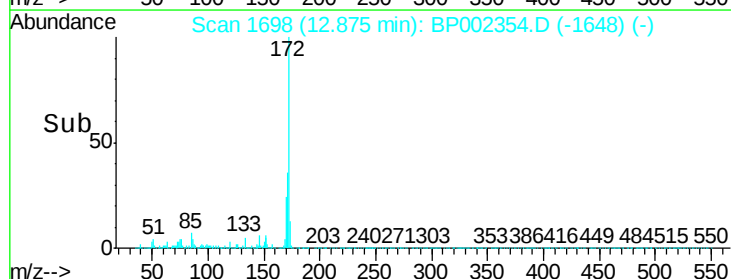
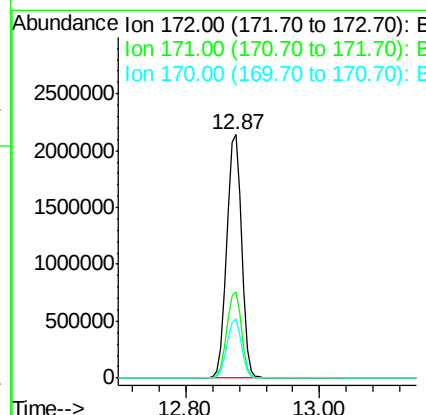
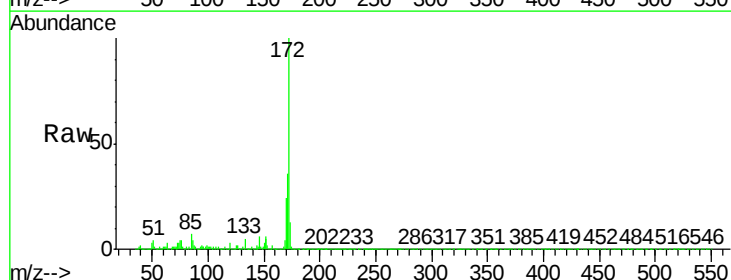




#50
Dimethylphthalate
Concen: 11.181 ng
RT: 13.72 min Scan# 1841
Delta R.T. -0.01 min
Lab File: BP002354.D
Acq: 02 Jun 2020 13:11




Instrument :
BNA_P
ClientSampleId :
PL-02-052920


Tot Ion:163 Resp: 395685
Ion Ratio Lower Upper
163 100
194 4.2 3.2 4.8
164 9.6 8.1 12.1

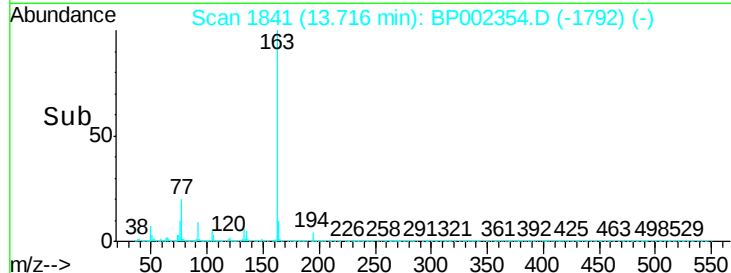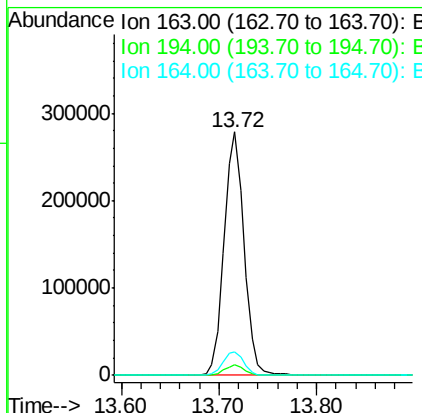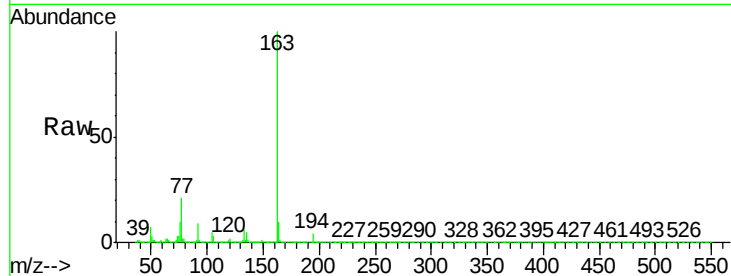

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.01 min Scan# 2401
Delta R.T. -0.01 min
Lab File: BP002354.D
Acq: 02 Jun 2020 13:11

Tgt Ion:188 Resp: 1105235
Ion Ratio Lower Upper
188 100
94 10.5 8.7 13.1
80 11.6 9.3 13.9


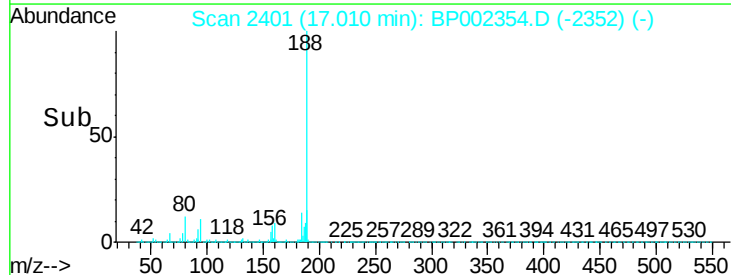
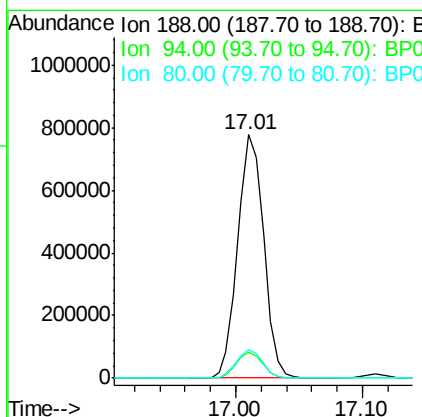





#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.12 min Scan# 3099
Delta R.T. -0.01 min
Lab File: BP002354.D
Acq: 02 Jun 2020 13:11




Instrument :
BNA_P
ClientSampleId :
PL-02-052920


Tot Ion:240 Resp: 1111262
Ion Ratio Lower Upper
240 100
120 12.6 8.7 13.1
236 26.5 21.0 31.4

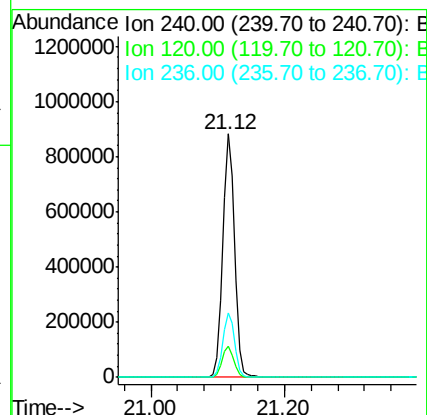

#79
Terphenyl-d14
Concen: 104.614 ng
RT: 19.60 min Scan# 2842
Delta R.T. 0.00 min
Lab File: BP002354.D
Acq: 02 Jun 2020 13:11

Tgt Ion:244 Resp: 4800458
Ion Ratio Lower Upper
244 100
212 8.4 6.4 9.6
122 10.8 9.4 14.0

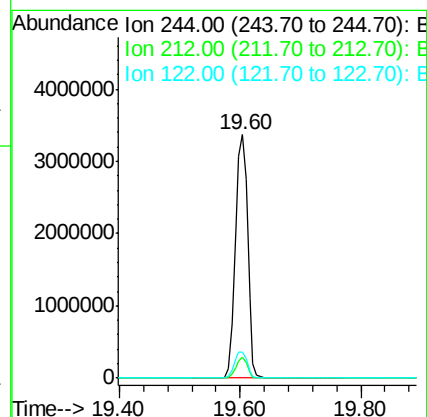



#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.33 min Scan# 3475
Delta R.T. -0.01 min
Lab File: BP002354.D
Acq: 02 Jun 2020 13:11

Instrument :
BNA_P
ClientSampleId :
PL-02-052920

Tot Ion:264 Resp: 1186091

Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.4	29.2
265	21.3	17.8	26.6

