


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060220\
 Data File : BP002349.D
 Acq On : 02 Jun 2020 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP052720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 02 12:11:53 2020

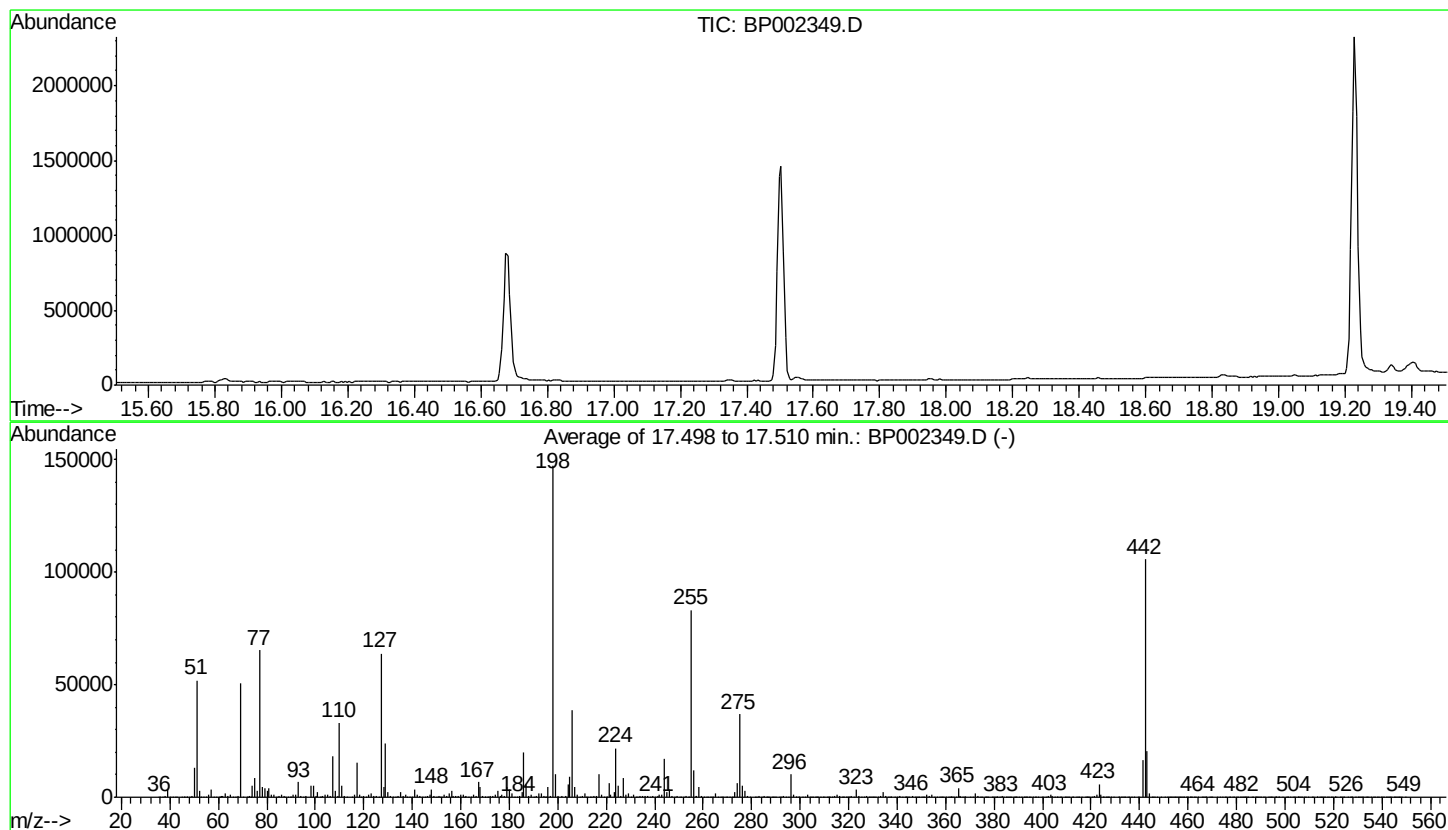

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	52065	PASS
68	69	0.00	2	1.5	762	PASS
69	198	0.00	100	34.3	50577	PASS
70	69	0.00	2	0.4	220	PASS
127	198	10	80	43.2	63730	PASS
197	198	0.00	2	0.4	541	PASS
198	198	100	100	100.0	147359	PASS
199	198	5	9	7.0	10281	PASS
275	198	10	60	24.9	36755	PASS
365	198	1	100	2.7	4000	PASS
441	198	0.01	100	11.3	16645	PASS
442	198	50	100	71.6	105544	PASS
443	442	15	24	19.4	20487	PASS