

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060221\  
 Data File : BP005669.D  
 Acq On : 02 Jun 2021 17:14  
 Operator : CG/JU  
 Sample : M2574-01 2X  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 NB-07-060121

Quant Time: Jun 02 17:43:35 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052721.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu May 27 16:11:11 2021  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc  | Units | Dev(Min) |
|-----------------------------|--------|------|----------|-------|-------|----------|
| -----                       |        |      |          |       |       |          |
| Internal Standards          |        |      |          |       |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.987  | 152  | 343182   | 20.00 | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.799 | 136  | 1332484  | 20.00 | ng    | 0.00     |
| 39) Acenaphthene-d10        | 14.610 | 164  | 807153   | 20.00 | ng    | 0.00     |
| 64) Phenanthrene-d10        | 17.351 | 188  | 1613087  | 20.00 | ng    | # 0.00   |
| 76) Chrysene-d12            | 21.422 | 240  | 1456766  | 20.00 | ng    | # 0.00   |
| 86) Perylene-d12            | 23.868 | 264  | 1638912  | 20.00 | ng    | 0.00     |
|                             |        |      |          |       |       |          |
| System Monitoring Compounds |        |      |          |       |       |          |
| 5) 2-Fluorophenol           | 5.546  | 112  | 955718   | 43.30 | ng    | 0.00     |
| 7) Phenol-d6                | 7.146  | 99   | 1162464  | 38.63 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 9.152  | 82   | 749307   | 31.27 | ng    | 0.00     |
| 42) 2,4,6-Tribromophenol    | 16.092 | 330  | 642154   | 62.04 | ng    | 0.00     |
| 45) 2-Fluorobiphenyl        | 13.240 | 172  | 1833364  | 30.06 | ng    | 0.00     |
| 79) Terphenyl-d14           | 19.898 | 244  | 2528167  | 32.57 | ng    | 0.00     |
|                             |        |      |          |       |       |          |
| Target Compounds            |        |      |          |       |       | Qvalue   |
| 26) 2-Nitrophenol           | 9.899  | 139  | 15       | 4.16  | ng    | # 1      |
| 32) Benzoic acid            | 10.093 | 122  | 153      | 5.03  | ng    | # 1      |
| 48) 2-Nitroaniline          | 13.710 | 65   | 134      | 4.50  | ng    | # 41     |
| 50) Dimethylphthalate       | 14.063 | 163  | 180464   | 2.81  | ng    | 100      |
| 51) 2,6-Dinitrotoluene      | 14.187 | 165  | 151      | 5.07  | ng    | # 26     |
| 53) 3-Nitroaniline          | 14.510 | 138  | 251      | 3.67  | ng    | # 39     |
| 54) 2,4-Dinitrophenol       | 14.722 | 184  | 39       | 6.53  | ng    | # 1      |
| 56) 4-Nitrophenol           | 14.669 | 139  | 344      | 3.77  | ng    | 92       |
| 57) 2,4-Dinitrotoluene      | 14.963 | 165  | 681      | 4.30  | ng    | # 57     |
| 62) 4-Nitroaniline          | 15.657 | 138  | 1434     | 3.72  | ng    | # 38     |
| 71) Phenanthrene            | 17.392 | 178  | 657085   | 6.54  | ng    | 99       |
| 75) Fluoranthene            | 19.351 | 202  | 1153434  | 9.56  | ng    | 97       |
| 78) Pyrene                  | 19.704 | 202  | 1055400  | 10.27 | ng    | 98       |
| 80) Butylbenzylphthalate    | 20.739 | 149  | 2889     | 4.19  | ng    | 91       |
| 81) Benzo(a)anthracene      | 21.404 | 228  | 586177   | 5.48  | ng    | 96       |
| 83) Chrysene                | 21.457 | 228  | 520191   | 5.02  | ng    | 96       |
| 87) Indeno(1,2,3-cd)pyrene  | 26.427 | 276  | 376397   | 2.70  | ng    | # 94     |
| 88) Benzo(b)fluoranthene    | 23.121 | 252  | 744296   | 6.26  | ng    | # 92     |
| 89) Benzo(k)fluoranthene    | 23.121 | 252  | 744296   | 6.61  | ng    | # 90     |
| 90) Benzo(a)pyrene          | 23.757 | 252  | 542061   | 5.01  | ng    | # 91     |
| 92) Benzo(g,h,i)perylene    | 27.215 | 276  | 366297   | 3.14  | ng    | # 93     |
| -----                       |        |      |          |       |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060221\  
Data File : BP005669.D  
Acq On : 02 Jun 2021 17:14  
Operator : CG/JU  
Sample : M2574-01 2X  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121

Quant Time: Jun 02 17:43:35 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052721.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 27 16:11:11 2021  
Response via : Initial Calibration




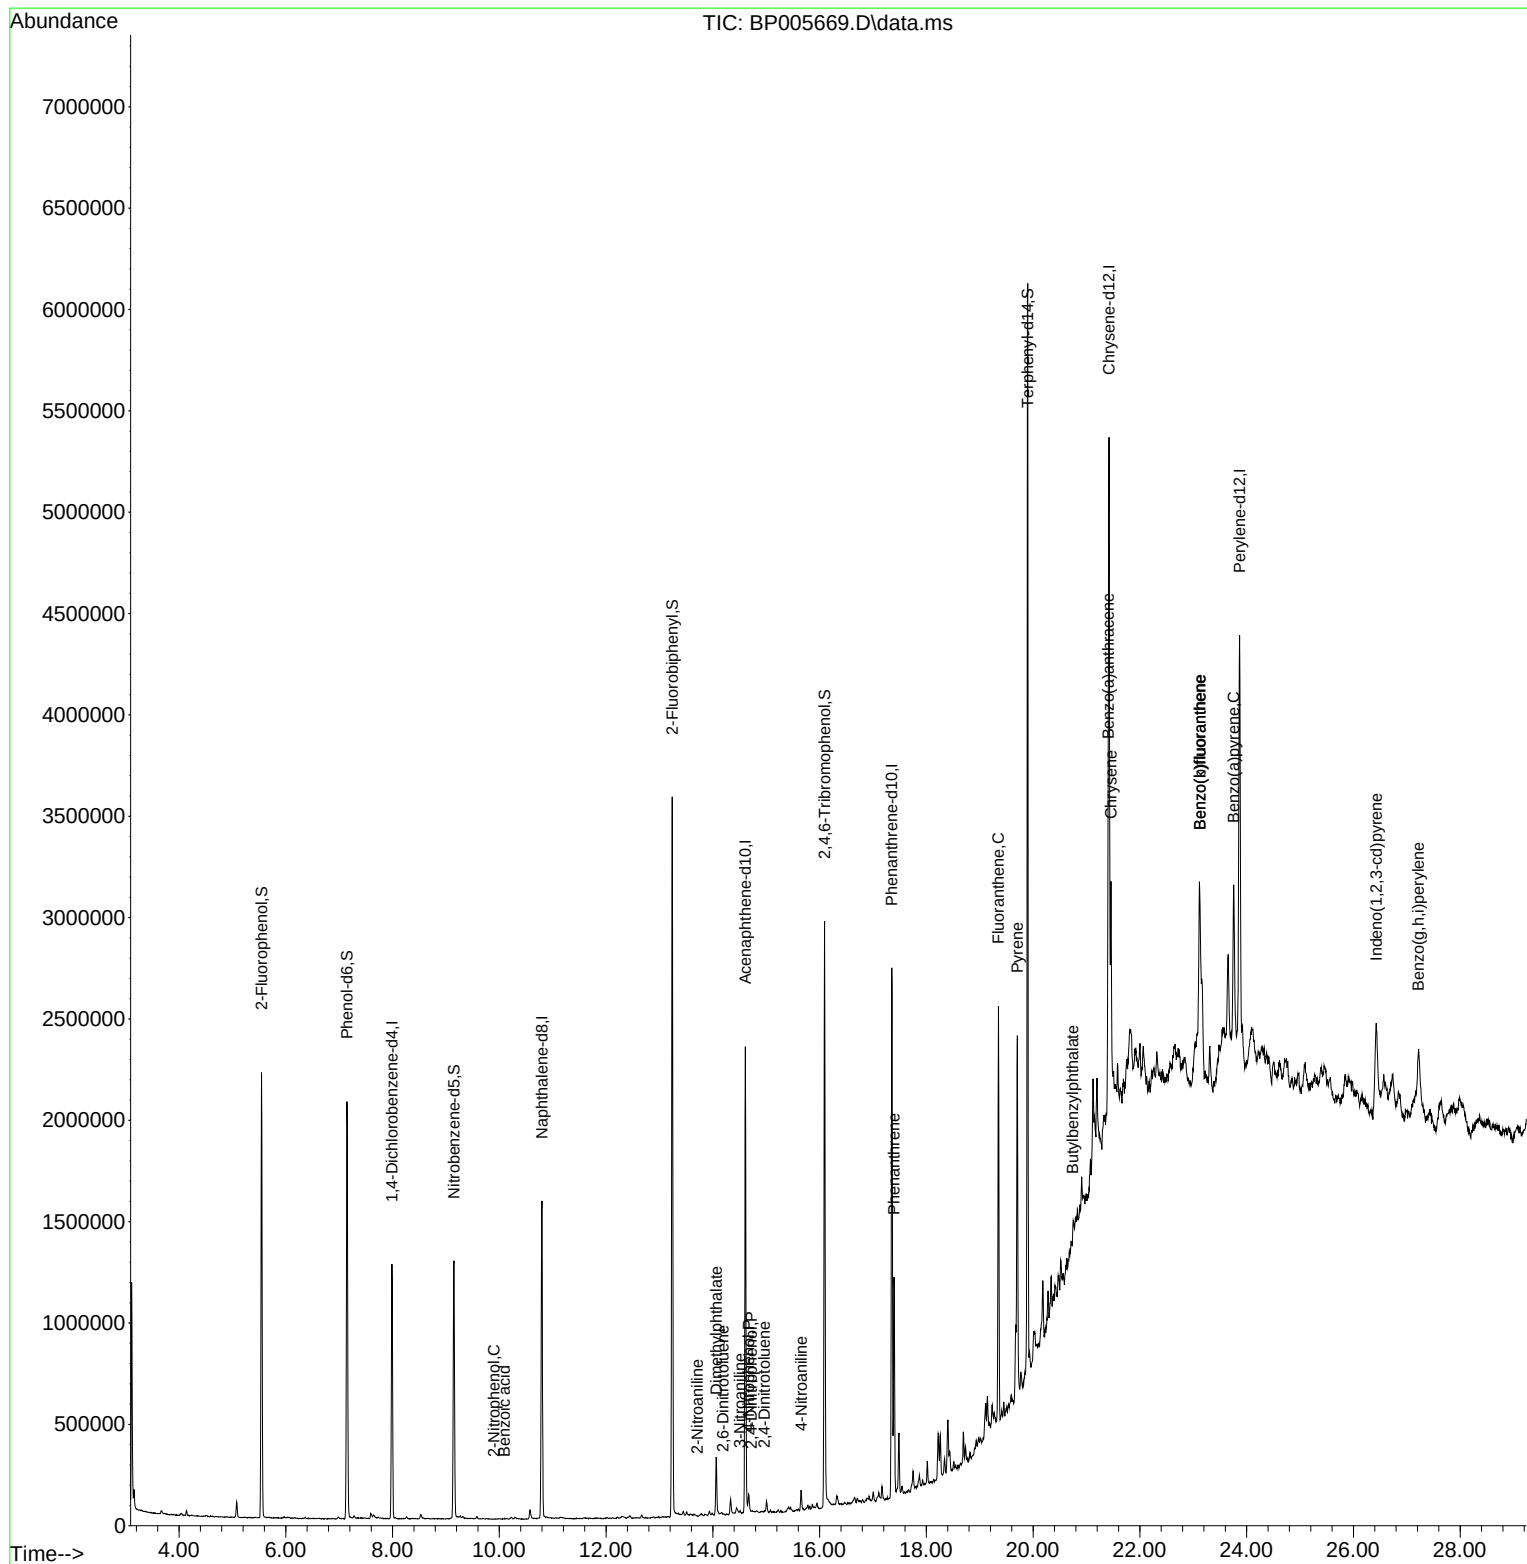




#1  
1,4-Dichlorobenzene-d4  
Concen: 20.00 ng  
RT: 7.987 min Scan# 833  
Delta R.T. -0.006 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion:152 Resp: 343182  
Ion Ratio Lower Upper  
152 100  
150 158.3 119.8 179.8  
115 58.4 49.0 73.4



#5  
2-Fluorophenol  
Concen: 43.30 ng  
RT: 5.546 min Scan# 418  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:112 Resp: 955718  
Ion Ratio Lower Upper  
112 100  
64 52.0 33.6 50.4#  
63 28.8 18.6 27.8#









#7  
Phenol-d6  
Concen: 38.63 ng  
RT: 7.146 min Scan# 690  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121

Tgt Ion: 99 Resp: 1162464




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 99  | 100   |       |       |
| 42  | 16.9  | 12.9  | 19.3  |
| 71  | 35.2  | 26.7  | 40.1  |

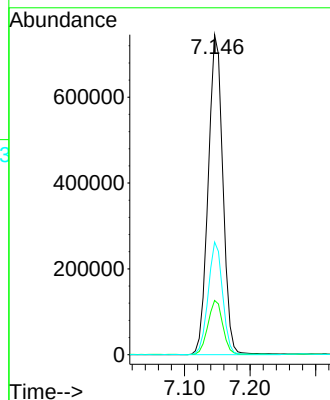


#21  
Naphthalene-d8  
Concen: 20.00 ng  
RT: 10.799 min Scan# 1311  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:136 Resp: 1332484

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 136 | 100   |       |       |
| 137 | 10.6  | 8.9   | 13.3  |
| 54  | 6.3   | 5.0   | 7.4   |
| 68  | 5.3   | 3.7   | 5.5   |



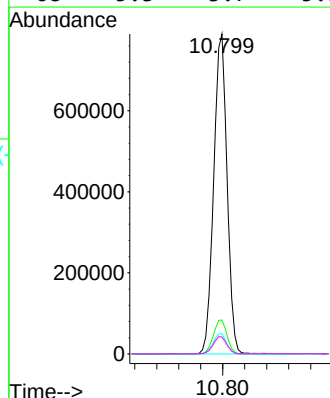





#23  
Nitrobenzene-d5  
Concen: 31.27 ng  
RT: 9.152 min Scan# 1031  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion: 82 Resp: 749307  
Ion Ratio Lower Upper  
82 100  
128 46.3 30.5 45.7#  
54 42.6 33.9 50.9

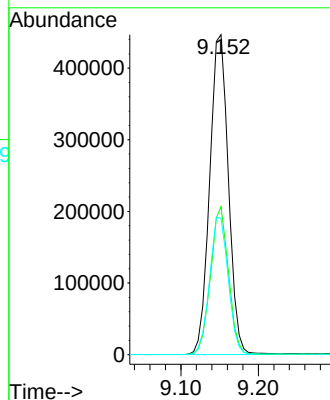

#26  
2-Nitrophenol  
Concen: 4.16 ng  
RT: 9.899 min Scan# 1158  
Delta R.T. -0.012 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:139 Resp: 15  
Ion Ratio Lower Upper  
139 100  
109 464.0 40.7 61.1#  
65 396.0 47.8 71.6#



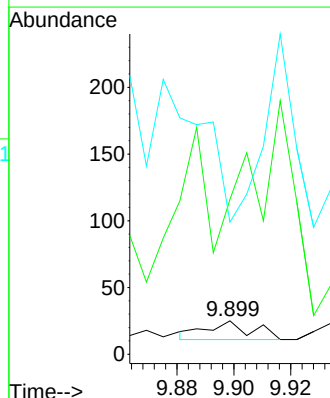





#32  
Benzoic acid  
Concen: 5.03 ng  
RT: 10.093 min Scan# 1191  
Delta R.T. 0.006 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion:122 Resp: 153  
Ion Ratio Lower Upper  
122 100  
105 154.9 105.1 145.1#  
77 306.9 69.6 109.6#

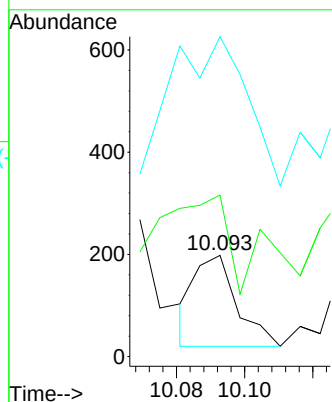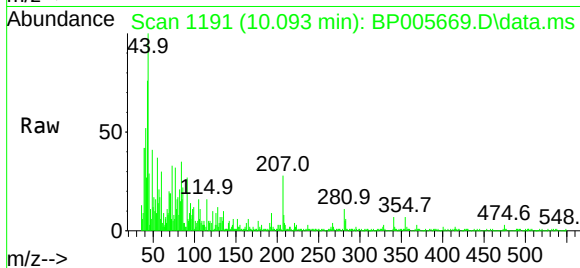

#39  
Acenaphthene-d10  
Concen: 20.00 ng  
RT: 14.610 min Scan# 1959  
Delta R.T. 0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:164 Resp: 807153  
Ion Ratio Lower Upper  
164 100  
162 98.8 73.5 110.3  
160 44.8 40.6 61.0




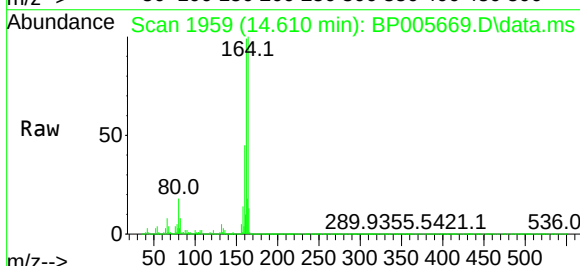




#42  
2,4,6-Tribromophenol  
Concen: 62.04 ng  
RT: 16.092 min Scan# 2211  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion:330 Resp: 642154  
Ion Ratio Lower Upper  
330 100  
332 96.8 76.3 114.5  
141 24.9 22.8 34.2

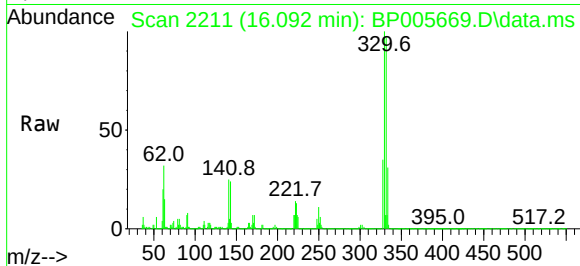

#45  
2-Fluorobiphenyl  
Concen: 30.06 ng  
RT: 13.240 min Scan# 1726  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:172 Resp: 1833364  
Ion Ratio Lower Upper  
172 100  
171 35.1 28.1 42.1  
170 23.1 19.6 29.4




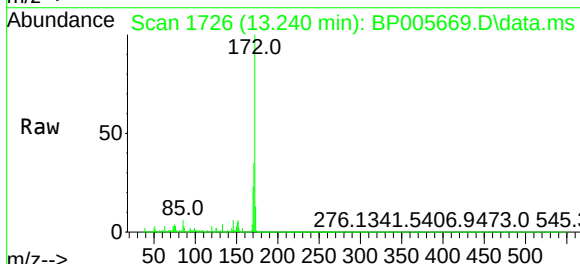




#48  
2-Nitroaniline  
Concen: 4.50 ng  
RT: 13.710 min Scan# 1806  
Delta R.T. 0.017 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121

Tgt Ion: 65 Resp: 134  
Ion Ratio Lower Upper  
65 100  
92 26.6 48.8 73.2#  
138 23.6 69.5 104.3#

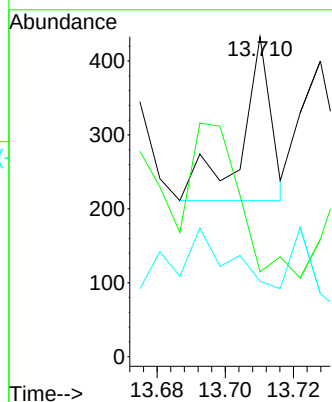


#50  
Dimethylphthalate  
Concen: 2.81 ng  
RT: 14.063 min Scan# 1866  
Delta R.T. -0.006 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion: 163 Resp: 180464  
Ion Ratio Lower Upper  
163 100  
194 4.6 3.9 5.9  
164 10.1 8.1 12.1

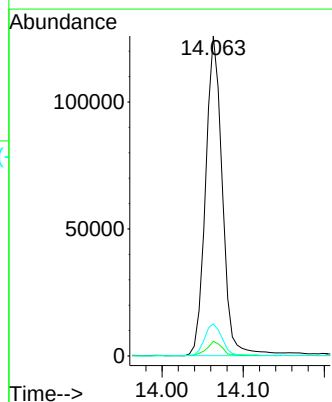









#51  
2,6-Dinitrotoluene  
Concen: 5.07 ng  
RT: 14.187 min Scan# 1887  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion:165 Resp: 151  
Ion Ratio Lower Upper  
165 100  
63 192.7 67.4 101.0#  
89 61.5 73.8 110.6#



#53  
3-Nitroaniline  
Concen: 3.67 ng  
RT: 14.510 min Scan# 1942  
Delta R.T. 0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:138 Resp: 251  
Ion Ratio Lower Upper  
138 100  
108 63.2 10.2 15.4#  
92 70.2 108.1 162.1#







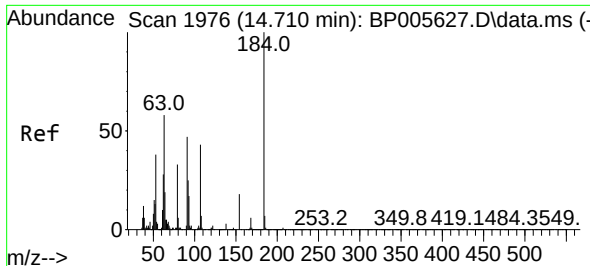

#54  
2,4-Dinitrophenol  
Concen: 6.53 ng  
RT: 14.722 min Scan# 1978  
Delta R.T. 0.012 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion:184 Resp: 39  
Ion Ratio Lower Upper  
184 100  
63 602.6 51.2 76.8#  
154 1261.5 55.8 83.8#

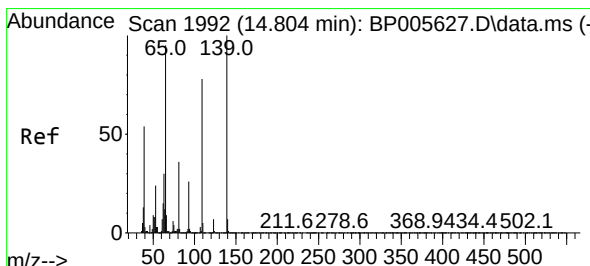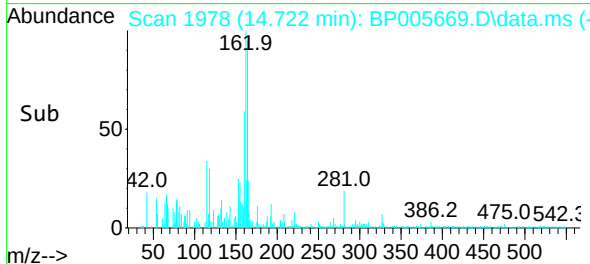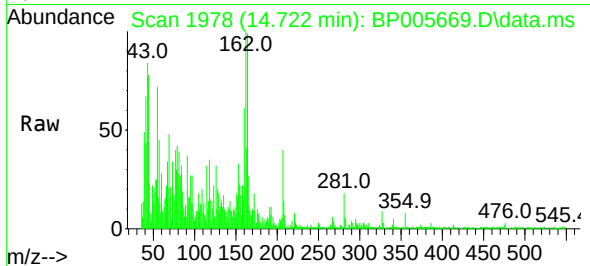

#56  
4-Nitrophenol  
Concen: 3.77 ng  
RT: 14.669 min Scan# 1969  
Delta R.T. -0.135 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:139 Resp: 344  
Ion Ratio Lower Upper  
139 100  
109 145.0 122.8 162.8  
65 112.2 110.0 150.0


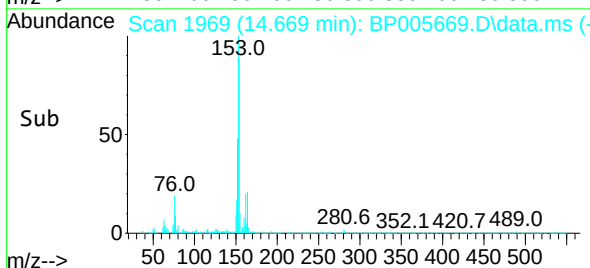
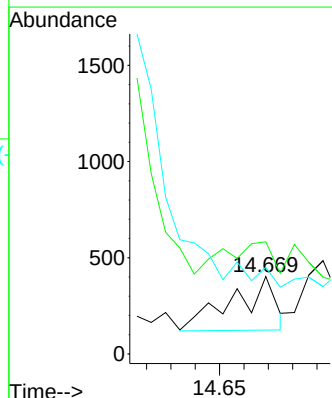
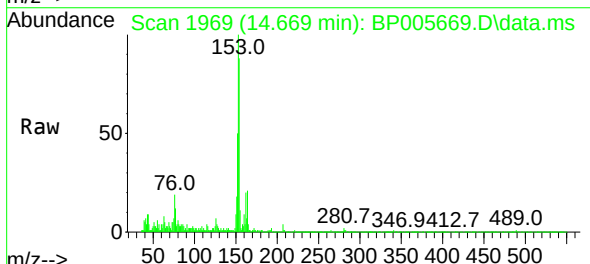




#57  
2,4-Dinitrotoluene  
Concen: 4.30 ng  
RT: 14.963 min Scan# 2019  
Delta R.T. 0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion:165 Resp: 681  
Ion Ratio Lower Upper  
165 100  
63 56.9 56.7 85.1  
89 48.8 85.8 128.6#  
182 56.2 3.0 4.6#

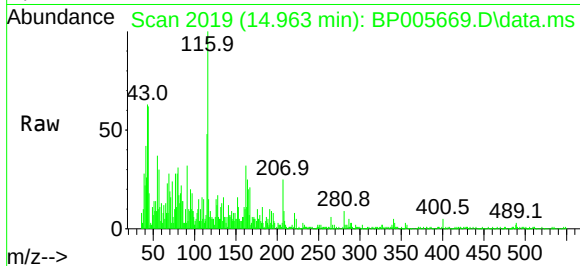

#62  
4-Nitroaniline  
Concen: 3.72 ng  
RT: 15.657 min Scan# 2137  
Delta R.T. -0.012 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:138 Resp: 1434  
Ion Ratio Lower Upper  
138 100  
92 43.5 50.9 90.9#  
108 72.1 154.7 194.7#




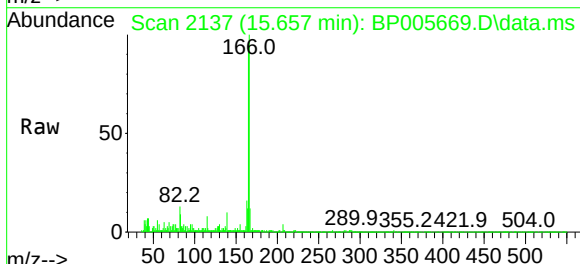




#64  
Phenanthrene-d10  
Concen: 20.00 ng  
RT: 17.351 min Scan# 2425  
Delta R.T. 0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion:188 Resp: 1613087  
Ion Ratio Lower Upper  
188 100  
94 7.9 5.0 7.6#  
80 8.7 5.9 8.9

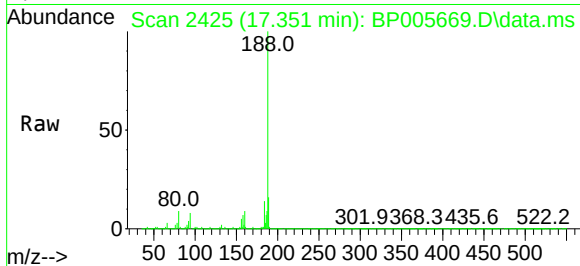

#71  
Phenanthrene  
Concen: 6.54 ng  
RT: 17.392 min Scan# 2432  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:178 Resp: 657085  
Ion Ratio Lower Upper  
178 100  
176 19.9 15.4 23.2  
179 15.9 12.3 18.5




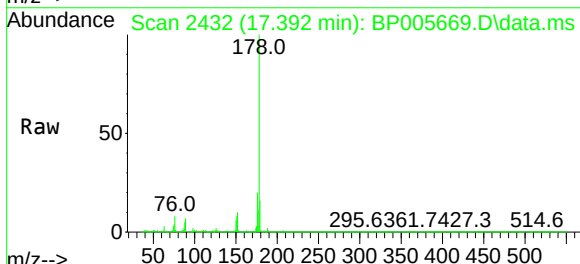




#75  
Fluoranthene  
Concen: 9.56 ng  
RT: 19.351 min Scan# 2765  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion:202 Resp: 1153434  
Ion Ratio Lower Upper  
202 100  
101 9.1 0.0 26.1  
203 17.8 0.0 37.2

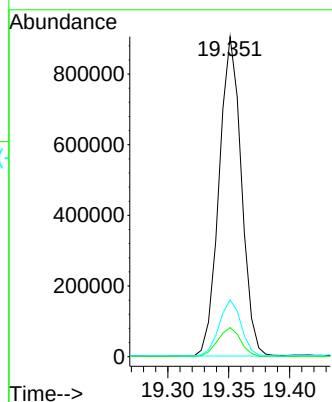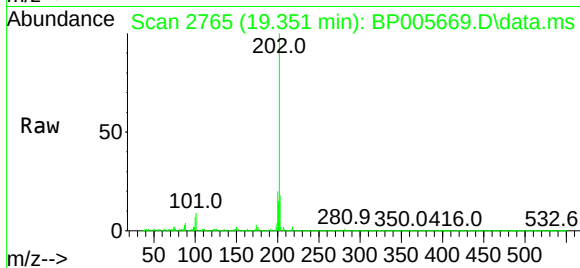

#76  
Chrysene-d12  
Concen: 20.00 ng  
RT: 21.422 min Scan# 3117  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:240 Resp: 1456766  
Ion Ratio Lower Upper  
240 100  
120 8.9 4.2 6.2#  
236 25.7 20.2 30.2


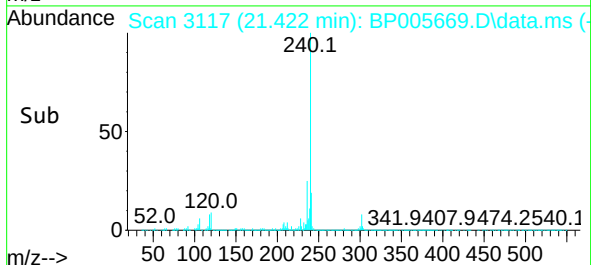

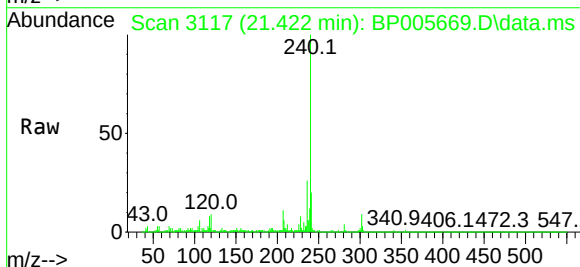




#78  
 Pyrene  
 Concen: 10.27 ng  
 RT: 19.704 min Scan# 2825  
 Delta R.T. 0.006 min  
 Lab File: BP005669.D  
 Acq: 02 Jun 2021 17:14




Instrument :  
 BNA\_P  
 ClientSampleId :  
 NB-07-060121


Tgt Ion:202 Resp: 1055400  
 Ion Ratio Lower Upper  
 202 100  
 200 21.5 16.9 25.3  
 203 18.4 13.8 20.6

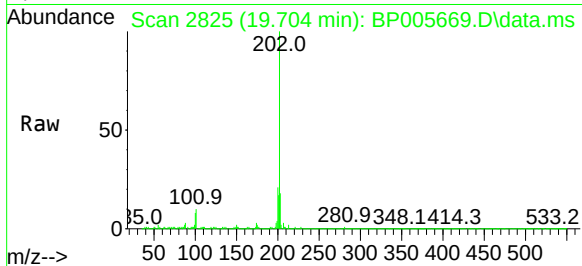

#79  
 Terphenyl-d14  
 Concen: 32.57 ng  
 RT: 19.898 min Scan# 2858  
 Delta R.T. -0.000 min  
 Lab File: BP005669.D  
 Acq: 02 Jun 2021 17:14

Tgt Ion:244 Resp: 2528167  
 Ion Ratio Lower Upper  
 244 100  
 212 6.9 5.8 8.6  
 122 8.3 5.2 7.8#




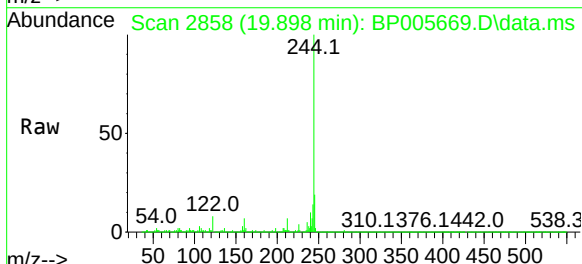




#80  
Butylbenzylphthalate  
Concen: 4.19 ng  
RT: 20.739 min Scan# 3001  
Delta R.T. 0.170 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion:149 Resp: 2889  
Ion Ratio Lower Upper  
149 100  
91 65.9 60.2 90.4  
206 31.2 23.9 35.9

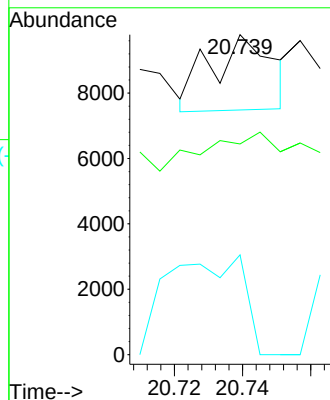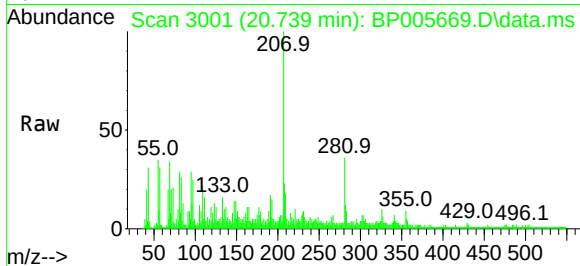

#81  
Benzo(a)anthracene  
Concen: 5.48 ng  
RT: 21.404 min Scan# 3114  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:228 Resp: 586177  
Ion Ratio Lower Upper  
228 100  
226 28.8 21.2 31.8  
229 21.3 15.6 23.4

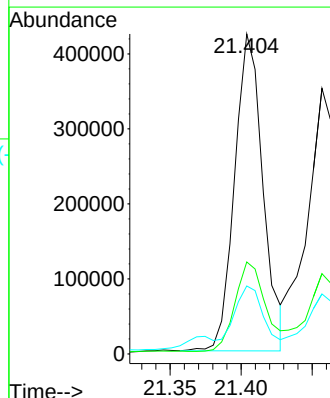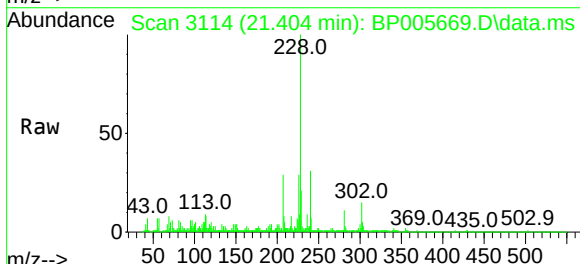



#83

Chrysene

Concen: 5.02 ng

RT: 21.457 min Scan# 3123

Delta R.T. -0.000 min

Lab File: BP005669.D

Acq: 02 Jun 2021 17:14





Tgt Ion:228 Resp: 520191

Ion Ratio Lower Upper

228 100

226 30.2 24.8 37.2

229 22.6 15.4 23.0

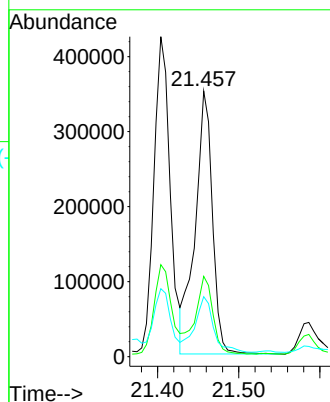

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.868 min Scan# 3533

Delta R.T. 0.006 min

Lab File: BP005669.D

Acq: 02 Jun 2021 17:14




Tgt Ion:264 Resp: 1638912

Ion Ratio Lower Upper


264 100

260 24.0 20.6 30.8

265 22.8 19.0 28.6

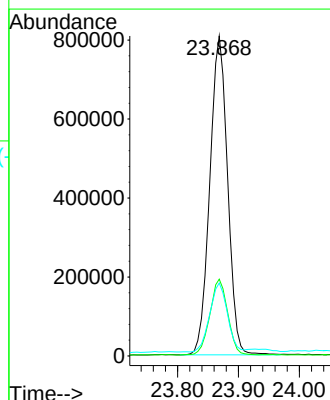







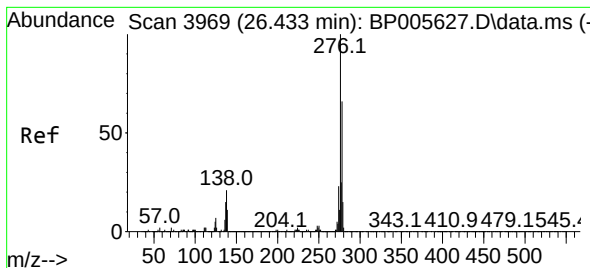

#87  
Indeno(1,2,3-cd)pyrene  
Concen: 2.70 ng  
RT: 26.427 min Scan# 3968  
Delta R.T. -0.006 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion:276 Resp: 376397  
Ion Ratio Lower Upper  
276 100  
138 16.8 8.4 12.6#  
277 24.9 20.6 31.0

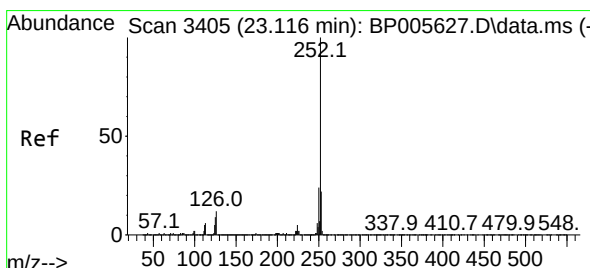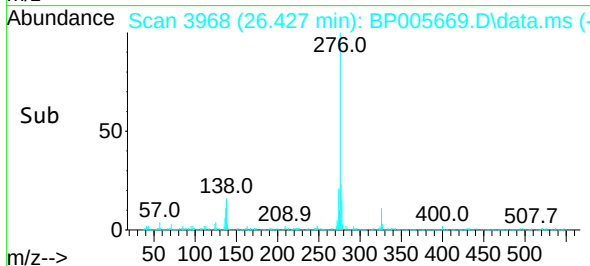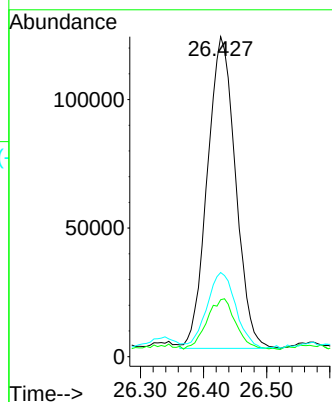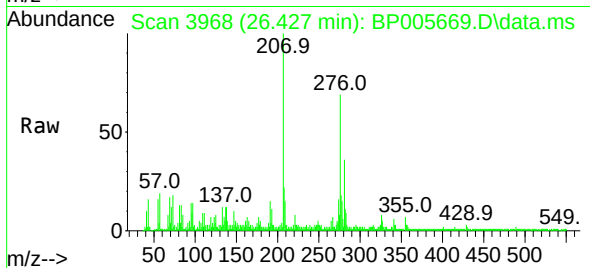

#88  
Benzo(b)fluoranthene  
Concen: 6.26 ng  
RT: 23.121 min Scan# 3406  
Delta R.T. 0.006 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14

Tgt Ion:252 Resp: 744296  
Ion Ratio Lower Upper  
252 100  
253 25.1 18.2 27.2  
125 12.2 3.4 5.0#


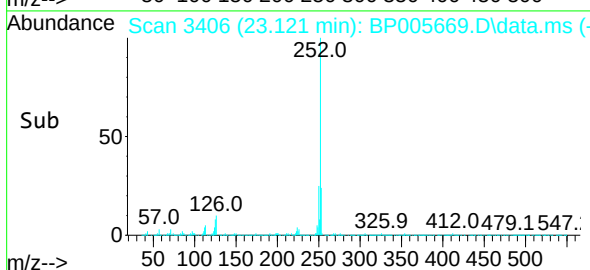

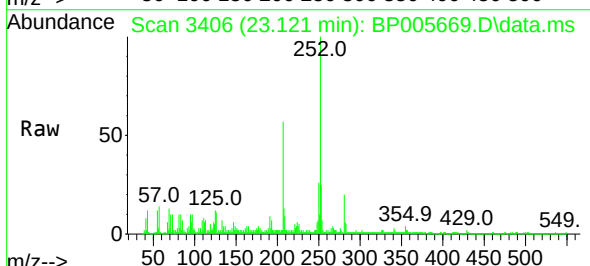




#89  
Benzo(k)fluoranthene  
Concen: 6.61 ng  
RT: 23.121 min Scan# 3406  
Delta R.T. -0.047 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14




Instrument :  
BNA\_P  
ClientSampleId :  
NB-07-060121


Tgt Ion:252 Resp: 744296  
Ion Ratio Lower Upper  
252 100  
253 25.1 17.2 25.8  
125 12.2 3.8 5.6#

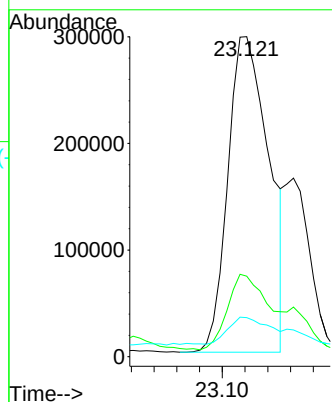

#90  
Benzo(a)pyrene  
Concen: 5.01 ng  
RT: 23.757 min Scan# 3514  
Delta R.T. -0.000 min  
Lab File: BP005669.D  
Acq: 02 Jun 2021 17:14


Tgt Ion:252 Resp: 542061  
Ion Ratio Lower Upper  
252 100  
253 24.0 17.1 25.7  
125 12.1 3.8 5.6#

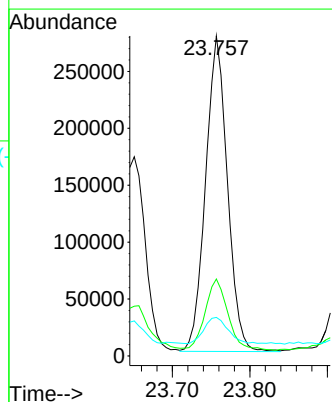



#92  
 Benzo(g,h,i)perylene  
 Concen: 3.14 ng  
 RT: 27.215 min Scan# 4102  
 Delta R.T. -0.012 min  
 Lab File: BP005669.D  
 Acq: 02 Jun 2021 17:14

Instrument :  
 BNA\_P  
 ClientSampleId :  
 NB-07-060121



Tgt Ion: 276 Resp: 366297  

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 276 | 100   |       |       |
| 277 | 25.3  | 19.8  | 29.8  |
| 138 | 17.4  | 7.7   | 11.5  |

