

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060221\
 Data File : BP005675.D
 Acq On : 02 Jun 2021 20:38
 Operator : CG/JU
 Sample : M2580-14 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 18-B5(2-4)

Quant Time: Jun 03 02:43:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.993	152	365272	20.00	ng	0.00
21) Naphthalene-d8	10.798	136	1405878	20.00	ng	# 0.00
39) Acenaphthene-d10	14.616	164	870719	20.00	ng	0.00
64) Phenanthrene-d10	17.357	188	1726298	20.00	ng	# 0.00
76) Chrysene-d12	21.427	240	1543444	20.00	ng	# 0.00
86) Perylene-d12	23.880	264	1757568	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.552	112	803460	34.20	ng	0.00
7) Phenol-d6	7.152	99	972901	30.38	ng	0.00
23) Nitrobenzene-d5	9.152	82	599337	23.71	ng	0.00
42) 2,4,6-Tribromophenol	16.098	330	545121	48.82	ng	0.00
45) 2-Fluorobiphenyl	13.245	172	1547646	23.52	ng	0.00
79) Terphenyl-d14	19.898	244	2122127	25.80	ng	0.00
Target Compounds						
						Qvalue
26) 2-Nitrophenol	9.910	139	49	4.16	ng	# 1
32) Benzoic acid	10.022	122	93	5.02	ng	# 45
48) 2-Nitroaniline	13.687	65	229	4.50	ng	# 63
50) Dimethylphthalate	14.069	163	177045	2.56	ng	98
51) 2,6-Dinitrotoluene	14.145	165	128	5.07	ng	90
52) Acenaphthene	14.675	154	172378	2.96	ng	97
53) 3-Nitroaniline	14.510	138	160	3.66	ng	# 69
54) 2,4-Dinitrophenol	14.710	184	164	6.55	ng	# 1
56) 4-Nitrophenol	14.822	139	3111	3.97	ng	# 12
57) 2,4-Dinitrotoluene	14.969	165	825	4.30	ng	# 33
58) Fluorene	15.657	166	213174	2.99	ng	99
62) 4-Nitroaniline	15.651	138	3237	3.82	ng	# 1
71) Phenanthrene	17.404	178	3775630	35.11	ng	100
72) Anthracene	17.492	178	1042679	9.82	ng	100
73) Carbazole	17.757	167	248772	2.38	ng	99
75) Fluoranthene	19.357	202	5182169	40.14	ng	95
78) Pyrene	19.710	202	4758115	43.69	ng	98
80) Butylbenzylphthalate	20.569	149	20404	4.55	ng	99
81) Benzo(a)anthracene	21.410	228	2650897	23.40	ng	97
83) Chrysene	21.463	228	2361238	21.53	ng	97
84) Bis(2-ethylhexyl)phtha...	21.327	149	172037	2.80	ng	99
87) Indeno(1,2,3-cd)pyrene	26.451	276	1706393	11.41	ng	# 95
88) Benzo(b)fluoranthene	23.133	252	3167871	24.84	ng	# 97
89) Benzo(k)fluoranthene	23.133	252	3167871	26.22	ng	# 95
90) Benzo(a)pyrene	23.768	252	2412324	20.79	ng	# 93
91) Dibenzo(a,h)anthracene	26.456	278	467619	3.60	ng	# 84
92) Benzo(g,h,i)perylene	27.251	276	1669798	13.34	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060221\
Data File : BP005675.D
Acq On : 02 Jun 2021 20:38
Operator : CG/JU
Sample : M2580-14 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)

Quant Time: Jun 03 02:43:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration




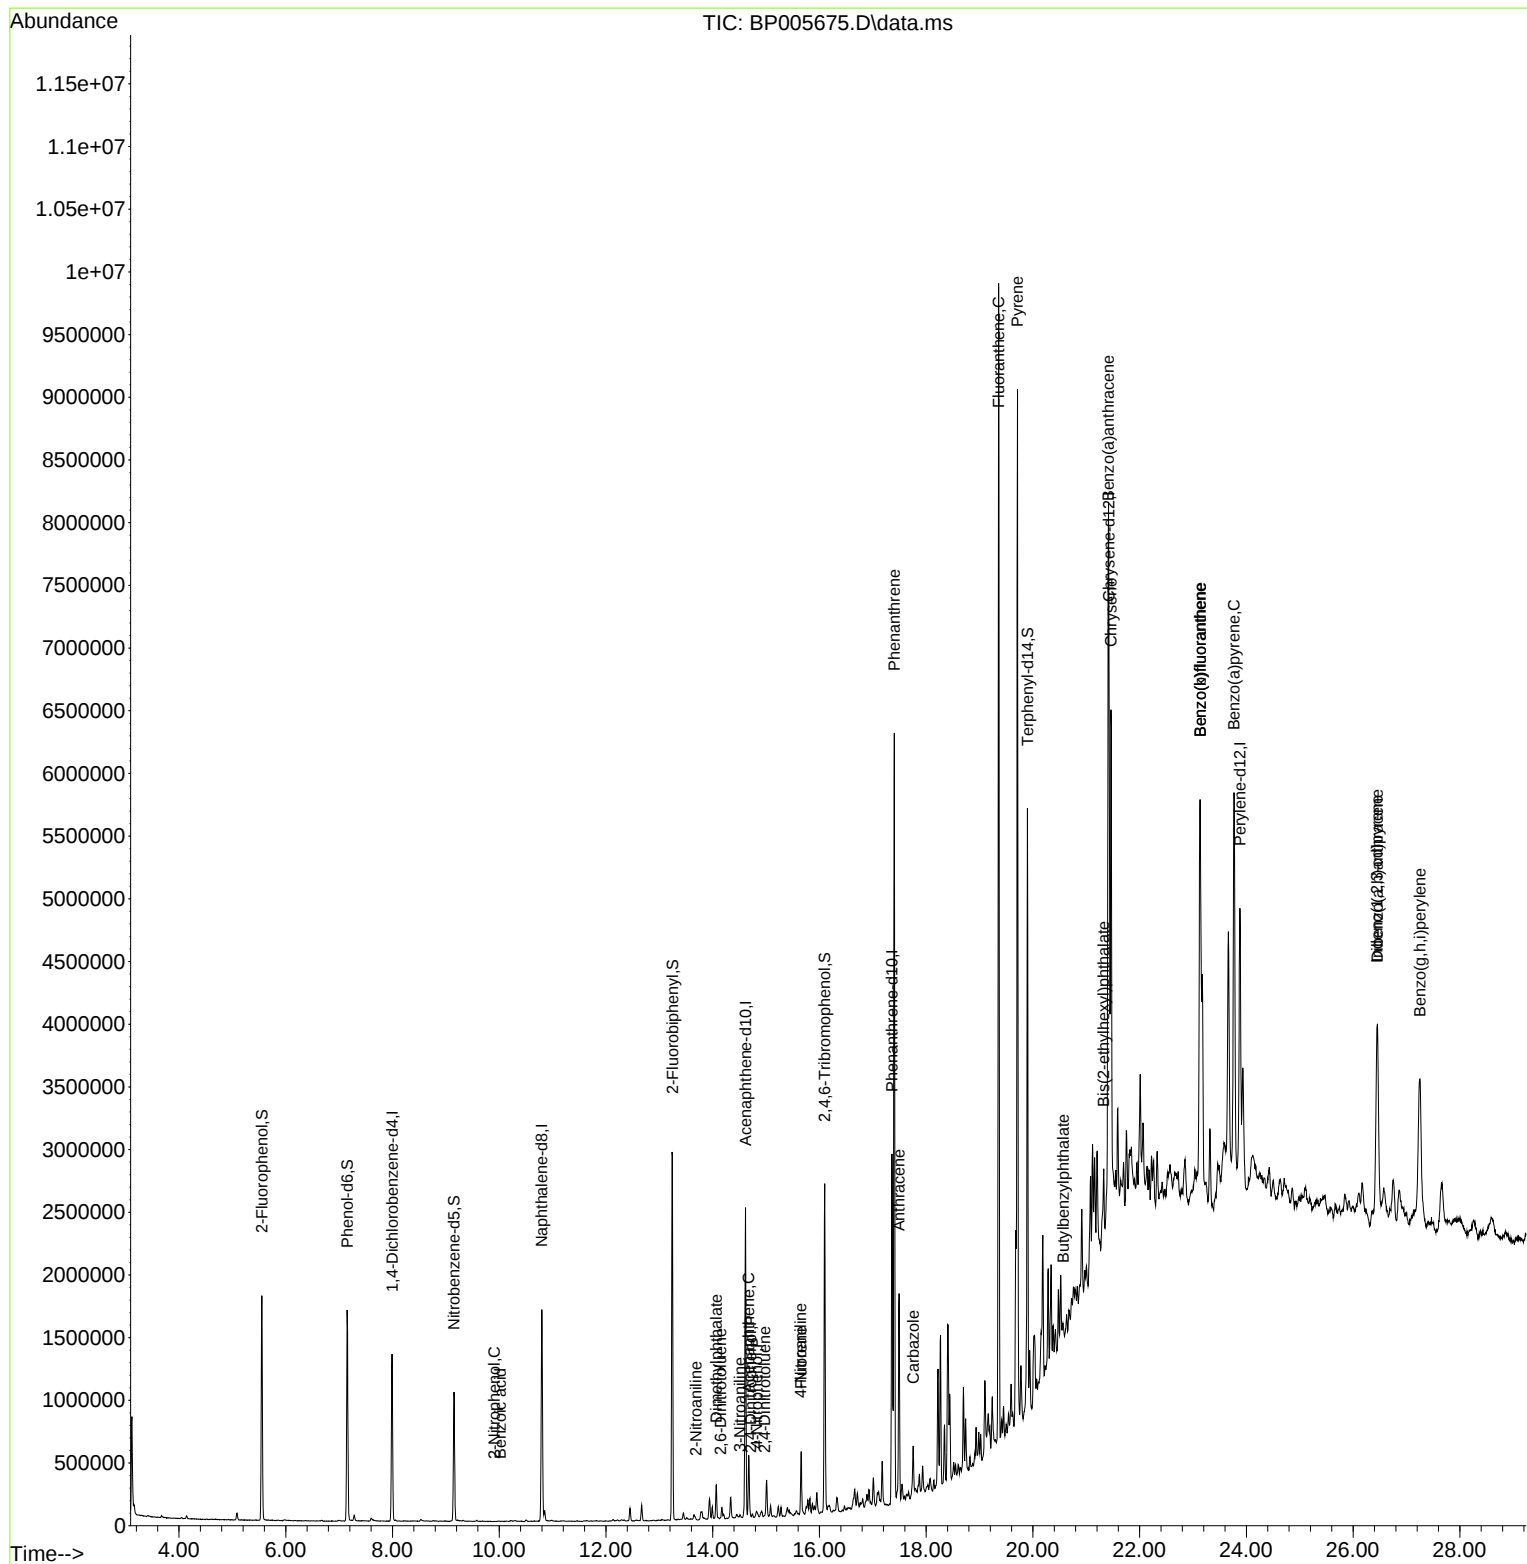




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.993 min Scan# 834
Delta R.T. -0.000 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:152 Resp: 365272
Ion Ratio Lower Upper
152 100
150 156.4 119.8 179.8
115 57.3 49.0 73.4



#5
2-Fluorophenol
Concen: 34.20 ng
RT: 5.552 min Scan# 419
Delta R.T. 0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:112 Resp: 803460
Ion Ratio Lower Upper
112 100
64 52.5 33.6 50.4#
63 28.2 18.6 27.8#


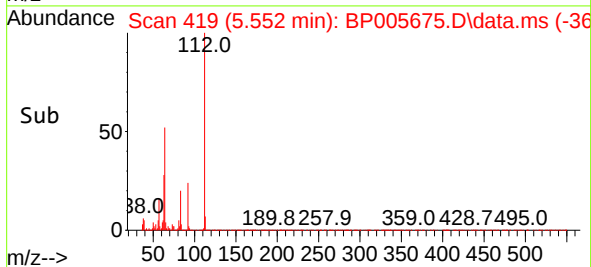

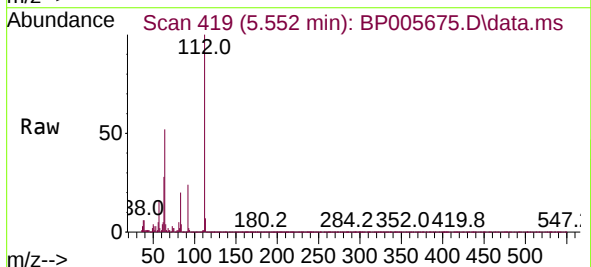




#7
Phenol-d6
Concen: 30.38 ng
RT: 7.152 min Scan# 691
Delta R.T. 0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion: 99 Resp: 972901
Ion Ratio Lower Upper
99 100
42 16.7 12.9 19.3
71 34.1 26.7 40.1



#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.798 min Scan# 1311
Delta R.T. -0.001 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:136 Resp: 1405878
Ion Ratio Lower Upper
136 100
137 10.9 8.9 13.3
54 6.3 5.0 7.4
68 5.5 3.7 5.5#



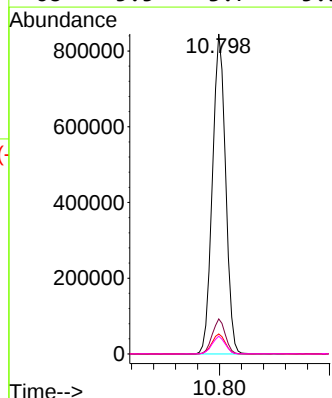





#23
Nitrobenzene-d5
Concen: 23.71 ng
RT: 9.152 min Scan# 1031
Delta R.T. -0.000 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion: 82 Resp: 599337
Ion Ratio Lower Upper
82 100
128 43.9 30.5 45.7
54 42.7 33.9 50.9



#26
2-Nitrophenol
Concen: 4.16 ng
RT: 9.910 min Scan# 1160
Delta R.T. -0.001 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion: 139 Resp: 49
Ion Ratio Lower Upper
139 100
109 118.9 40.7 61.1#
65 181.1 47.8 71.6#


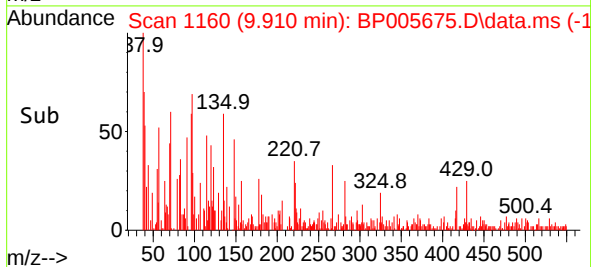

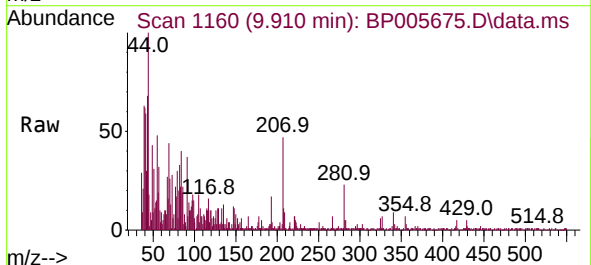




#32
Benzoic acid
Concen: 5.02 ng
RT: 10.022 min Scan# 1179
Delta R.T. -0.065 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:122 Resp: 93
Ion Ratio Lower Upper
122 100
105 105.8 105.1 145.1
77 191.5 69.6 109.6#

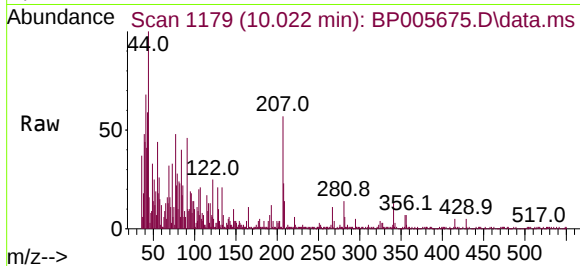

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.616 min Scan# 1960
Delta R.T. 0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:164 Resp: 870719
Ion Ratio Lower Upper
164 100
162 100.7 73.5 110.3
160 44.7 40.6 61.0




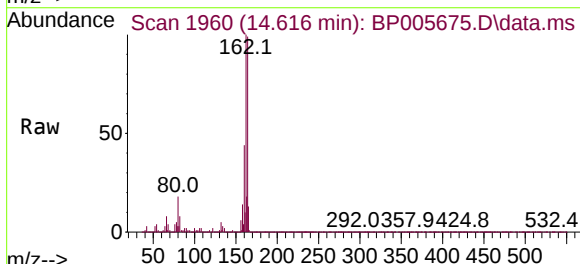




#42
2,4,6-Tribromophenol
Concen: 48.82 ng
RT: 16.098 min Scan# 2212
Delta R.T. 0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion: 330 Resp: 545121
Ion Ratio Lower Upper
330 100
332 96.6 76.3 114.5
141 24.9 22.8 34.2

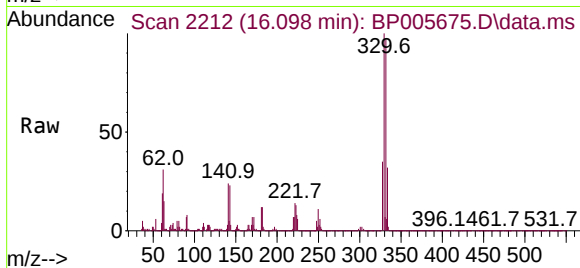

#45
2-Fluorobiphenyl
Concen: 23.52 ng
RT: 13.245 min Scan# 1727
Delta R.T. 0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion: 172 Resp: 1547646
Ion Ratio Lower Upper
172 100
171 34.7 28.1 42.1
170 23.2 19.6 29.4


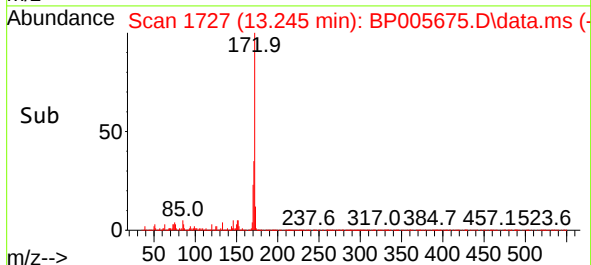

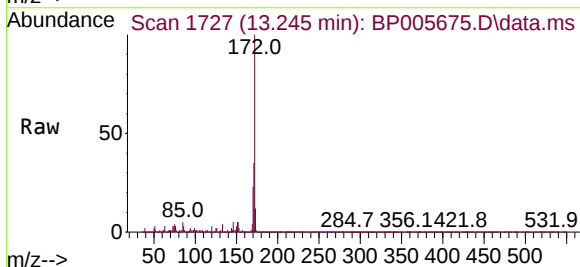




#48
2-Nitroaniline
Concen: 4.50 ng
RT: 13.687 min Scan# 1802
Delta R.T. -0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion: 65 Resp: 229
Ion Ratio Lower Upper
65 100
92 76.2 48.8 73.2#
138 41.9 69.5 104.3#

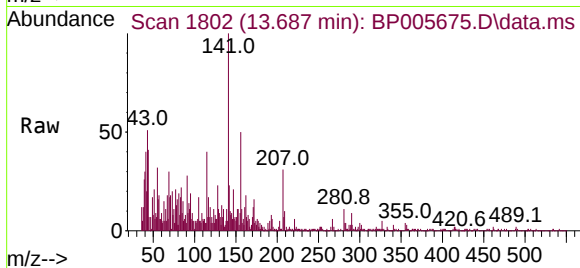

#50
Dimethylphthalate
Concen: 2.56 ng
RT: 14.069 min Scan# 1867
Delta R.T. -0.000 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion: 163 Resp: 177045
Ion Ratio Lower Upper
163 100
194 4.6 3.9 5.9
164 9.3 8.1 12.1




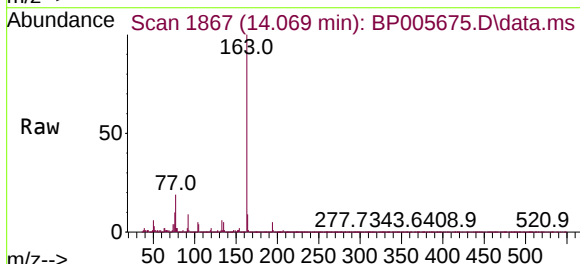




#51
2,6-Dinitrotoluene
Concen: 5.07 ng
RT: 14.145 min Scan# 1880
Delta R.T. -0.042 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:165	Resp:	128
Ion Ratio	Lower	Upper
165	100	
63	94.1	67.4 101.0
89	83.3	73.8 110.6

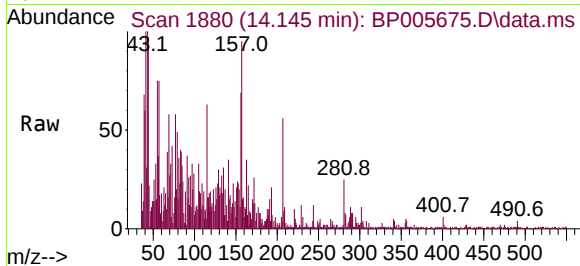

#52
Acenaphthene
Concen: 2.96 ng
RT: 14.675 min Scan# 1970
Delta R.T. -0.000 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:154	Resp:	172378
Ion Ratio	Lower	Upper
154	100	
153	113.2	90.9 136.3
152	54.2	48.5 72.7




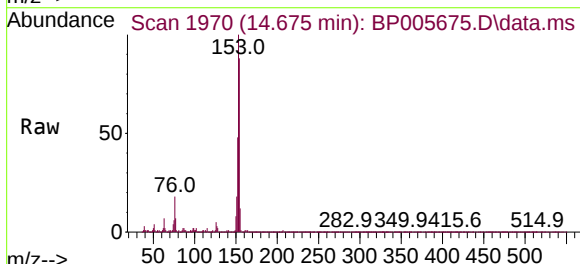




#53
3-Nitroaniline
Concen: 3.66 ng
RT: 14.510 min Scan# 1942
Delta R.T. 0.000 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:138 Resp: 160
Ion Ratio Lower Upper
138 100
108 55.2 10.2 15.4#
92 106.6 108.1 162.1#



#54
2,4-Dinitrophenol
Concen: 6.55 ng
RT: 14.710 min Scan# 1976
Delta R.T. 0.000 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:184 Resp: 164
Ion Ratio Lower Upper
184 100
63 216.4 51.2 76.8#
154 797.3 55.8 83.8#



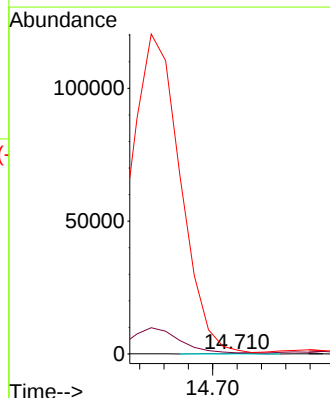





#56
4-Nitrophenol
Concen: 3.97 ng
RT: 14.822 min Scan# 1995
Delta R.T. 0.018 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:139 Resp: 3111
Ion Ratio Lower Upper
139 100
109 34.8 122.8 162.8#
65 26.7 110.0 150.0#

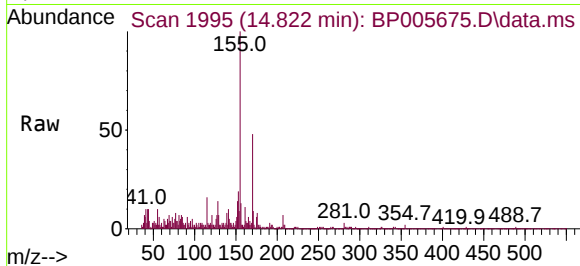

#57
2,4-Dinitrotoluene
Concen: 4.30 ng
RT: 14.969 min Scan# 2020
Delta R.T. 0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:165 Resp: 825
Ion Ratio Lower Upper
165 100
63 31.9 56.7 85.1#
89 34.1 85.8 128.6#
182 118.0 3.0 4.6#




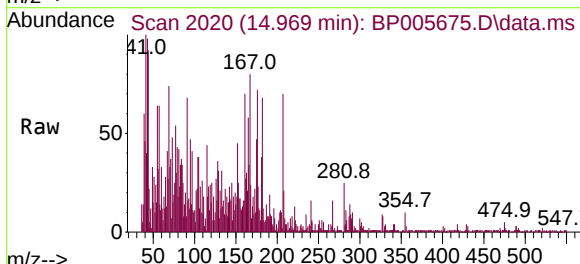




#58
Fluorene
Concen: 2.99 ng
RT: 15.657 min Scan# 2137
Delta R.T. -0.000 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:166 Resp: 213174
Ion Ratio Lower Upper
166 100
165 98.8 78.8 118.2
167 14.4 10.9 16.3

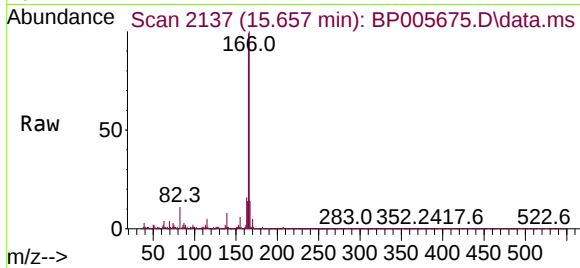

#62
4-Nitroaniline
Concen: 3.82 ng
RT: 15.651 min Scan# 2136
Delta R.T. -0.018 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:138 Resp: 3237
Ion Ratio Lower Upper
138 100
92 13.7 50.9 90.9#
108 15.9 154.7 194.7#




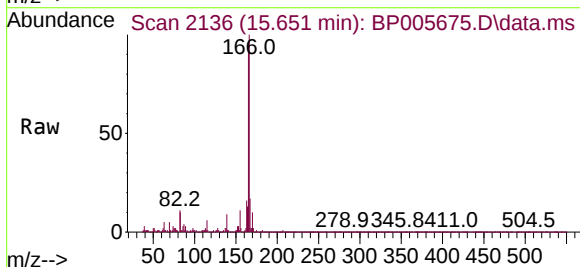




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.357 min Scan# 2426
Delta R.T. 0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:188 Resp: 1726298
Ion Ratio Lower Upper
188 100
94 8.0 5.0 7.6#
80 8.6 5.9 8.9

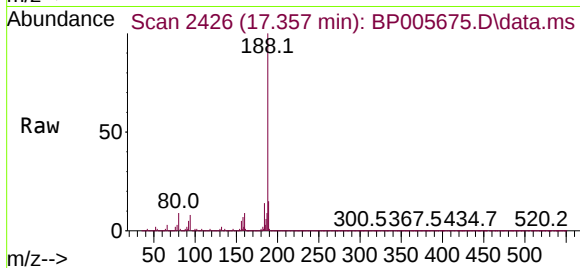

#71
Phenanthrene
Concen: 35.11 ng
RT: 17.404 min Scan# 2434
Delta R.T. 0.012 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:178 Resp: 3775630
Ion Ratio Lower Upper
178 100
176 19.6 15.4 23.2
179 15.4 12.3 18.5

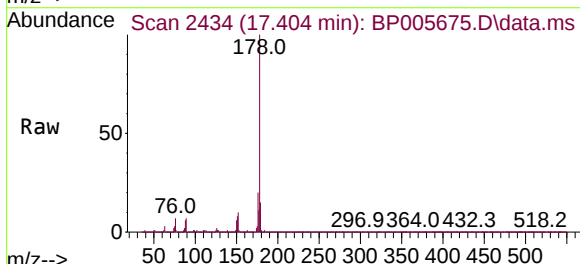



#72

Anthracene

Concen: 9.82 ng

RT: 17.492 min Scan# 2449





Delta R.T. 0.006 min

Lab File: BP005675.D

Acq: 02 Jun 2021 20:38

Tgt Ion:178 Resp: 1042679

Ion	Ratio	Lower	Upper
178	100		
176	18.7	15.2	22.8
179	15.9	12.6	19.0

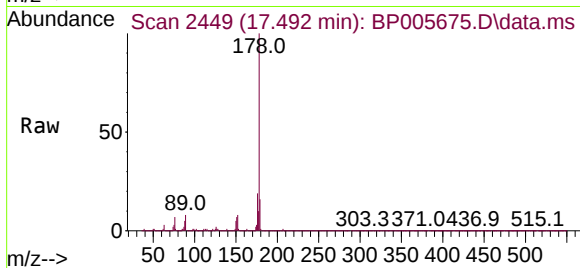

#73

Carbazole

Concen: 2.38 ng

RT: 17.757 min Scan# 2494




Delta R.T. 0.006 min


Lab File: BP005675.D

Acq: 02 Jun 2021 20:38

Tgt Ion:167 Resp: 248772

Ion	Ratio	Lower	Upper
167	100		
166	22.4	17.4	26.0
139	12.5	10.4	15.6




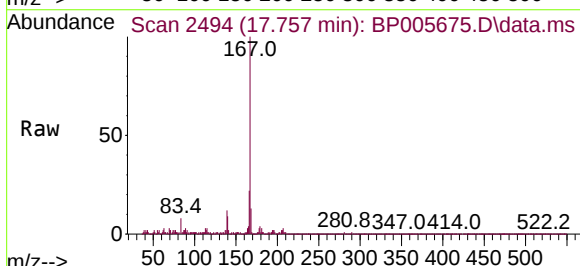




#75
Fluoranthene
Concen: 40.14 ng
RT: 19.357 min Scan# 2766
Delta R.T. 0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:202 Resp: 5182169
Ion Ratio Lower Upper
202 100
101 9.3 0.0 26.1
203 18.4 0.0 37.2



#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.427 min Scan# 3118
Delta R.T. 0.005 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:240 Resp: 1543444
Ion Ratio Lower Upper
240 100
120 9.1 4.2 6.2#
236 26.5 20.2 30.2









#78
Pyrene
Concen: 43.69 ng
RT: 19.710 min Scan# 2826
Delta R.T. 0.012 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:202 Resp: 4758115
Ion Ratio Lower Upper
202 100
200 21.9 16.9 25.3
203 18.4 13.8 20.6



#79
Terphenyl-d14
Concen: 25.80 ng
RT: 19.898 min Scan# 2858
Delta R.T. -0.000 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:244 Resp: 2122127
Ion Ratio Lower Upper
244 100
212 7.1 5.8 8.6
122 8.6 5.2 7.8#









#80
Butylbenzylphthalate
Concen: 4.55 ng
RT: 20.569 min Scan# 2972
Delta R.T. -0.000 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:	149	Resp:	20404
Ion Ratio	Lower	Upper	
149	100		
91	75.9	60.2	90.4
206	29.7	23.9	35.9

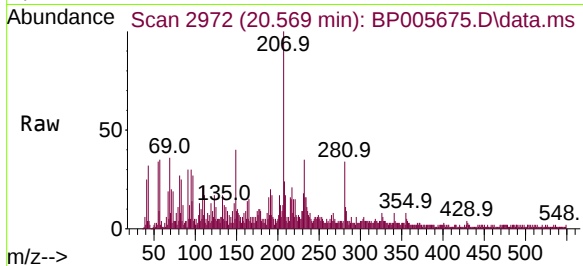

#81
Benzo(a)anthracene
Concen: 23.40 ng
RT: 21.410 min Scan# 3115
Delta R.T. 0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:	228	Resp:	2650897
Ion Ratio	Lower	Upper	
228	100		
226	27.9	21.2	31.8
229	21.0	15.6	23.4




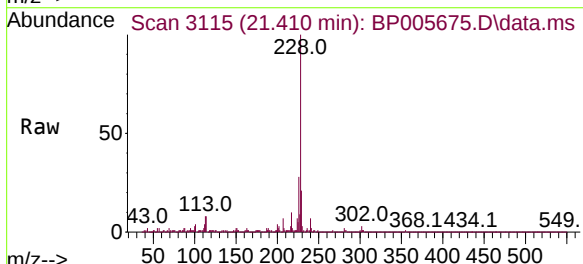




#83
Chrysene
Concen: 21.53 ng
RT: 21.463 min Scan# 3124
Delta R.T. 0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:228 Resp: 2361238
Ion Ratio Lower Upper
228 100
226 30.9 24.8 37.2
229 22.6 15.4 23.0

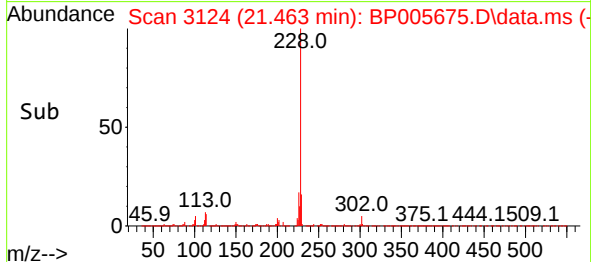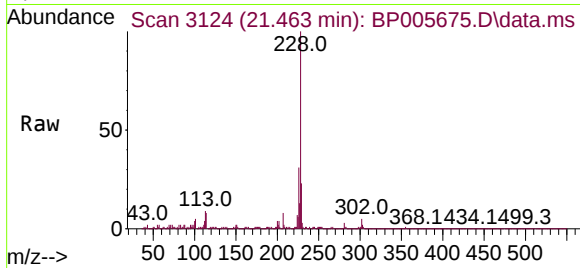

#84
Bis(2-ethylhexyl)phthalate
Concen: 2.80 ng
RT: 21.327 min Scan# 3101
Delta R.T. -0.000 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:149 Resp: 172037
Ion Ratio Lower Upper
149 100
167 30.1 23.8 35.8
279 7.6 5.7 8.5

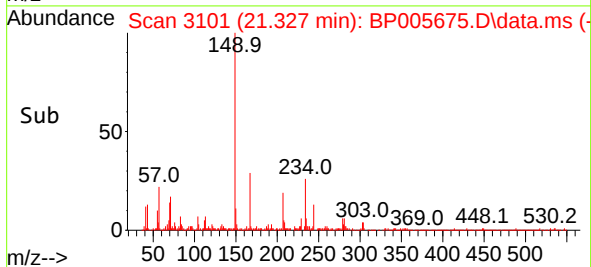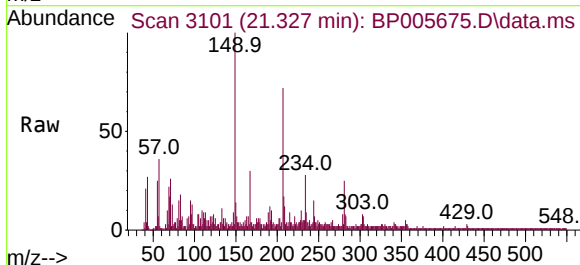



#86

Perylene-d12

Concen: 20.00 ng

RT: 23.880 min Scan# 3535





Delta R.T. 0.017 min

Lab File: BP005675.D

Acq: 02 Jun 2021 20:38

Tgt Ion:264 Resp: 1757568

Ion	Ratio	Lower	Upper
264	100		
260	24.1	20.6	30.8
265	22.9	19.0	28.6

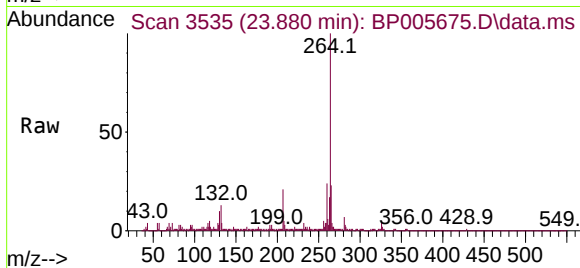

#87

Indeno(1,2,3-cd)pyrene

Concen: 11.41 ng

RT: 26.451 min Scan# 3972




Delta R.T. 0.017 min


Lab File: BP005675.D

Acq: 02 Jun 2021 20:38

Tgt Ion:276 Resp: 1706393

Ion	Ratio	Lower	Upper
276	100		
138	16.2	8.4	12.6
277	25.3	20.6	31.0



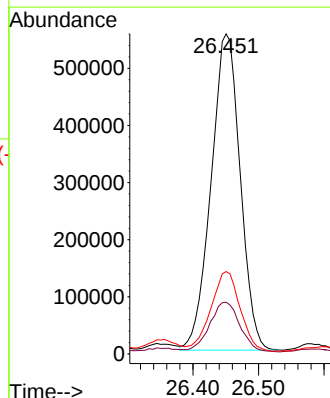
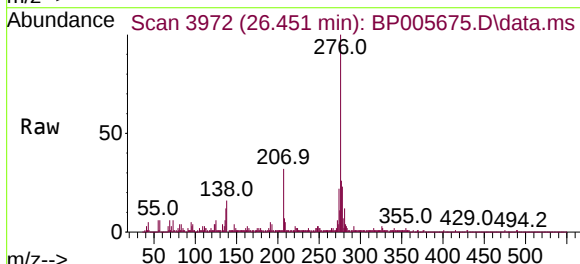




#88
Benzo(b)fluoranthene
Concen: 24.84 ng
RT: 23.133 min Scan# 3408
Delta R.T. 0.017 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:252 Resp: 3167871
Ion Ratio Lower Upper
252 100
253 23.3 18.2 27.2
125 8.4 3.4 5.0#

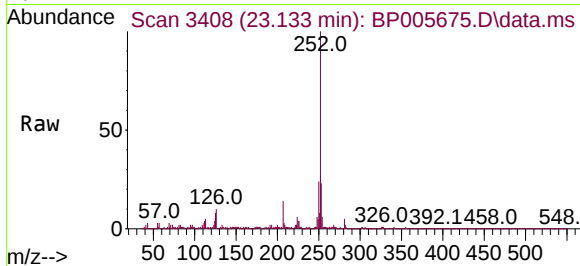

#89
Benzo(k)fluoranthene
Concen: 26.22 ng
RT: 23.133 min Scan# 3408
Delta R.T. -0.035 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Tgt Ion:252 Resp: 3167871
Ion Ratio Lower Upper
252 100
253 23.3 17.2 25.8
125 8.4 3.8 5.6#




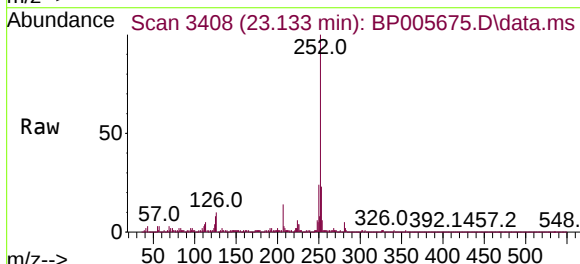


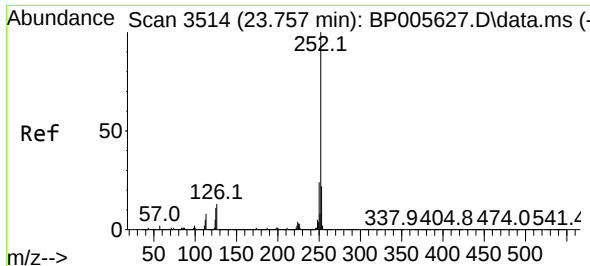

#90
Benzo(a)pyrene
Concen: 20.79 ng
RT: 23.768 min Scan# 3516
Delta R.T. 0.012 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38




Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)


Tgt Ion:252 Resp: 2412324
Ion Ratio Lower Upper
252 100
253 23.9 17.1 25.7
125 9.4 3.8 5.6#

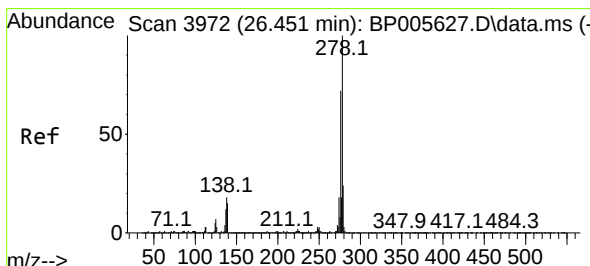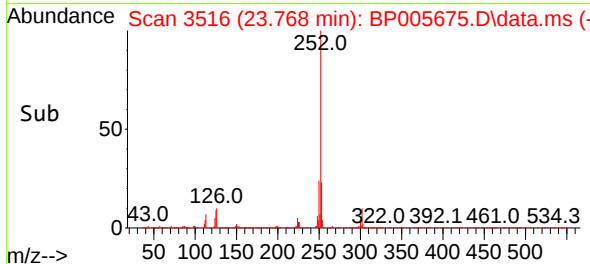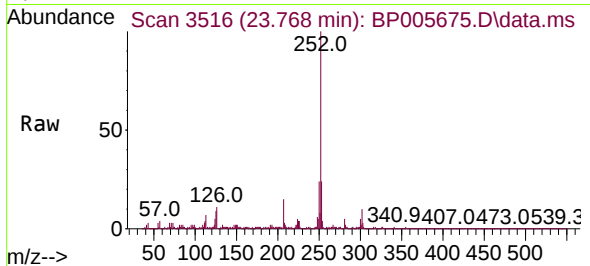

#91
Dibenzo(a,h)anthracene
Concen: 3.60 ng
RT: 26.456 min Scan# 3973
Delta R.T. 0.006 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38


Tgt Ion:278 Resp: 467619
Ion Ratio Lower Upper
278 100
139 0.0 5.0 7.6#
279 30.6 18.6 28.0#

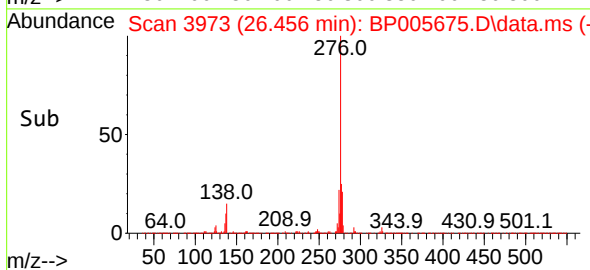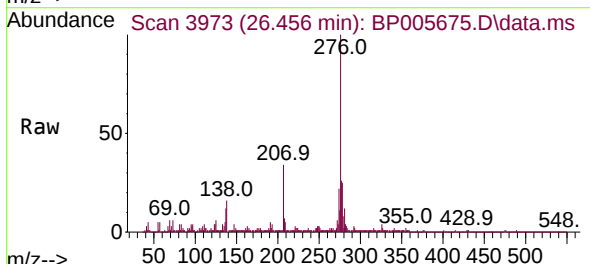



#92
Benzo(g,h,i)perylene
Concen: 13.34 ng
RT: 27.251 min Scan# 4108
Delta R.T. 0.023 min
Lab File: BP005675.D
Acq: 02 Jun 2021 20:38

Instrument :
BNA_P
ClientSampleId :
18-B5(2-4)



Tgt Ion:276 Resp: 1669798
Ion Ratio Lower Upper
276 100
277 24.6 19.8 29.8
138 16.4 7.7 11.5#

