
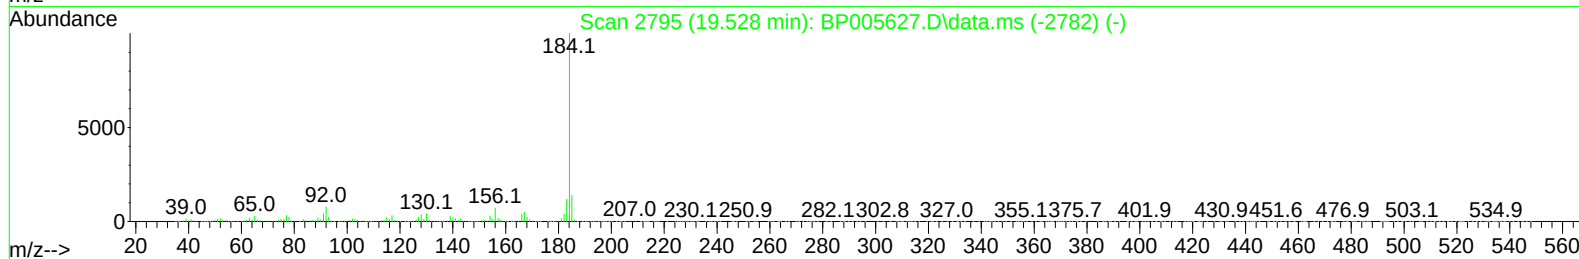
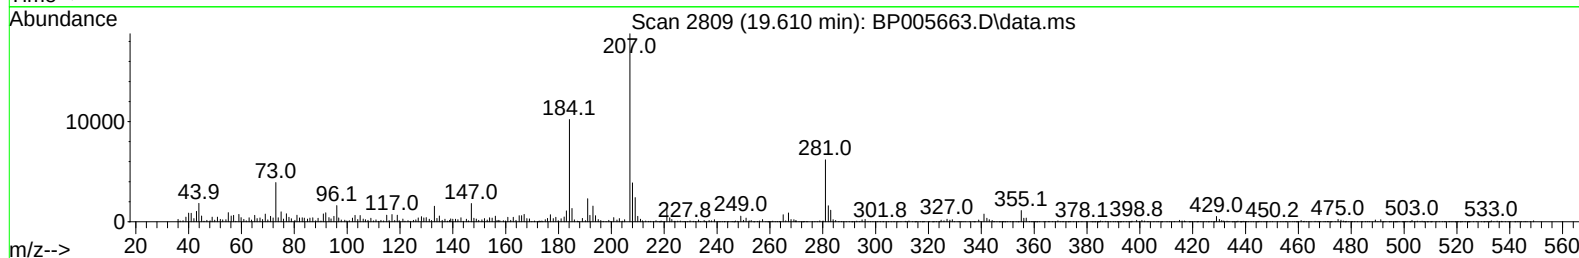


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060221\
Data File : BP005663.D
Acq On : 02 Jun 2021 13:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 14:02:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration

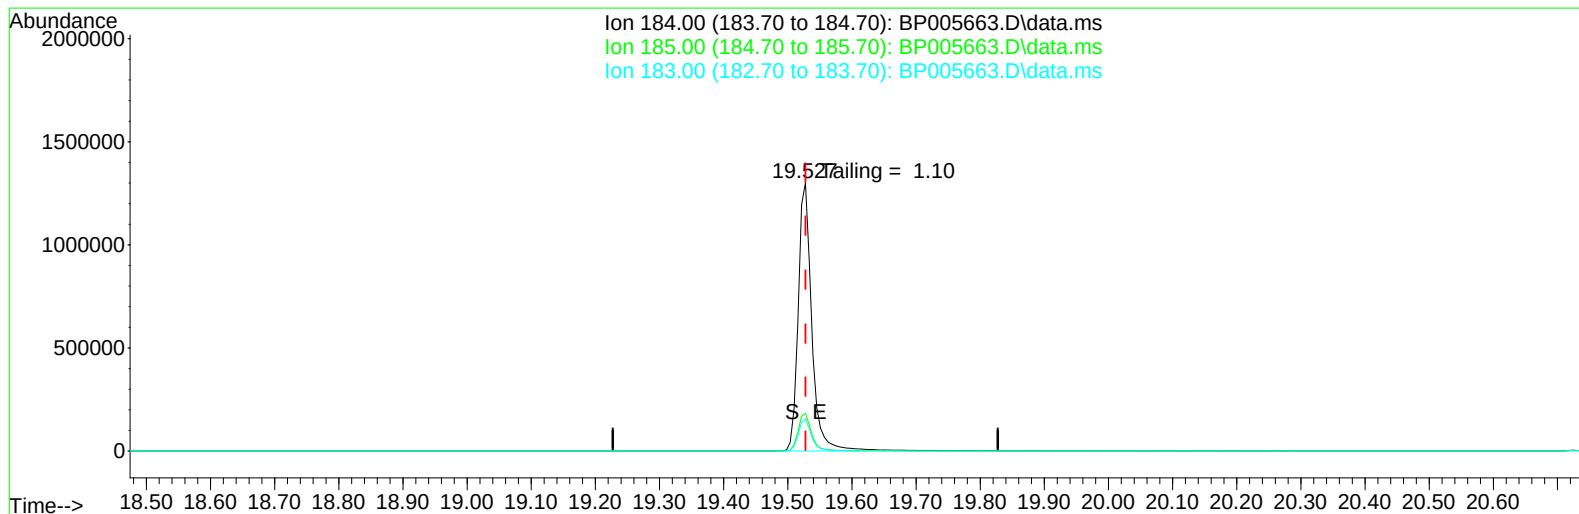




TIC: BP005663.D\data.ms

(77) Benzidine**19.527min (-0.000) 949883.69 ng****response 1912190**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.09
183.00	12.30	11.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060221\
Data File : BP005663.D
Acq On : 02 Jun 2021 13:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 14:02:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration

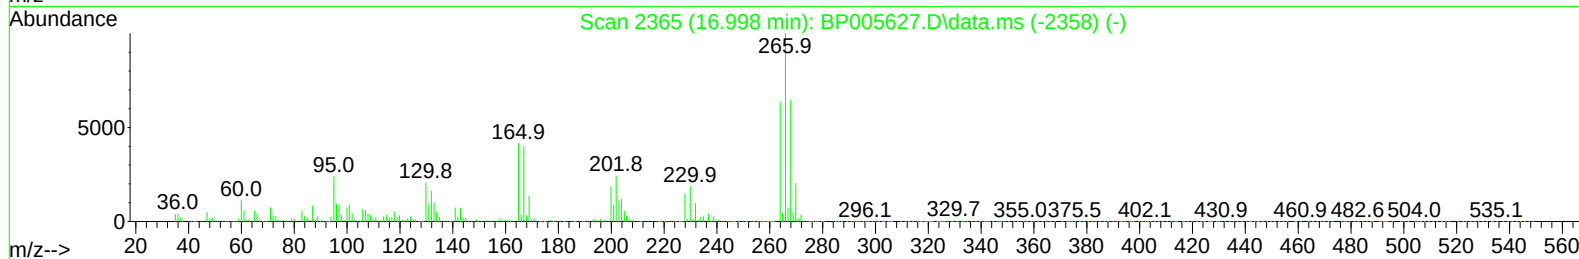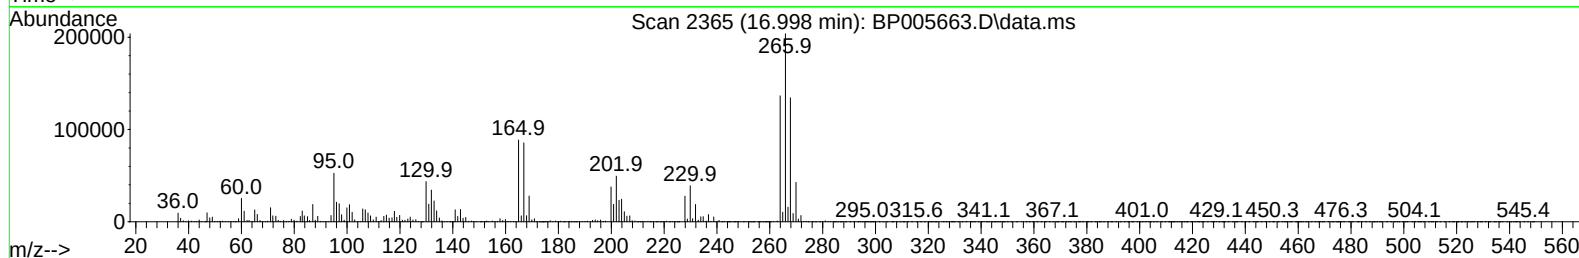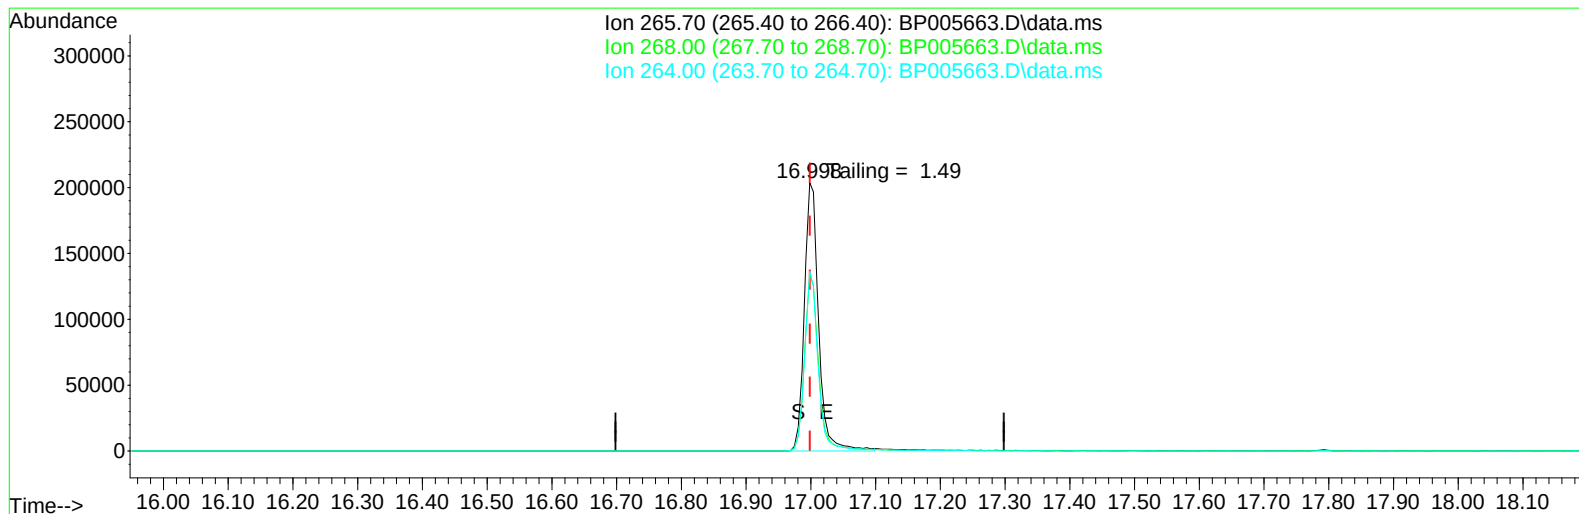

TIC: BP005663.D\data.ms

(70) Pentachlorophenol (C)

16.998min (-0.000) 2604027.80 ng

response 318470

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.92
264.00	67.10	66.96
0.00	0.00	0.00