

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060221\
 Data File : BP005679.D
 Acq On : 02 Jun 2021 22:54
 Operator : CG/JU
 Sample : M2580-02 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 18-B1(2-4)

Quant Time: Jun 03 02:44:54 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.993	152	341055	20.00	ng	0.00
21) Naphthalene-d8	10.804	136	1334318	20.00	ng	0.00
39) Acenaphthene-d10	14.616	164	827002	20.00	ng	0.00
64) Phenanthrene-d10	17.357	188	1584481	20.00	ng	# 0.00
76) Chrysene-d12	21.427	240	1358040	20.00	ng	# 0.00
86) Perylene-d12	23.880	264	1552993	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.552	112	149552	6.82	ng	0.00
7) Phenol-d6	7.152	99	182836	6.11	ng	0.00
23) Nitrobenzene-d5	9.158	82	107996	4.50	ng	0.00
42) 2,4,6-Tribromophenol	16.098	330	80106	7.55	ng	0.00
45) 2-Fluorobiphenyl	13.246	172	305355	4.89	ng	0.00
79) Terphenyl-d14	19.898	244	405952	5.61	ng	0.00
Target Compounds						Qvalue
71) Phenanthrene	17.404	178	296011	3.00	ng	99
75) Fluoranthene	19.357	202	477007	4.03	ng	97
78) Pyrene	19.710	202	409485	4.27	ng	98
81) Benzo(a)anthracene	21.410	228	237001	2.38	ng	# 93
83) Chrysene	21.463	228	211908	2.20	ng	# 93
88) Benzo(b)fluoranthene	23.127	252	306998	2.72	ng	# 76
90) Benzo(a)pyrene	23.768	252	237777	2.32	ng	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060221\
Data File : BP005679.D
Acq On : 02 Jun 2021 22:54
Operator : CG/JU
Sample : M2580-02 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)

Quant Time: Jun 03 02:44:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration




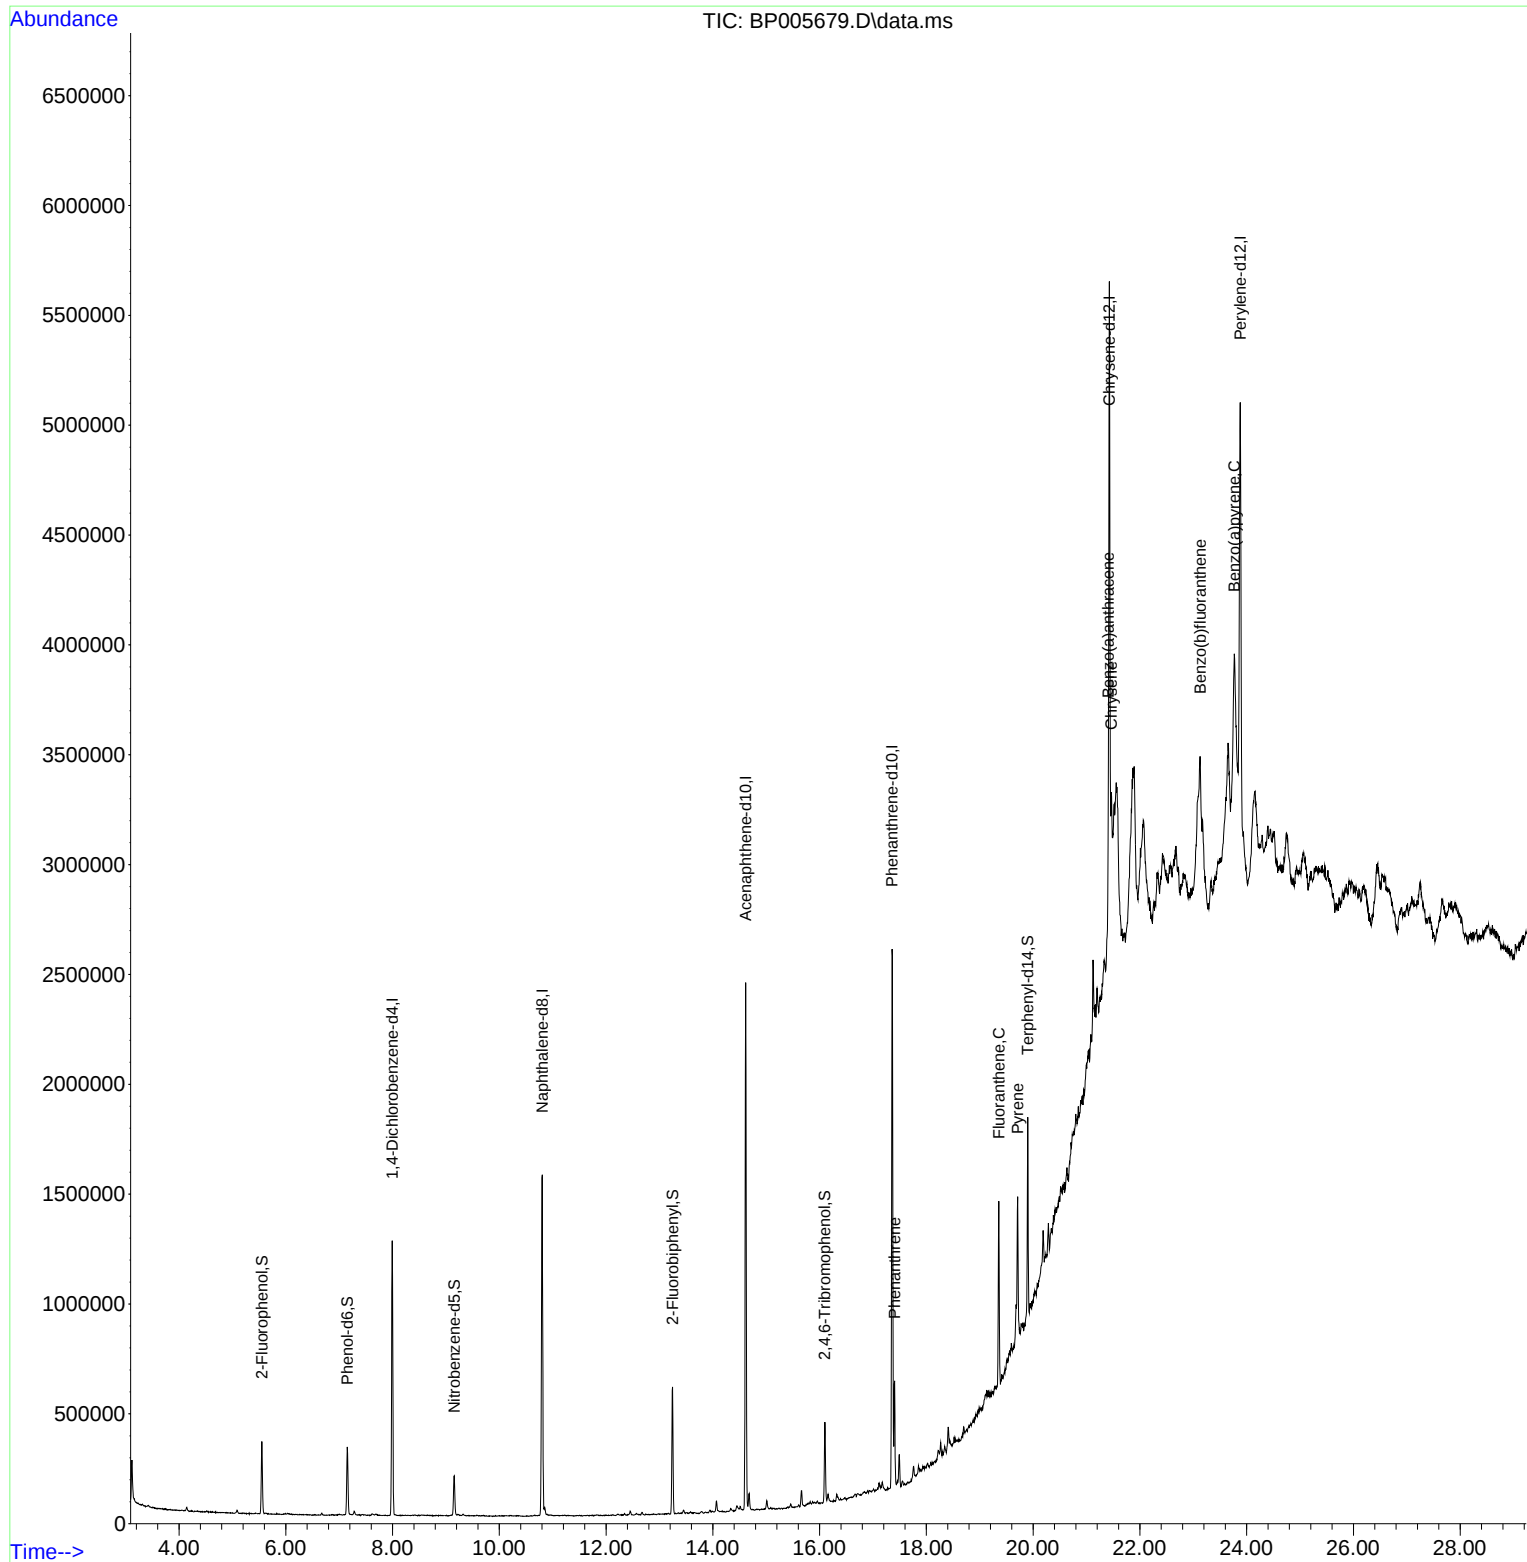




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.993 min Scan# 834
Delta R.T. -0.000 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54




Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)


Tgt Ion:152 Resp: 341055
Ion Ratio Lower Upper
152 100
150 154.6 119.8 179.8
115 56.5 49.0 73.4

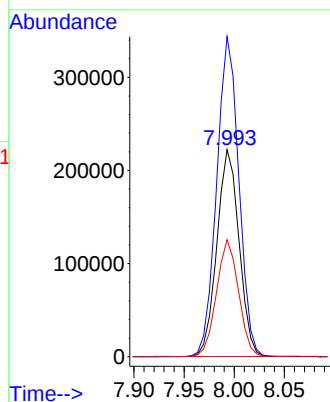

#5
2-Fluorophenol
Concen: 6.82 ng
RT: 5.552 min Scan# 419
Delta R.T. 0.006 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54

Tgt Ion:112 Resp: 149552
Ion Ratio Lower Upper
112 100
64 54.3 33.6 50.4#
63 28.2 18.6 27.8#


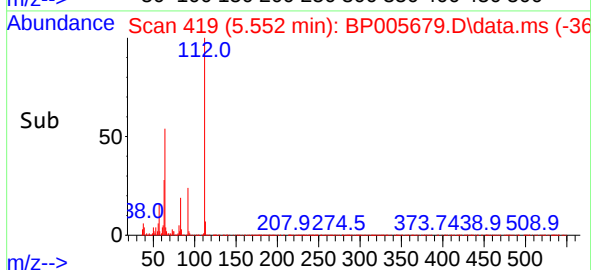
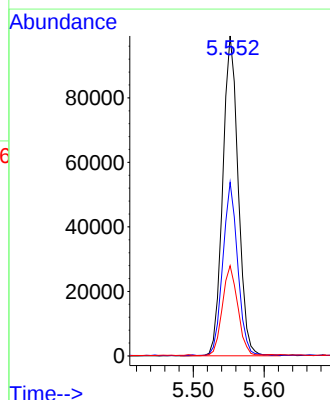





#7
Phenol-d6
Concen: 6.11 ng
RT: 7.152 min Scan# 691
Delta R.T. 0.006 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54




Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)


Tgt Ion: 99 Resp: 182836
Ion Ratio Lower Upper
99 100
42 17.9 12.9 19.3
71 34.2 26.7 40.1

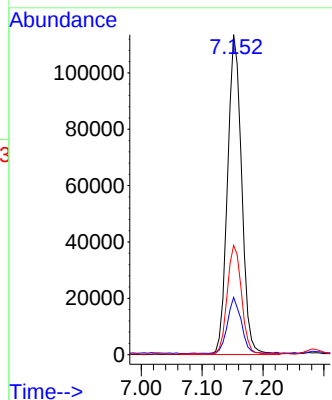

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.804 min Scan# 1312
Delta R.T. 0.005 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54

Tgt Ion:136 Resp: 1334318
Ion Ratio Lower Upper
136 100
137 11.0 8.9 13.3
54 6.1 5.0 7.4
68 5.4 3.7 5.5


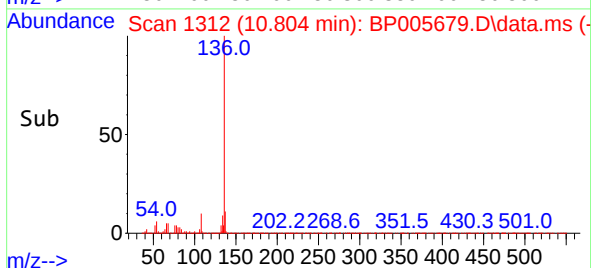
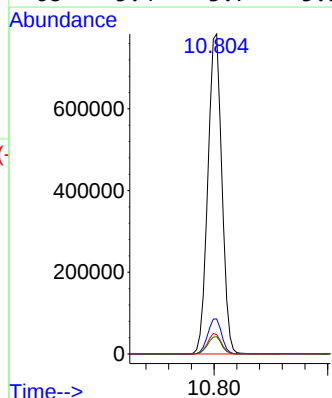





#23
Nitrobenzene-d5
Concen: 4.50 ng
RT: 9.158 min Scan# 1032
Delta R.T. 0.006 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54




Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)


Tgt Ion: 82 Resp: 107996
Ion Ratio Lower Upper
82 100
128 44.2 30.5 45.7
54 43.9 33.9 50.9

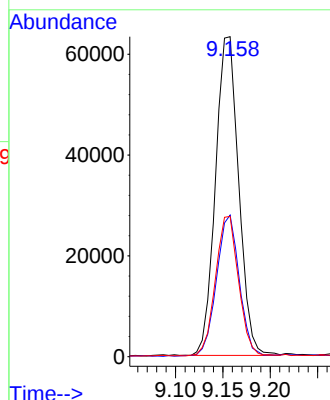

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.616 min Scan# 1960
Delta R.T. 0.006 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54

Tgt Ion: 164 Resp: 827002
Ion Ratio Lower Upper
164 100
162 99.9 73.5 110.3
160 43.5 40.6 61.0


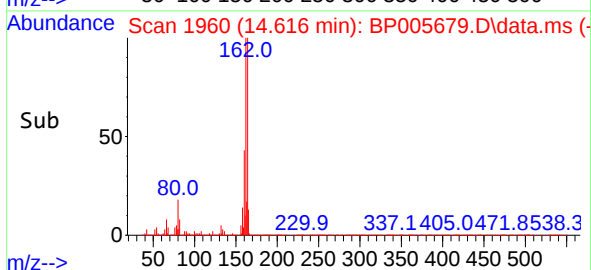
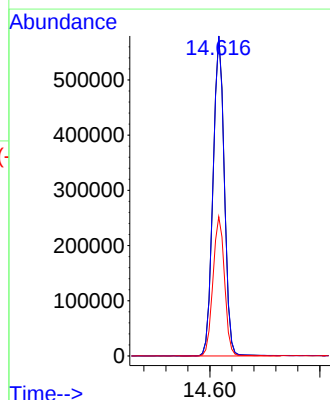





#42
2,4,6-Tribromophenol
Concen: 7.55 ng
RT: 16.098 min Scan# 2212
Delta R.T. 0.006 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54




Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)


Tgt Ion: 330 Resp: 80106
Ion Ratio Lower Upper
330 100
332 99.0 76.3 114.5
141 26.5 22.8 34.2

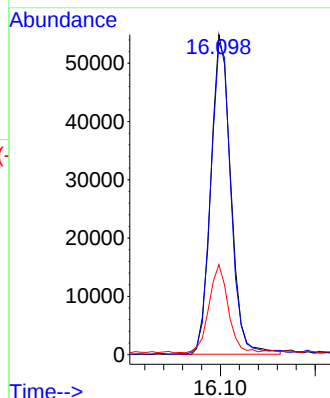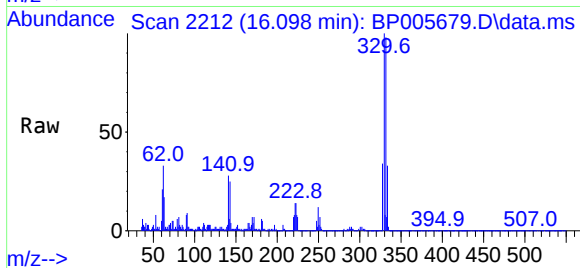

#45
2-Fluorobiphenyl
Concen: 4.89 ng
RT: 13.246 min Scan# 1727
Delta R.T. 0.006 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54

Tgt Ion: 172 Resp: 305355
Ion Ratio Lower Upper
172 100
171 34.9 28.1 42.1
170 23.7 19.6 29.4


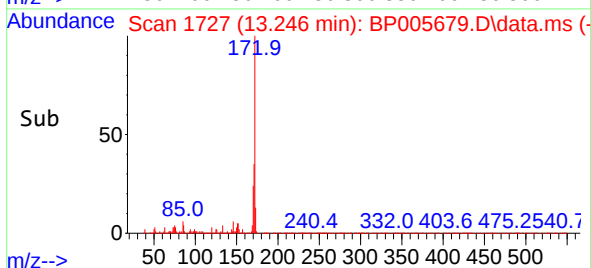
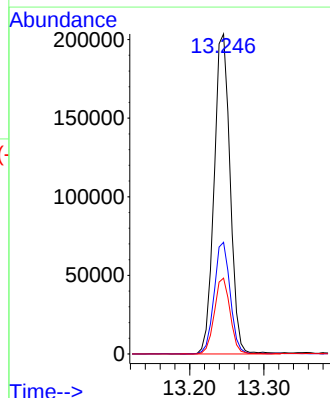
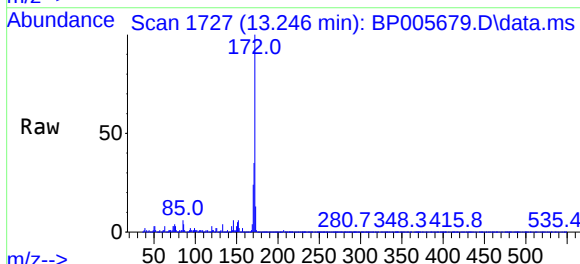




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.357 min Scan# 2426
Delta R.T. 0.006 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54




Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)


Tgt Ion:188 Resp: 1584481
Ion Ratio Lower Upper
188 100
94 8.3 5.0 7.6#
80 8.4 5.9 8.9

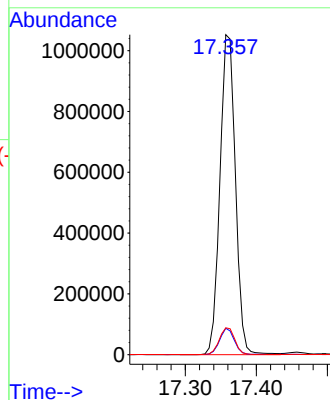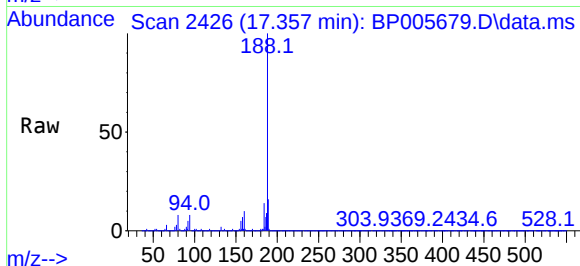

#71
Phenanthrene
Concen: 3.00 ng
RT: 17.404 min Scan# 2434
Delta R.T. 0.012 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54

Tgt Ion:178 Resp: 296011
Ion Ratio Lower Upper
178 100
176 19.3 15.4 23.2
179 16.1 12.3 18.5


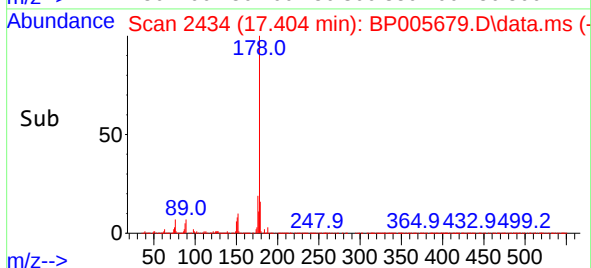
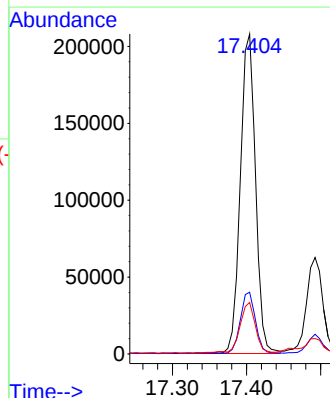
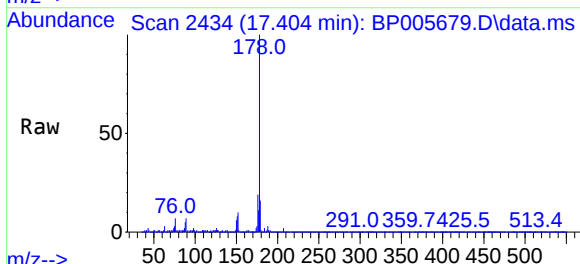




#75
Fluoranthene
Concen: 4.03 ng
RT: 19.357 min Scan# 2766
Delta R.T. 0.006 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54




Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)


Tgt Ion:	202	Resp:	477007
Ion	Ratio	Lower	Upper
202	100		
101	9.0	0.0	26.1
203	17.7	0.0	37.2

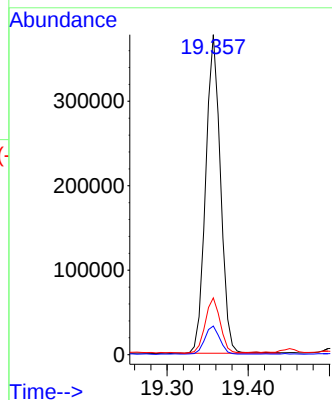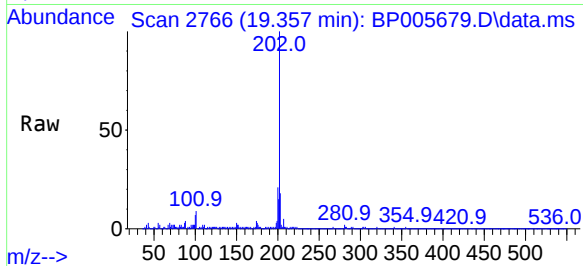

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.427 min Scan# 3118
Delta R.T. 0.005 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54

Tgt Ion:	240	Resp:	1358040
Ion	Ratio	Lower	Upper
240	100		
120	8.7	4.2	6.2#
236	25.7	20.2	30.2


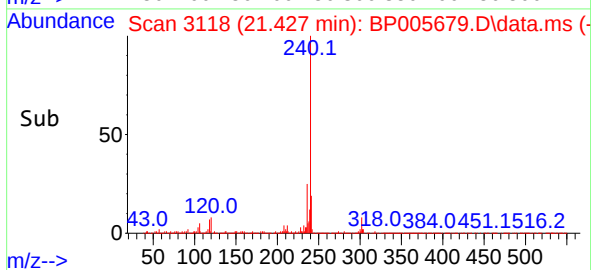
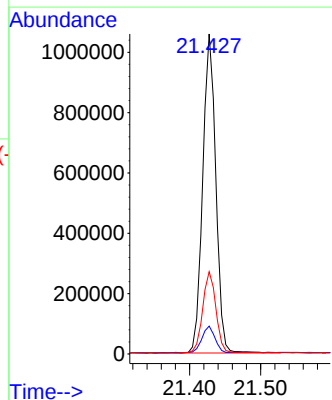
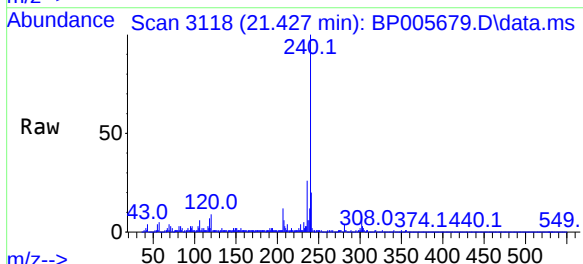




#78
Pyrene
Concen: 4.27 ng
RT: 19.710 min Scan# 2826
Delta R.T. 0.012 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54




Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)


Tgt Ion:	202	Resp:	409485
Ion Ratio	Lower	Upper	
202	100		
200	21.3	16.9	25.3
203	18.5	13.8	20.6

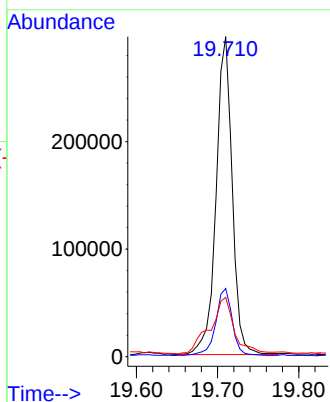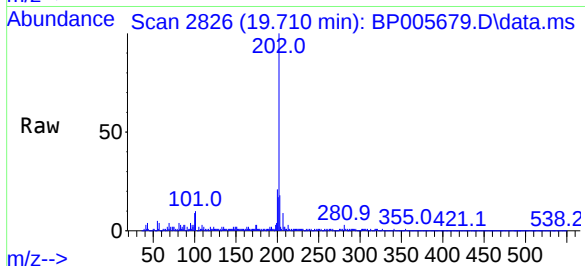

#79
Terphenyl-d14
Concen: 5.61 ng
RT: 19.898 min Scan# 2858
Delta R.T. -0.000 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54

Tgt Ion:	244	Resp:	405952
Ion Ratio	Lower	Upper	
244	100		
212	6.6	5.8	8.6
122	8.5	5.2	7.8#


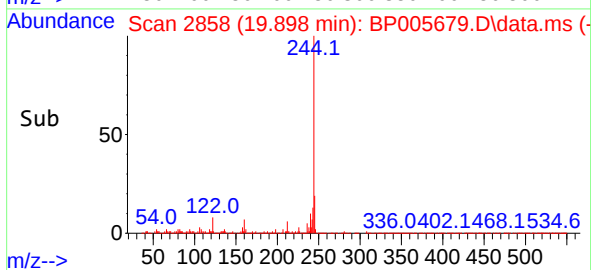
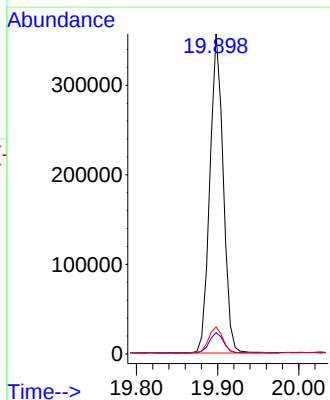
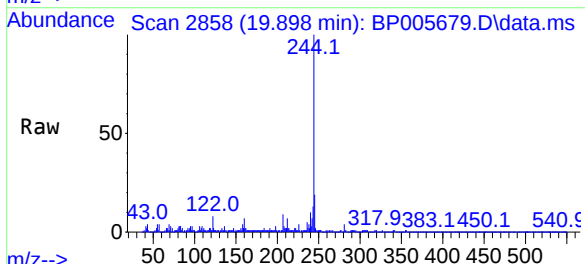




#81
Benzo(a)anthracene
Concen: 2.38 ng
RT: 21.410 min Scan# 3115
Delta R.T. 0.006 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54




Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)


Tgt Ion:228 Resp: 237001
Ion Ratio Lower Upper
228 100
226 29.4 21.2 31.8
229 23.7 15.6 23.4#

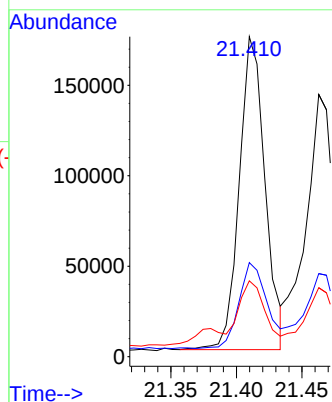

#83
Chrysene
Concen: 2.20 ng
RT: 21.463 min Scan# 3124
Delta R.T. 0.006 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54

Tgt Ion:228 Resp: 211908
Ion Ratio Lower Upper
228 100
226 31.7 24.8 37.2
229 26.3 15.4 23.0#


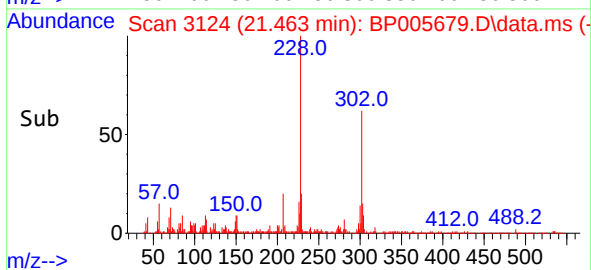
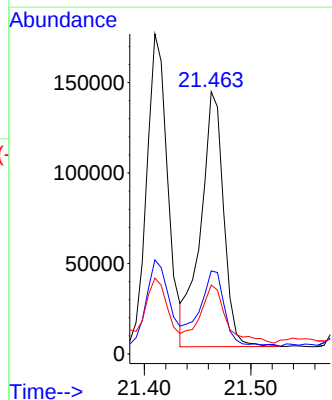





#86
Perylene-d12
Concen: 20.00 ng
RT: 23.880 min Scan# 3535
Delta R.T. 0.018 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54




Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)


Tgt Ion:264 Resp: 1552993
Ion Ratio Lower Upper
264 100
260 24.3 20.6 30.8
265 23.3 19.0 28.6

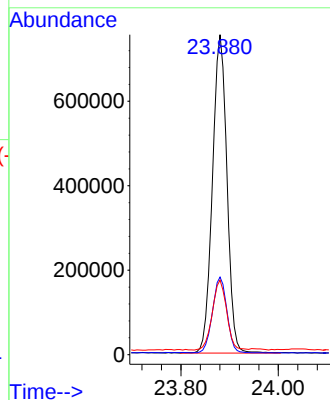

#88
Benzo(b)fluoranthene
Concen: 2.72 ng
RT: 23.127 min Scan# 3407
Delta R.T. 0.012 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54

Tgt Ion:252 Resp: 306998
Ion Ratio Lower Upper
252 100
253 32.9 18.2 27.2#
125 17.8 3.4 5.0#

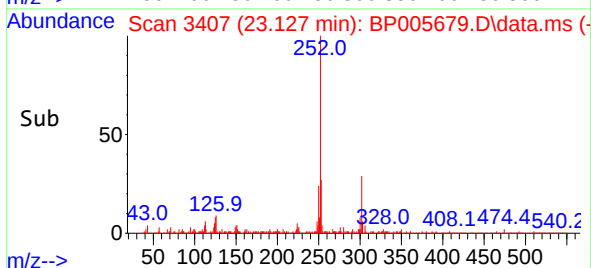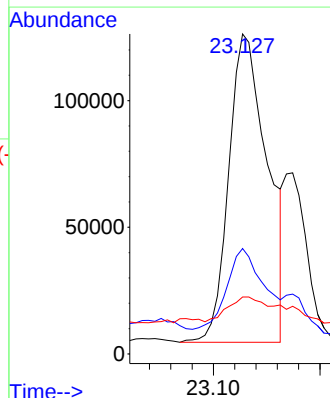

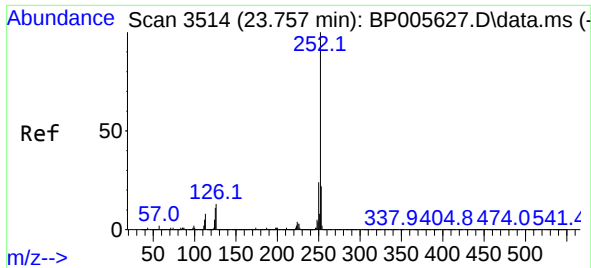

#90
Benzo(a)pyrene
Concen: 2.32 ng
RT: 23.768 min Scan# 3516
Delta R.T. 0.012 min
Lab File: BP005679.D
Acq: 02 Jun 2021 22:54

Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)

Tgt Ion:252 Resp: 237777
Ion Ratio Lower Upper
252 100
253 27.5 17.1 25.7#
125 18.7 3.8 5.6#

