
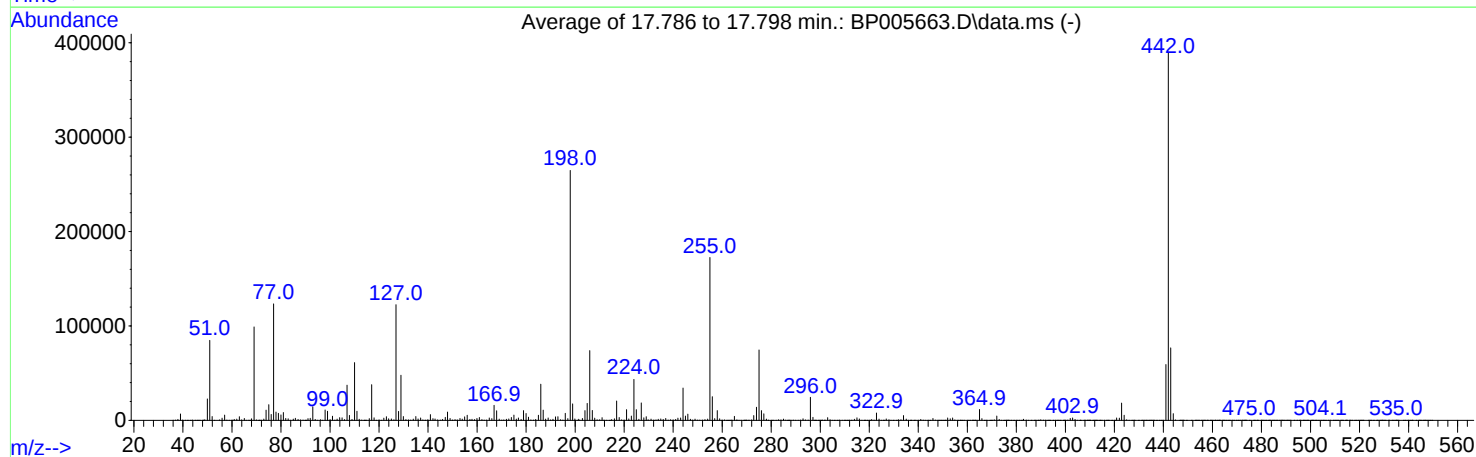


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060221\  
 Data File : BP005663.D  
 Acq On : 02 Jun 2021 13:09  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052721.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu May 27 16:11:11 2021

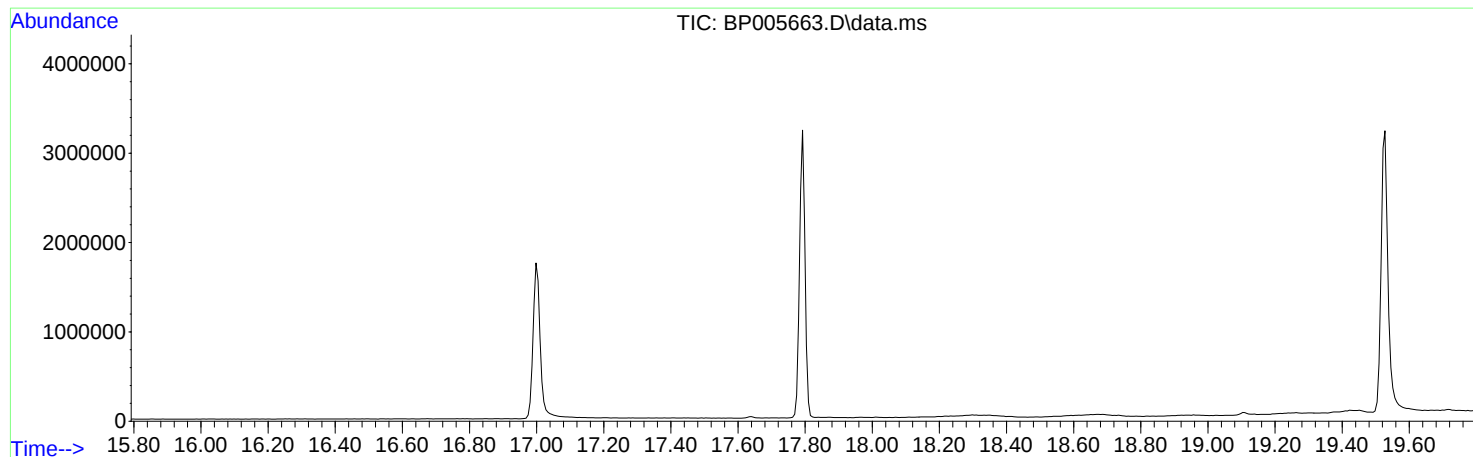




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 32.0         | 84812      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1753       | PASS                |
| 69             | 198             | 0.00            | 100             | 37.4         | 99070      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 573        | PASS                |
| 127            | 198             | 10              | 80              | 46.3         | 122485     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.7          | 1831       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 264823     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 17476      | PASS                |
| 275            | 198             | 10              | 60              | 28.2         | 74563      | PASS                |
| 365            | 198             | 1               | 100             | 4.4          | 11582      | PASS                |
| 441            | 198             | 0.01            | 100             | 22.3         | 59157      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 389696     | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 76739      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060221\  
 Data File : BP005663.D  
 Acq On : 02 Jun 2021 13:09  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 02 14:02:11 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052721.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu May 27 16:11:11 2021  
 Response via : Initial Calibration

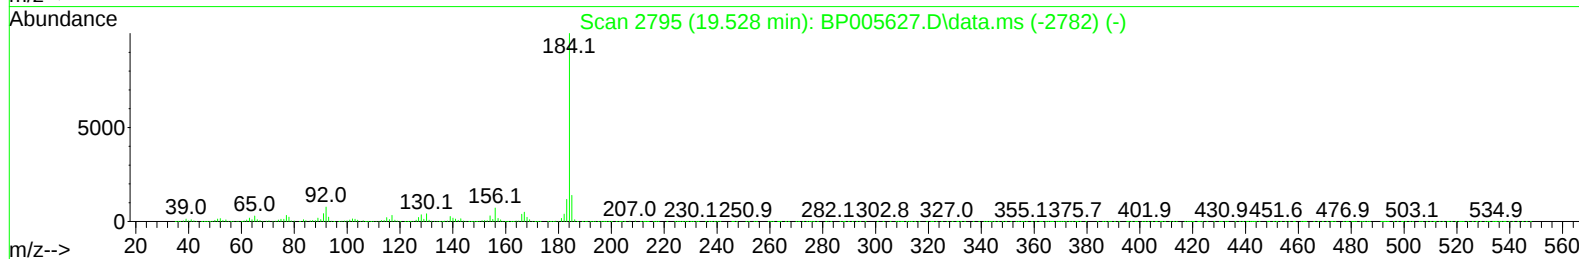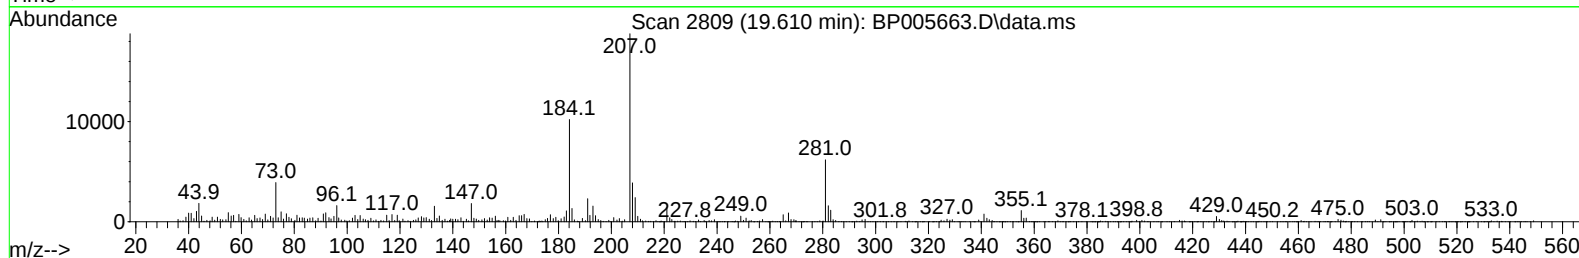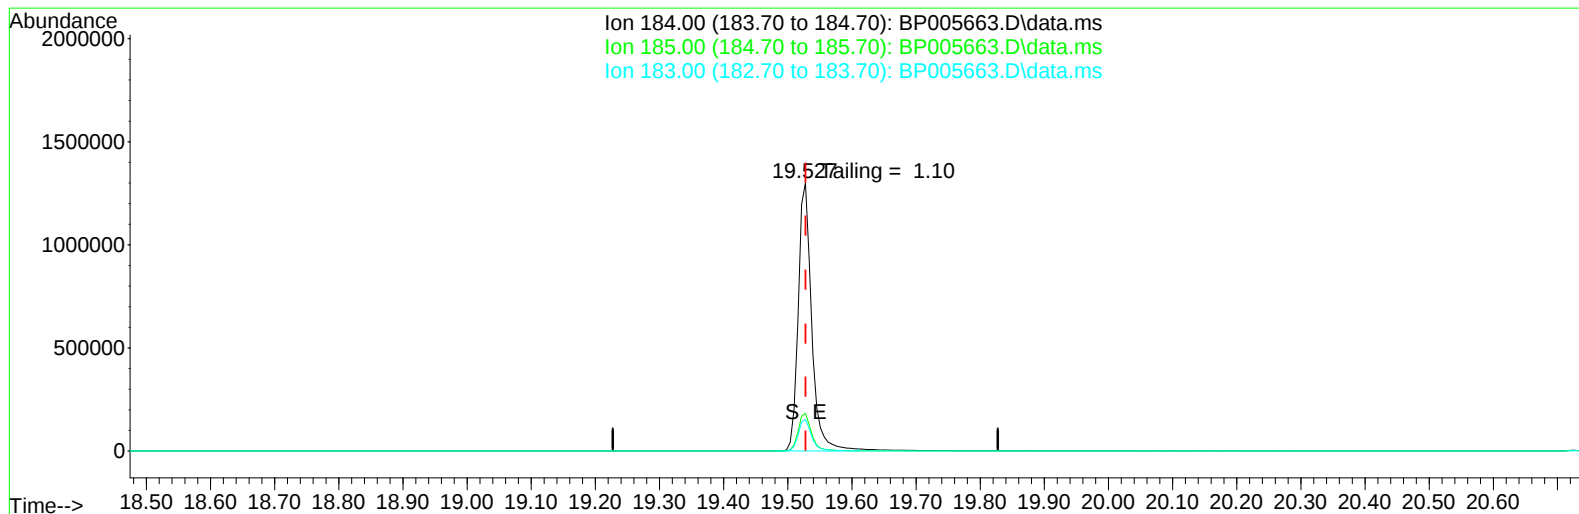

TIC: BP005663.D\data.ms

**(77) Benzidine**

**19.527min (-0.000) 949883.69 ng**




**response 1912190**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 14.09  |
| 183.00 | 12.30  | 11.75  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060221\  
 Data File : BP005663.D  
 Acq On : 02 Jun 2021 13:09  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 02 14:02:11 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052721.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu May 27 16:11:11 2021  
 Response via : Initial Calibration

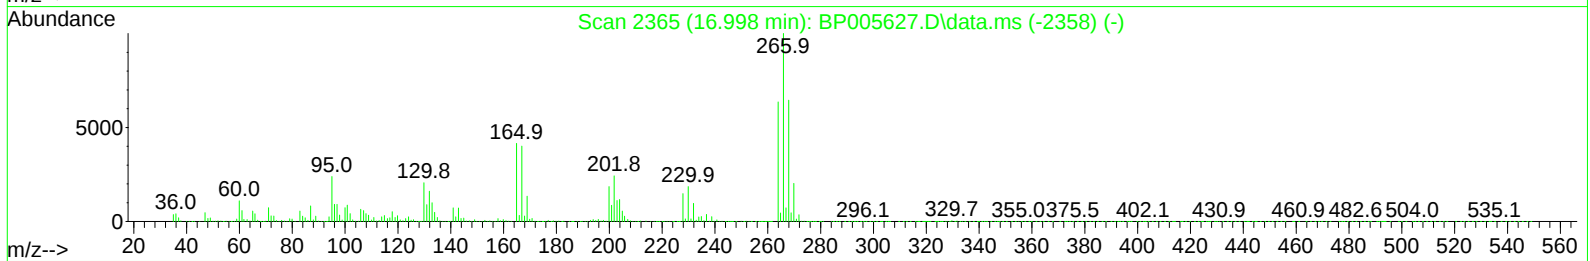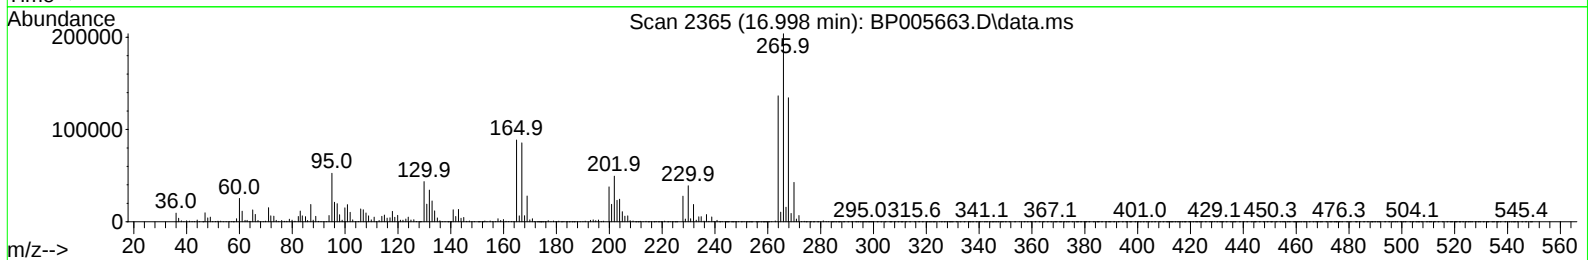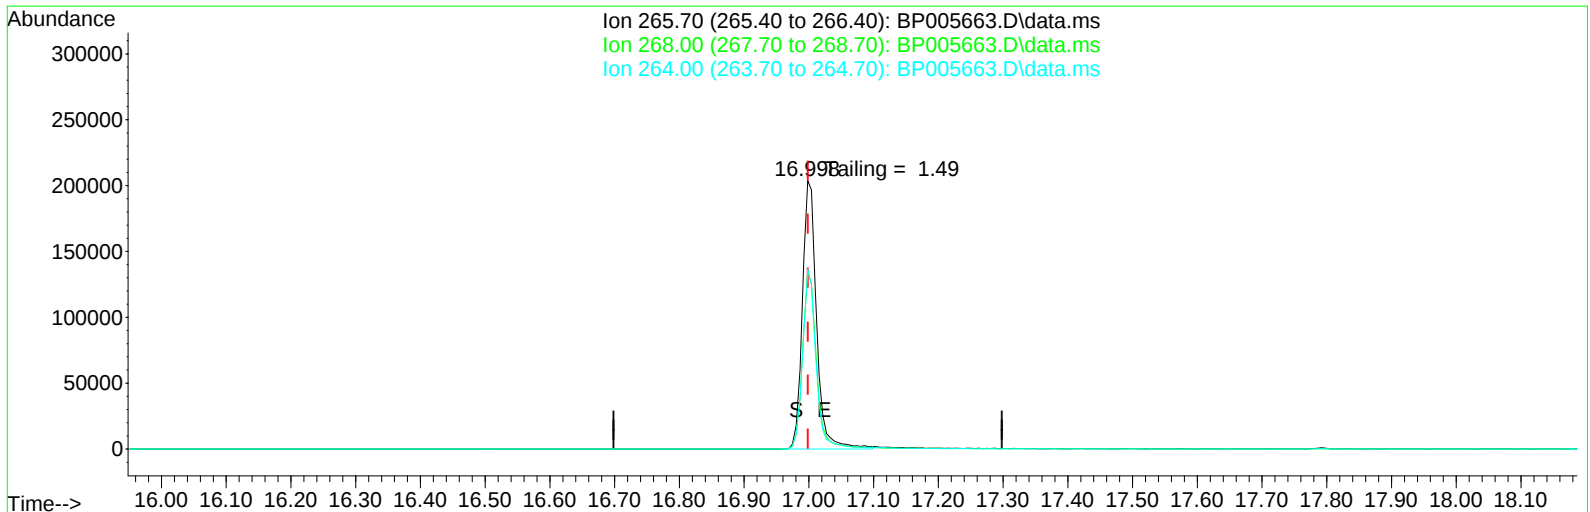

TIC: BP005663.D\data.ms

**(70) Pentachlorophenol (C)**

16.998min (-0.000) 2604027.80 ng

response 318470

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.70  | 65.92  |
| 264.00 | 67.10  | 66.96  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/2/2021      | BNA_P            | <u>BP005663.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 929605           | 20.72              |
| DDD           | 33708            | 20.29              |
| DDE           | 2085             | 19.81              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 35793         | 965398           | 3.71               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP