
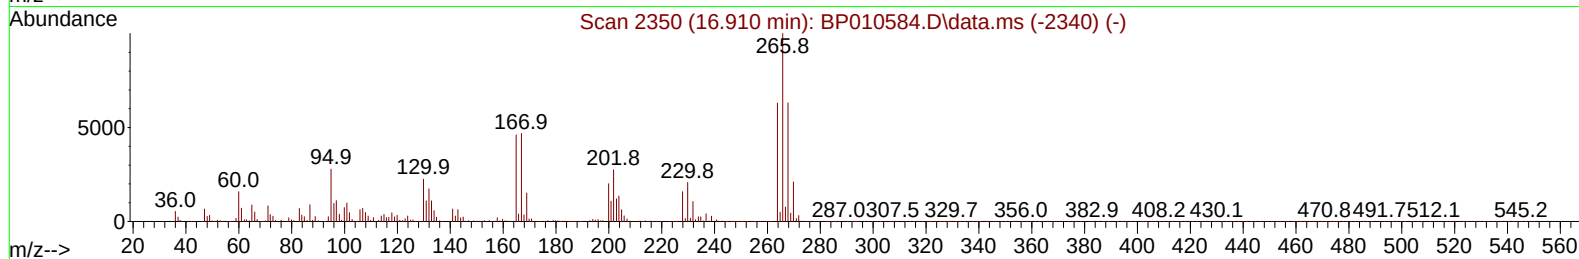
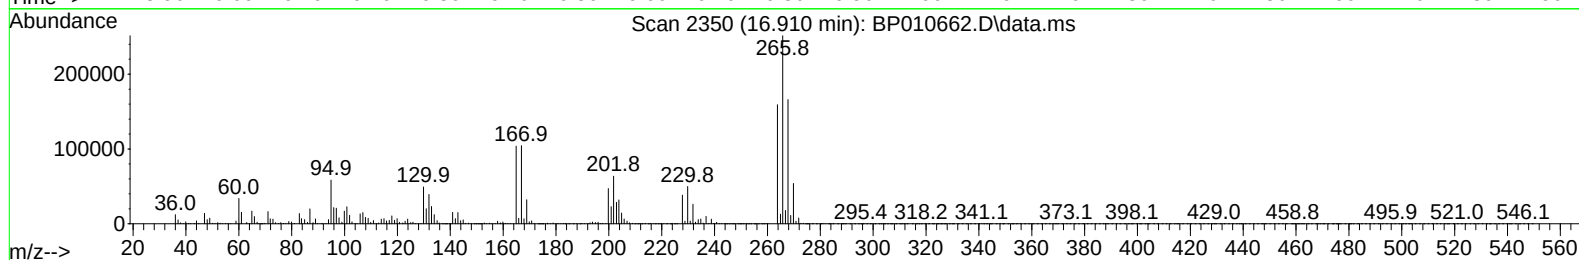


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060222\
 Data File : BP010662.D
 Acq On : 02 Jun 2022 09:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 06:03:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 28 02:18:04 2022
 Response via : Initial Calibration

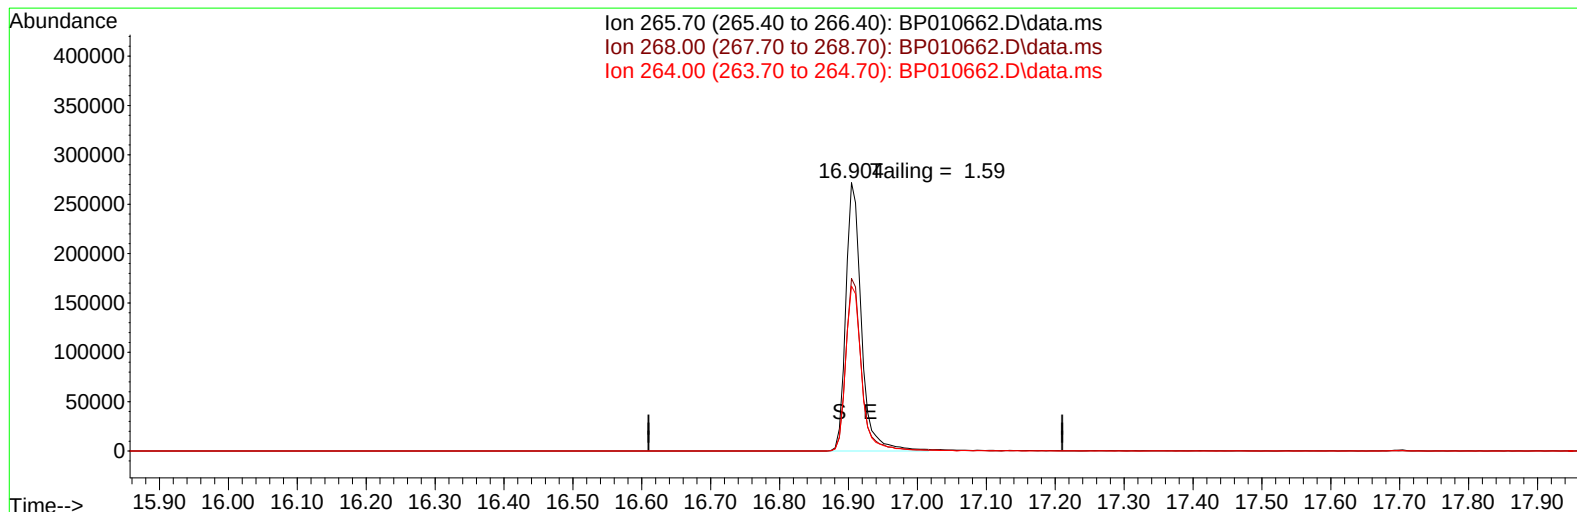

TIC: BP010662.D\data.ms

(70) Pentachlorophenol (C)




16.910min (-16.910) 0.00 ng

response 0

Ion	Exp%	Act%
265.70	100.00	0.00
268.00	63.10	0.00#
264.00	63.00	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060222\
Data File : BP010662.D
Acq On : 02 Jun 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 06:03:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 28 02:18:04 2022
Response via : Initial Calibration

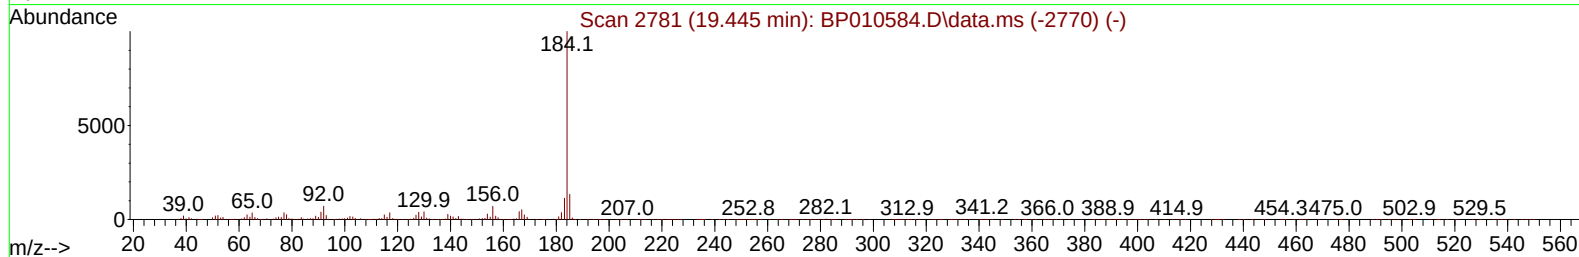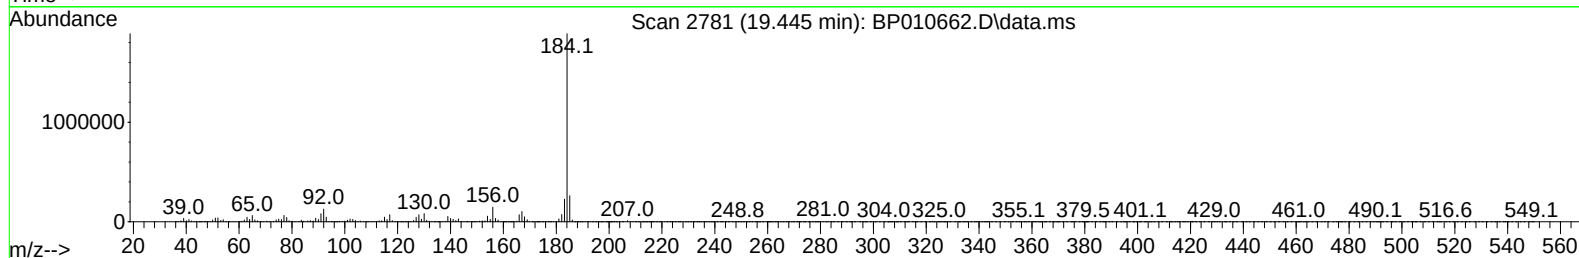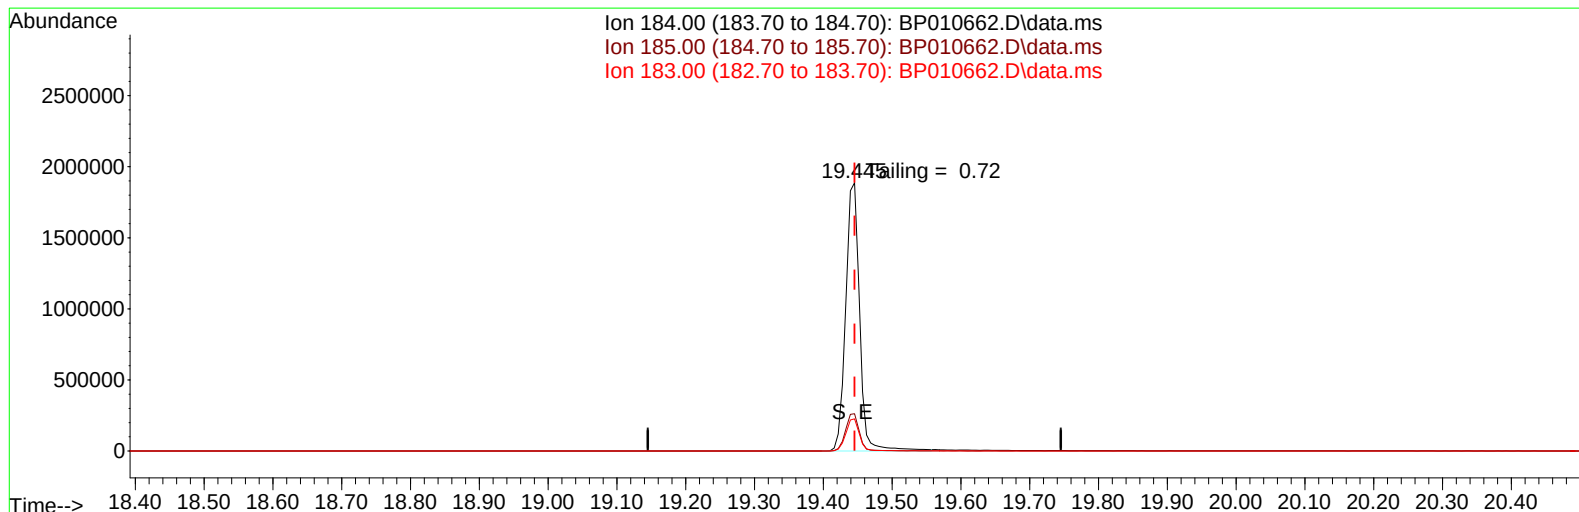

TIC: BP010662.D\data.ms

(77) Benzidine**19.445min (0.000) 572473.95 ng****response 2353327**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.90
183.00	11.30	12.00
0.00	0.00	0.00