

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060222\
 Data File : BP010668.D
 Acq On : 02 Jun 2022 13:24
 Operator : CG/JU
 Sample : N3087-08DL2 50X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MW-14DL2

Quant Time: Jun 02 15:20:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 28 02:18:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	145067	20.000	ng	0.00
21) Naphthalene-d8	10.657	136	591750	20.000	ng	-0.01
39) Acenaphthene-d10	14.492	164	374452	20.000	ng	-0.01
64) Phenanthrene-d10	17.251	188	767291	20.000	ng	0.00
76) Chrysene-d12	21.339	240	726917	20.000	ng	0.00
86) Perylene-d12	23.751	264	726603	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.452	112	8014	1.008	ng	0.00
7) Phenol-d6	7.052	99	5063	0.448	ng	0.01
23) Nitrobenzene-d5	9.028	82	18133	1.449	ng	0.00
42) 2,4,6-Tribromophenol	15.998	330	9763	2.303	ng	0.00
45) 2-Fluorobiphenyl	13.122	172	39937	1.514	ng	0.00
79) Terphenyl-d14	19.804	244	65753	1.699	ng	-0.01
Target Compounds						
						Qvalue
31) Naphthalene	10.710	128	1267465	40.658	ng	100
37) 2-Methylnaphthalene	12.316	142	149959	6.894	ng	100
38) 1-Methylnaphthalene	12.534	142	181647	8.551	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060222\
Data File : BP010668.D
Acq On : 02 Jun 2022 13:24
Operator : CG/JU
Sample : N3087-08DL2 50X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-14DL2

Quant Time: Jun 02 15:20:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 28 02:18:04 2022
Response via : Initial Calibration




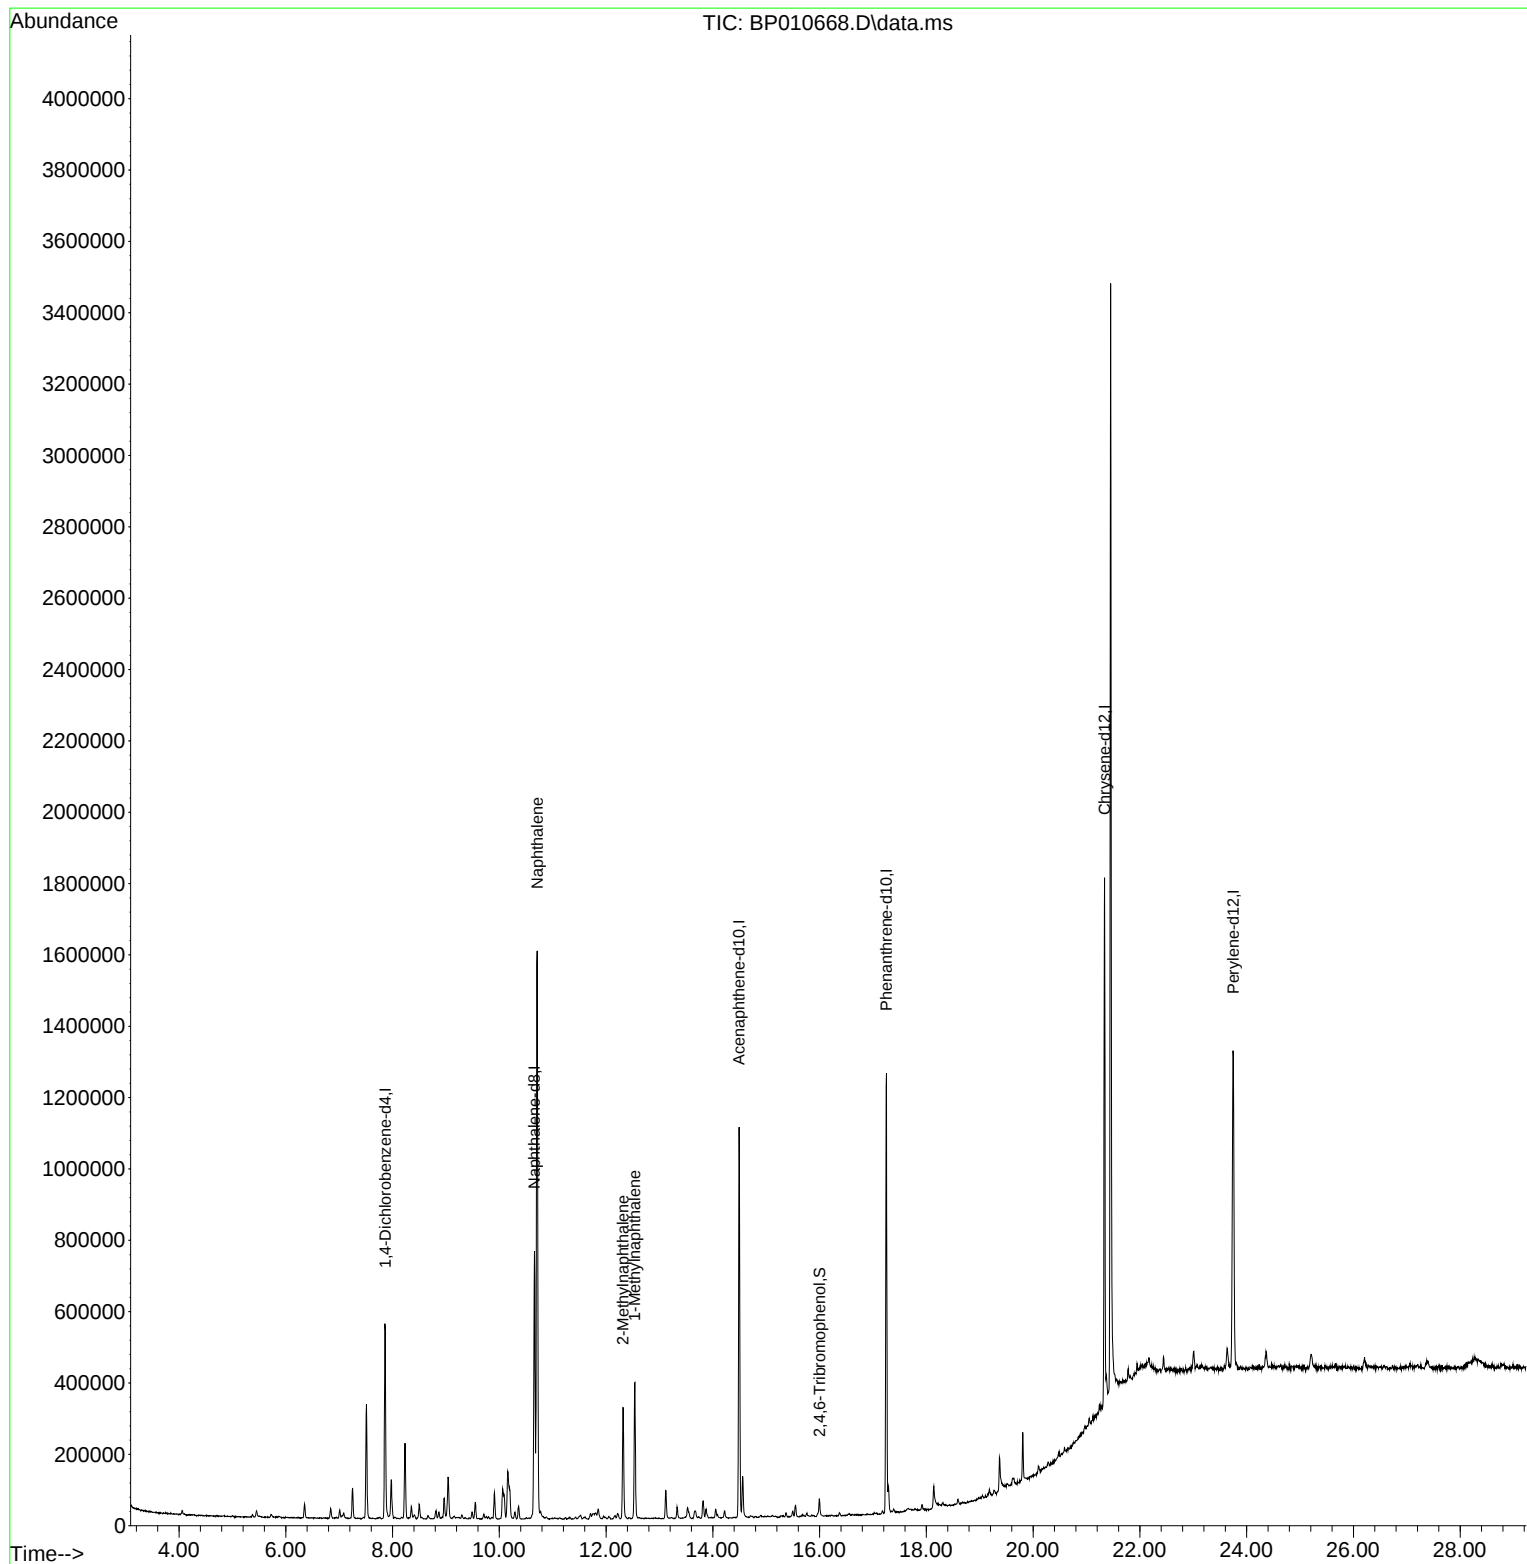




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.863 min Scan# 81
Delta R.T. -0.006 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24




Instrument :
BNA_P
ClientSampleId :
MW-14DL2


Tgt Ion:152 Resp: 145067
Ion Ratio Lower Upper
152 100
150 150.9 123.4 185.2
115 58.6 51.3 76.9

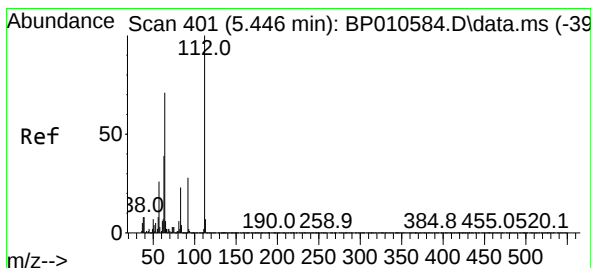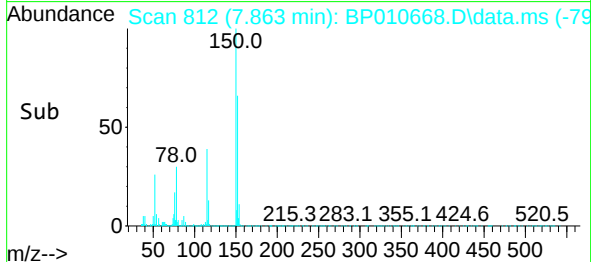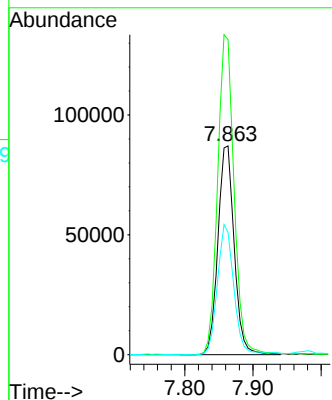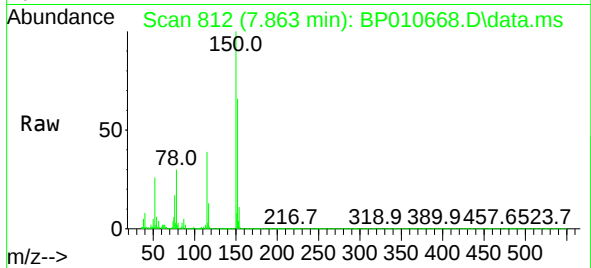

#5
2-Fluorophenol
Concen: 1.008 ng
RT: 5.452 min Scan# 402
Delta R.T. 0.006 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24

Tgt Ion:112 Resp: 8014
Ion Ratio Lower Upper
112 100
64 70.8 56.9 85.3
63 40.0 31.2 46.8


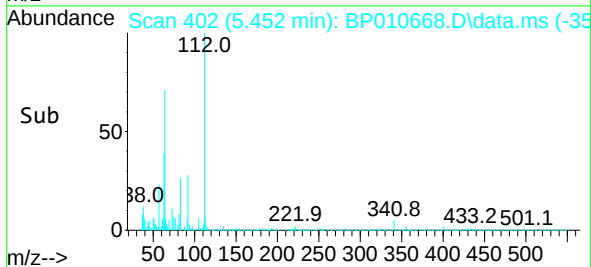
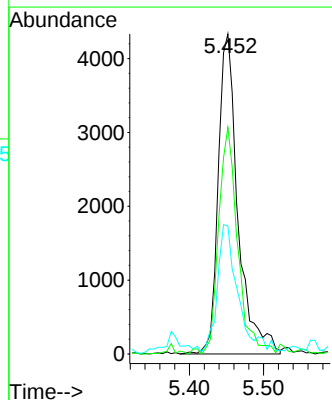
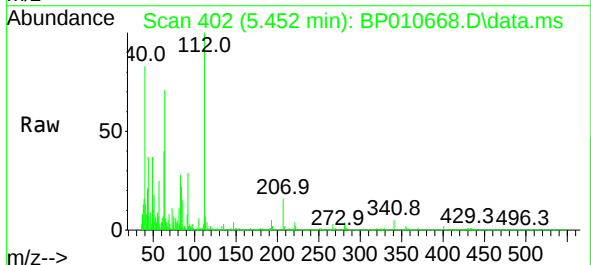


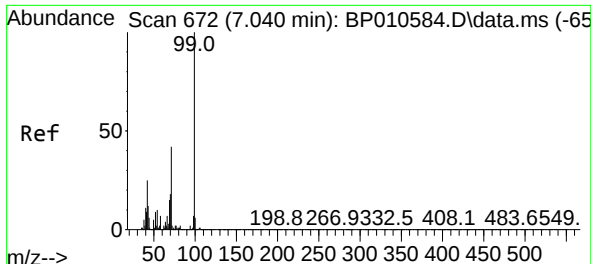

#7
Phenol-d6
Concen: 0.448 ng
RT: 7.052 min Scan# 61
Delta R.T. 0.012 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24




Instrument :
BNA_P
ClientSampleId :
MW-14DL2


Tgt Ion: 99 Resp: 5063
Ion Ratio Lower Upper
99 100
42 32.3 20.3 30.5#
71 45.8 33.9 50.9

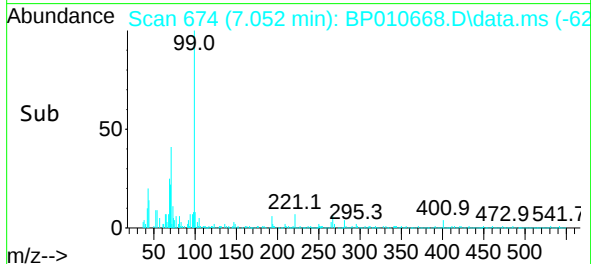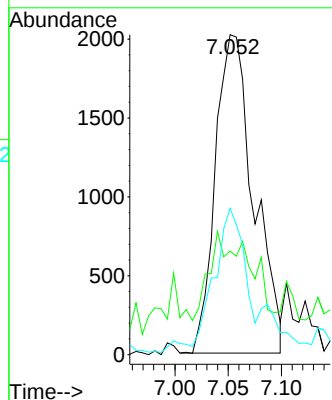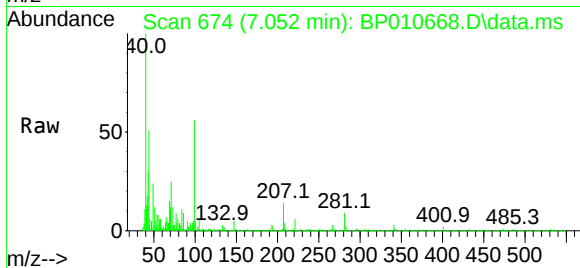

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.657 min Scan# 1287
Delta R.T. -0.012 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24

Tgt Ion:136 Resp: 591750
Ion Ratio Lower Upper
136 100
137 11.1 9.0 13.4
54 10.3 8.7 13.1
68 6.4 4.8 7.2


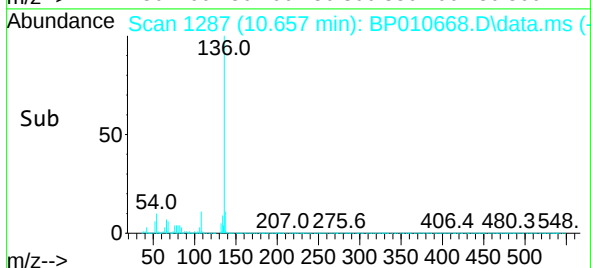
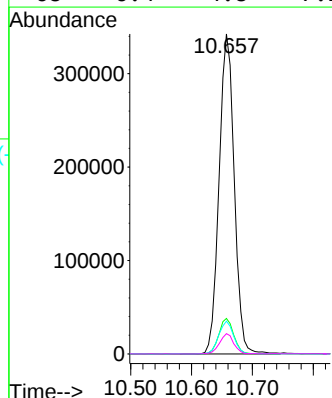
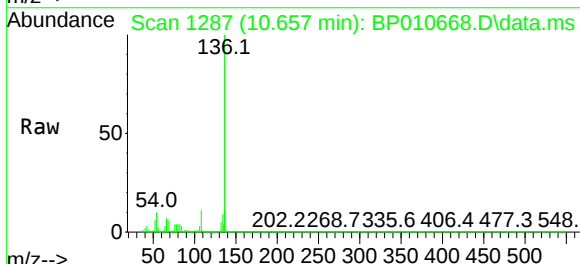




#23
Nitrobenzene-d5
Concen: 1.449 ng
RT: 9.028 min Scan# 1010
Delta R.T. 0.000 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24




Instrument :
BNA_P
ClientSampleId :
MW-14DL2


Tgt Ion: 82 Resp: 18133
Ion Ratio Lower Upper
82 100
128 41.0 31.3 46.9
54 55.8 49.8 74.8

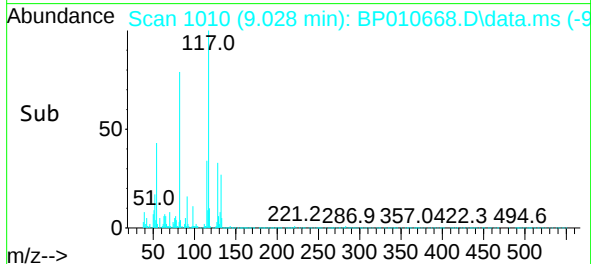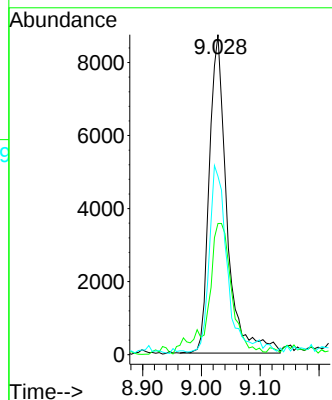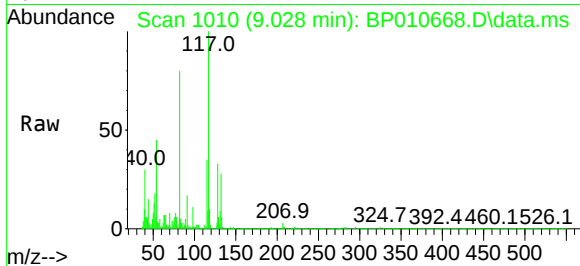

#31
Naphthalene
Concen: 40.658 ng
RT: 10.710 min Scan# 1296
Delta R.T. -0.006 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24

Tgt Ion: 128 Resp: 1267465
Ion Ratio Lower Upper
128 100
129 10.7 8.6 12.8
127 13.1 10.3 15.5


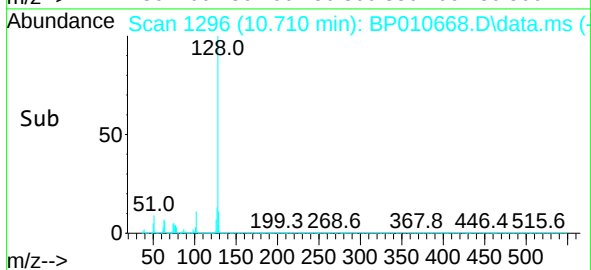
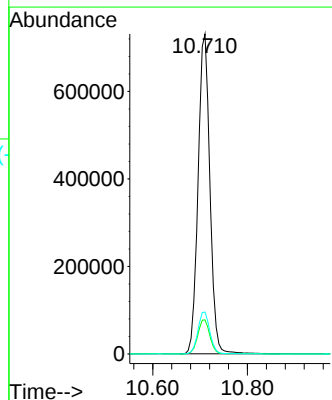
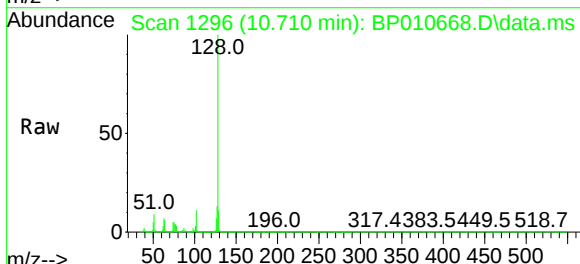




#37
2-Methylnaphthalene
Concen: 6.894 ng
RT: 12.316 min Scan# 1569
Delta R.T. -0.012 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24




Instrument :
BNA_P
ClientSampleId :
MW-14DL2


Tgt Ion:142 Resp: 149959
Ion Ratio Lower Upper
142 100
141 89.2 71.3 106.9
115 38.9 31.4 47.2

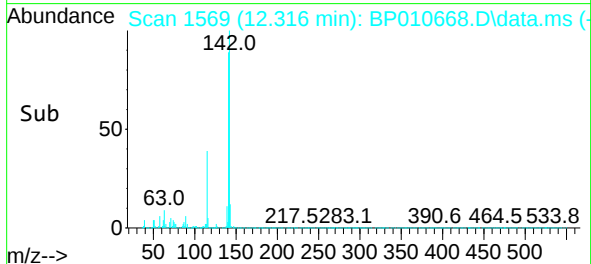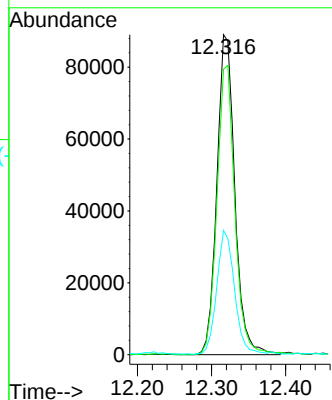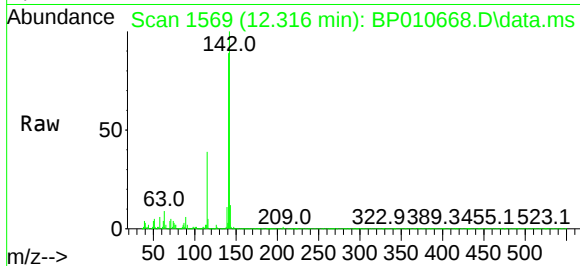

#38
1-Methylnaphthalene
Concen: 8.551 ng
RT: 12.534 min Scan# 1606
Delta R.T. -0.012 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24

Tgt Ion:142 Resp: 181647
Ion Ratio Lower Upper
142 100
141 90.8 72.6 108.8
116 4.1 3.3 4.9


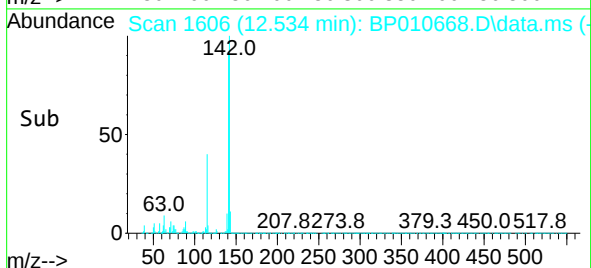
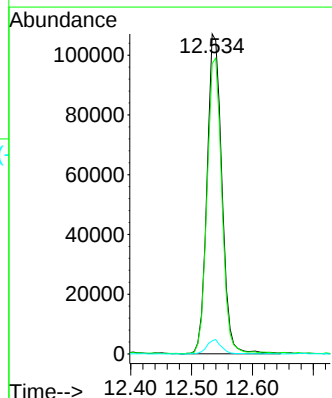
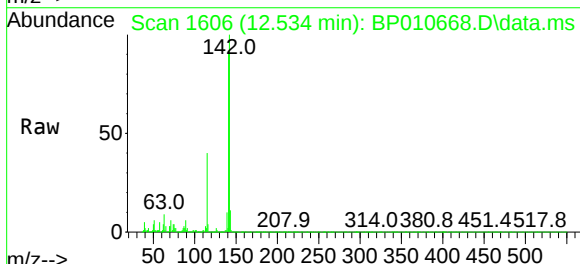




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.492 min Scan# 1939
Delta R.T. -0.012 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24




Instrument :
BNA_P
ClientSampleId :
MW-14DL2


Tgt Ion:164 Resp: 374452
Ion Ratio Lower Upper
164 100
162 101.1 81.9 122.9
160 42.9 34.6 51.8

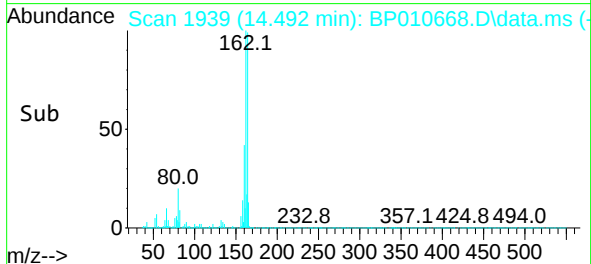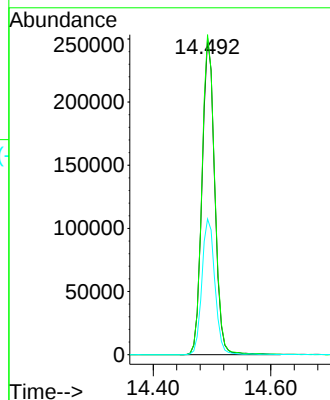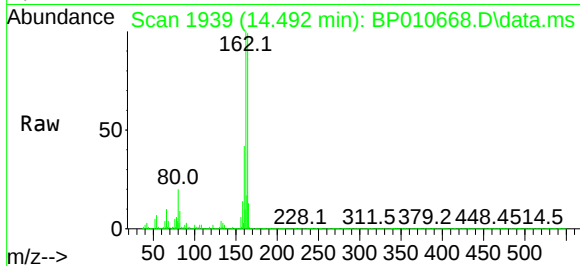

#42
2,4,6-Tribromophenol
Concen: 2.303 ng
RT: 15.998 min Scan# 2195
Delta R.T. 0.005 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24

Tgt Ion:330 Resp: 9763
Ion Ratio Lower Upper
330 100
332 99.8 78.1 117.1
141 39.0 31.4 47.2

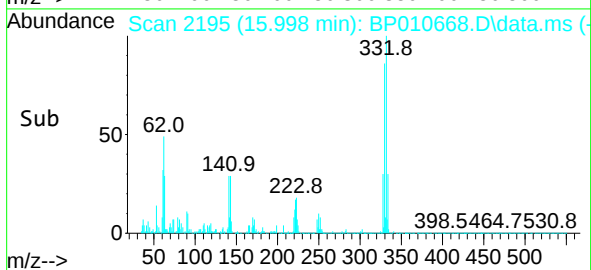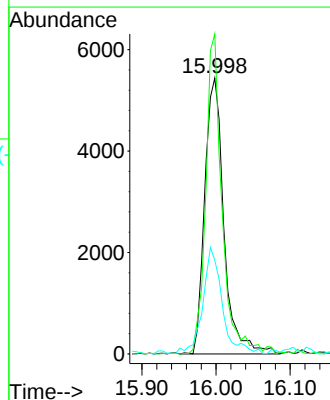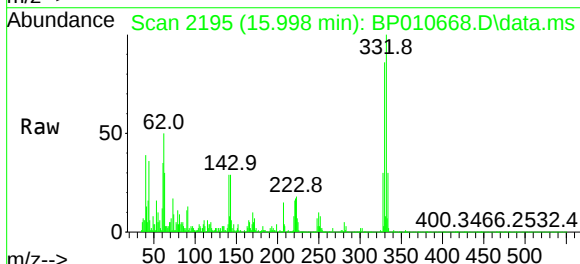

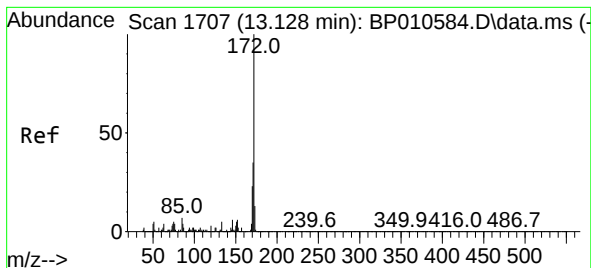

#45

2-Fluorobiphenyl

Concen: 1.514 ng

RT: 13.122 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP010668.D

Acq: 02 Jun 2022 13:24

Instrument :

BNA_P

ClientSampleId :

MW-14DL2





Tgt Ion:172 Resp: 39937

Ion Ratio Lower Upper

172 100

171 35.8 27.9 41.9

170 22.7 18.2 27.2

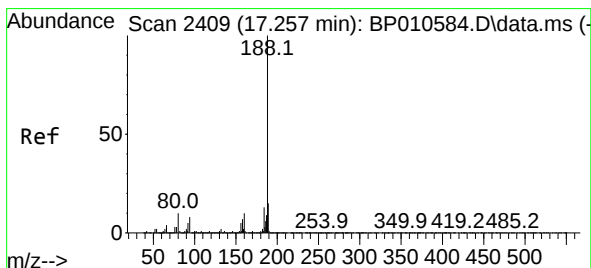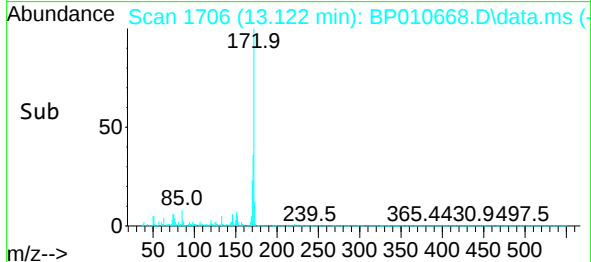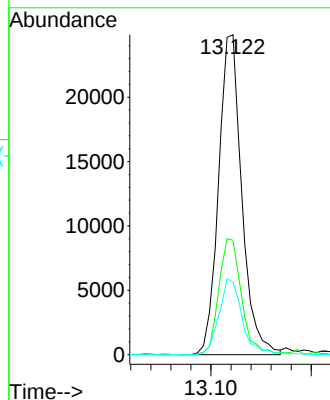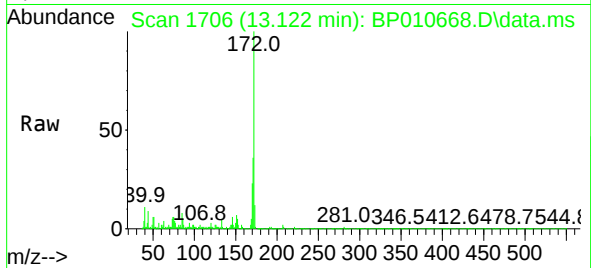

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.251 min Scan# 2408

Delta R.T. -0.006 min

Lab File: BP010668.D

Acq: 02 Jun 2022 13:24




Tgt Ion:188 Resp: 767291


Ion Ratio Lower Upper

188 100

94 8.4 6.6 10.0

80 10.1 8.0 12.0


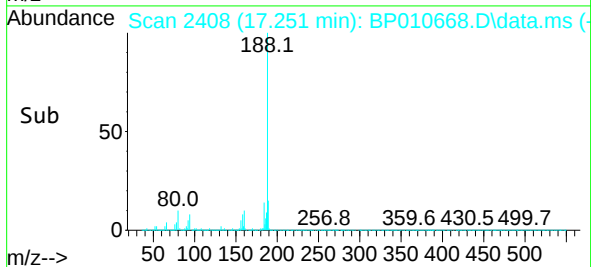
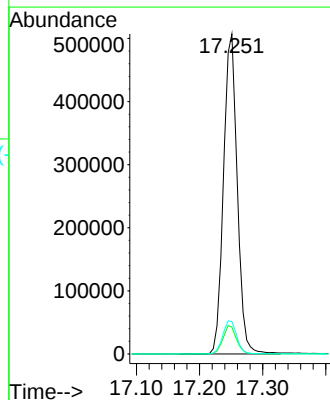
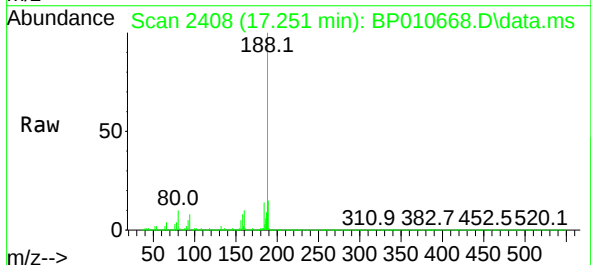




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.339 min Scan# 31
Delta R.T. 0.000 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24




Instrument :
BNA_P
ClientSampleId :
MW-14DL2


Tgt Ion:240 Resp: 726917
Ion Ratio Lower Upper
240 100
120 9.0 8.6 12.8
236 25.7 19.8 29.6

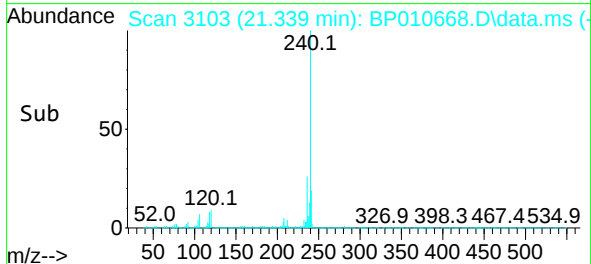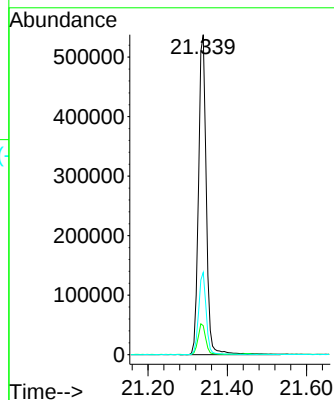

#79
Terphenyl-d14
Concen: 1.699 ng
RT: 19.804 min Scan# 2842
Delta R.T. -0.012 min
Lab File: BP010668.D
Acq: 02 Jun 2022 13:24

Tgt Ion:244 Resp: 65753
Ion Ratio Lower Upper
244 100
212 7.5 5.8 8.8
122 9.6 7.6 11.4

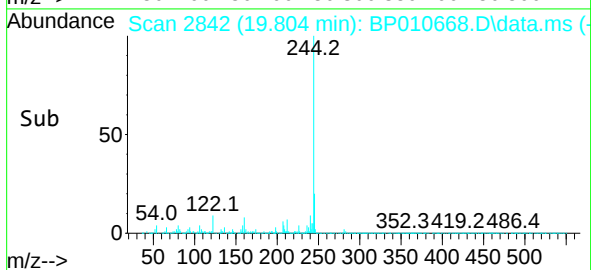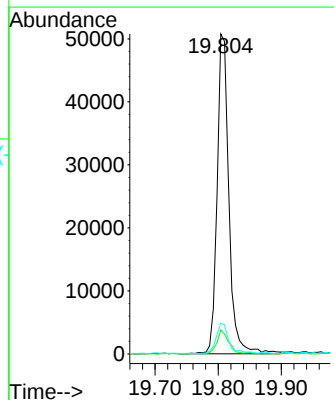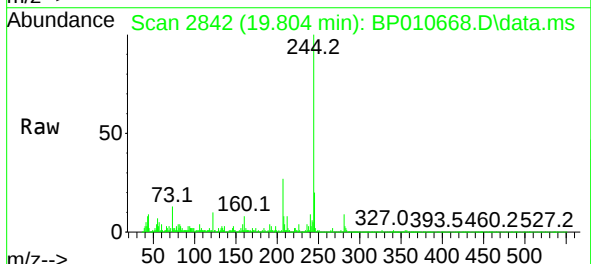

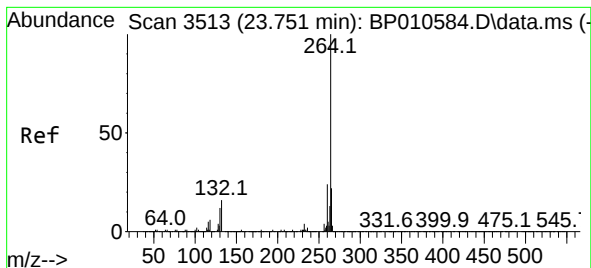

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.751 min Scan# 31

Delta R.T. -0.000 min

Lab File: BP010668.D


Acq: 02 Jun 2022 13:24

Instrument :

BNA_P

ClientSampleId :

MW-14DL2

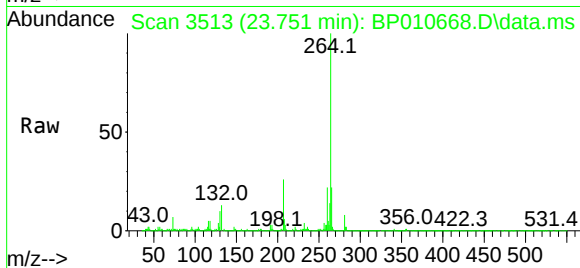

Tgt Ion:264 Resp: 726603

Ion Ratio Lower Upper

264 100

260 22.2 19.3 28.9

265 21.9 18.0 27.0

