

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060222\
 Data File : BP010664.D
 Acq On : 02 Jun 2022 11:05
 Operator : CG/JU
 Sample : PB145143TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB145143TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	394	401	417	rBV	2635877	3900976	50.71%	10.736%
2	7.034	664	671	694	rBV	2528856	4175855	54.29%	11.493%
3	7.857	804	811	818	rBV	427043	683228	8.88%	1.880%
4	9.022	999	1009	1024	rBV	1557324	2724479	35.42%	7.498%
5	10.657	1280	1287	1303	rBV	537295	984760	12.80%	2.710%
6	13.116	1697	1705	1727	rBV	3911824	6002613	78.03%	16.521%
7	14.498	1932	1940	1953	rBV	845217	1348410	17.53%	3.711%
8	15.992	2185	2194	2213	rBV	2946201	4602201	59.83%	12.666%
9	17.251	2401	2408	2420	rBV	998946	1560573	20.29%	4.295%
10	19.810	2837	2843	2853	rBV	6306187	7692408	100.00%	21.171%
11	21.339	3098	3103	3109	rBV	850072	1200398	15.60%	3.304%
12	21.451	3118	3122	3132	rBV	271949	455183	5.92%	1.253%
13	23.751	3507	3513	3526	rVB	468398	1003233	13.04%	2.761%




Sum of corrected areas: 36334317

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060222\
Data File : BP010664.D
Acq On : 02 Jun 2022 11:05
Operator : CG/JU
Sample : PB145143TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145143TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

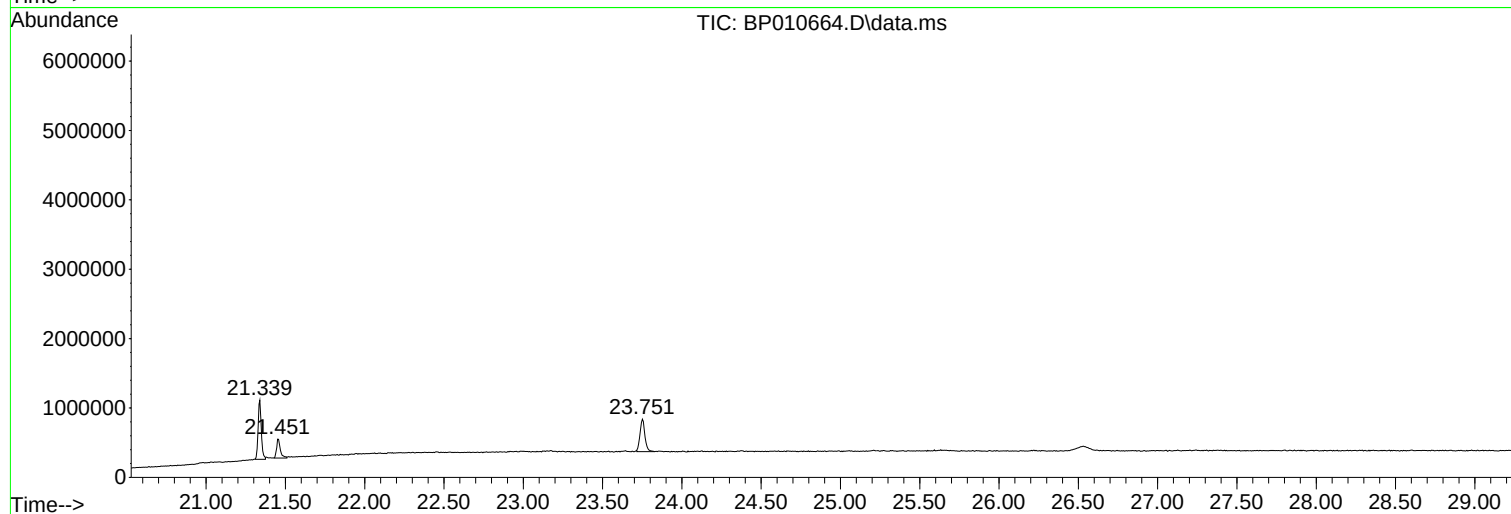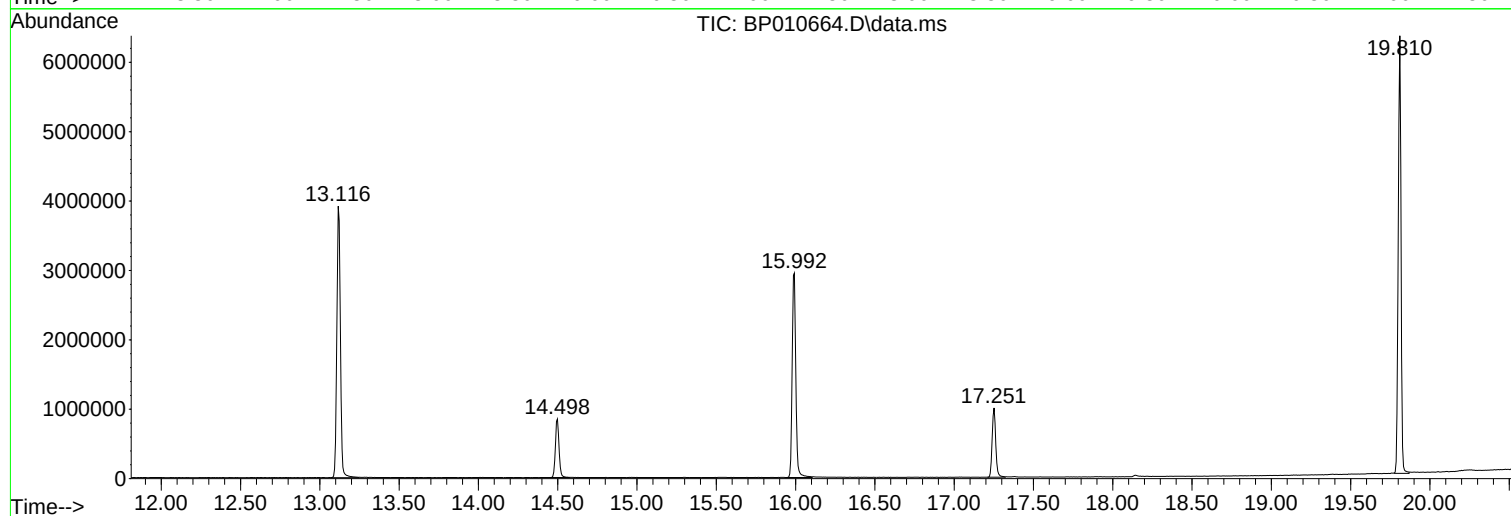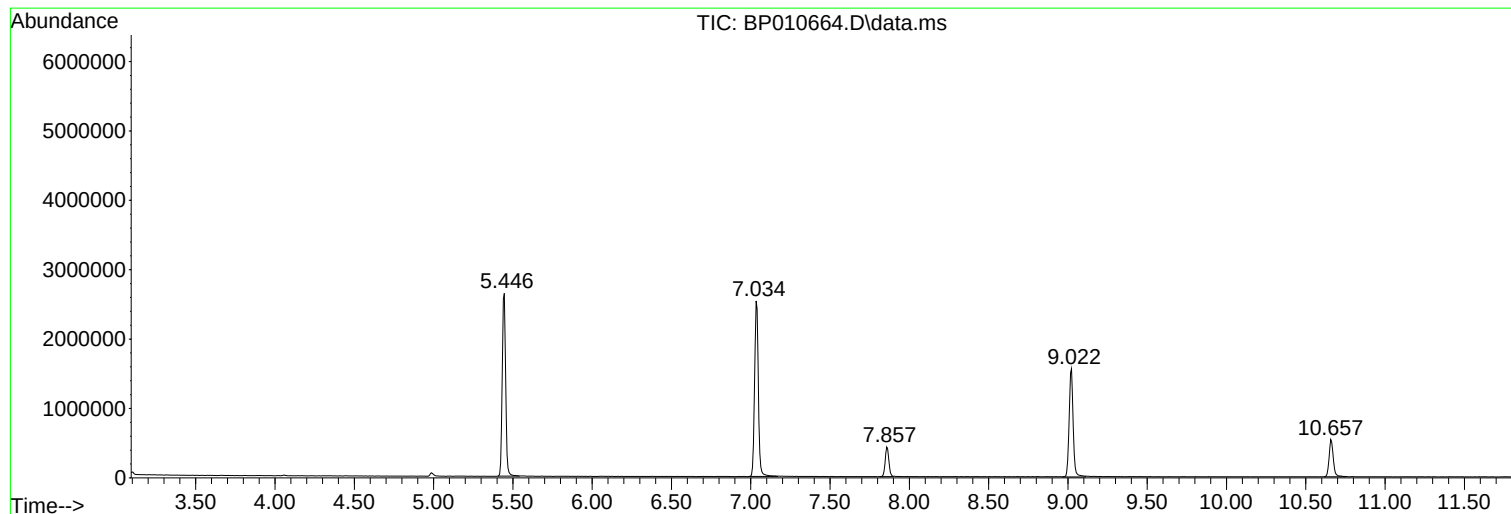

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060222\
Data File : BP010664.D
Acq On : 02 Jun 2022 11:05
Operator : CG/JU
Sample : PB145143TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145143TB










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.451	7.58 ng	455183	Chrysene-d12	21.339

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	98
2			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	50
3			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19N03S	1000483-83-4	46
4			Benzoic acid, 2-(diphenylphosphi...	306	C19H15O2P	017261-28-8	38
5			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	38

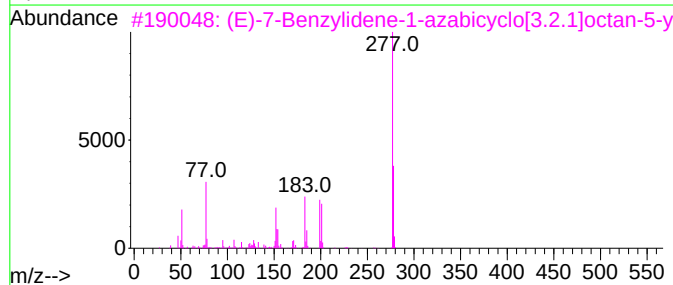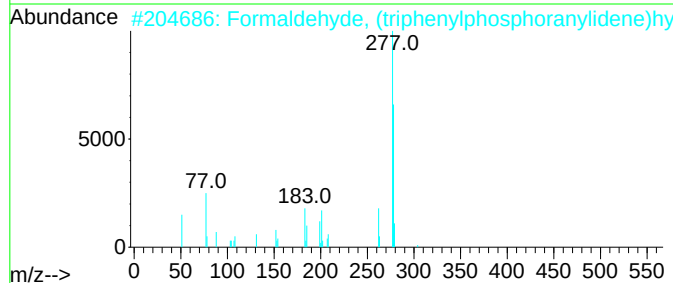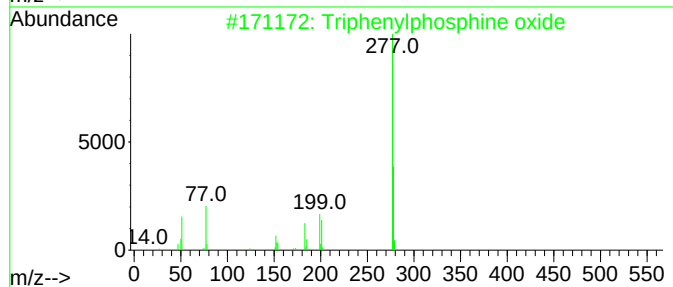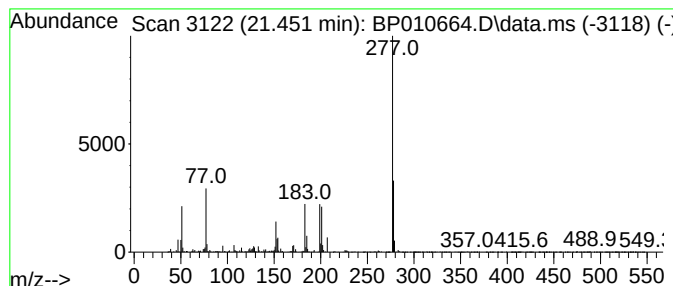

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060222\
Data File : BP010664.D
Acq On : 02 Jun 2022 11:05
Operator : CG/JU
Sample : PB145143TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145143TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	21.451	7.6	ng	455183	5	21.339	1200400	20.0