DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060222\
Data File : BP010662.D
Acq On : 02 Jun 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat May 28 02:18:04 2022

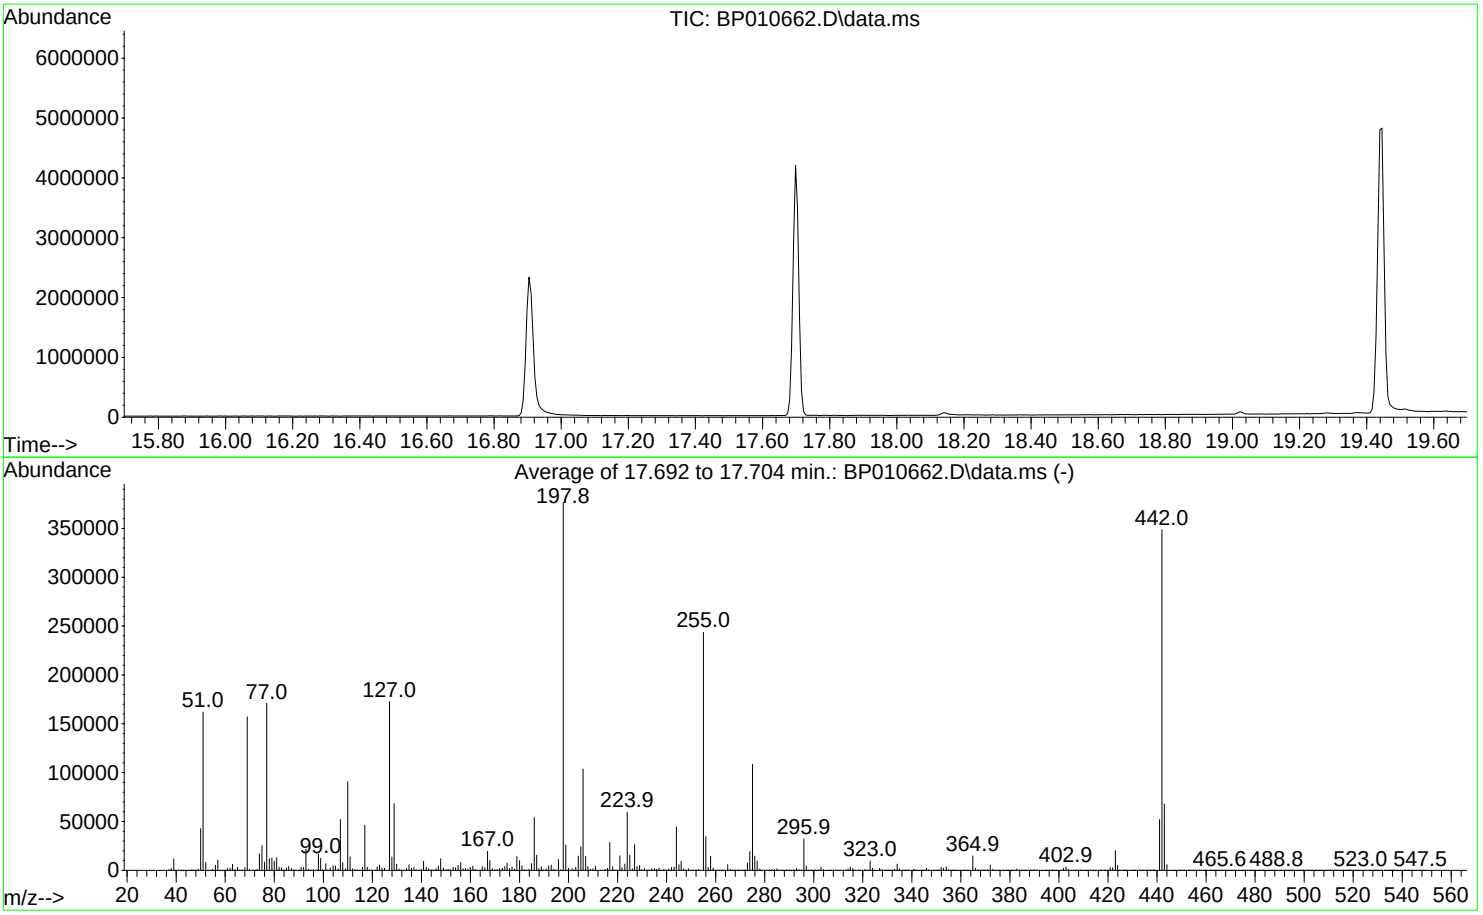

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	161901	PASS
68	69	0.00	2	1.8	2893	PASS
69	198	0.00	100	41.8	157203	PASS
70	69	0.00	2	0.6	913	PASS
127	198	10	80	45.8	172609	PASS
197	198	0.00	2	0.2	630	PASS
198	198	100	100	100.0	376490	PASS
199	198	5	9	6.9	26088	PASS
275	198	10	60	28.8	108445	PASS
365	198	1	100	3.9	14756	PASS
441	198	0.01	100	13.8	52113	PASS
442	442	100	100	100.0	348843	PASS
443	442	15	24	19.5	68021	PASS

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060222\
Data File : BP010662.D
Acq On : 02 Jun 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 03 06:03:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 28 02:18:04 2022
Response via : Initial Calibration

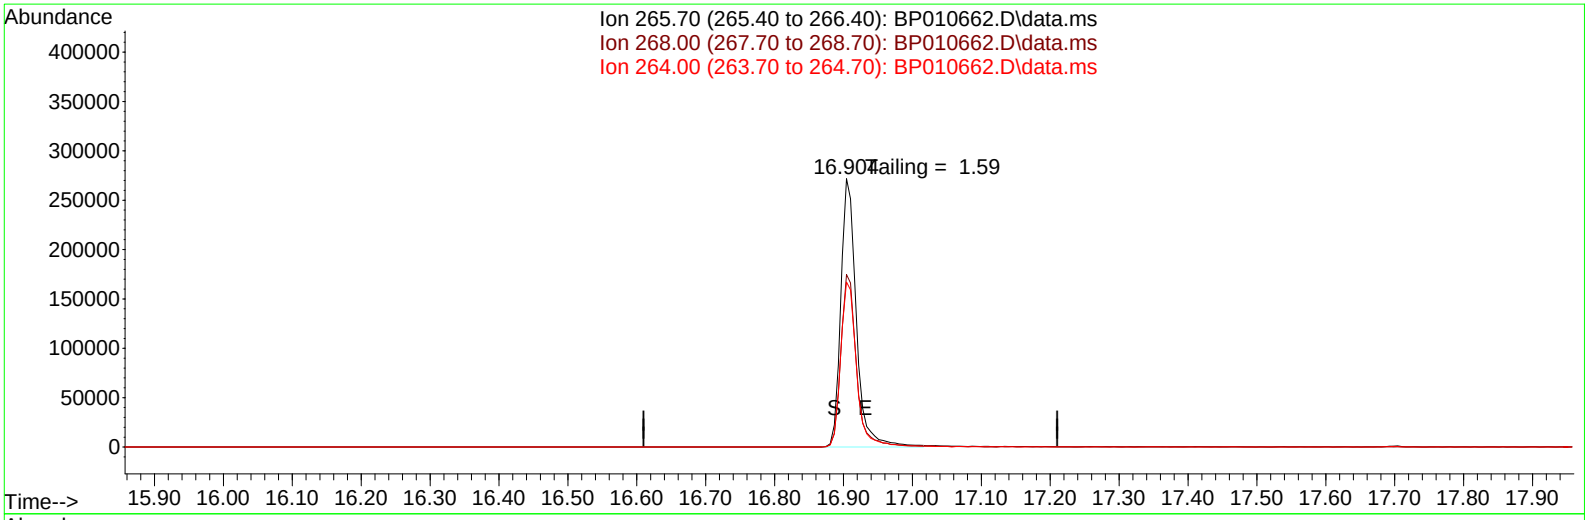

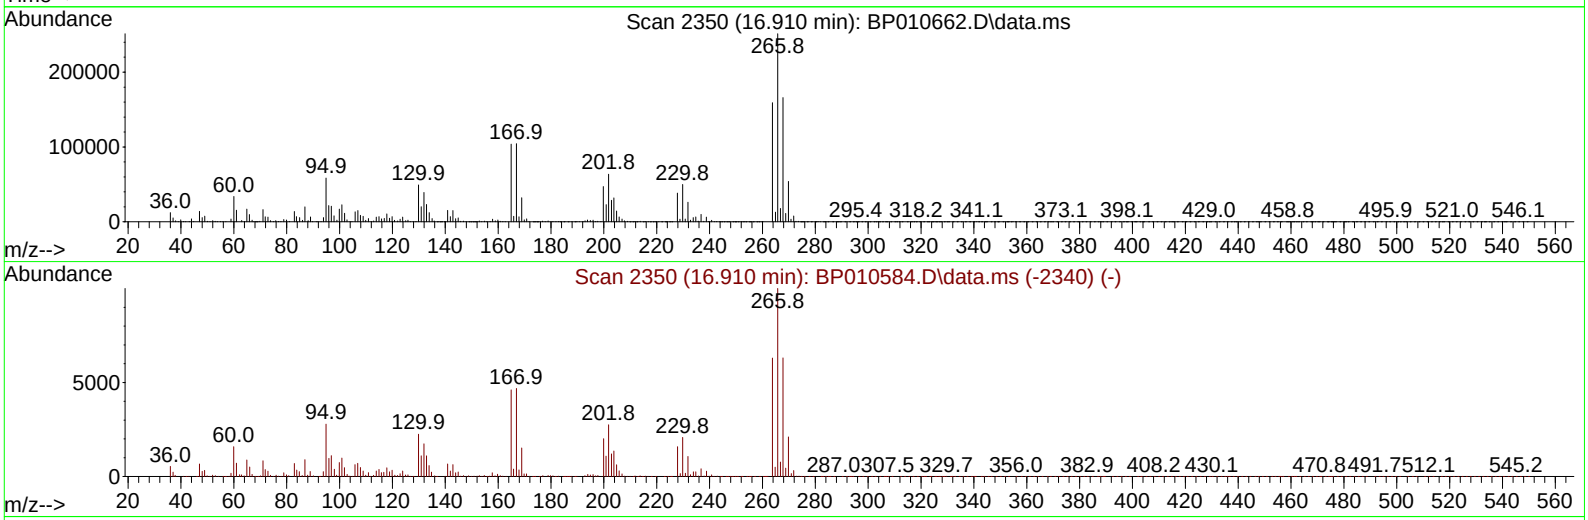

TIC: BP010662.D\data.ms

(70) Pentachlorophenol (C)

16.910min (-16.910) 0.00 ng

response 0

Ion	Exp%	Act%
265.70	100.00	0.00
268.00	63.10	0.00#
264.00	63.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060222\
Data File : BP010662.D
Acq On : 02 Jun 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 03 06:03:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 28 02:18:04 2022
Response via : Initial Calibration

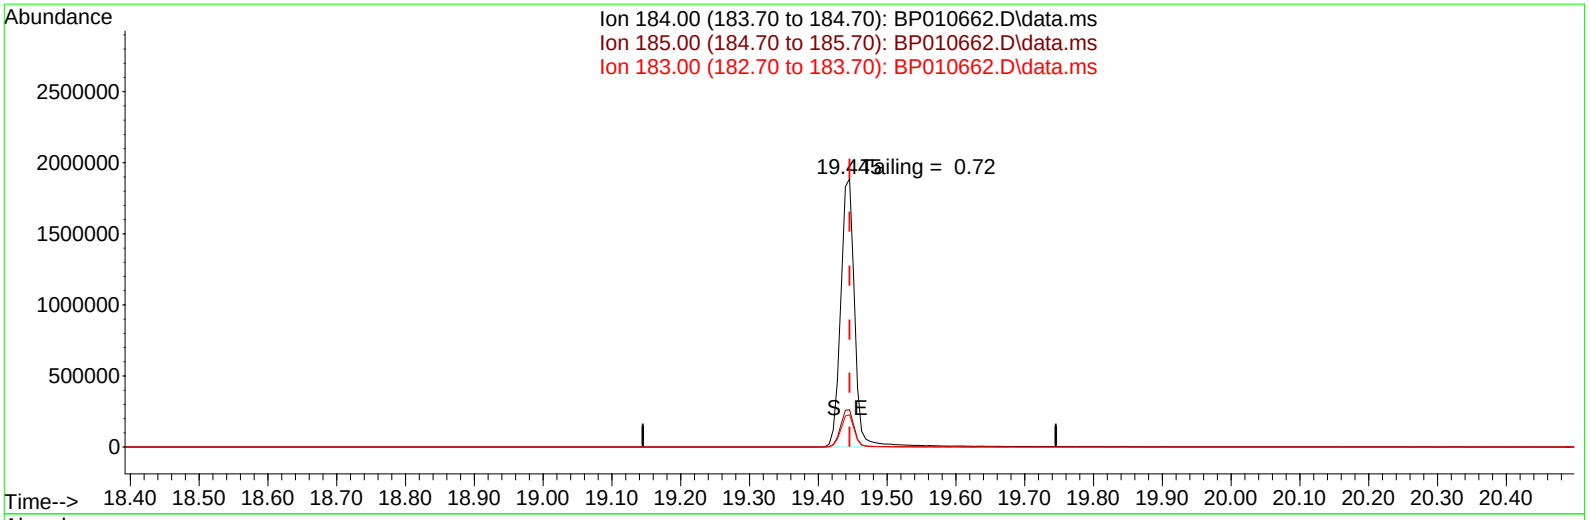

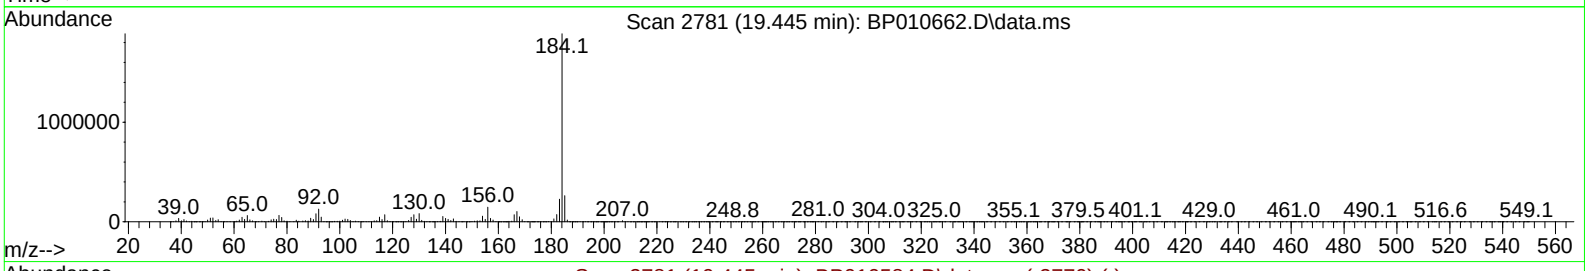

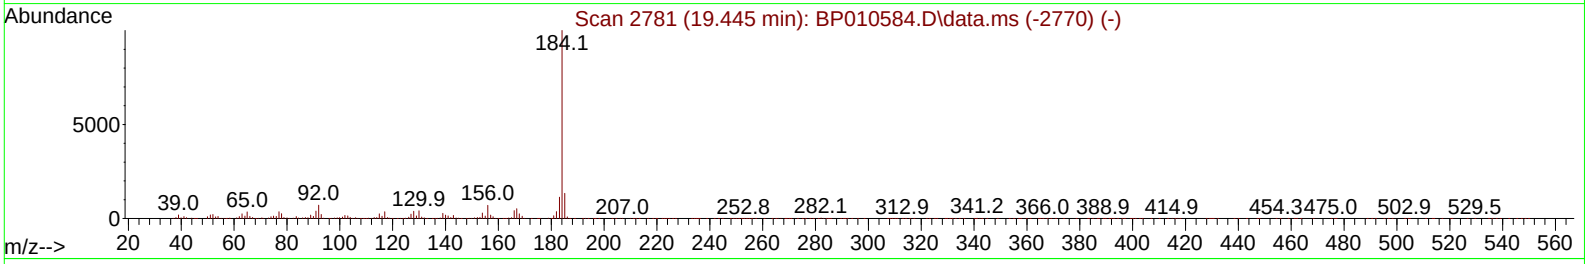

TIC: BP010662.D\data.ms

(77) Benzidine

19.445min (0.000) 572473.95 ng

response 2353327

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.90
183.00	11.30	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/2/2022	BNA_P	BP010662.D
Compound Name	**Response**	**Retention Time**
DDT	1441252	20.645
DDD	22284	20.216
DDE	2915	19.722
SUM(DDD+DDE)	**SUM(DDT+DDD+DDE)**	**% Breakdown Of DDT**
25199	1466451	1.72

Instrument :
BNA_P
ClientSampleId :
DFTPP