
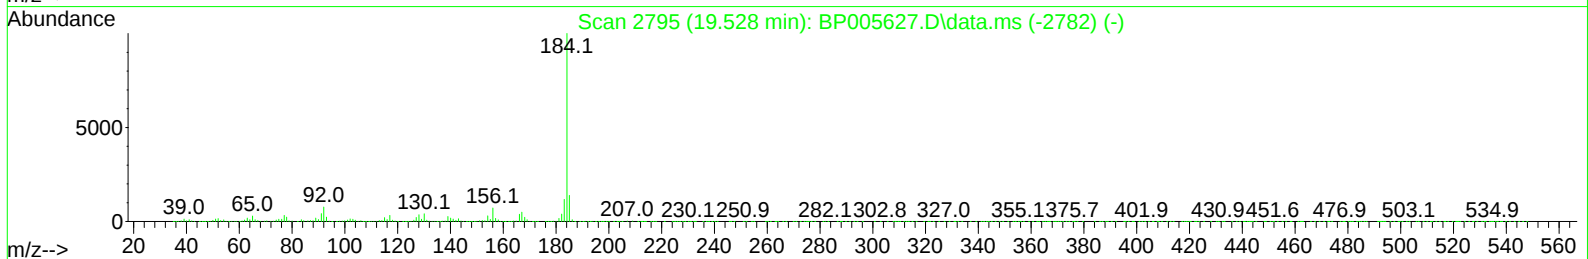
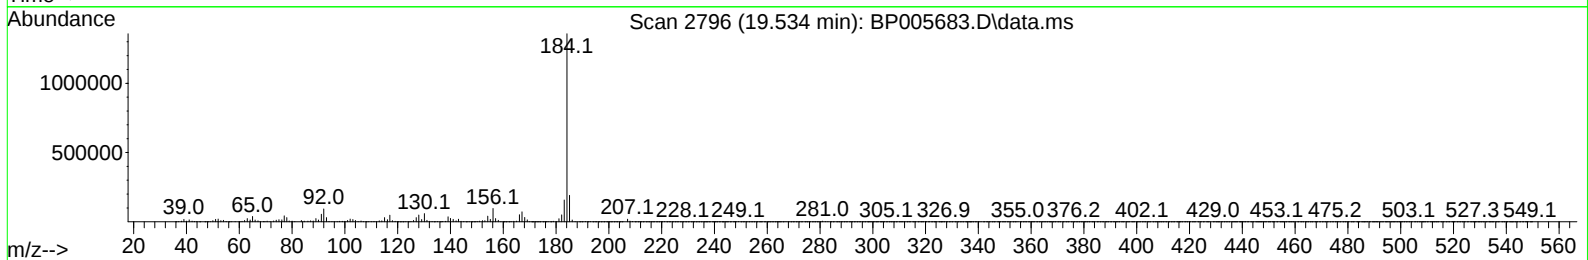


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060321\
 Data File : BP005683.D
 Acq On : 03 Jun 2021 12:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 13:35:14 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

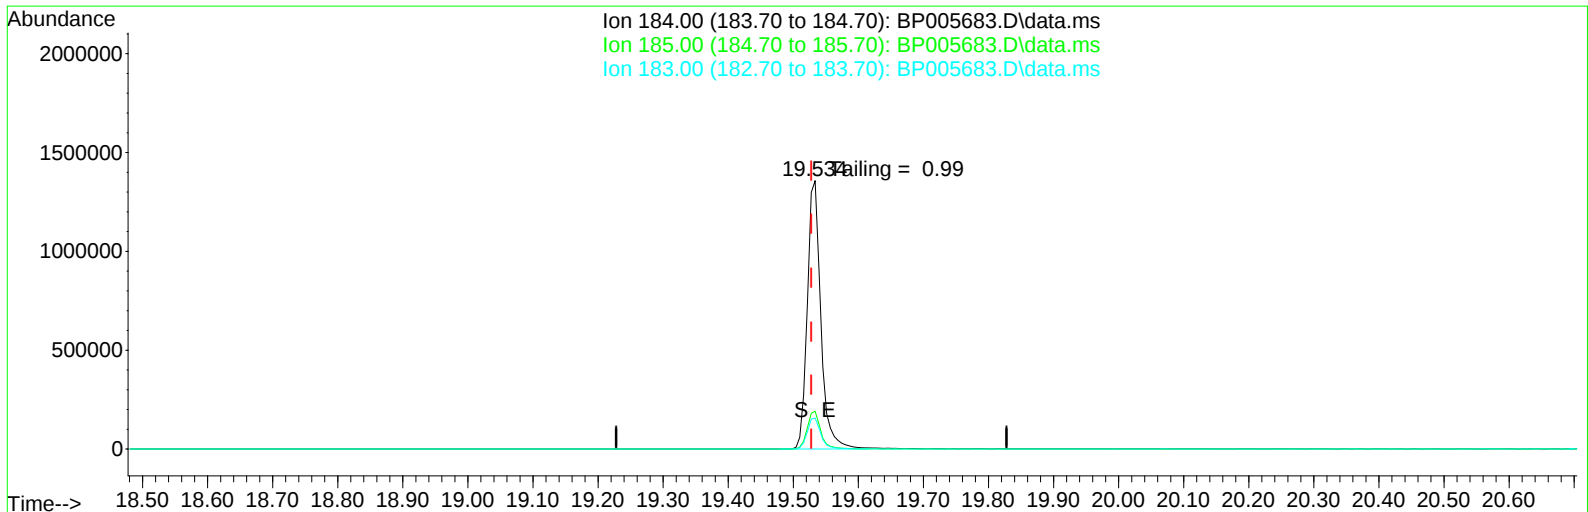

TIC: BP005683.D\data.ms

(77) Benzidine




19.534min (+ 0.006) 82930.22 ng

response 1974991

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.06
183.00	12.30	11.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060321\
Data File : BP005683.D
Acq On : 03 Jun 2021 12:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 13:35:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration

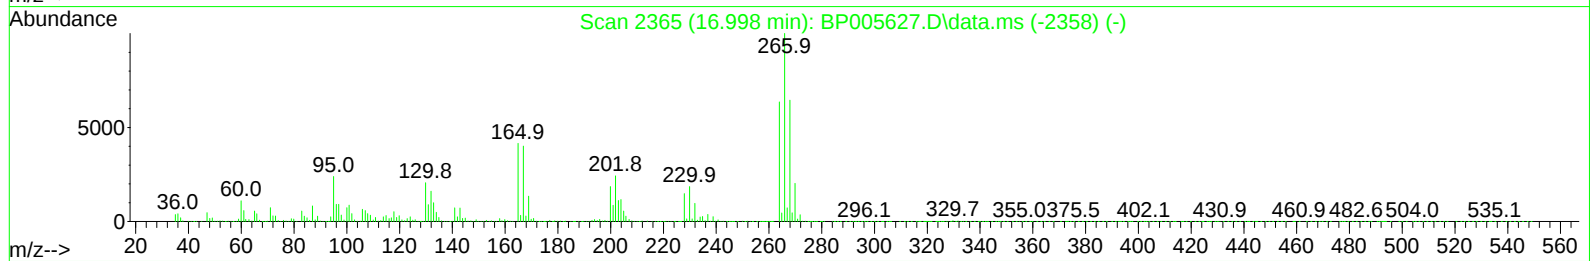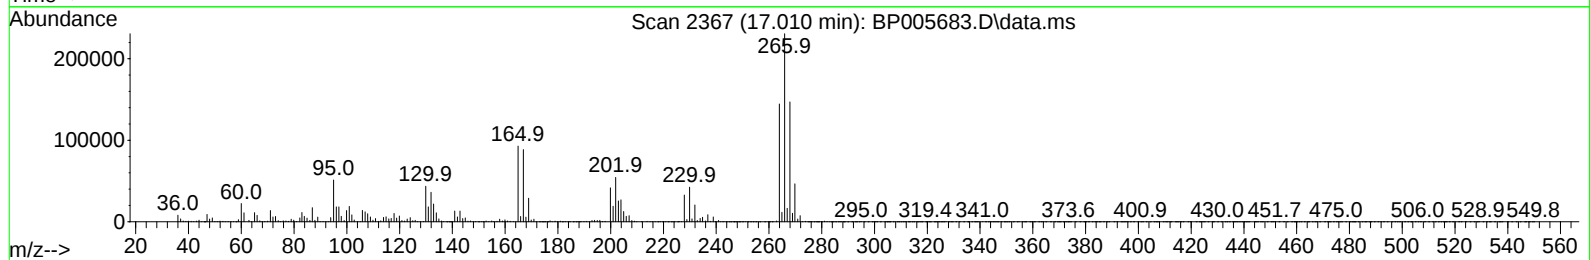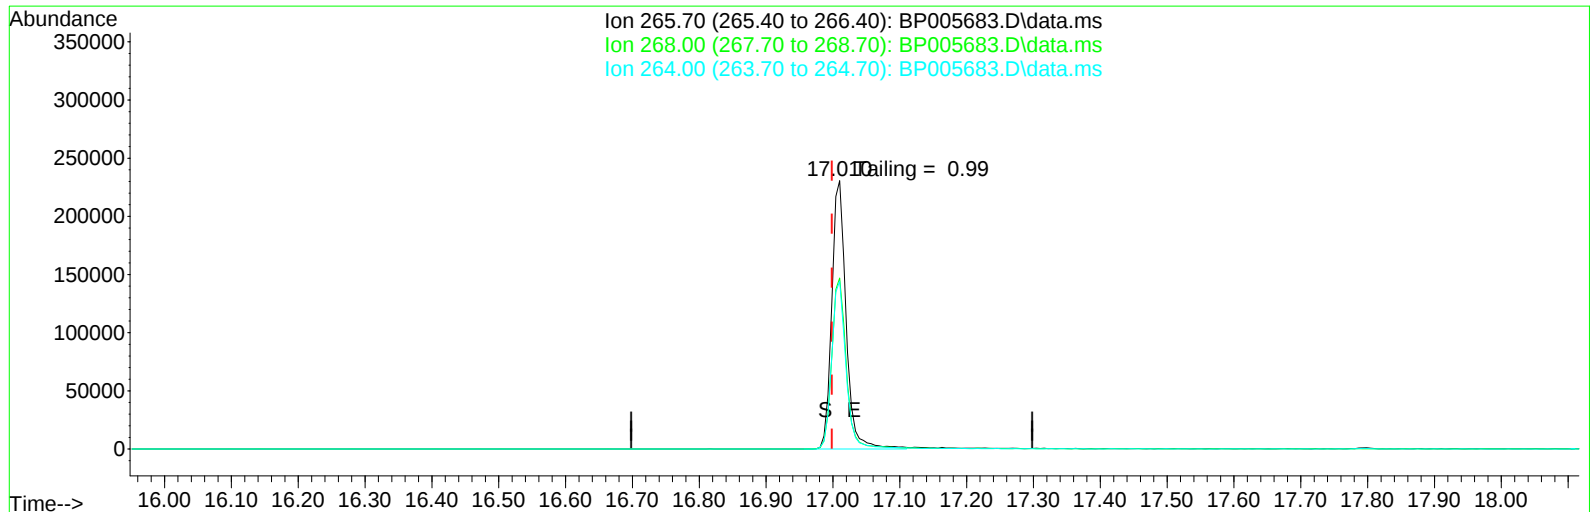

TIC: BP005683.D\data.ms

(70) Pentachlorophenol (C)

17.010min (+ 0.012) 134925.63 ng

response 345556

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.72
264.00	67.10	62.64
0.00	0.00	0.00