

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060321\
 Data File : BP005699.D
 Acq On : 03 Jun 2021 22:04
 Operator : CG/JU
 Sample : M2580-02 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 18-B1(2-4)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.546	411	418	426	rVB	198980	301448	11.23%	1.788%
2	7.146	683	690	700	rBV	200275	326527	12.16%	1.936%
3	7.987	823	833	840	rBV	706581	1153948	42.99%	6.843%
4	9.146	1023	1030	1038	rBV	121597	202977	7.56%	1.204%
5	10.793	1300	1310	1316	rBV	909094	1548312	57.68%	9.182%
6	13.234	1719	1725	1734	rVB	335625	494654	18.43%	2.934%
7	14.063	1860	1866	1870	rBV	30801	44691	1.66%	0.265%
8	14.610	1952	1959	1965	rBV	1394467	1988913	74.09%	11.795%
9	14.669	1965	1969	1977	rVB	41286	68408	2.55%	0.406%
10	15.004	2021	2026	2032	rBV	24717	40256	1.50%	0.239%
11	15.651	2131	2136	2140	rBV2	43986	58700	2.19%	0.348%
12	16.092	2206	2211	2217	rBV	207872	301002	11.21%	1.785%
13	17.351	2419	2425	2430	rBV	1656589	2373212	88.41%	14.074%
14	17.392	2430	2432	2437	rVB	303548	375249	13.98%	2.225%
15	17.486	2444	2448	2453	rVB	96724	128209	4.78%	0.760%
16	17.751	2491	2493	2498	rVB2	36900	48006	1.79%	0.285%
17	19.351	2760	2765	2770	rBV	585393	768575	28.63%	4.558%
18	19.698	2821	2824	2834	rVB	442761	612405	22.81%	3.632%
19	19.892	2853	2857	2861	rVB	606722	692370	25.79%	4.106%
20	21.422	3112	3117	3121	rBV	1948539	2684466	100.00%	15.920%
21	23.863	3528	3532	3541	rVB2	1337372	2649782	98.71%	15.714%




Sum of corrected areas: 16862110

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060321\
Data File : BP005699.D
Acq On : 03 Jun 2021 22:04
Operator : CG/JU
Sample : M2580-02 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

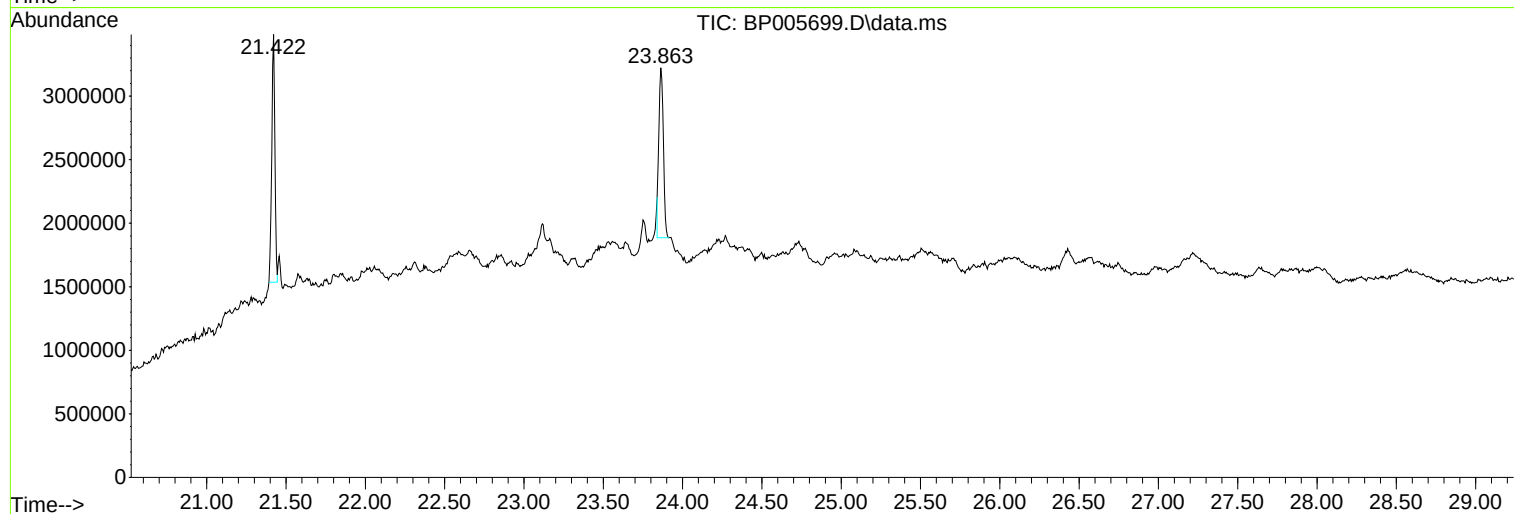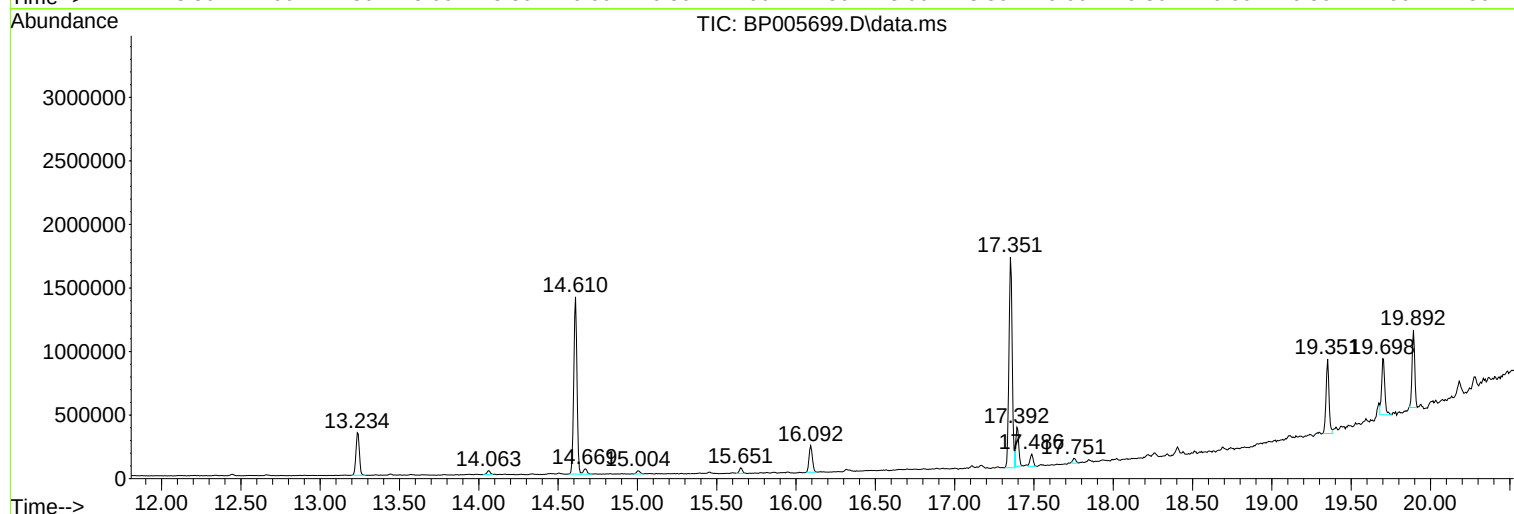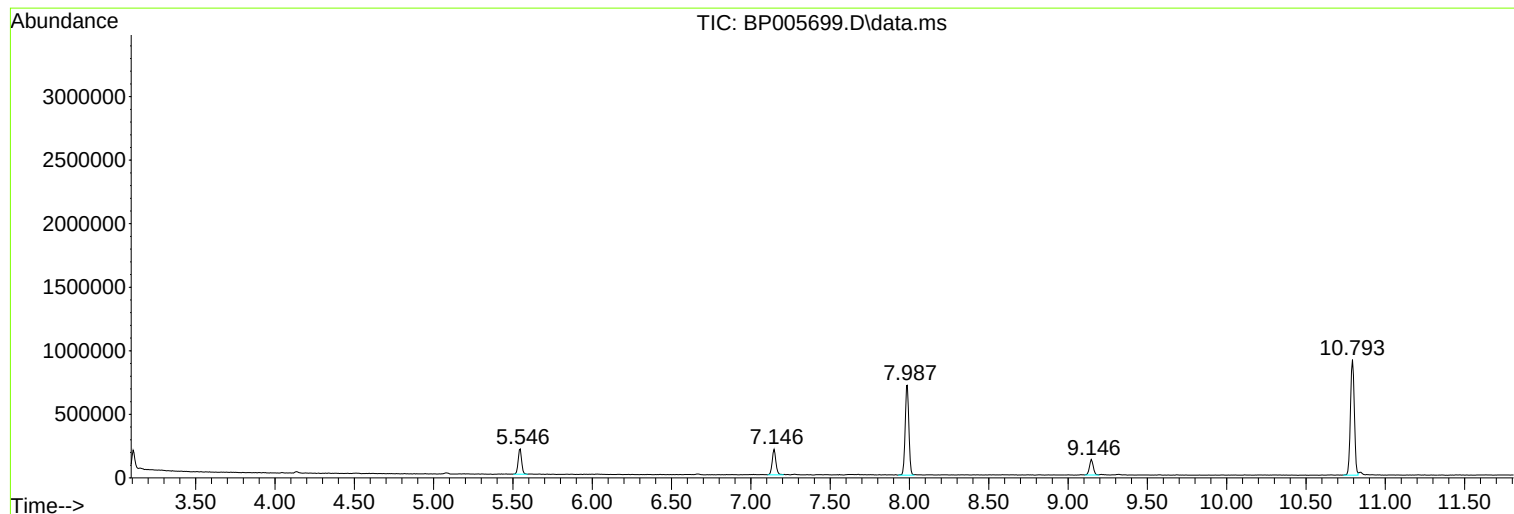

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060321\
Data File : BP005699.D
Acq On : 03 Jun 2021 22:04
Operator : CG/JU
Sample : M2580-02 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060321\
Data File : BP005699.D
Acq On : 03 Jun 2021 22:04
Operator : CG/JU
Sample : M2580-02 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
18-B1(2-4)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc