
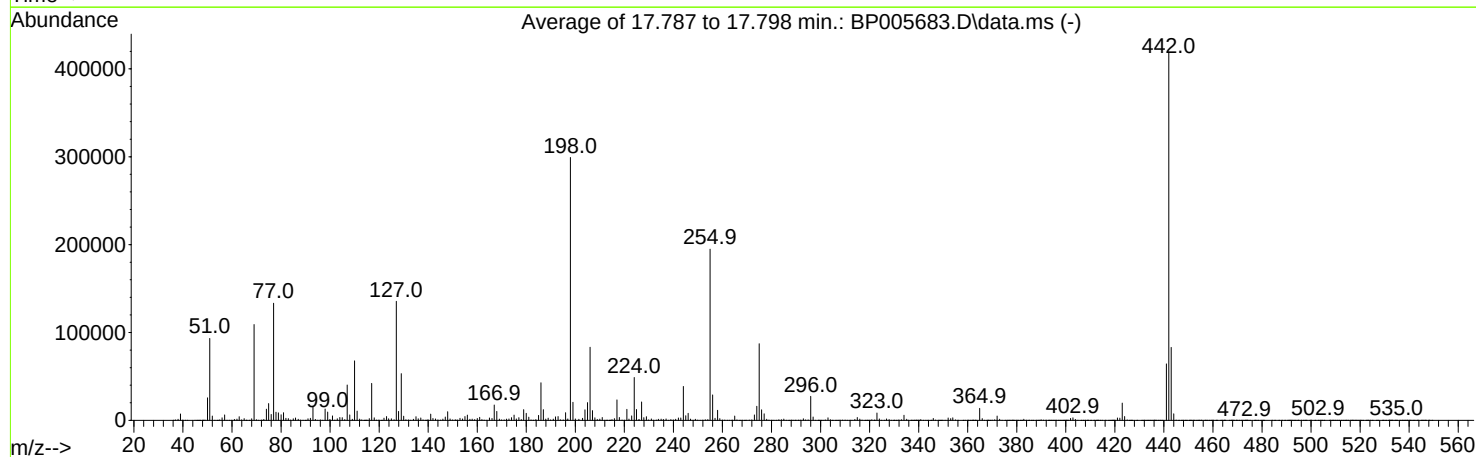


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060321\
 Data File : BP005683.D
 Acq On : 03 Jun 2021 12:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 27 16:11:11 2021

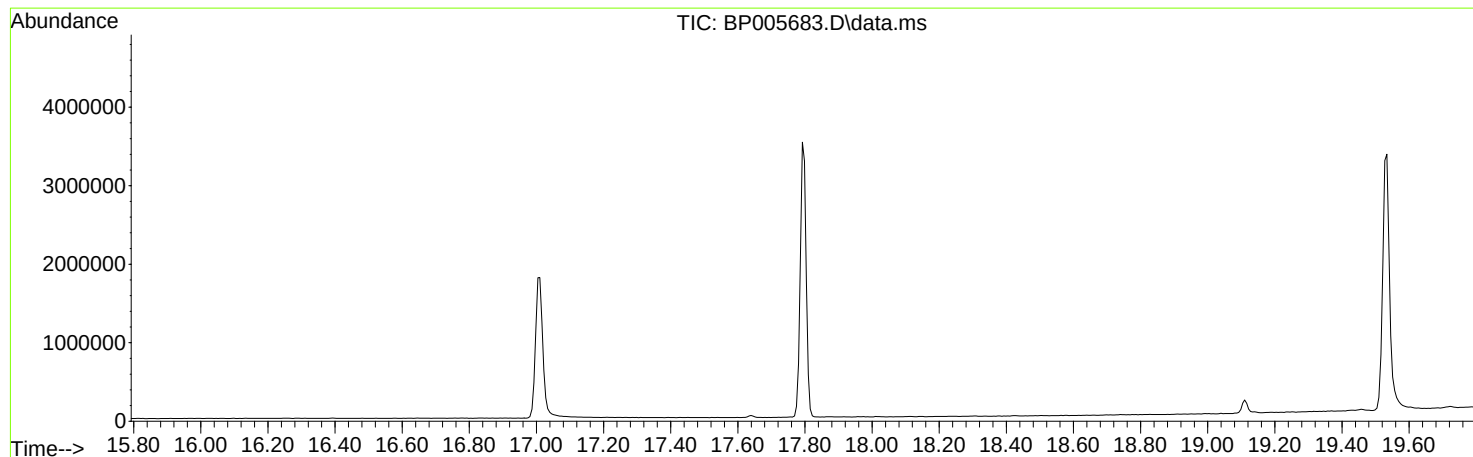

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	93295	PASS
68	69	0.00	2	1.7	1857	PASS
69	198	0.00	100	36.4	108993	PASS
70	69	0.00	2	0.6	689	PASS
127	198	10	80	45.3	135445	PASS
197	198	0.00	2	0.6	1669	PASS
198	198	100	100	100.0	299247	PASS
199	198	5	9	6.9	20632	PASS
275	198	10	60	29.2	87245	PASS
365	198	1	100	4.6	13720	PASS
441	198	0.01	100	21.5	64291	PASS
442	442	100	100	100.0	418659	PASS
443	442	15	24	19.8	83008	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/3/2021	BNA_P	<u>BP005683.D</u>
Compound Name	Response	Retention Time
DDT	1034716	20.73
DDD	66343	20.3
DDE	2667	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
69010	1103726	6.25

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060321\
 Data File : BP005683.D
 Acq On : 03 Jun 2021 12:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 03 13:35:14 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

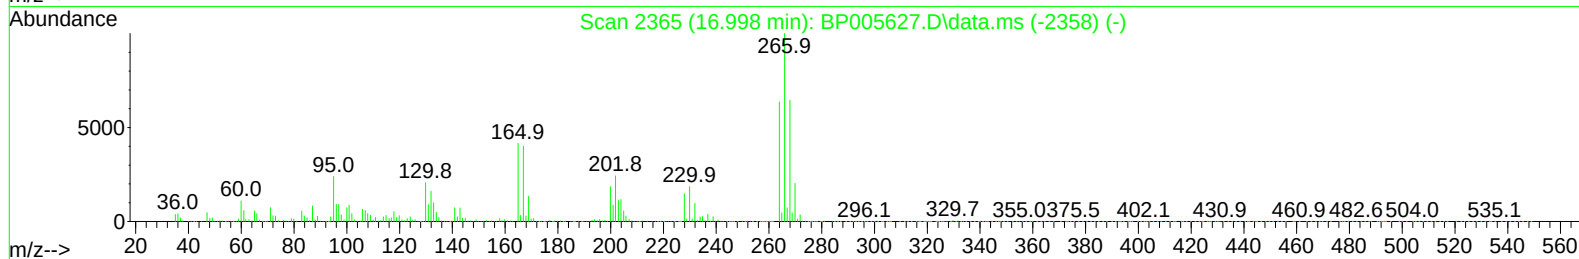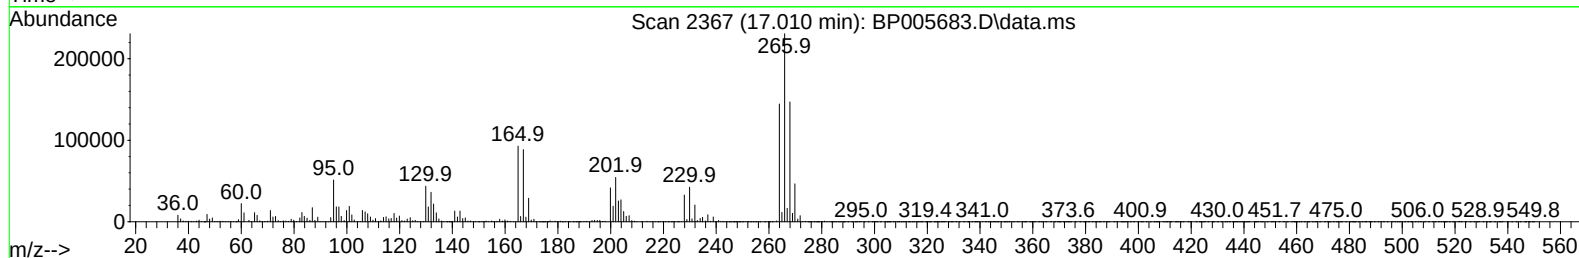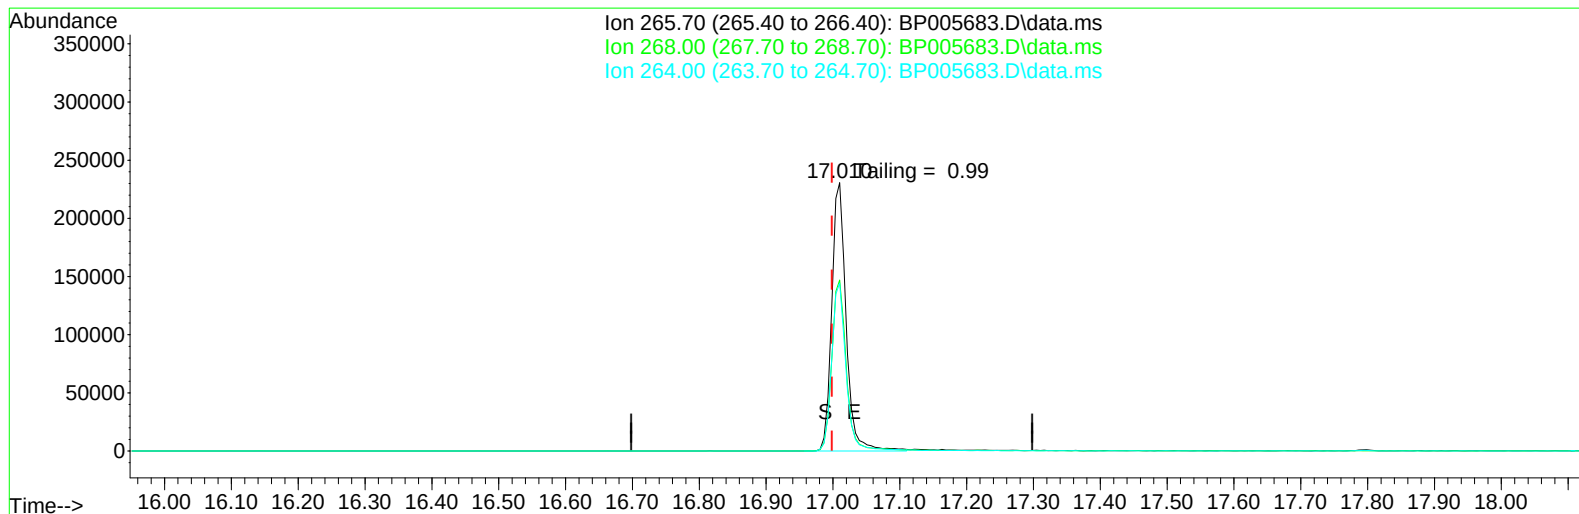

TIC: BP005683.D\data.ms

(70) Pentachlorophenol (C)

17.010min (+ 0.012) 134925.63 ng




response 345556

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.72
264.00	67.10	62.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060321\
 Data File : BP005683.D
 Acq On : 03 Jun 2021 12:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 03 13:35:14 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

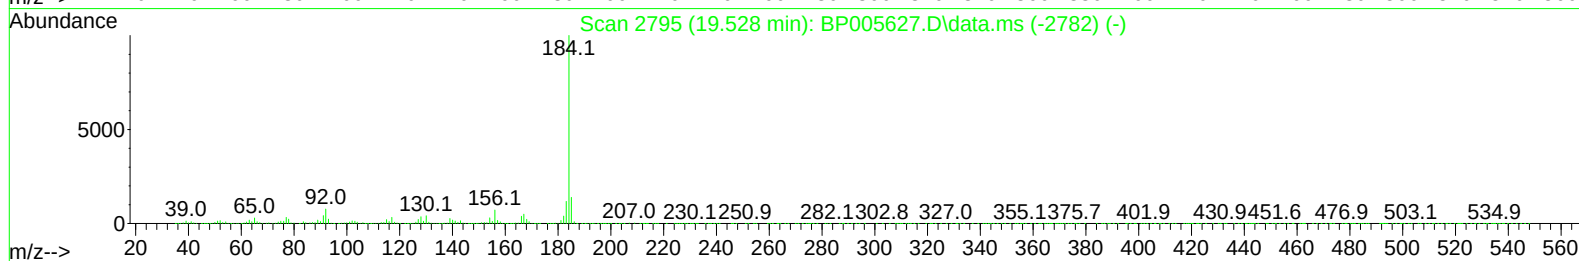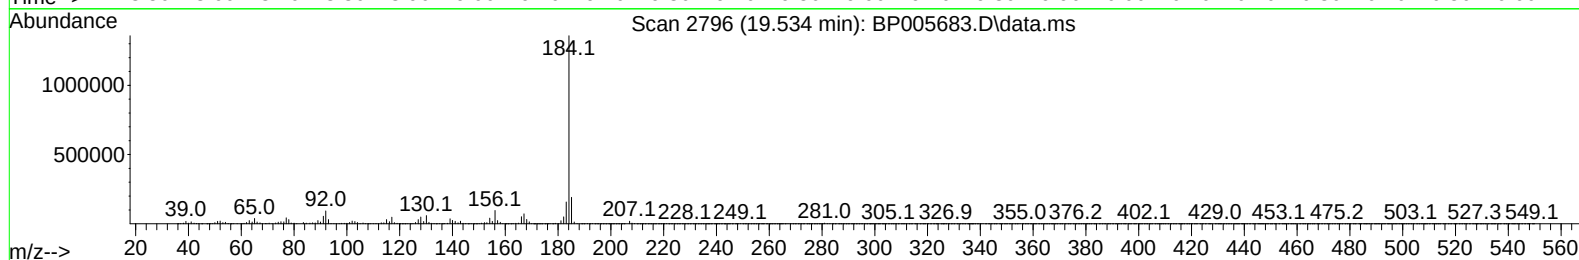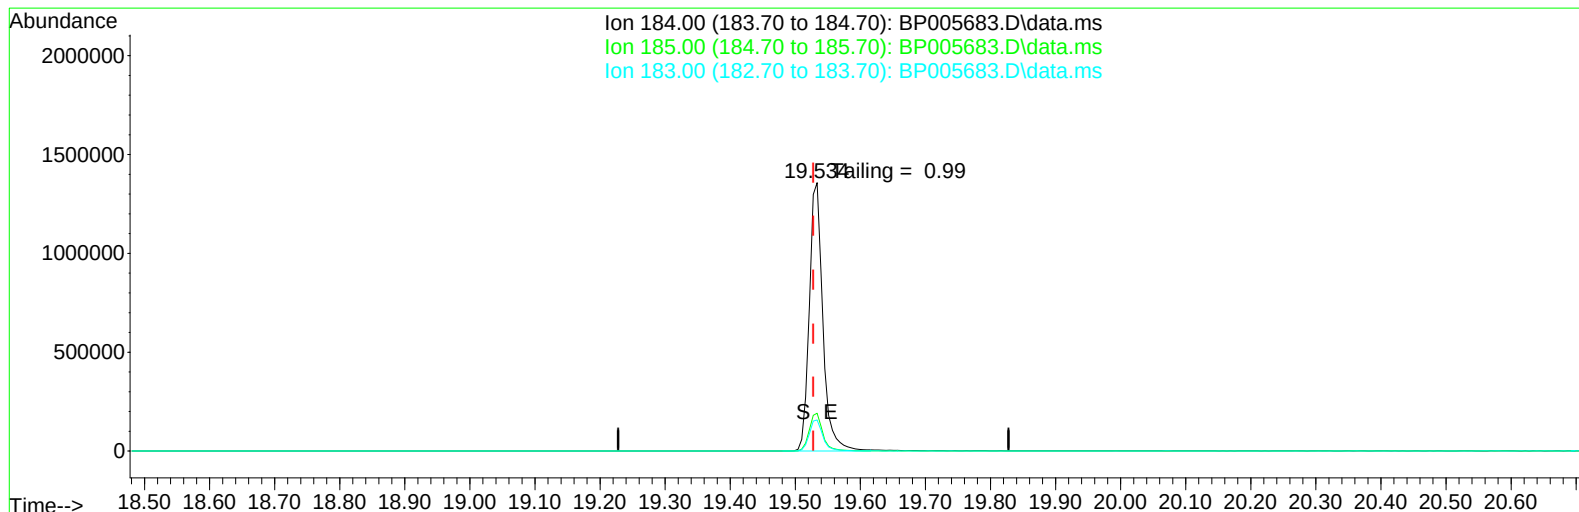

TIC: BP005683.D\data.ms

(77) Benzidine

19.534min (+ 0.006) 82930.22 ng

response 1974991

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.06
183.00	12.30	11.60
0.00	0.00	0.00