
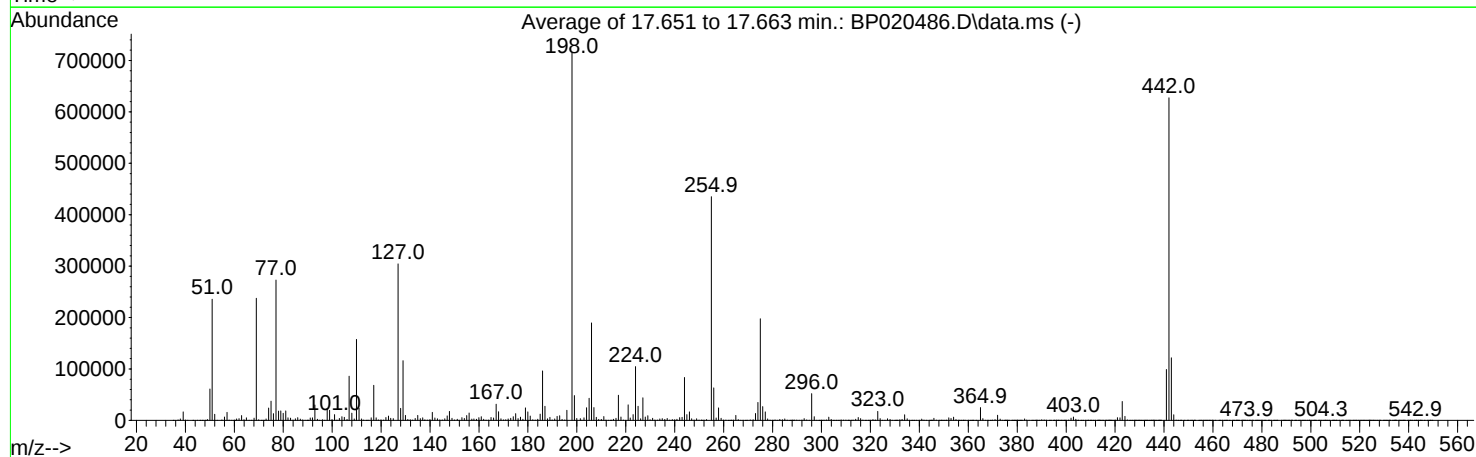


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060324\
Data File : BP020486.D
Acq On : 03 Jun 2024 09:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

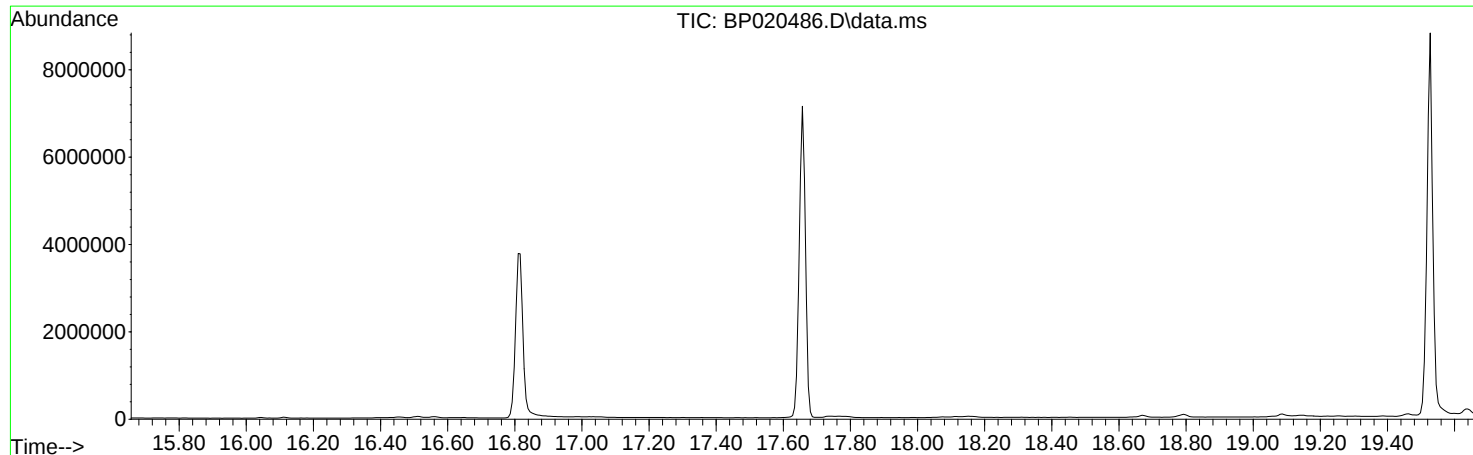




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	235517	PASS
68	69	0.00	2	1.9	4472	PASS
69	198	0.00	100	33.2	237419	PASS
70	69	0.00	2	0.5	1303	PASS
127	198	10	80	42.5	304230	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	715488	PASS
199	198	5	9	6.7	48232	PASS
275	198	10	60	27.6	197504	PASS
365	198	1	100	3.5	25061	PASS
441	198	0.01	100	13.8	98913	PASS
442	442	100	100	100.0	627541	PASS
443	442	15	24	19.4	121645	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060324\
Data File : BP020486.D
Acq On : 03 Jun 2024 09:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 03 13:06:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

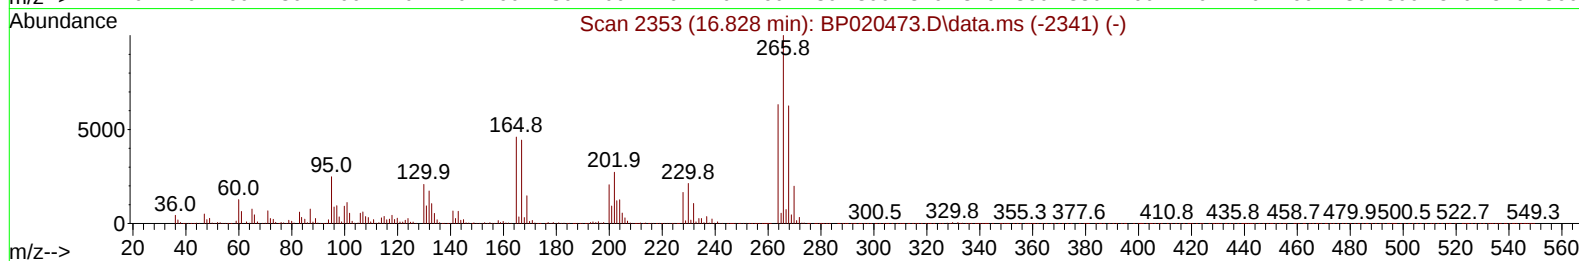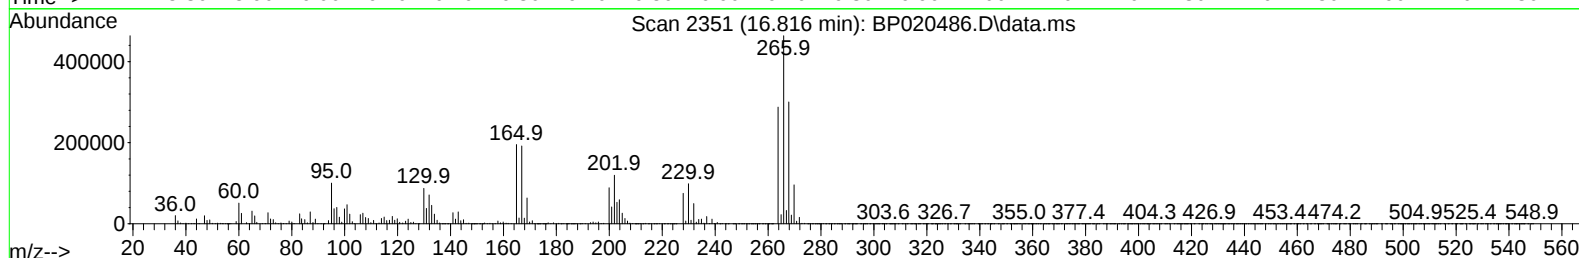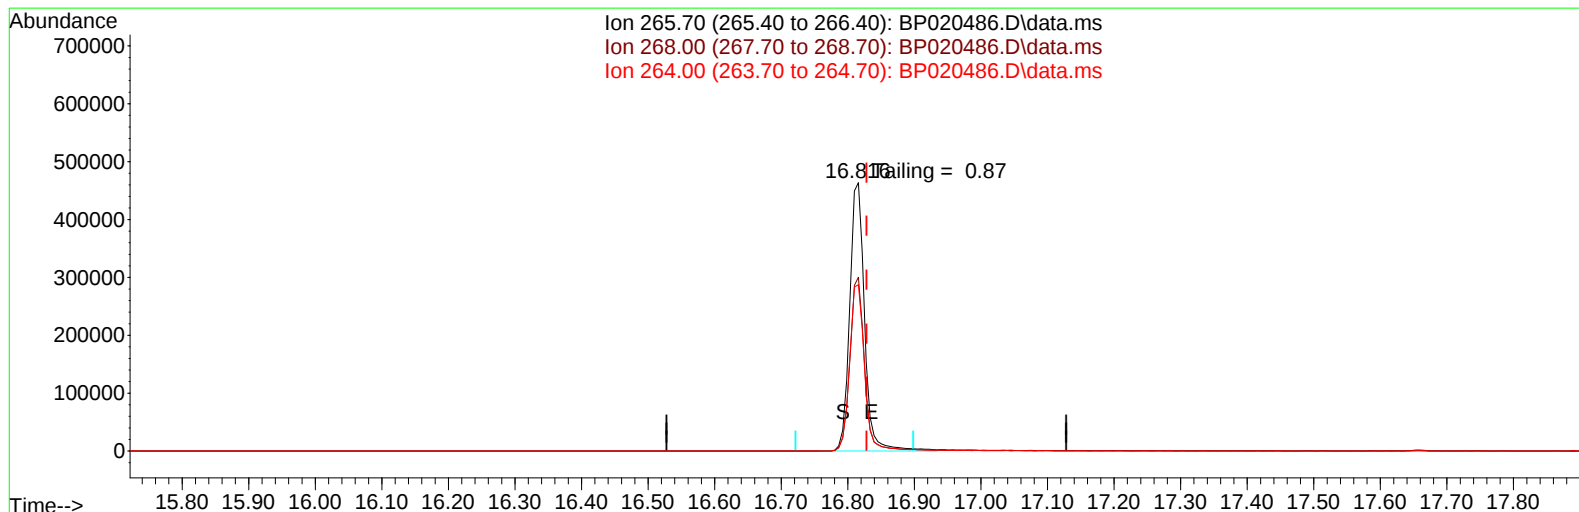

TIC: BP020486.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.012) 342698.26 ng m




response 721747

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.74
264.00	63.30	62.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060324\
Data File : BP020486.D
Acq On : 03 Jun 2024 09:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 03 13:06:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

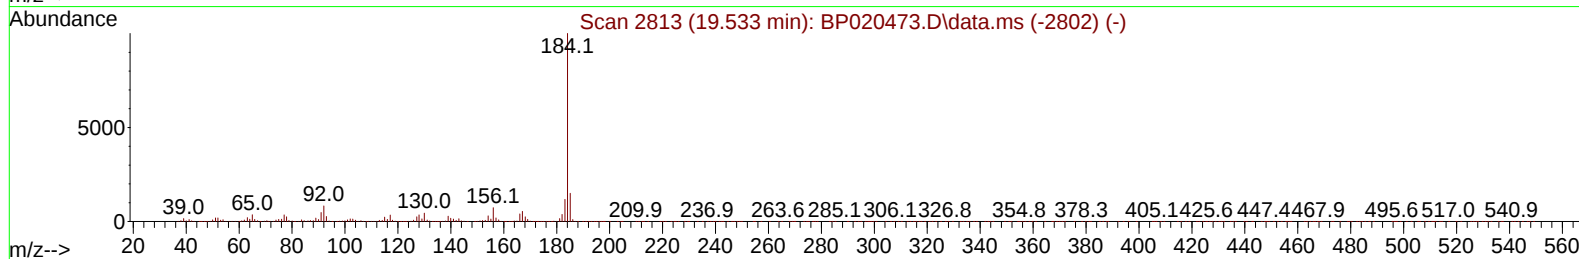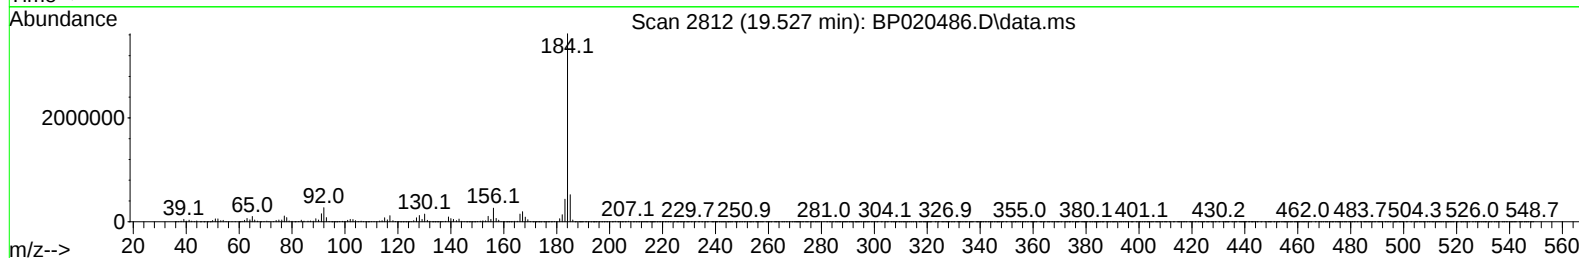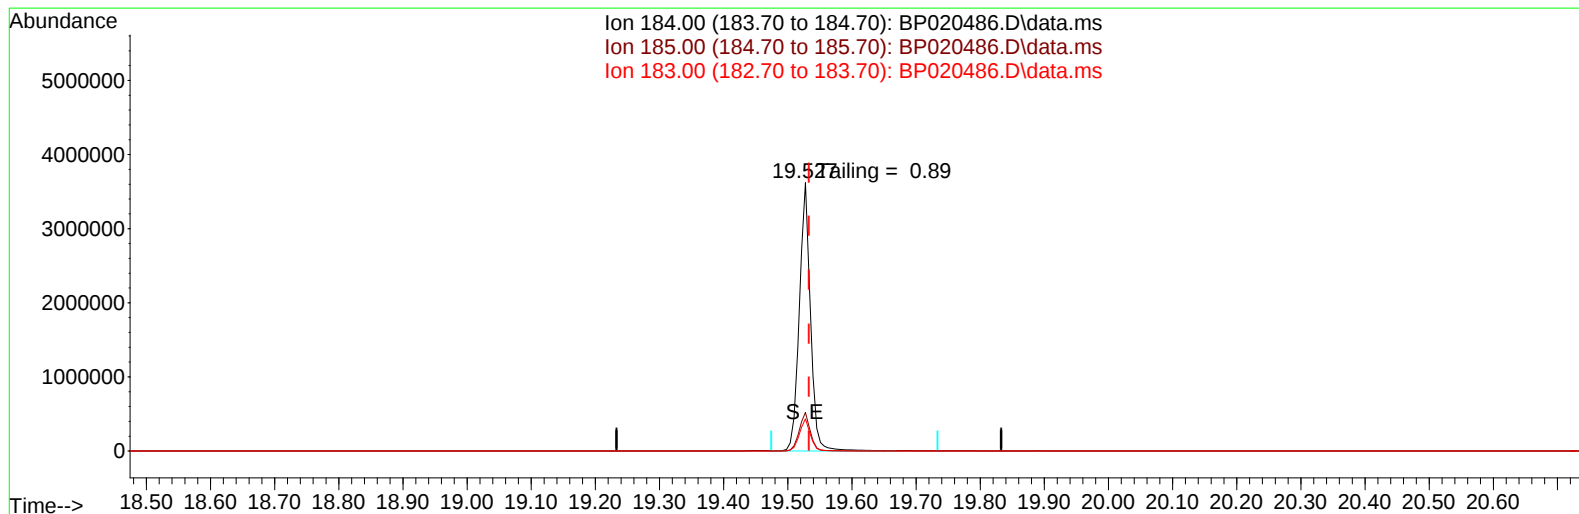

TIC: BP020486.D\data.ms

(77) Benzidine

19.527min (-0.006) 1963.12 ng

response 4334646

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.36
183.00	11.70	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/3/2024	BNA_P	<u>BP020486.D</u>
Compound Name	Response	Retention Time
DDT	2005442	20.822
DDD	25765	20.416
DDE	2529	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28294	2033736	1.39

Instrument :
BNA_P
ClientSampleId :
DFTPP