
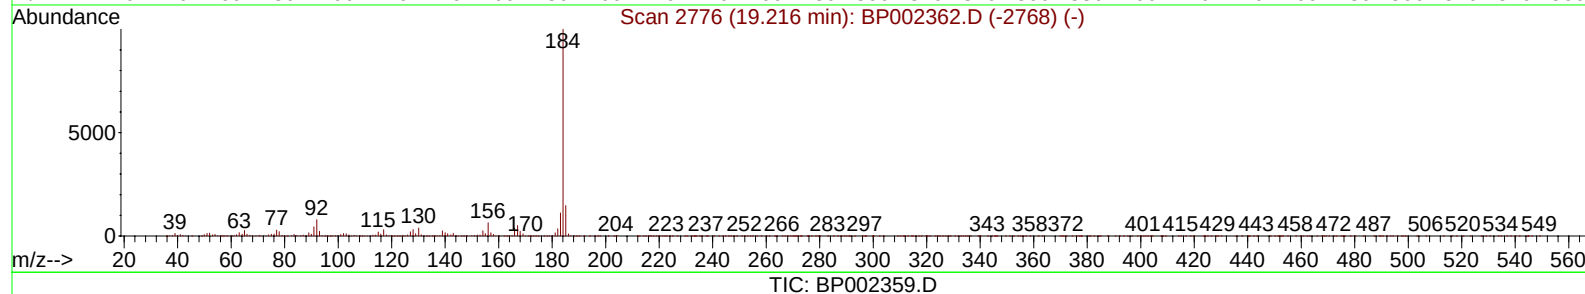
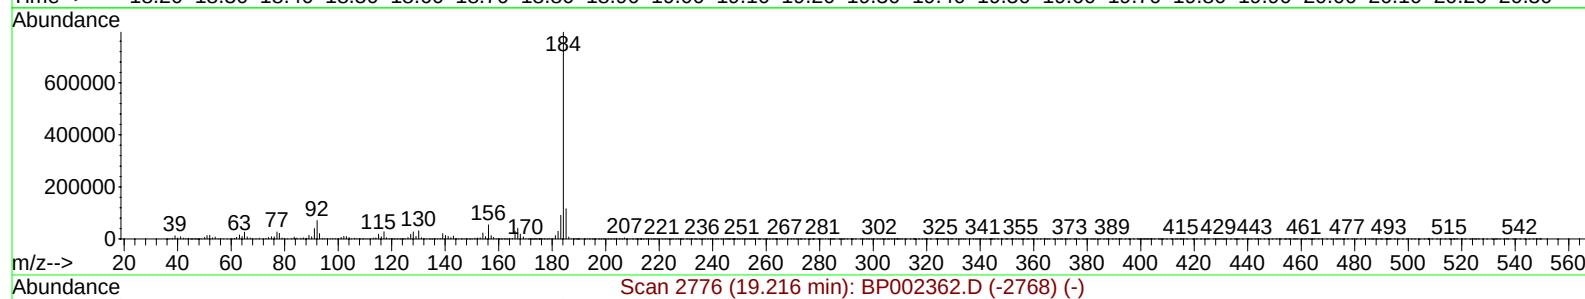


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP060420\
 Data File : BP002359.D
 Acq On : 04 Jun 2020 11:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 16:17:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 04 16:04:12 2020
 Response via : Initial Calibration

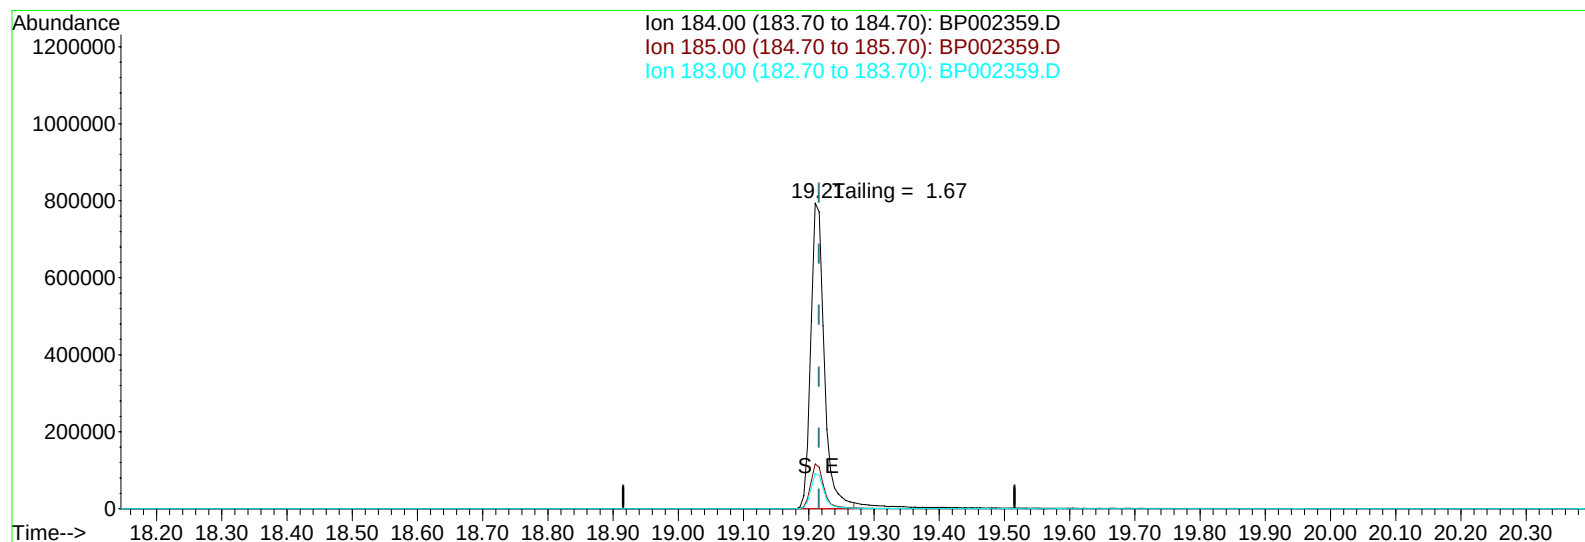

(77) Benzidine

19.210min (-0.006) 182478.41ng

response 1181768

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.64
183.00	11.10	11.46
0.00	0.00	0.00