


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060420\
 Data File : BP002359.D
 Acq On : 04 Jun 2020 11:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 04 16:24:14 2020

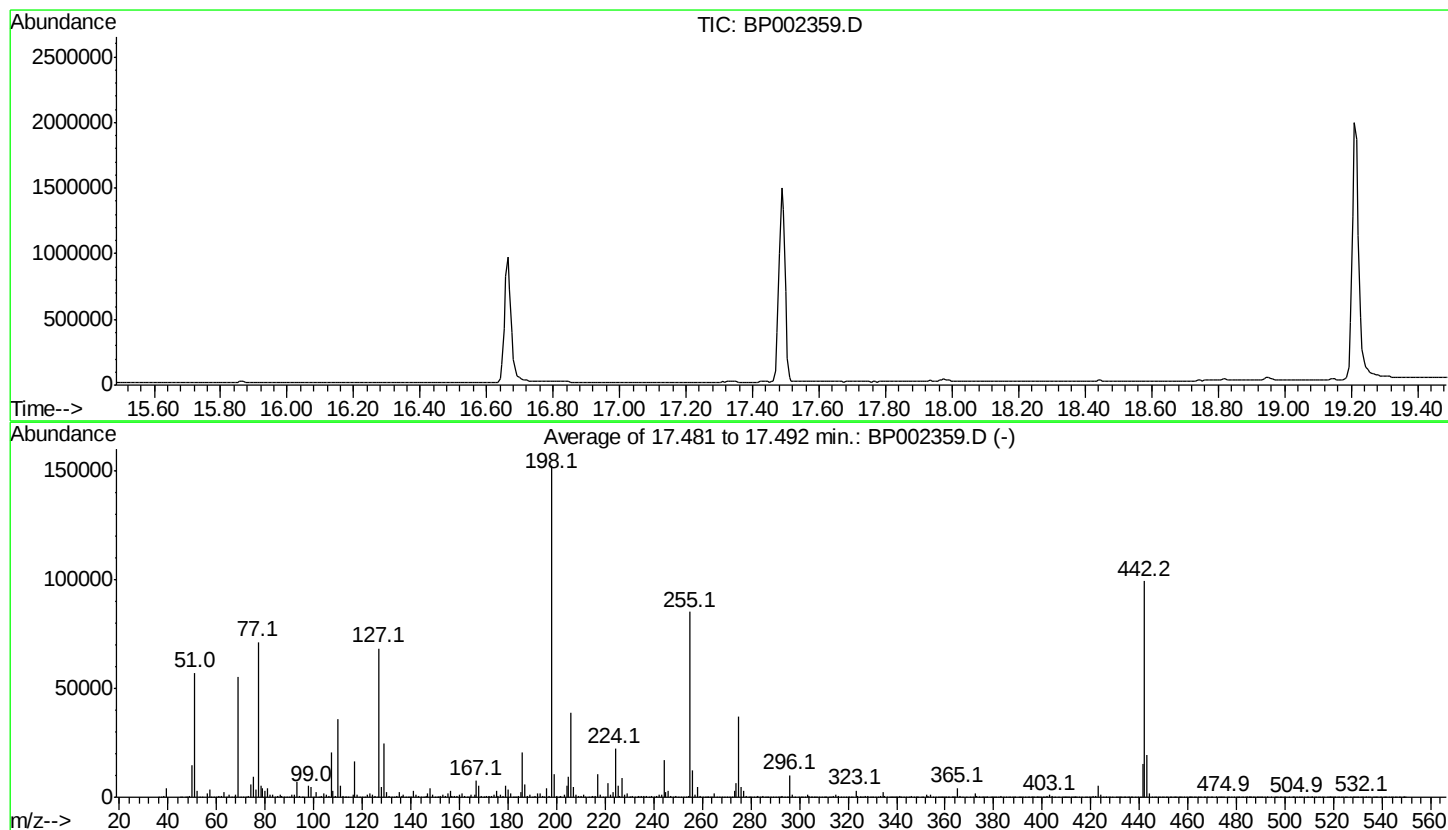

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	56988	PASS
68	69	0.00	2	1.6	905	PASS
69	198	0.00	100	36.3	55262	PASS
70	69	0.00	2	0.5	255	PASS
127	198	10	80	44.8	68188	PASS
197	198	0.00	2	0.5	712	PASS
198	198	100	100	100.0	152154	PASS
199	198	5	9	6.9	10456	PASS
275	198	10	60	24.4	37056	PASS
365	198	1	100	2.8	4286	PASS
441	198	0.01	100	10.1	15384	PASS
442	198	50	100	65.2	99141	PASS
443	442	15	24	19.4	19230	PASS