
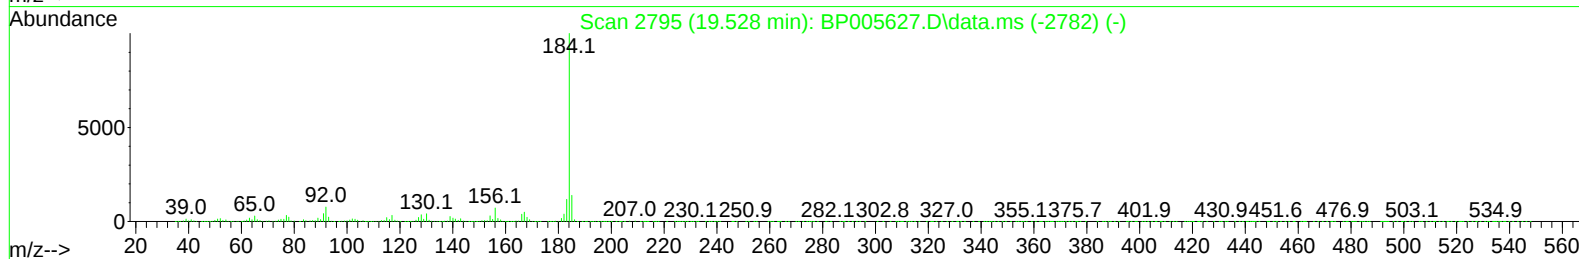
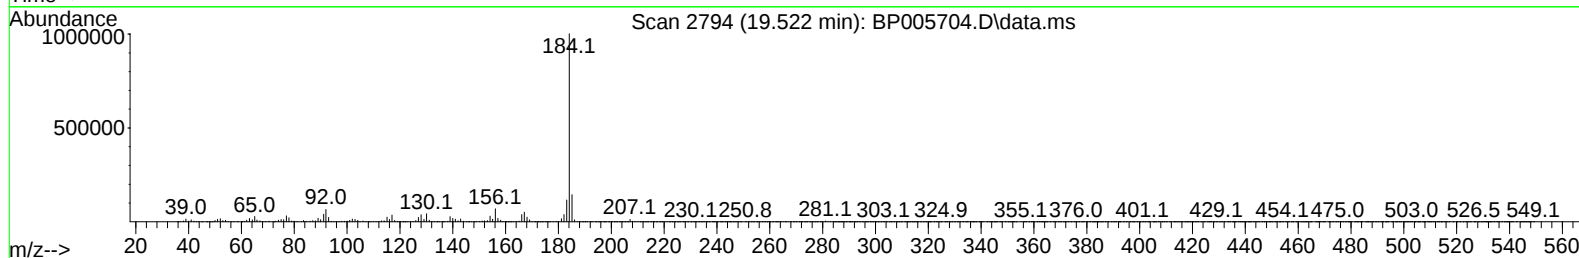


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060421\
Data File : BP005704.D
Acq On : 04 Jun 2021 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 11:25:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration

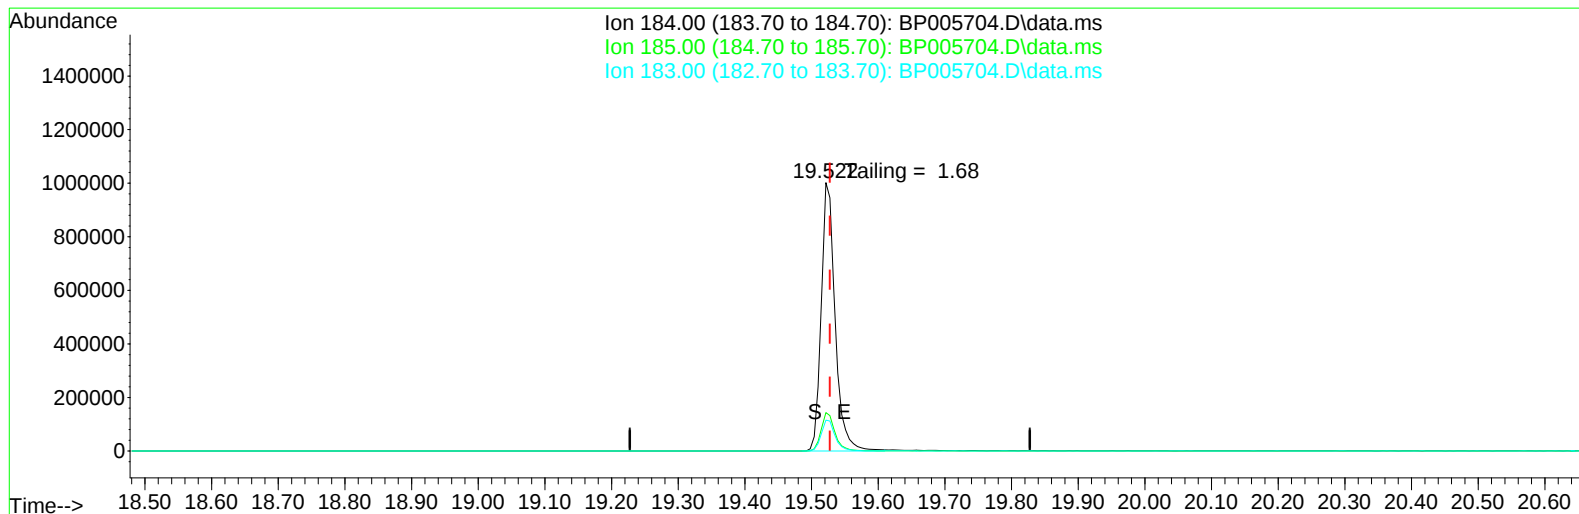




TIC: BP005704.D\data.ms

(77) Benzidine**19.522min (-0.006) 329927.63 ng****response 1459921**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.35
183.00	12.30	11.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060421\
Data File : BP005704.D
Acq On : 04 Jun 2021 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 11:25:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration

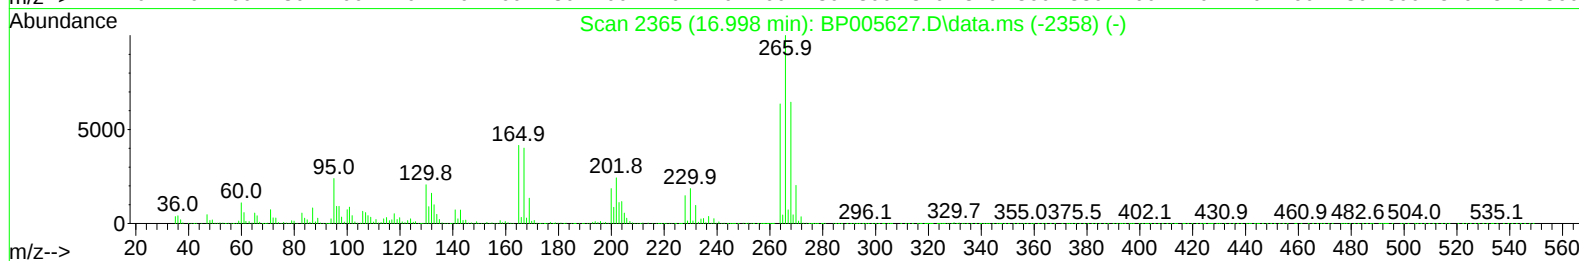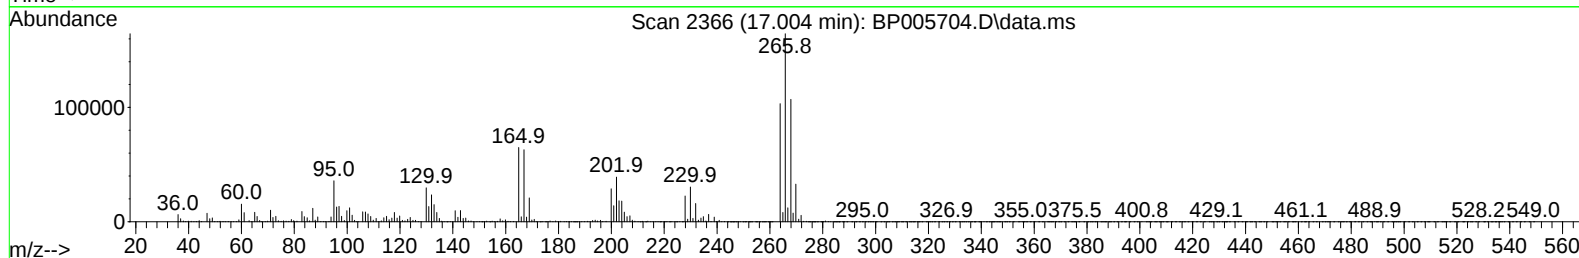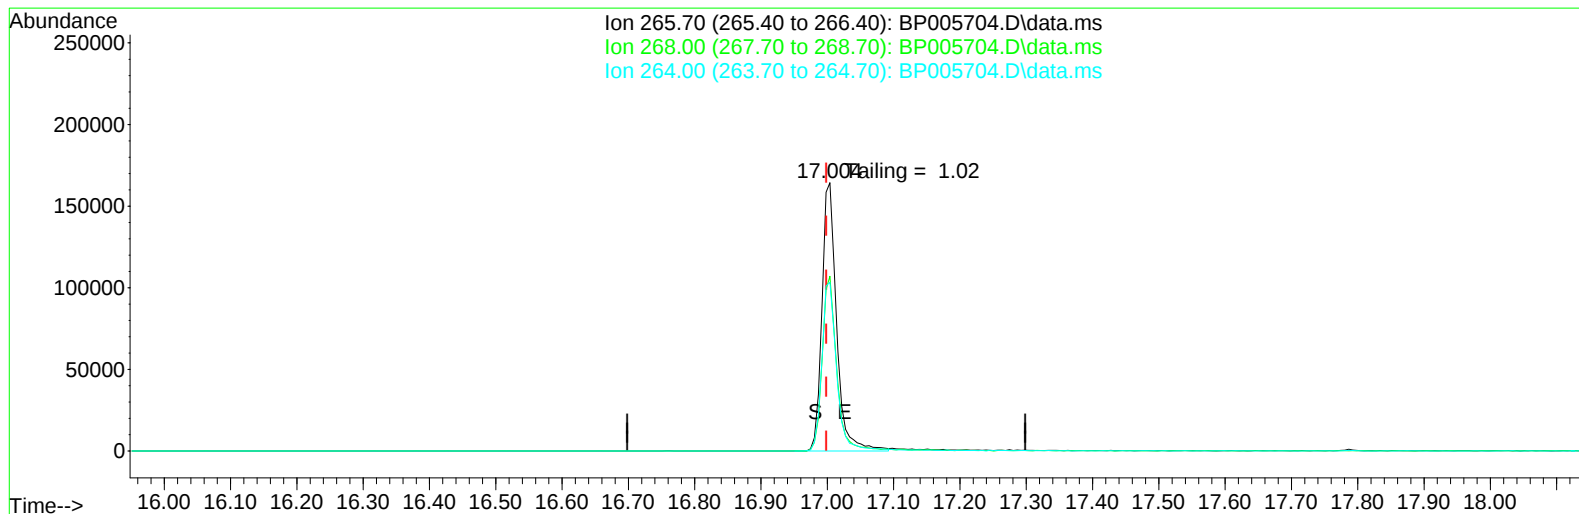

TIC: BP005704.D\data.ms

(70) Pentachlorophenol (C)

17.004min (+ 0.006) 196493.47 ng

response 255859

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.13
264.00	67.10	62.85
0.00	0.00	0.00