
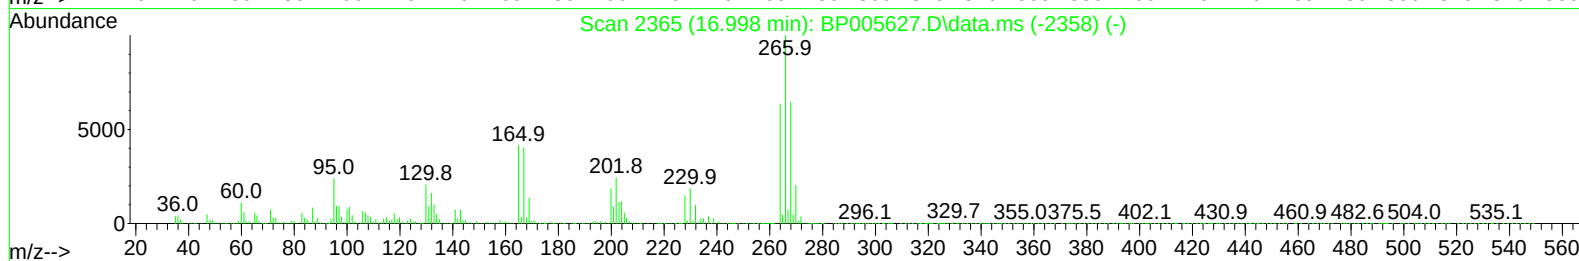
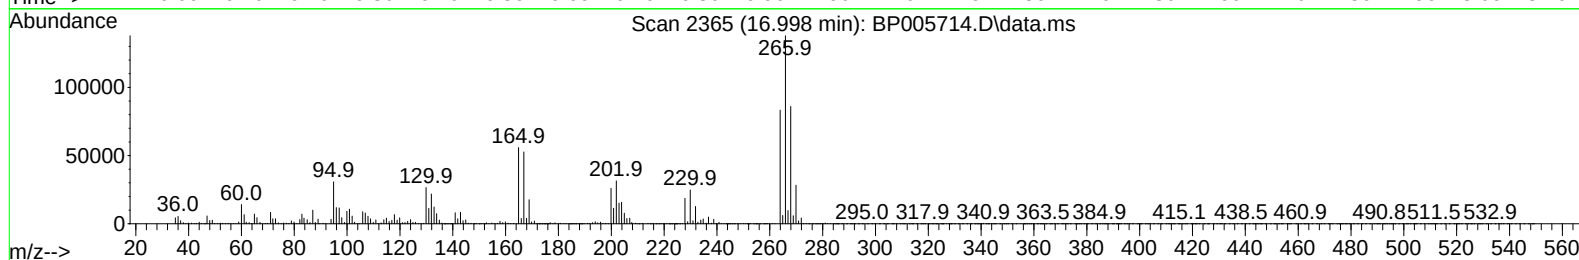


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060421\
 Data File : BP005714.D
 Acq On : 04 Jun 2021 16:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 17:08:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

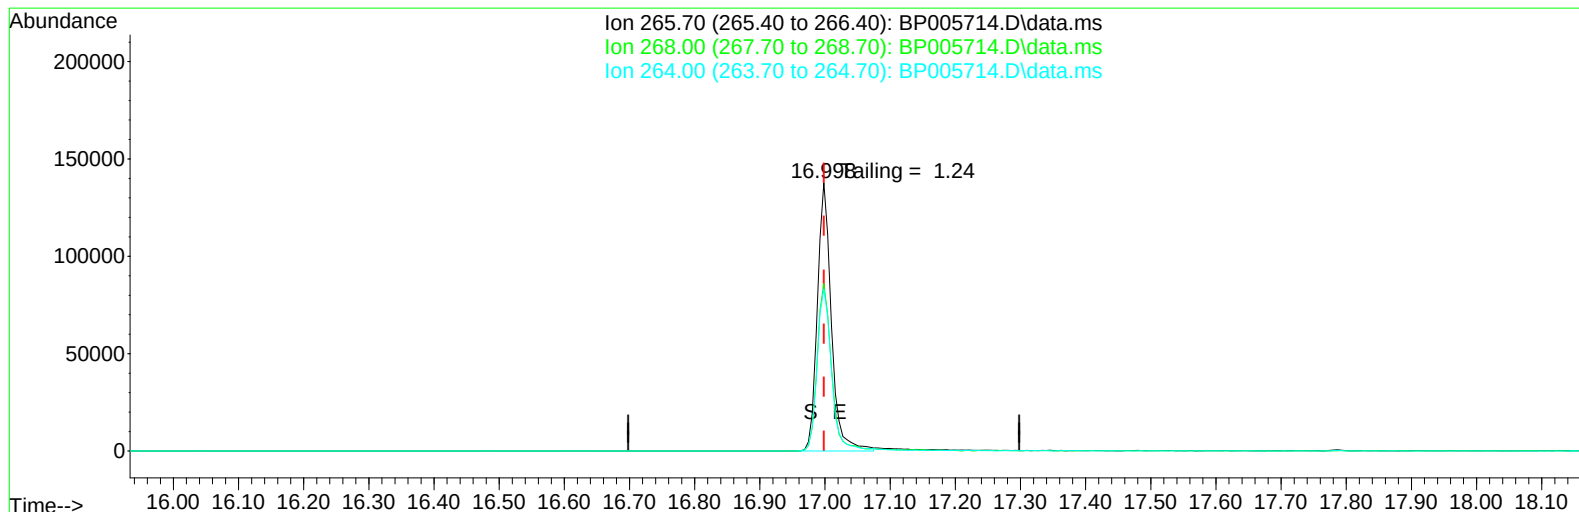

TIC: BP005714.D\data.ms

(70) Pentachlorophenol (C)




16.998min (-0.000) 81996.97 ng

response 211181

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.37
264.00	67.10	60.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060421\
Data File : BP005714.D
Acq On : 04 Jun 2021 16:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 17:08:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration

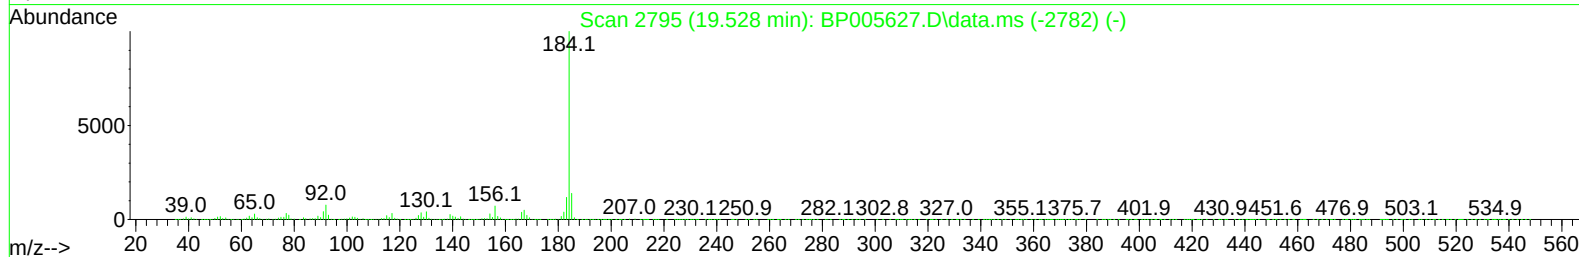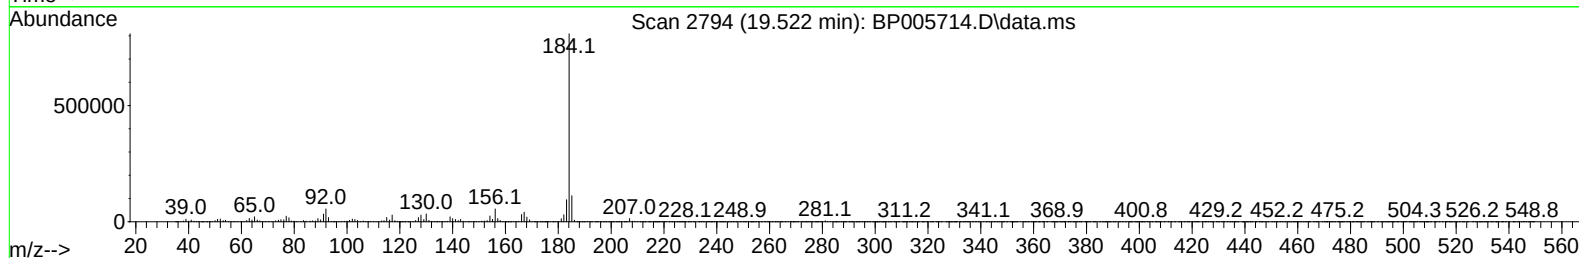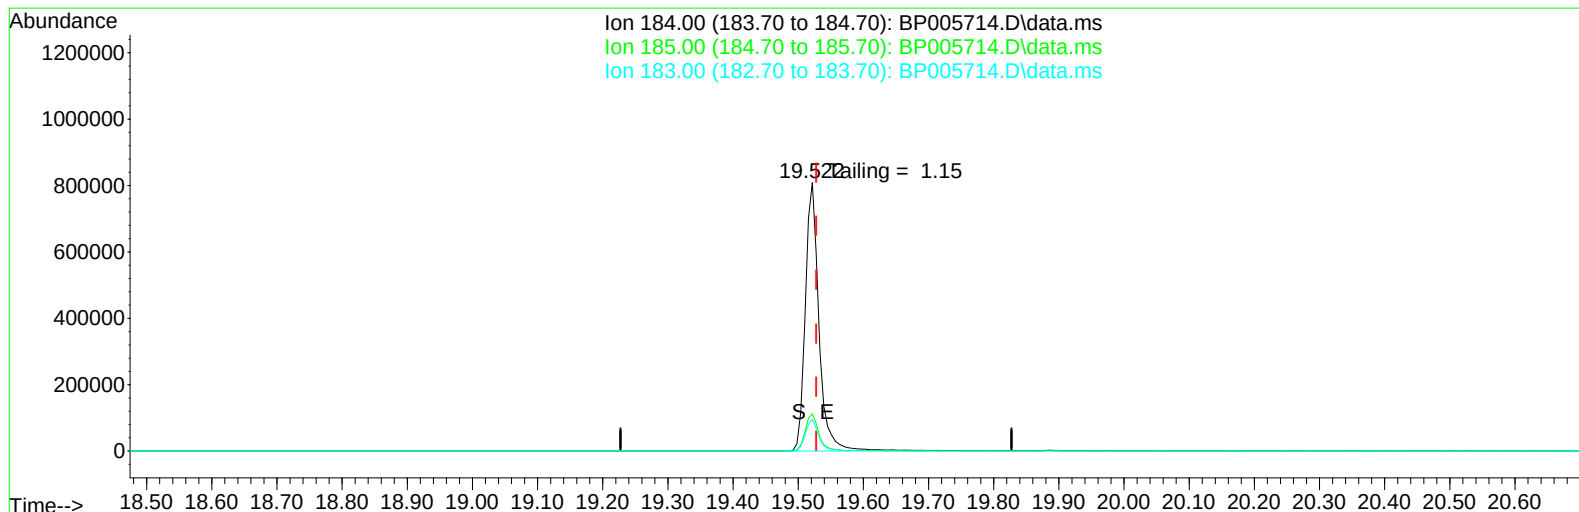

TIC: BP005714.D\data.ms

(77) Benzidine

19.522min (-0.006) 27923.57 ng

response 1177277

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.86
183.00	12.30	11.78
0.00	0.00	0.00