

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060421\
 Data File : BP005706.D
 Acq On : 04 Jun 2021 11:17
 Operator : CG/JU
 Sample : PB136792BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB136792BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.546	411	418	427	rBV	2318605	3475856	43.17%	10.185%
2	7.146	683	690	703	rBV	2177796	3421719	42.50%	10.027%
3	7.981	825	832	839	rVB	445362	697435	8.66%	2.044%
4	9.145	1022	1030	1041	rBV	1375725	2226820	27.66%	6.525%
5	10.787	1299	1309	1319	rBV	532541	921069	11.44%	2.699%
6	13.233	1717	1725	1741	rBV	3318323	5024512	62.40%	14.724%
7	14.604	1952	1958	1969	rBV	764353	1163639	14.45%	3.410%
8	16.092	2203	2211	2236	rBV	2683394	4079017	50.66%	11.953%
9	17.351	2418	2425	2438	rBV	934185	1413573	17.56%	4.142%
10	19.892	2851	2857	2865	rBV	6487822	8051737	100.00%	23.594%
11	21.415	3111	3116	3121	rBV	1333700	1767890	21.96%	5.181%
12	23.856	3525	3531	3540	rVB2	916836	1882460	23.38%	5.516%




Sum of corrected areas: 34125727

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060421\
Data File : BP005706.D
Acq On : 04 Jun 2021 11:17
Operator : CG/JU
Sample : PB136792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136792BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

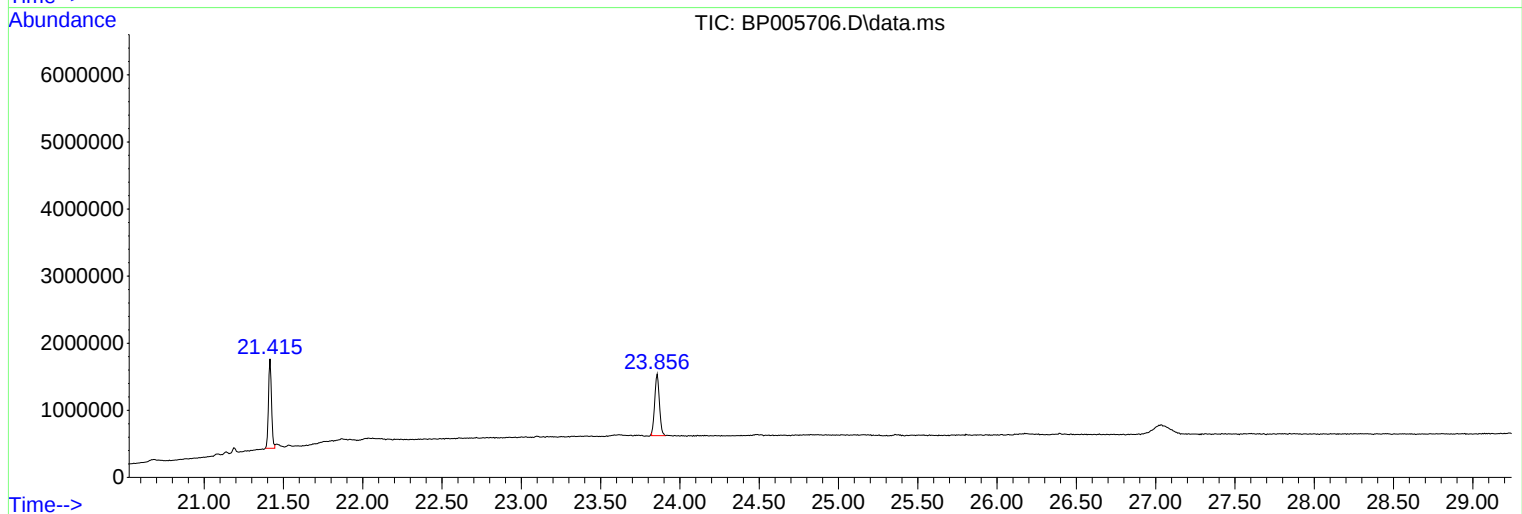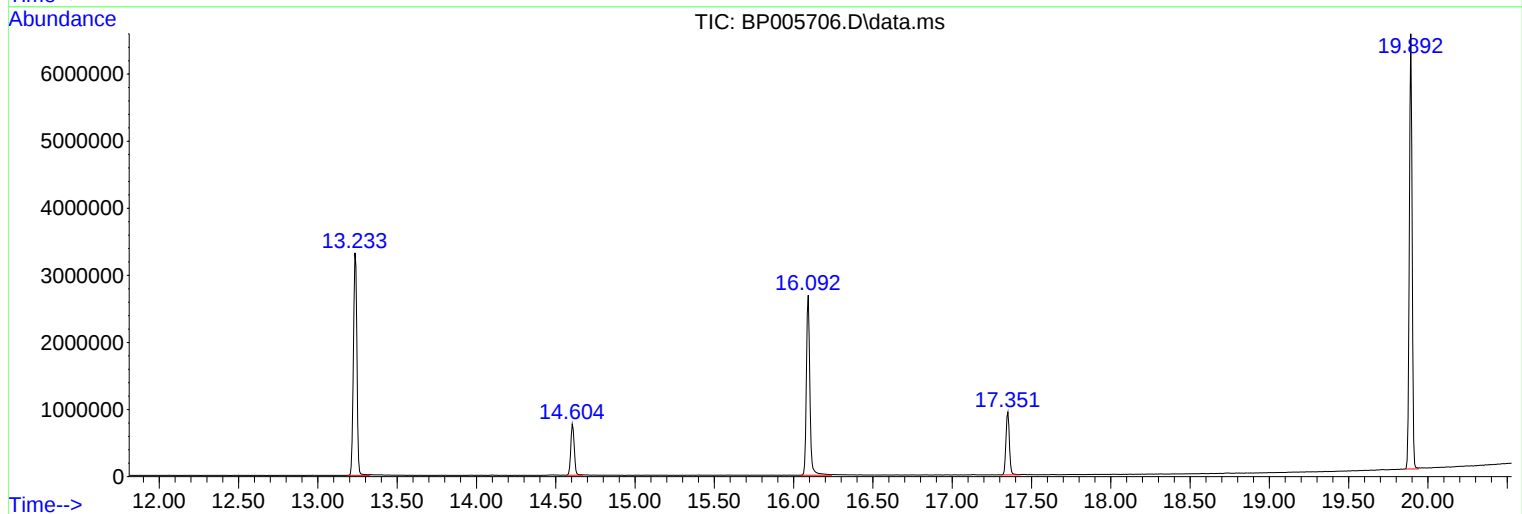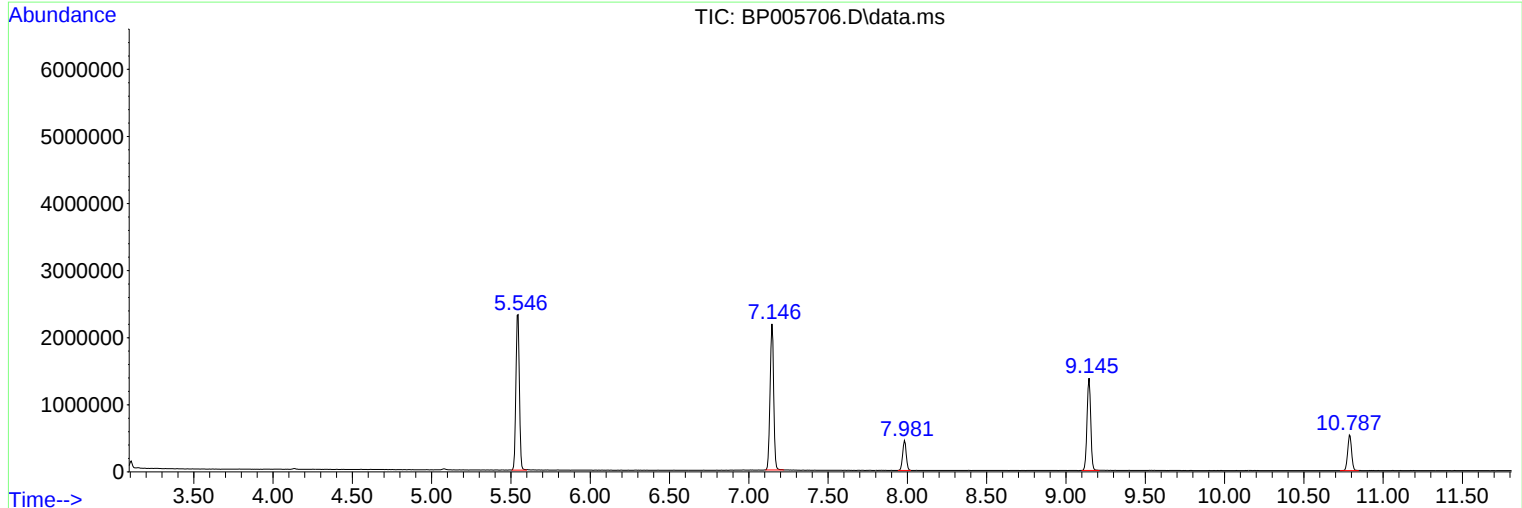

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060421\
Data File : BP005706.D
Acq On : 04 Jun 2021 11:17
Operator : CG/JU
Sample : PB136792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136792BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060421\
Data File : BP005706.D
Acq On : 04 Jun 2021 11:17
Operator : CG/JU
Sample : PB136792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136792BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------