
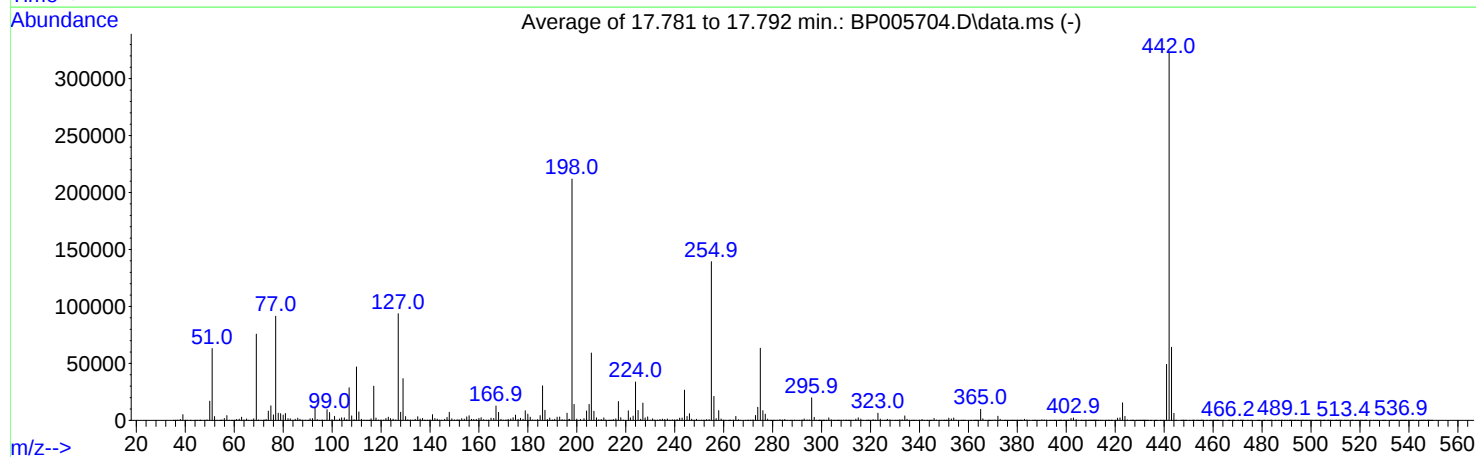


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060421\  
 Data File : BP005704.D  
 Acq On : 04 Jun 2021 09:26  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052721.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jun 07 12:13:53 2021

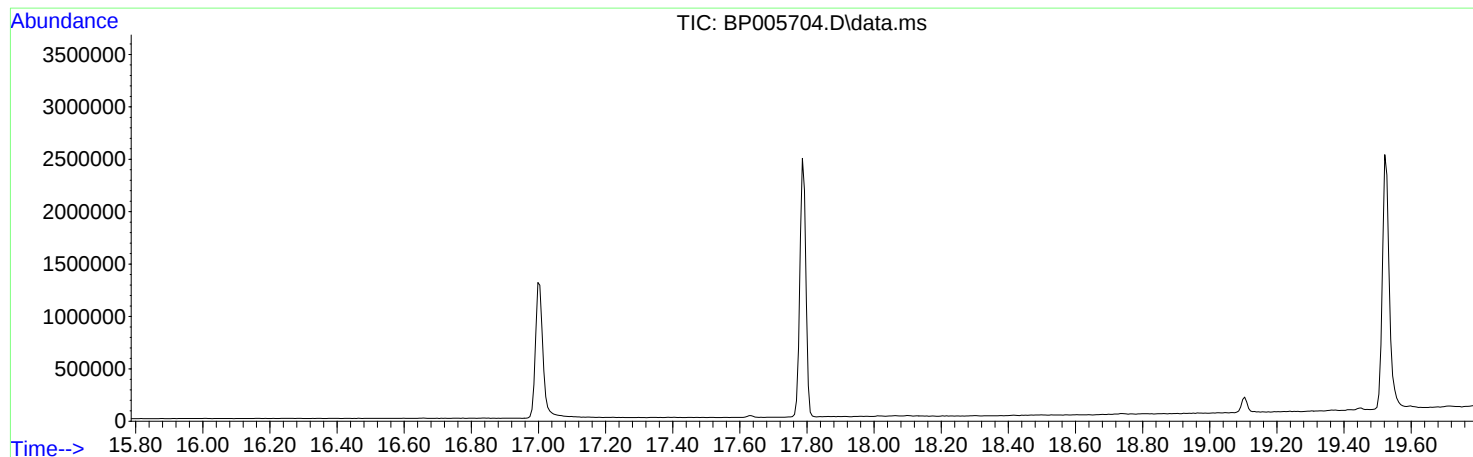




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2490

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 29.8      | 63059   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.9       | 1400    | PASS             |
| 69          | 198          | 0.00         | 100          | 35.7      | 75671   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 440     | PASS             |
| 127         | 198          | 10           | 80           | 44.2      | 93687   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 1050    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 211830  | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 14004   | PASS             |
| 275         | 198          | 10           | 60           | 29.9      | 63308   | PASS             |
| 365         | 198          | 1            | 100          | 4.6       | 9750    | PASS             |
| 441         | 198          | 0.01         | 100          | 23.2      | 49208   | PASS             |
| 442         | 442          | 100          | 100          | 100.0     | 322965  | PASS             |
| 443         | 442          | 15           | 24           | 19.9      | 64202   | PASS             |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060421\  
Data File : BP005704.D  
Acq On : 04 Jun 2021 09:26  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Jun 04 11:25:11 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052721.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 27 16:11:11 2021  
Response via : Initial Calibration

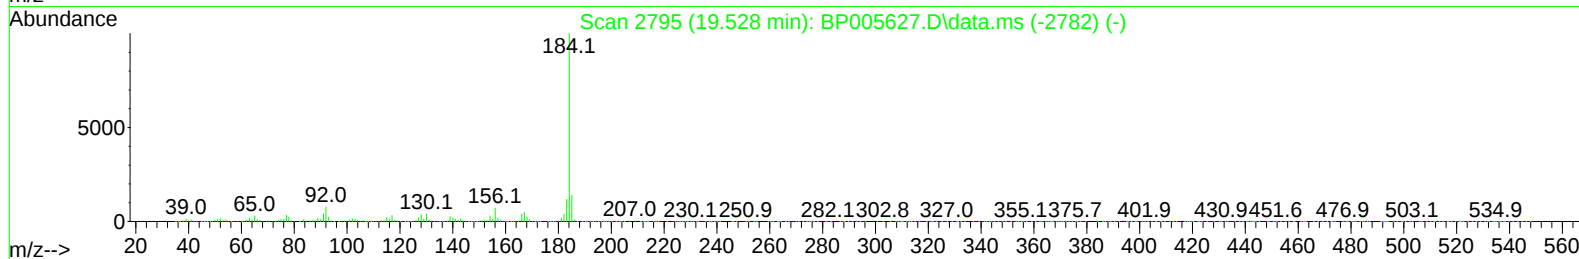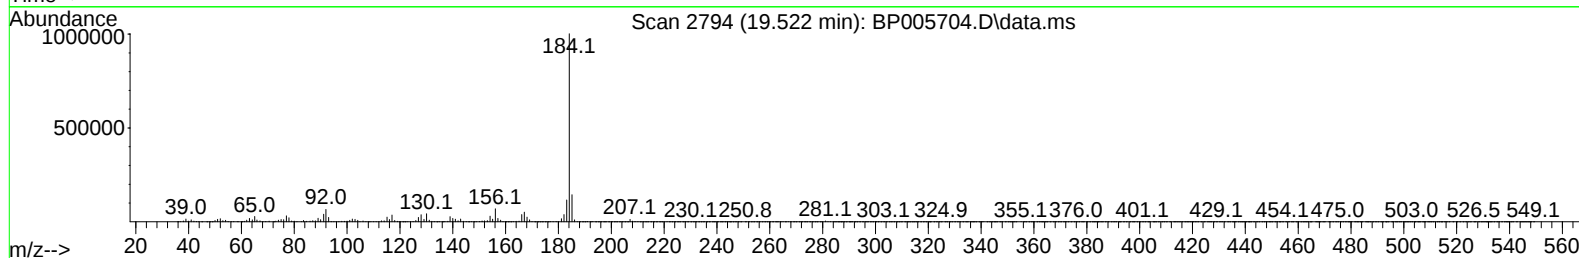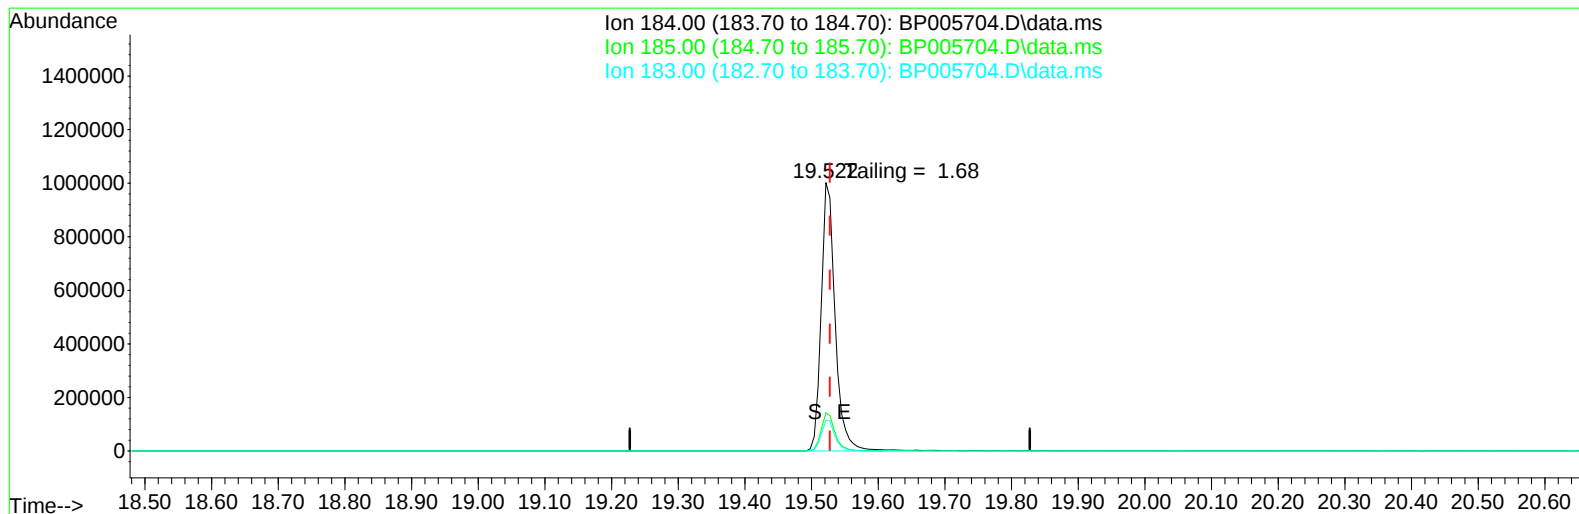

TIC: BP005704.D\data.ms

(77) Benzidine

19.522min (-0.006) 329927.63 ng




response 1459921

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 14.35  |
| 183.00 | 12.30  | 11.54  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060421\  
 Data File : BP005704.D  
 Acq On : 04 Jun 2021 09:26  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 04 11:25:11 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052721.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu May 27 16:11:11 2021  
 Response via : Initial Calibration

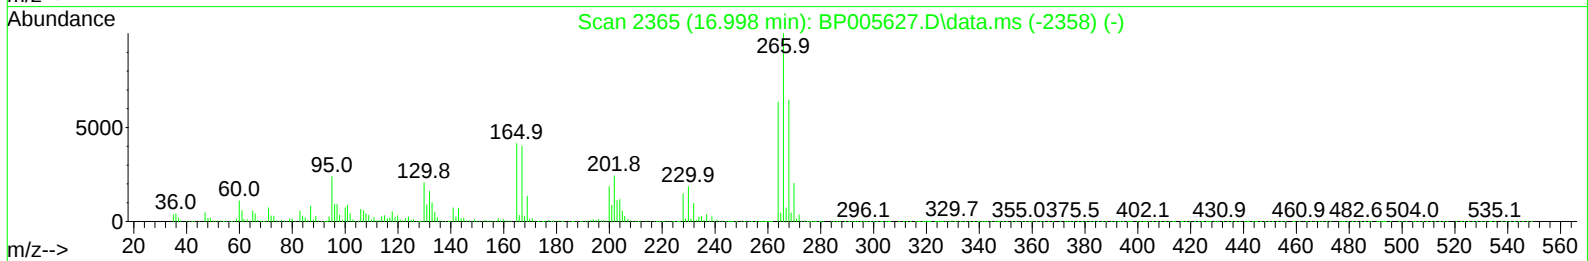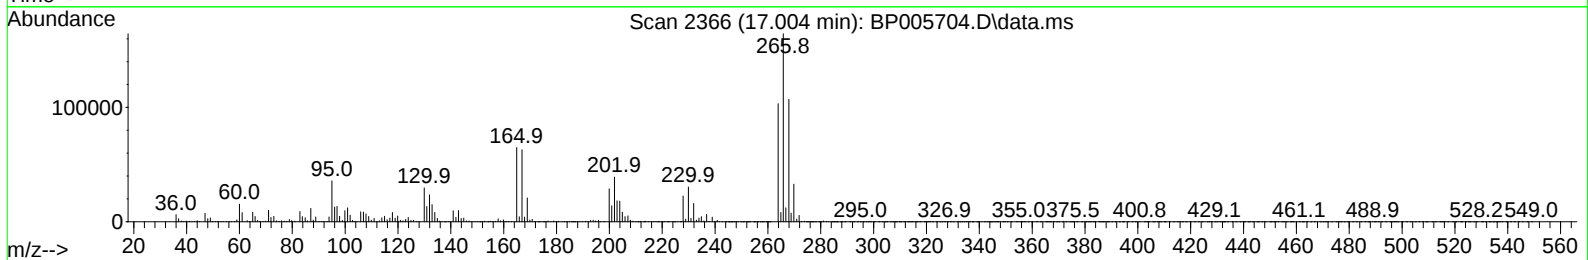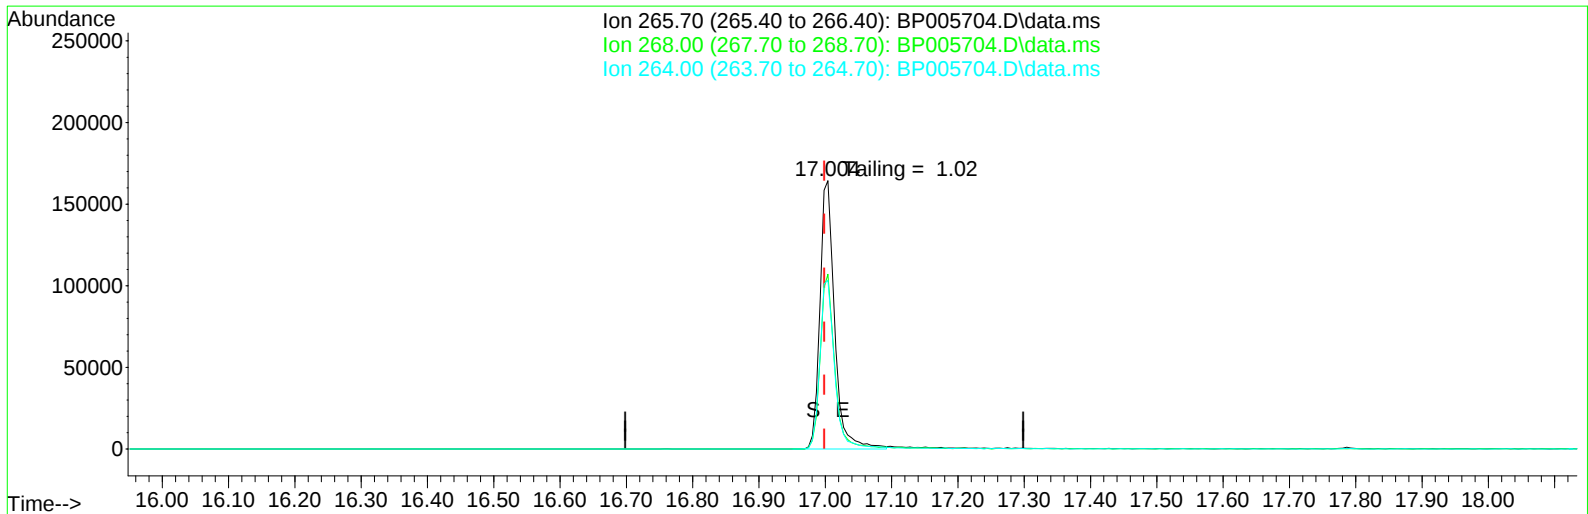

TIC: BP005704.D\data.ms

**(70) Pentachlorophenol (C)**

17.004min (+ 0.006) 196493.47 ng

response 255859

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.70  | 65.13  |
| 264.00 | 67.10  | 62.85  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/4/2021      | BNA_P            | BP005704.D         |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 764952           | 20.72              |
| DDD           | 45403            | 20.29              |
| DDE           | 3121             | 19.8               |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 48524         | 813476           | 5.97               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP