
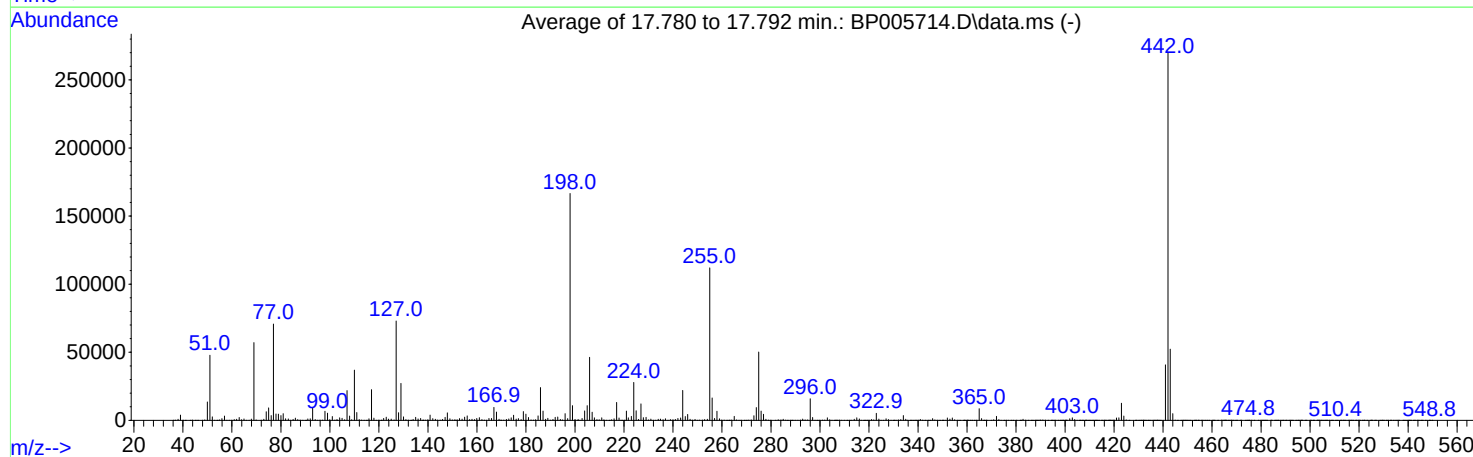


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060421\
 Data File : BP005714.D
 Acq On : 04 Jun 2021 16:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 07 12:13:53 2021

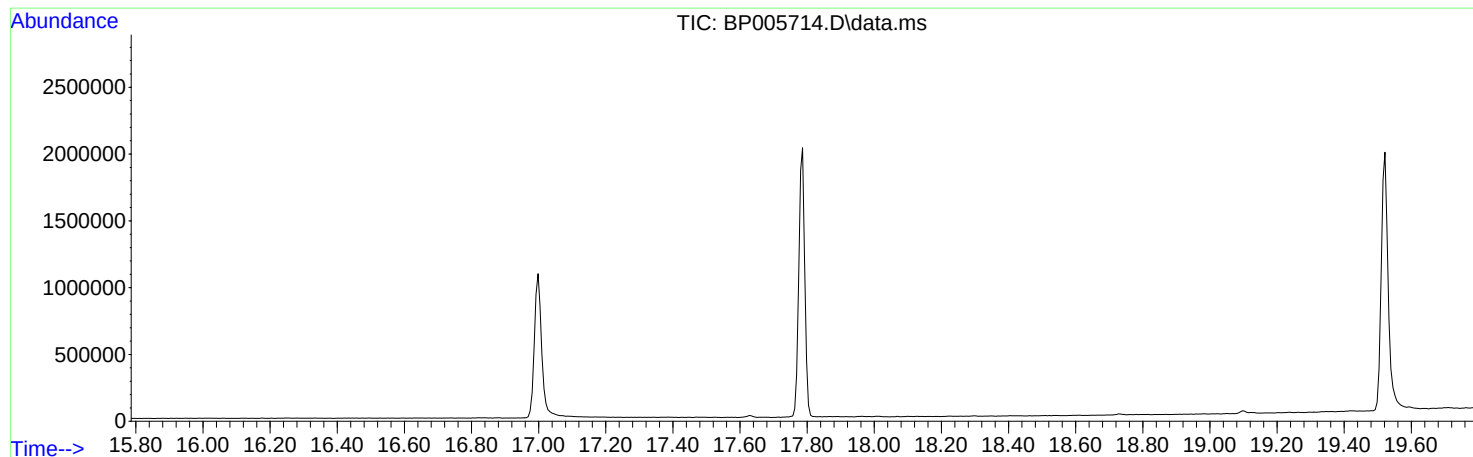




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	47853	PASS
68	69	0.00	2	1.7	955	PASS
69	198	0.00	100	34.3	57117	PASS
70	69	0.00	2	0.5	307	PASS
127	198	10	80	43.8	72917	PASS
197	198	0.00	2	0.8	1270	PASS
198	198	100	100	100.0	166667	PASS
199	198	5	9	6.5	10868	PASS
275	198	10	60	30.1	50192	PASS
365	198	1	100	5.2	8628	PASS
441	198	0.01	100	24.5	40765	PASS
442	442	100	100	100.0	270123	PASS
443	442	15	24	19.3	52241	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060421\
 Data File : BP005714.D
 Acq On : 04 Jun 2021 16:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 04 17:08:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

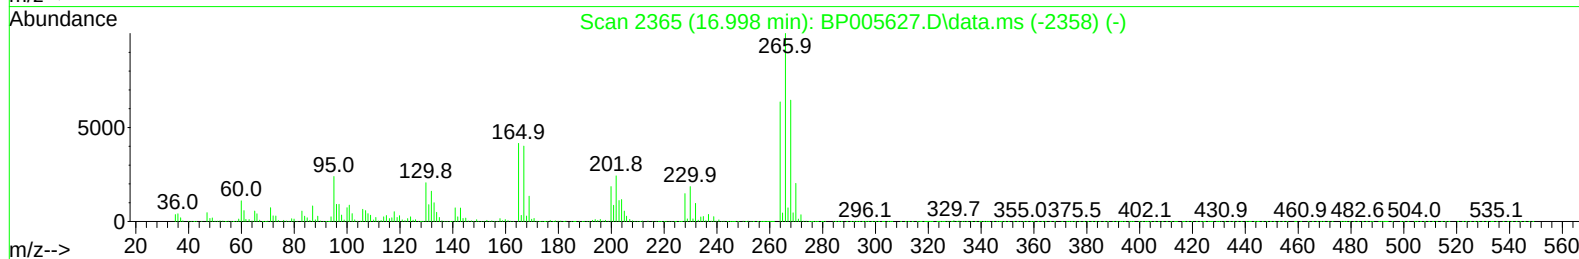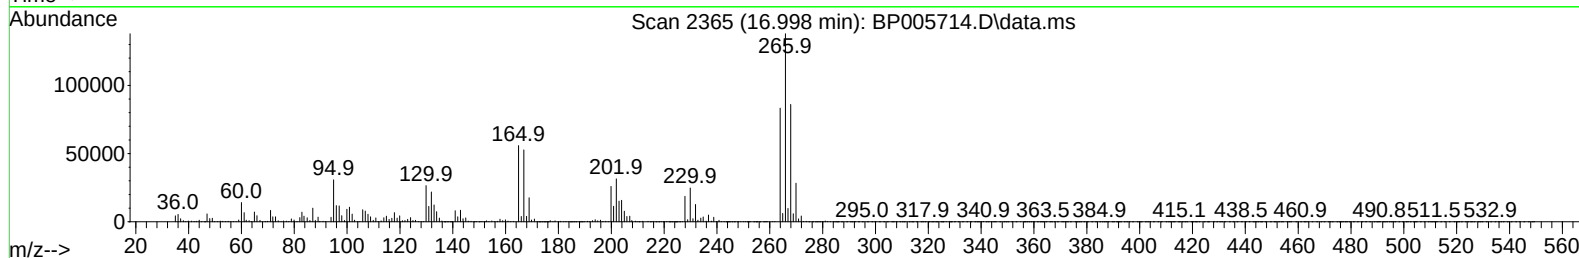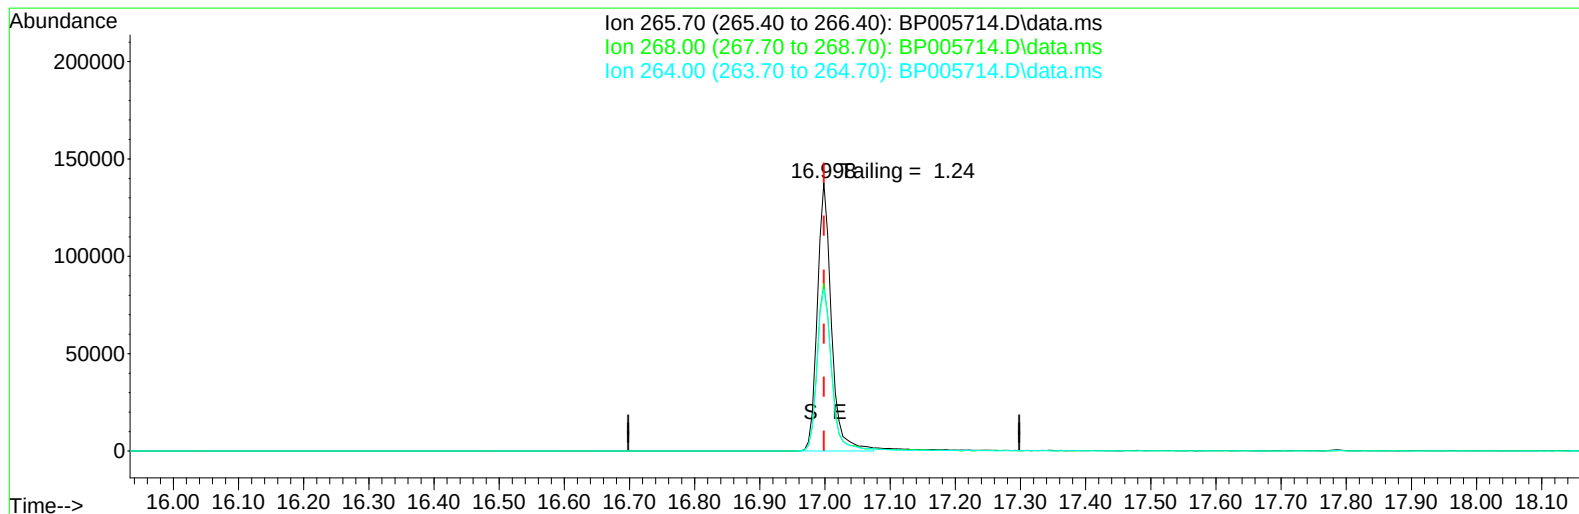

TIC: BP005714.D\data.ms

(70) Pentachlorophenol (C)

16.998min (-0.000) 81996.97 ng




response 211181

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.37
264.00	67.10	60.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060421\
Data File : BP005714.D
Acq On : 04 Jun 2021 16:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 04 17:08:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration

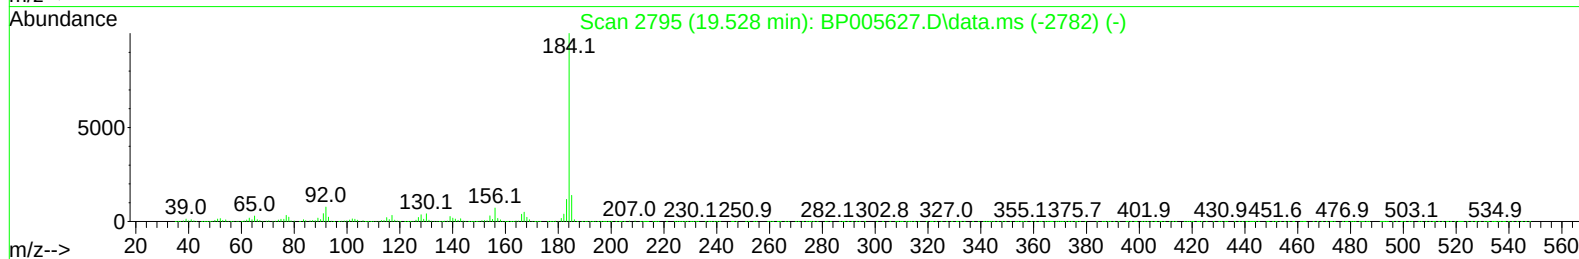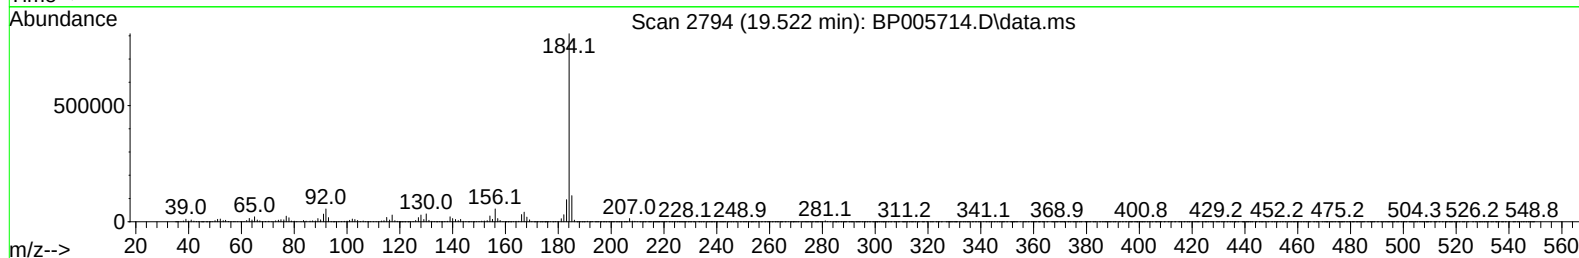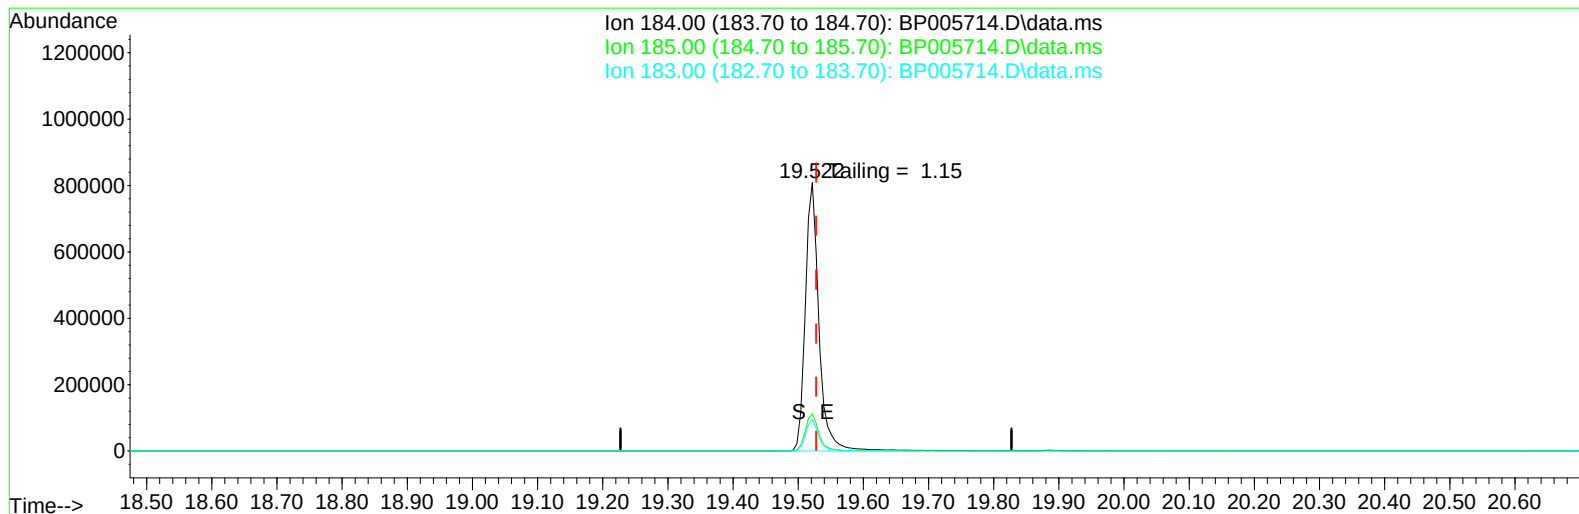

TIC: BP005714.D\data.ms

(77) Benzidine

19.522min (-0.006) 27923.57 ng

response 1177277

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.86
183.00	12.30	11.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/4/2021	BNA_P	<u>BP005714.D</u>
Compound Name	Response	Retention Time
DDT	613330	20.72
DDD	27407	20.29
DDE	2254	19.79
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29661	642991	4.61

Instrument :
BNA_P
ClientSampleId :
DFTPP