
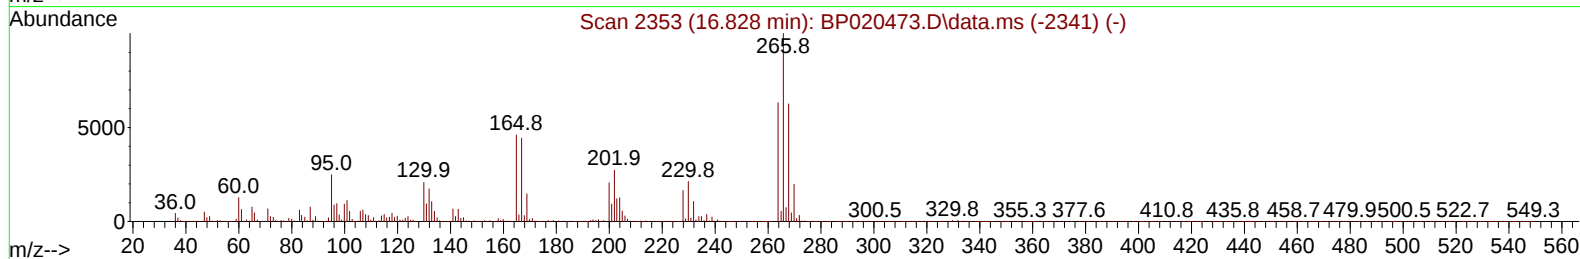
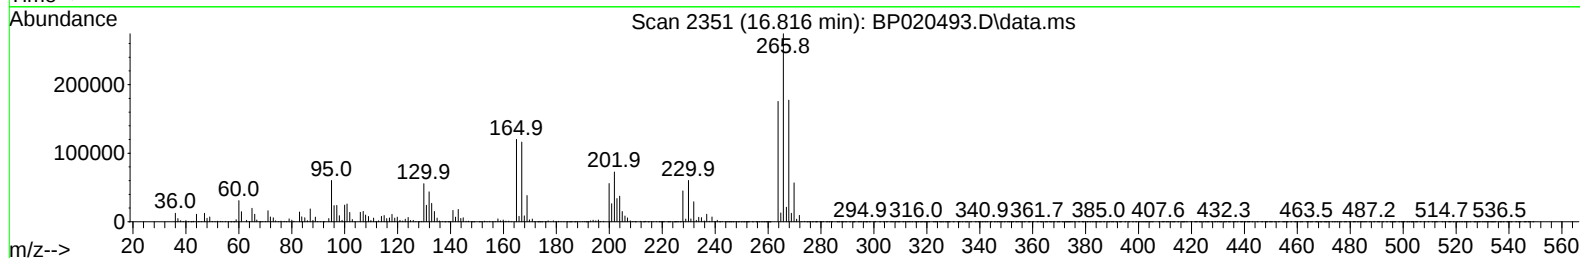


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060424\
Data File : BP020493.D
Acq On : 04 Jun 2024 11:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 13:05:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

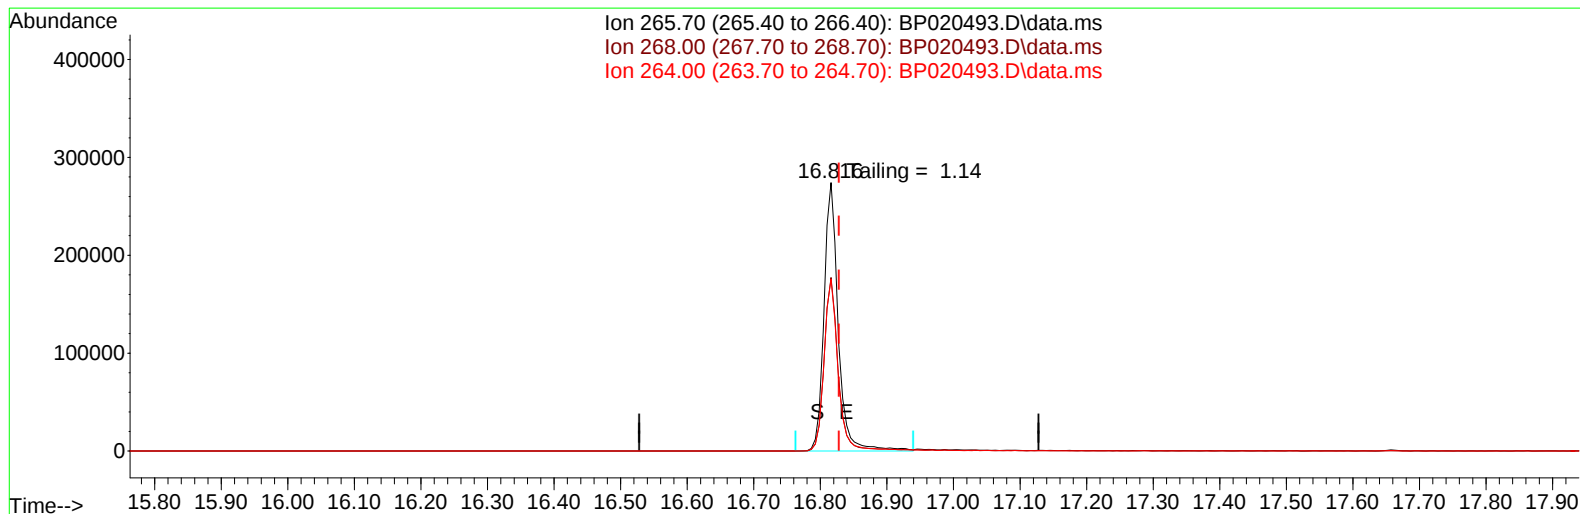

TIC: BP020493.D\data.ms

(70) Pentachlorophenol (C)




16.816min (-0.012) 290268.89 ng

response 409674

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.64
264.00	63.30	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060424\
Data File : BP020493.D
Acq On : 04 Jun 2024 11:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 13:05:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

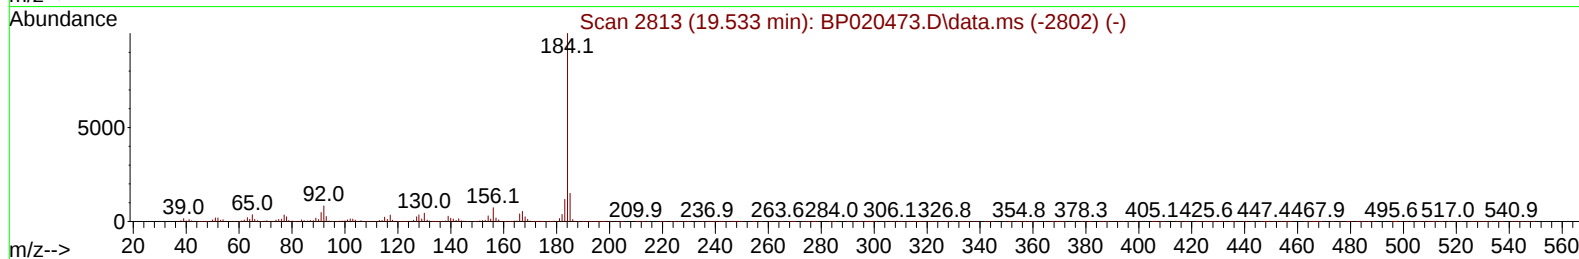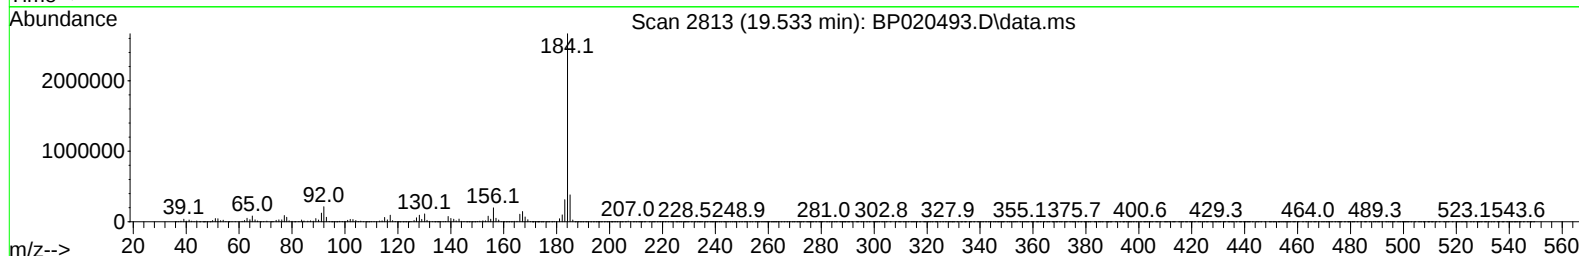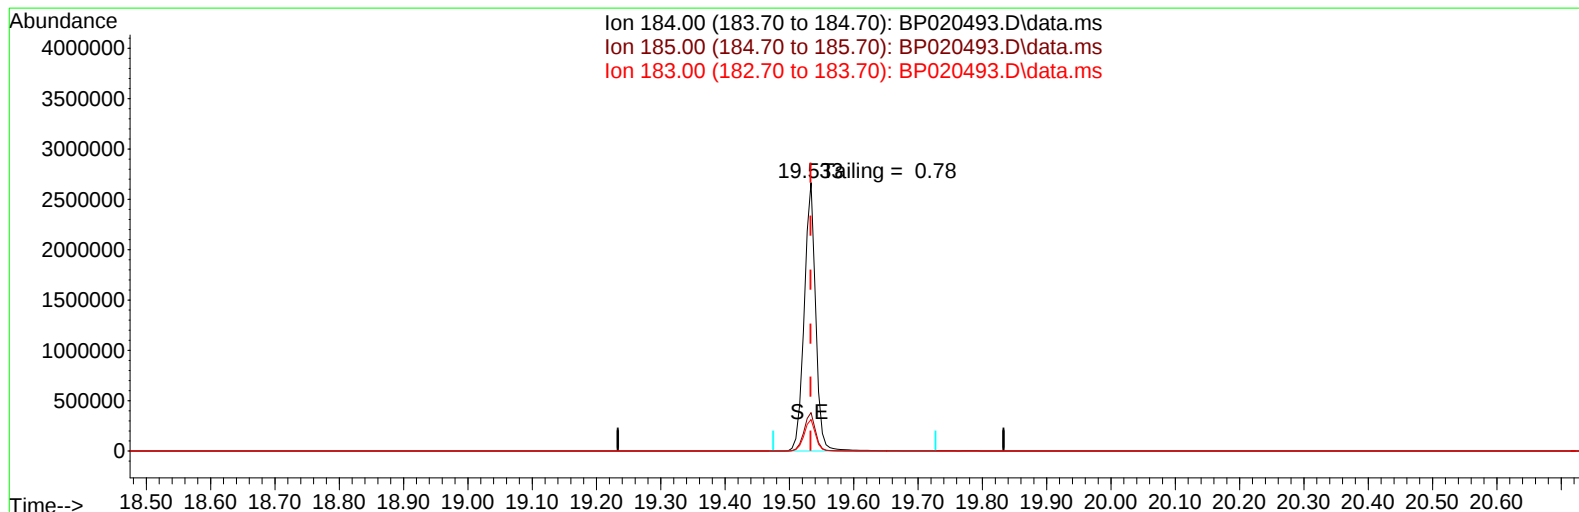

TIC: BP020493.D\data.ms

(77) Benzidine**19.533min (+ 0.000) 143964.92 ng****response 3302471**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.31
183.00	11.70	11.74
0.00	0.00	0.00