

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060424\
 Data File : BP020509.D
 Acq On : 05 Jun 2024 00:06
 Operator : MA/JU
 Sample : P2689-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BU-03-05312024

Quant Time: Jun 05 01:27:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 30 03:41:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	321175	20.000	ng	0.00
21) Naphthalene-d8	10.540	136	1323465	20.000	ng	0.00
39) Acenaphthene-d10	14.387	164	811843	20.000	ng	0.00
64) Phenanthrene-d10	17.198	188	1646526	20.000	ng	0.00
76) Chrysene-d12	21.645	240	1459117	20.000	ng	-0.02
86) Perylene-d12	25.009	264	1662415	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.381	112	1994453	111.185	ng	0.00
7) Phenol-d6	6.928	99	2702429	106.826	ng	0.00
23) Nitrobenzene-d5	8.904	82	1626881	67.290	ng	-0.02
42) 2,4,6-Tribromophenol	15.904	330	1058822	125.671	ng	0.00
45) 2-Fluorobiphenyl	13.004	172	3838408	70.482	ng	0.00
79) Terphenyl-d14	19.933	244	5765576	65.780	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060424\
Data File : BP020509.D
Acq On : 05 Jun 2024 00:06
Operator : MA/JU
Sample : P2689-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BU-03-05312024

Quant Time: Jun 05 01:27:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration




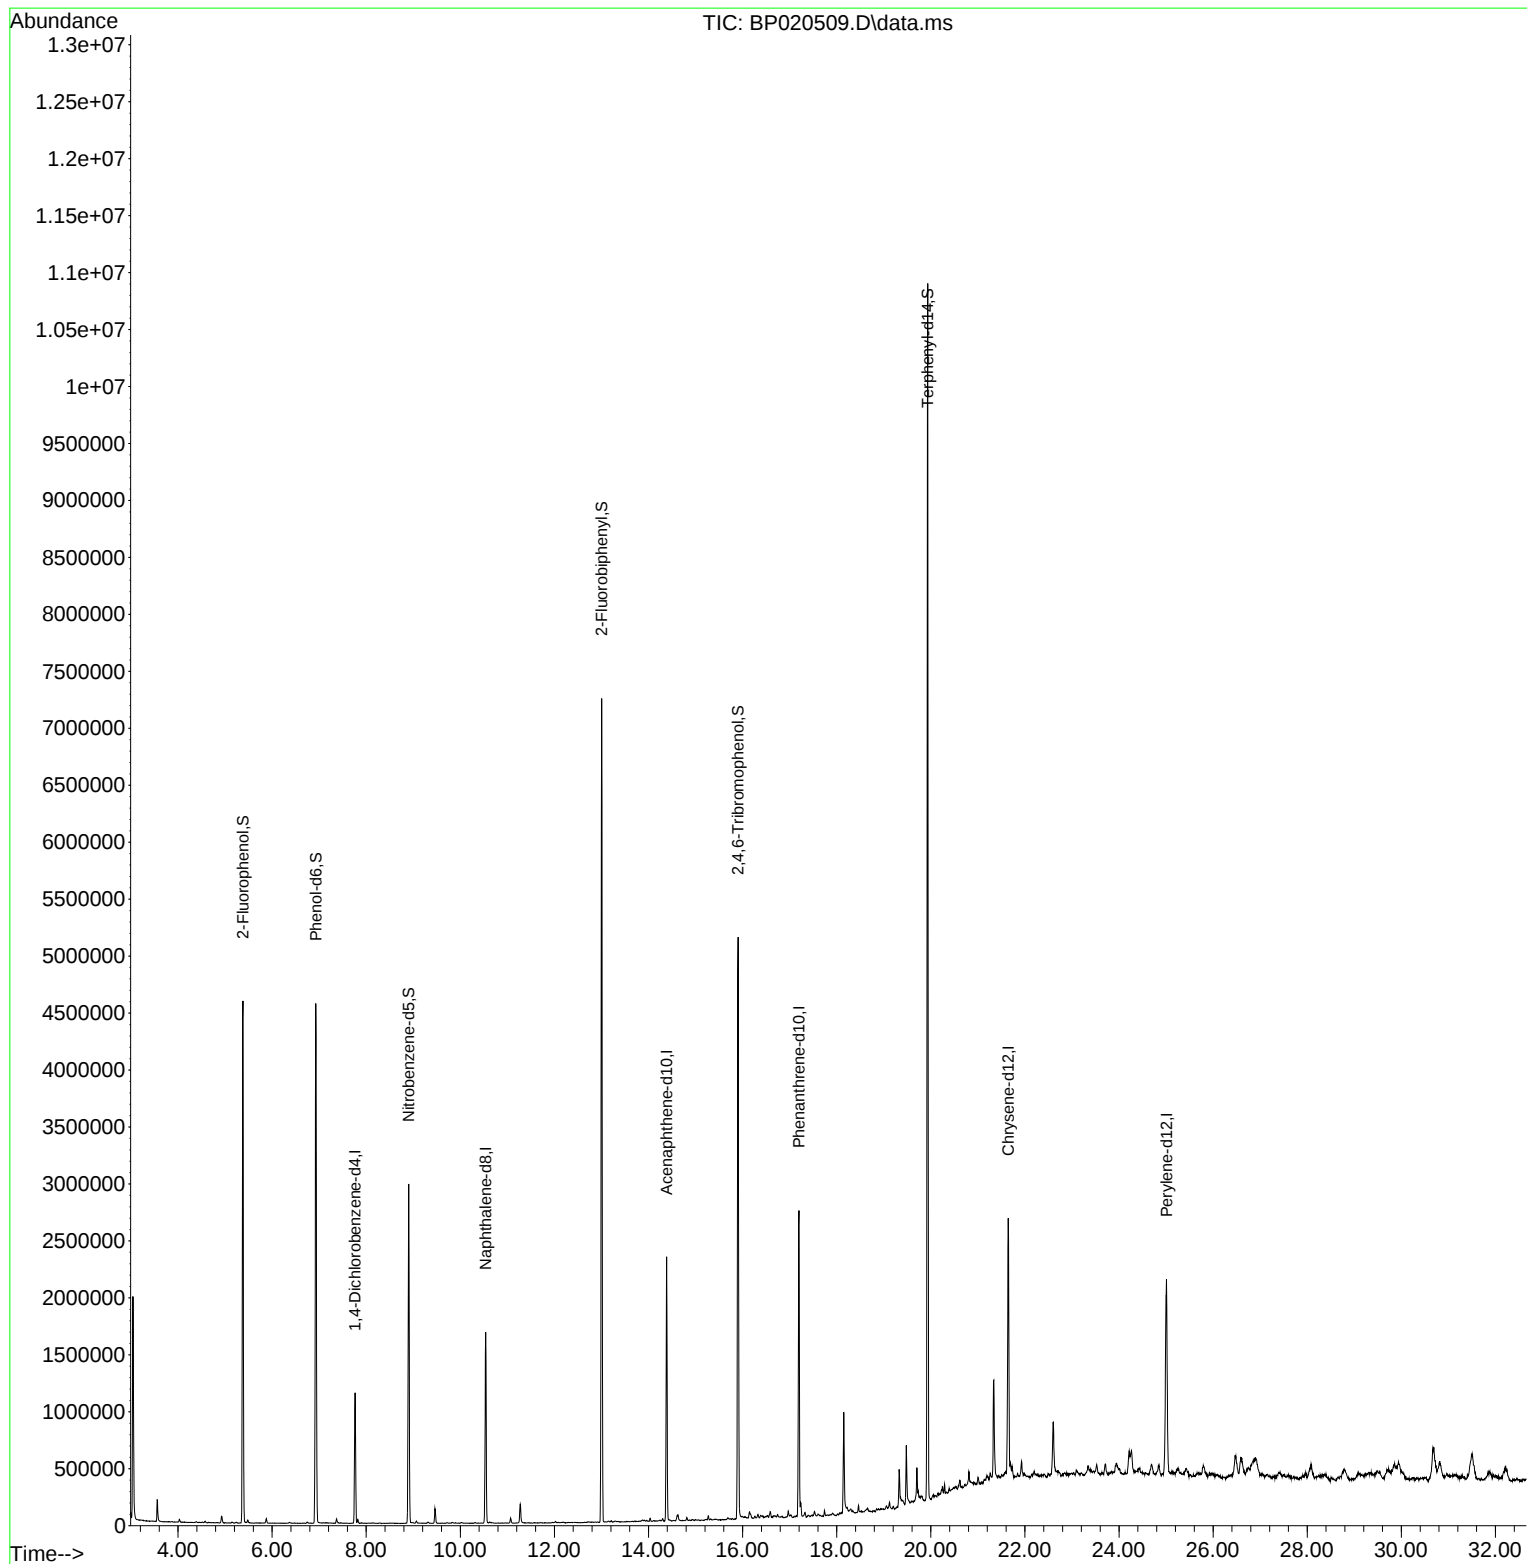


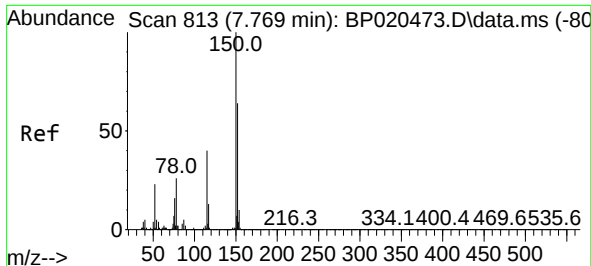

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.763 min Scan# 81
Delta R.T. -0.006 min
Lab File: BP020509.D
Acq: 05 Jun 2024 00:06




Instrument :
BNA_P
ClientSampleId :
BU-03-05312024


Tgt Ion:152 Resp: 321175
Ion Ratio Lower Upper
152 100
150 156.9 124.2 186.2
115 60.4 49.5 74.3

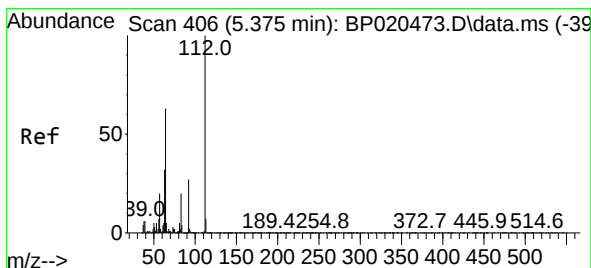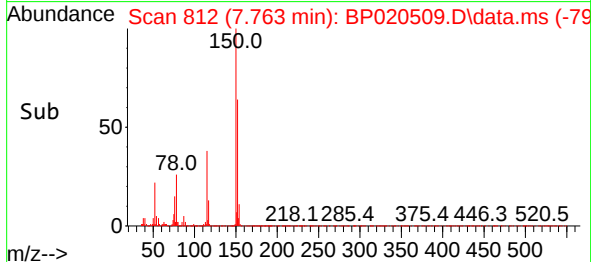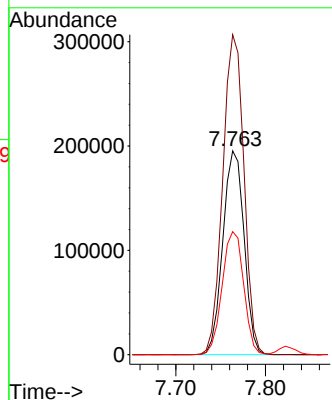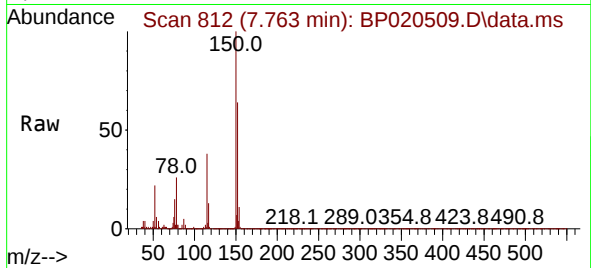

#5
2-Fluorophenol
Concen: 111.185 ng
RT: 5.381 min Scan# 407
Delta R.T. 0.006 min
Lab File: BP020509.D
Acq: 05 Jun 2024 00:06

Tgt Ion:112 Resp: 1994453
Ion Ratio Lower Upper
112 100
64 58.9 50.1 75.1
63 30.4 25.7 38.5


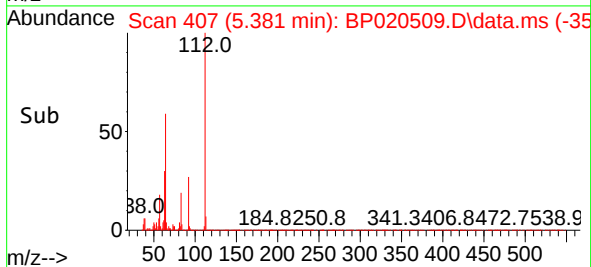
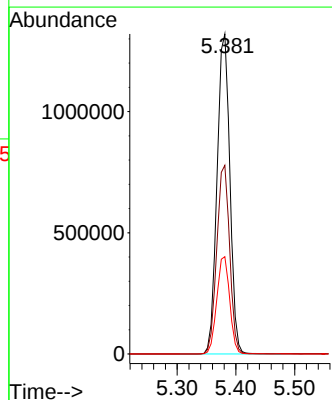
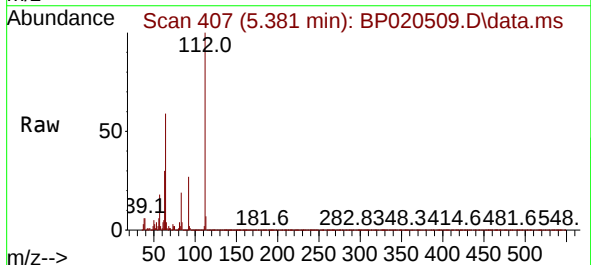


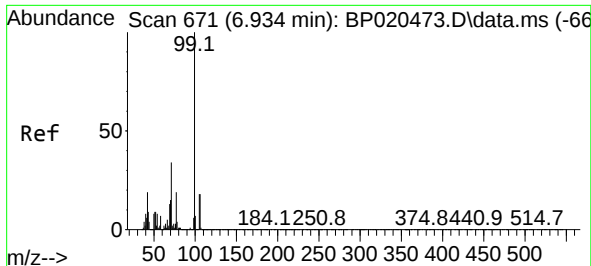

#7
Phenol-d6
Concen: 106.826 ng
RT: 6.928 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP020509.D
Acq: 05 Jun 2024 00:06




Instrument :
BNA_P
ClientSampleId :
BU-03-05312024


Tgt Ion: 99 Resp: 2702429
Ion Ratio Lower Upper
99 100
42 17.9 15.0 22.4
71 34.1 27.3 40.9

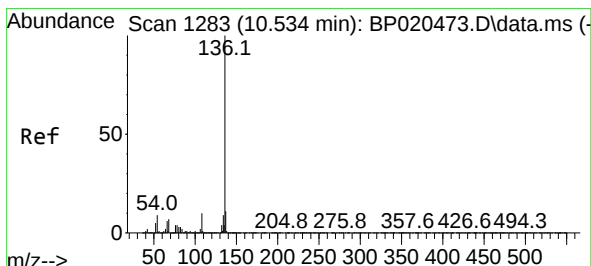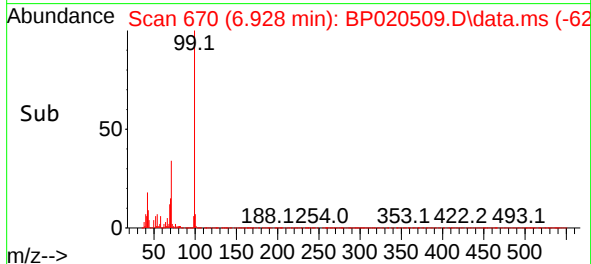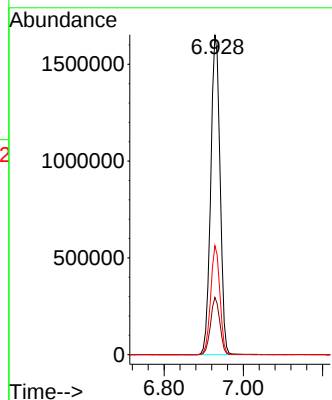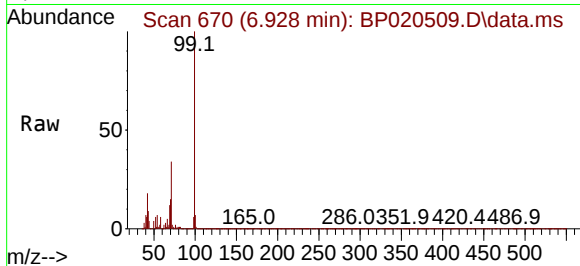

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.540 min Scan# 1284
Delta R.T. 0.006 min
Lab File: BP020509.D
Acq: 05 Jun 2024 00:06

Tgt Ion:136 Resp: 1323465
Ion Ratio Lower Upper
136 100
137 10.7 9.0 13.4
54 8.4 7.4 11.0
68 6.0 5.2 7.8


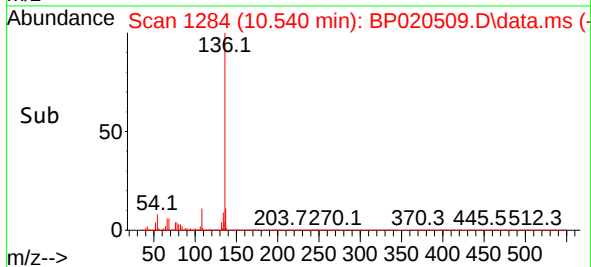
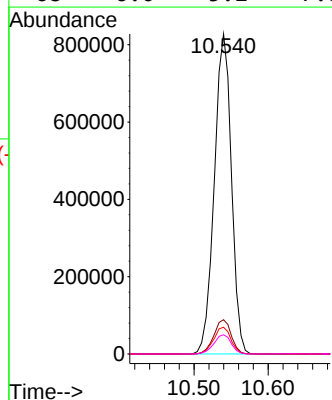
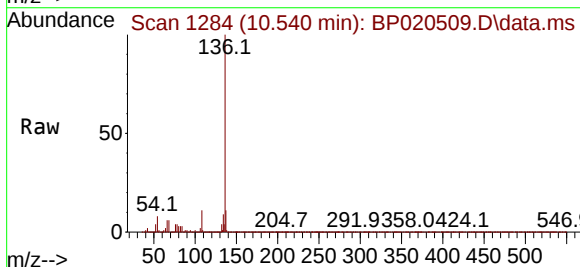


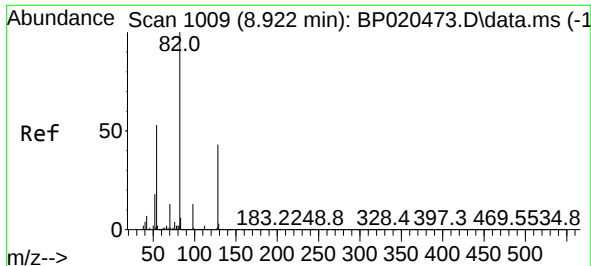

#23
Nitrobenzene-d5
Concen: 67.290 ng
RT: 8.904 min Scan# 1006
Delta R.T. -0.018 min
Lab File: BP020509.D
Acq: 05 Jun 2024 00:06




Instrument :
BNA_P
ClientSampleId :
BU-03-05312024


Tgt Ion: 82 Resp: 1626881
Ion Ratio Lower Upper
82 100
128 43.3 34.2 51.4
54 51.4 42.7 64.1

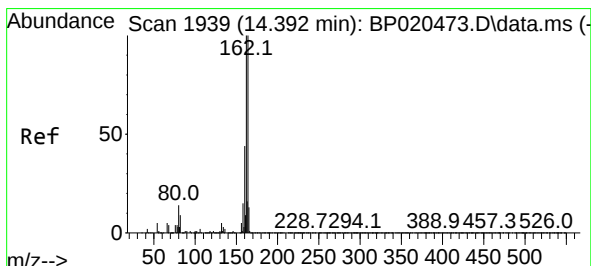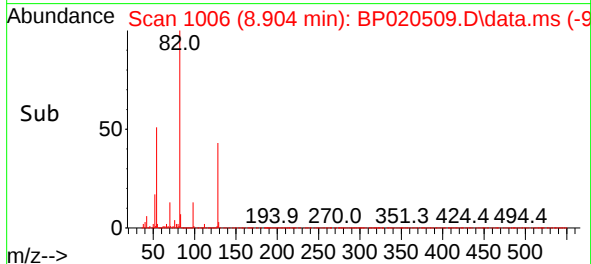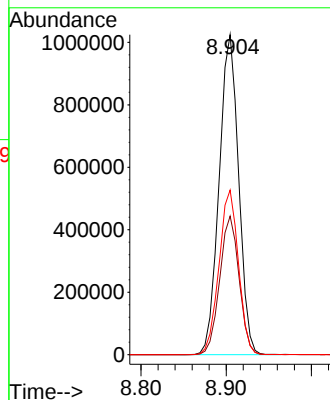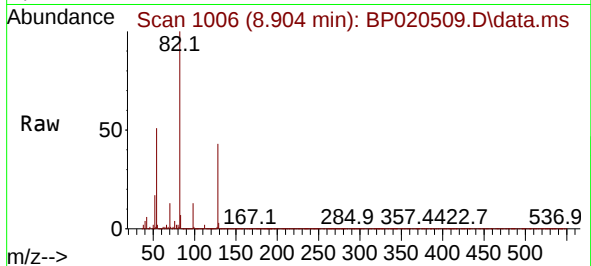

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.387 min Scan# 1938
Delta R.T. -0.005 min
Lab File: BP020509.D
Acq: 05 Jun 2024 00:06

Tgt Ion:164 Resp: 811843
Ion Ratio Lower Upper
164 100
162 101.1 80.3 120.5
160 44.6 35.4 53.2


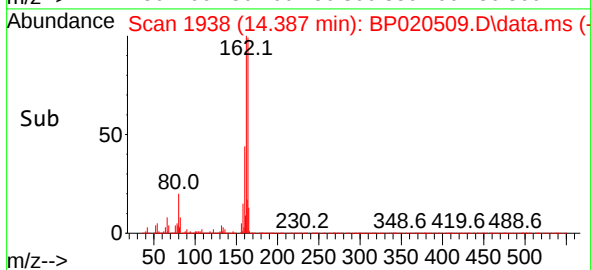
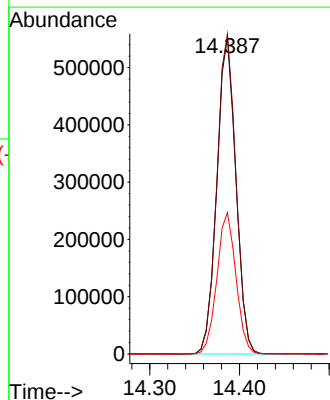
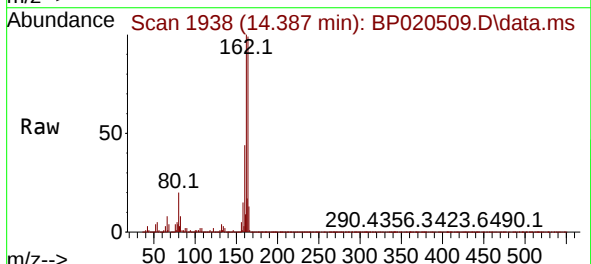


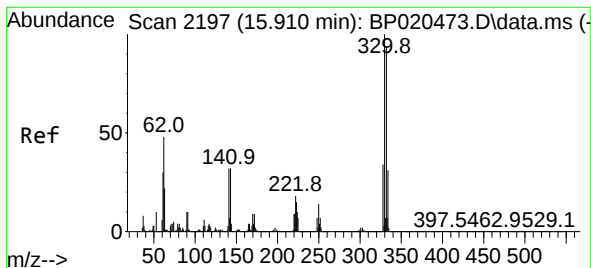

#42
2,4,6-Tribromophenol
Concen: 125.671 ng
RT: 15.904 min Scan# 2197
Delta R.T. -0.006 min
Lab File: BP020509.D
Acq: 05 Jun 2024 00:06




Instrument :
BNA_P
ClientSampleId :
BU-03-05312024


Tgt Ion:330 Resp: 1058822
Ion Ratio Lower Upper
330 100
332 97.2 76.6 114.8
141 31.9 27.1 40.7

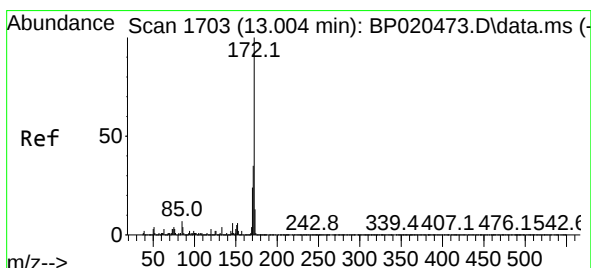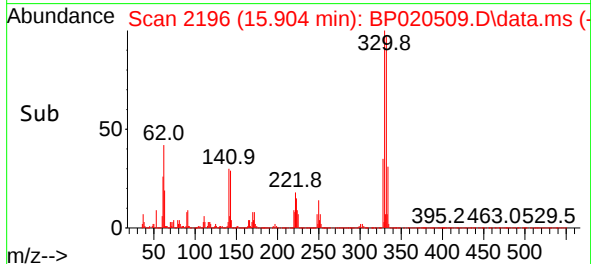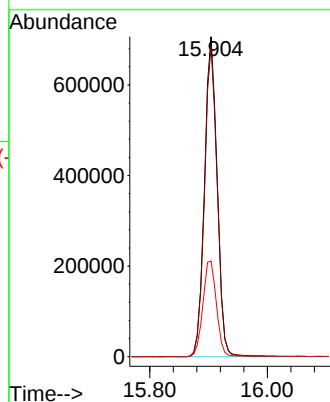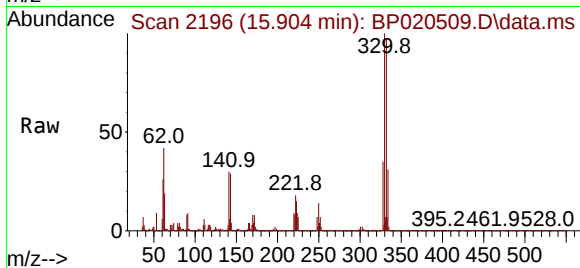

#45
2-Fluorobiphenyl
Concen: 70.482 ng
RT: 13.004 min Scan# 1703
Delta R.T. -0.000 min
Lab File: BP020509.D
Acq: 05 Jun 2024 00:06

Tgt Ion:172 Resp: 3838408
Ion Ratio Lower Upper
172 100
171 35.8 28.4 42.6
170 23.6 18.9 28.3

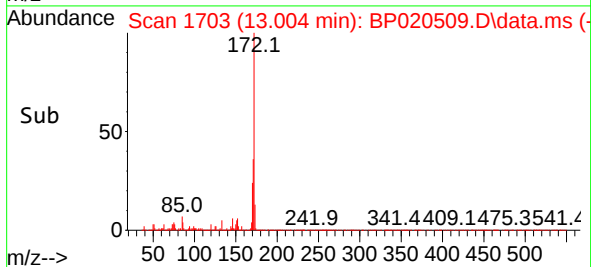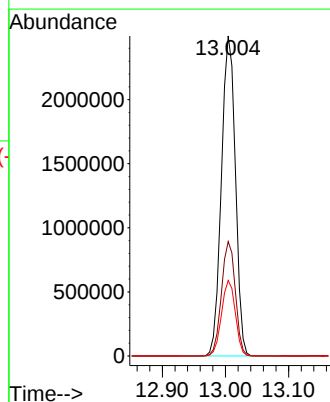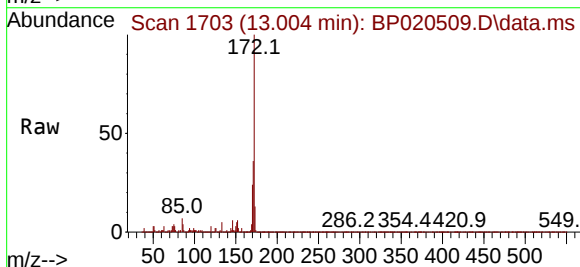

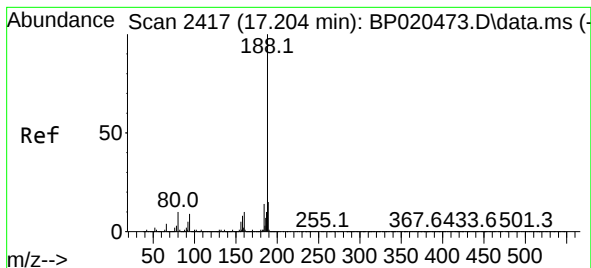

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.198 min Scan# 2416

Delta R.T. -0.006 min

Lab File: BP020509.D

Acq: 05 Jun 2024 00:06

Instrument :

BNA_P

ClientSampleId :

BU-03-05312024





Tgt Ion:188 Resp: 1646526

Ion Ratio Lower Upper

188 100

94 9.6 7.2 10.8

80 10.1 8.1 12.1

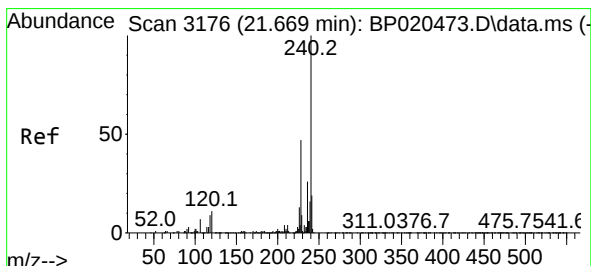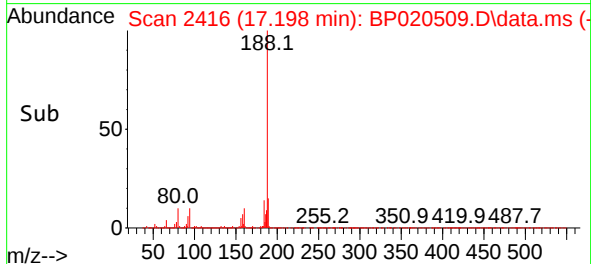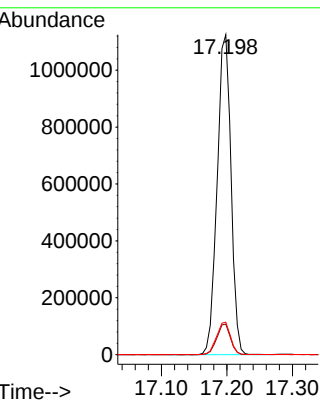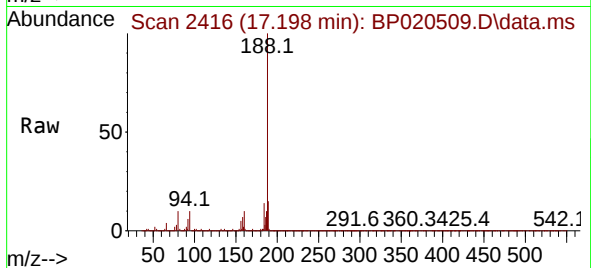

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.645 min Scan# 3172

Delta R.T. -0.024 min

Lab File: BP020509.D

Acq: 05 Jun 2024 00:06




Tgt Ion:240 Resp: 1459117


Ion Ratio Lower Upper

240 100

120 10.7 8.5 12.7

236 26.1 20.5 30.7

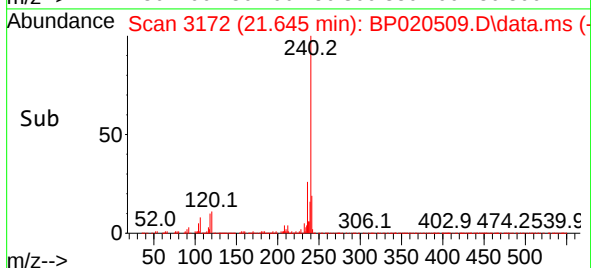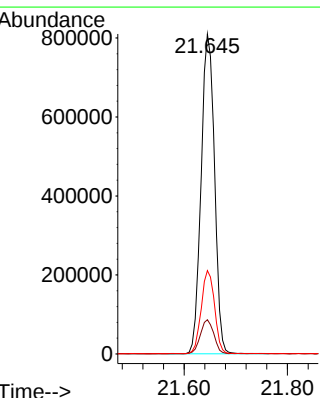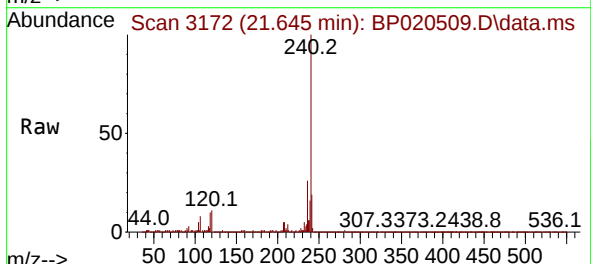

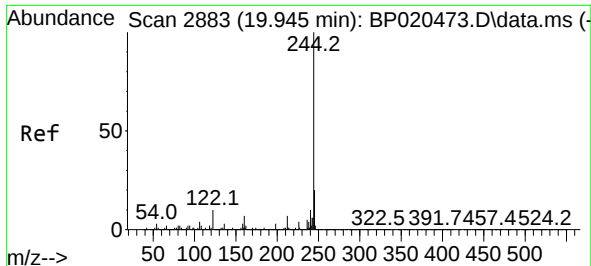

#79

Terphenyl-d14

Concen: 65.780 ng

RT: 19.933 min Scan# 21

Delta R.T. -0.012 min

Lab File: BP020509.D

Acq: 05 Jun 2024 00:06

Instrument :

BNA_P

ClientSampleId :

BU-03-05312024





Tgt Ion:244 Resp: 5765576

Ion Ratio Lower Upper

244 100

212 7.0 5.8 8.8

122 9.6 8.2 12.2

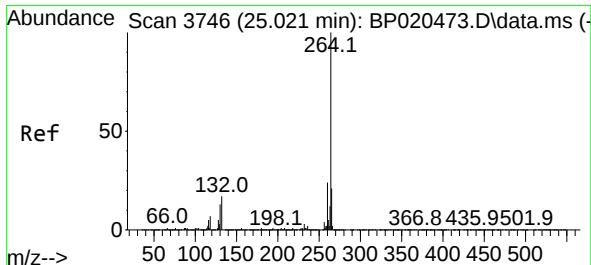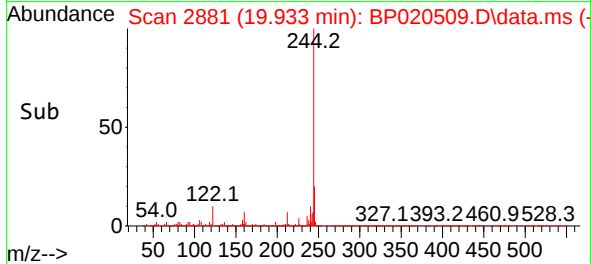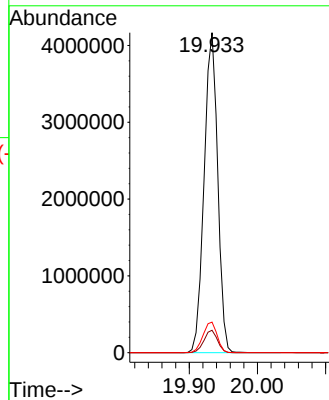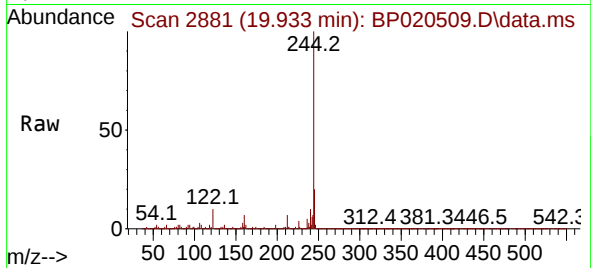

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.009 min Scan# 3744

Delta R.T. -0.012 min

Lab File: BP020509.D

Acq: 05 Jun 2024 00:06

Tgt Ion:264 Resp: 1662415

Ion Ratio Lower Upper

264 100

260 23.7 18.9 28.3

265 21.4 17.4 26.0

