
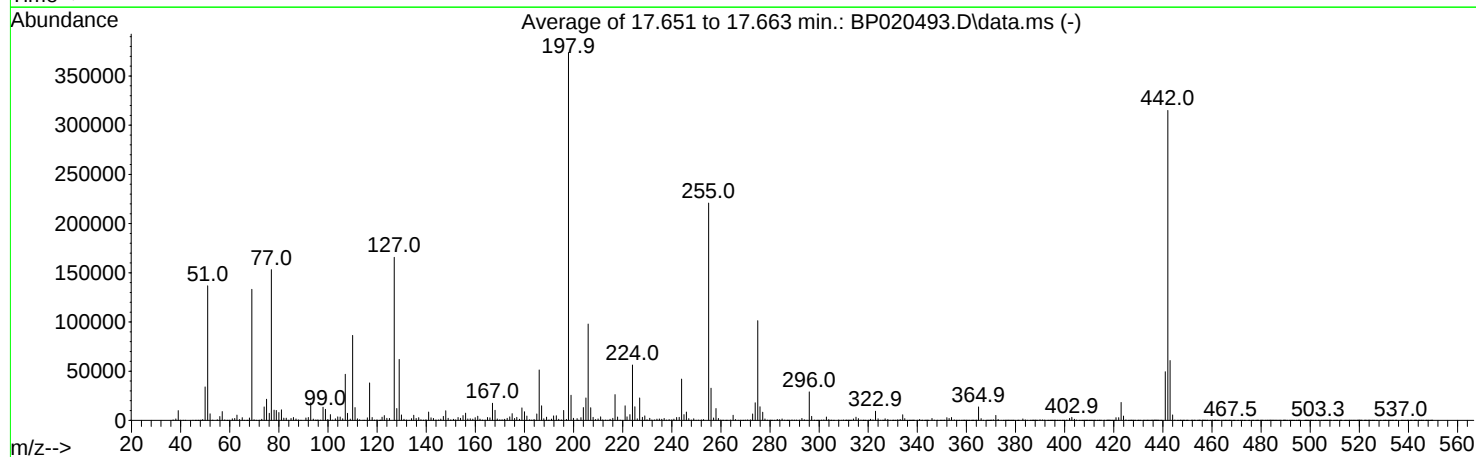


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060424\
Data File : BP020493.D
Acq On : 04 Jun 2024 11:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

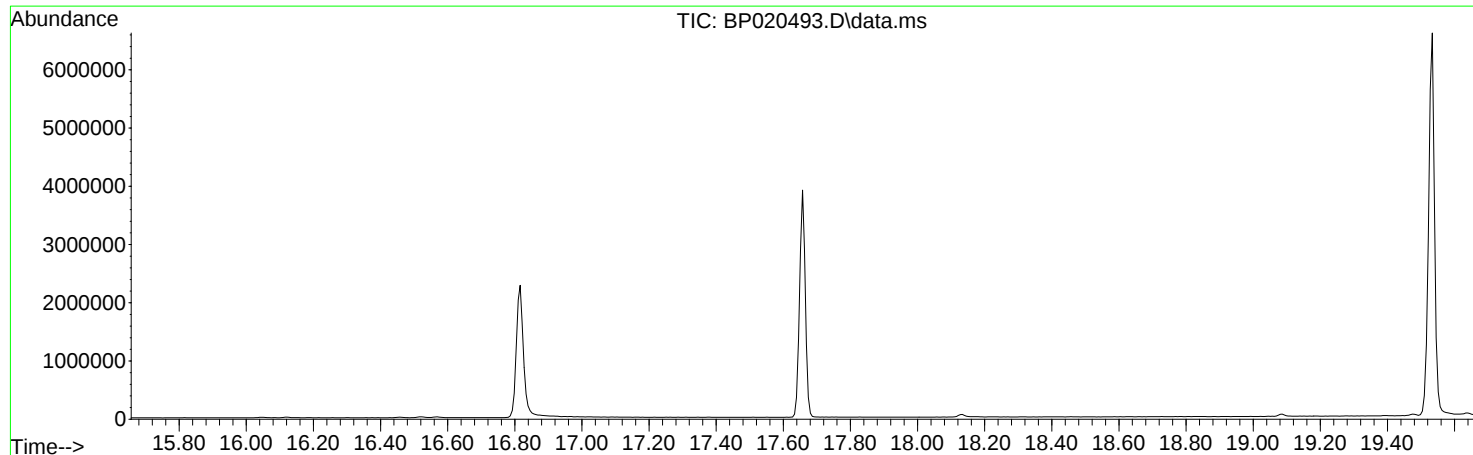




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	136717	PASS
68	69	0.00	2	1.8	2427	PASS
69	198	0.00	100	35.6	133197	PASS
70	69	0.00	2	0.5	660	PASS
127	198	10	80	44.3	165760	PASS
197	198	0.00	2	0.3	1026	PASS
198	198	100	100	100.0	373896	PASS
199	198	5	9	6.8	25469	PASS
275	198	10	60	27.1	101305	PASS
365	198	1	100	3.7	13713	PASS
441	198	0.01	100	13.2	49390	PASS
442	442	100	100	100.0	315093	PASS
443	442	15	24	19.3	60820	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060424\
Data File : BP020493.D
Acq On : 04 Jun 2024 11:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 04 13:05:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

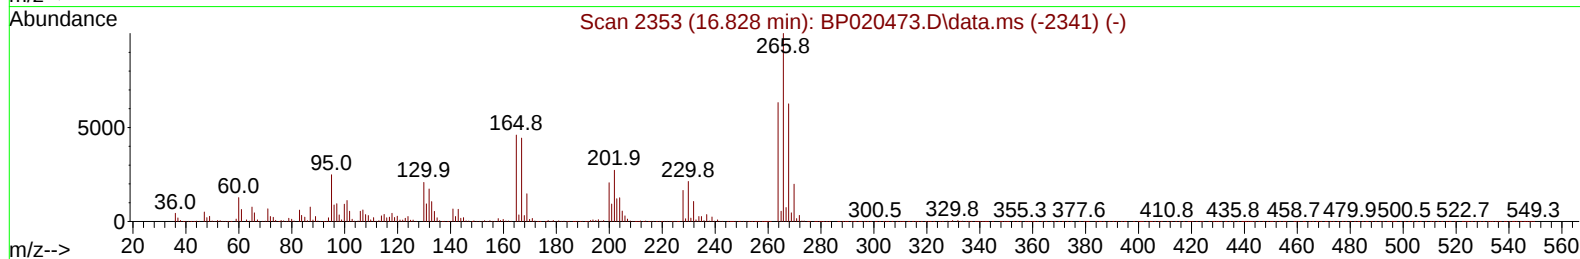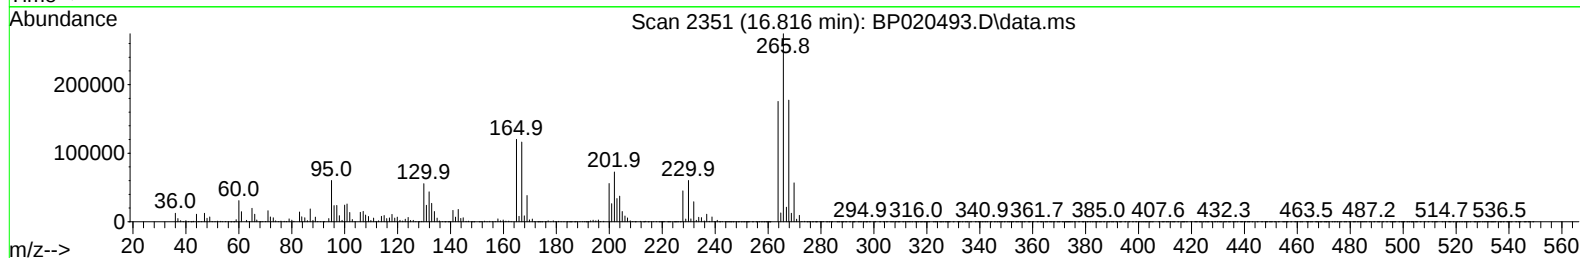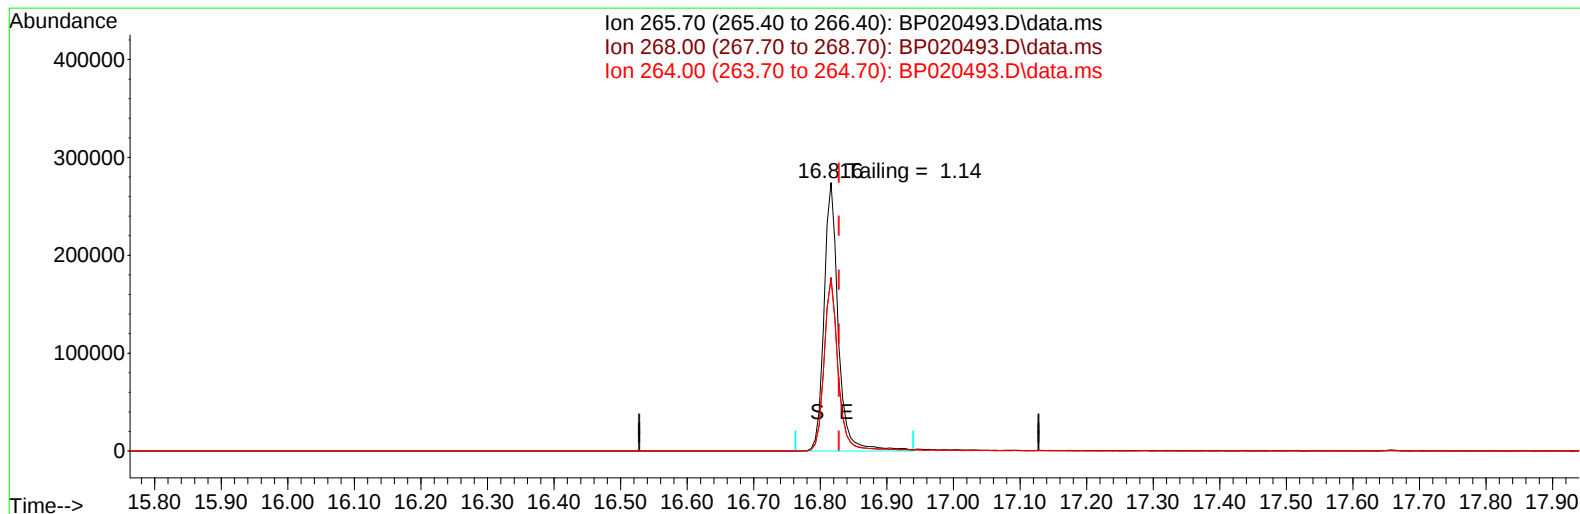

TIC: BP020493.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.012) 290268.89 ng




response 409674

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.64
264.00	63.30	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060424\
Data File : BP020493.D
Acq On : 04 Jun 2024 11:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 04 13:05:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

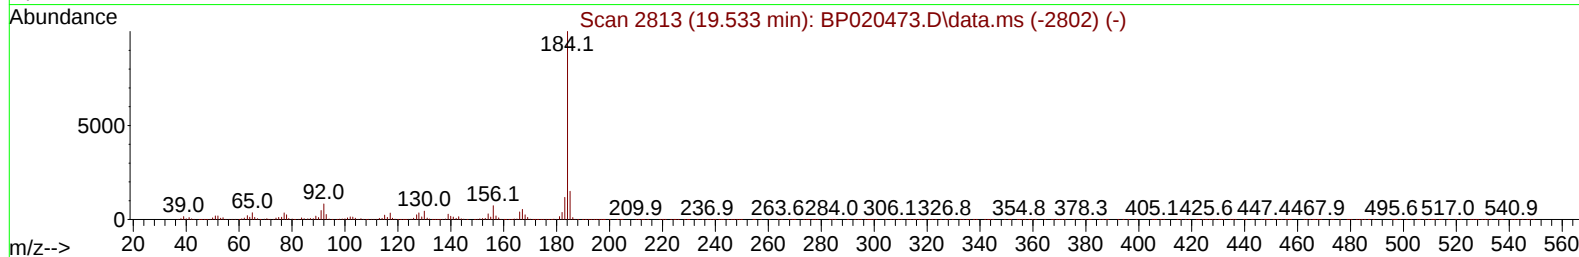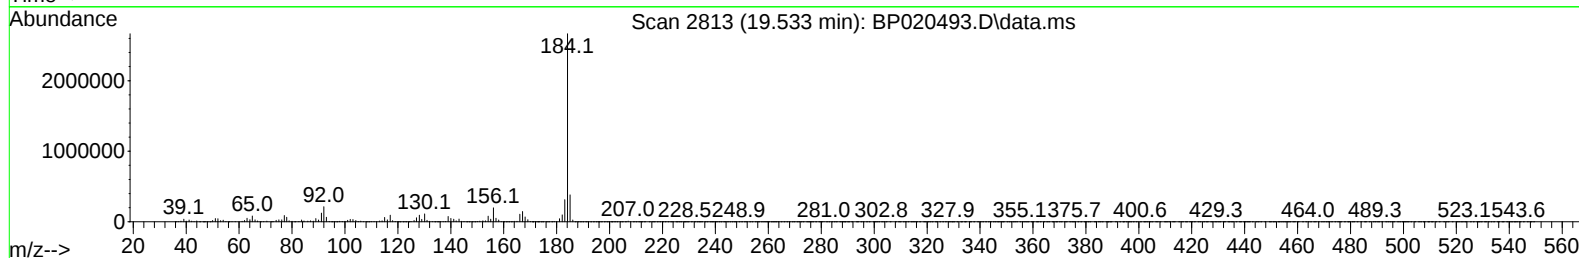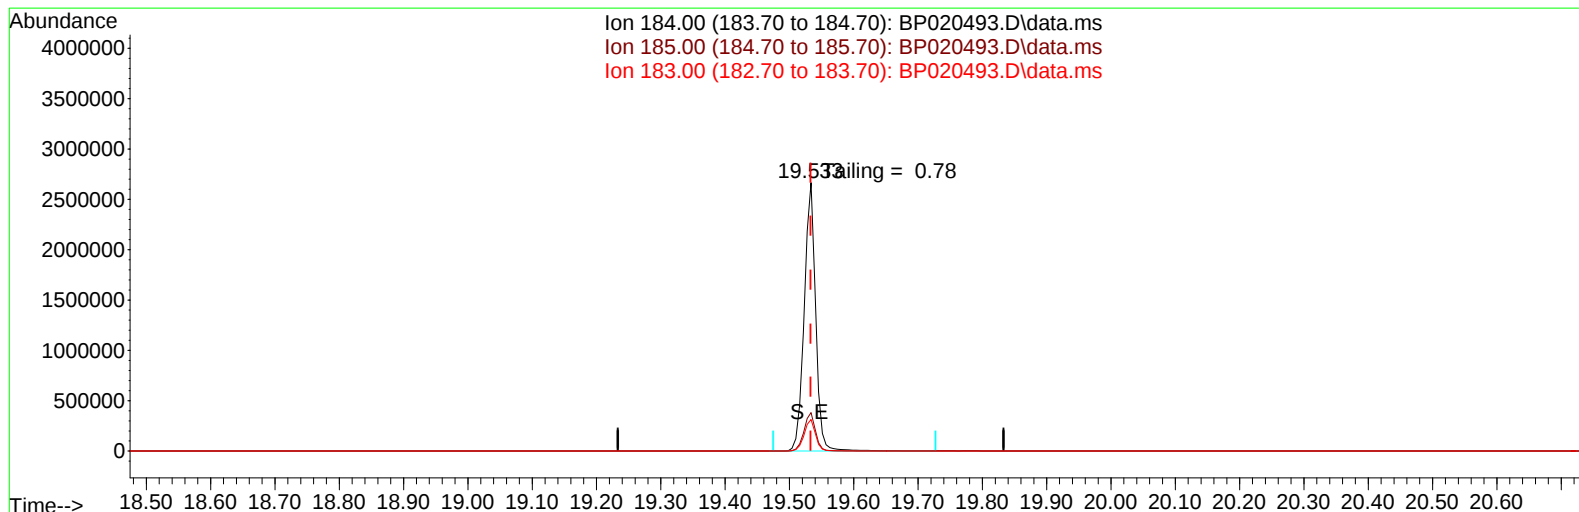

TIC: BP020493.D\data.ms

(77) Benzidine

19.533min (+ 0.000) 143964.92 ng

response 3302471

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.31
183.00	11.70	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/4/2024	BNA_P	<u>BP020493.D</u>
Compound Name	Response	Retention Time
DDT	1347670	20.827
DDD	26044	20.357
DDE	1327	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27371	1375041	1.99

Instrument :
BNA_P
ClientSampleId :
DFTPP