



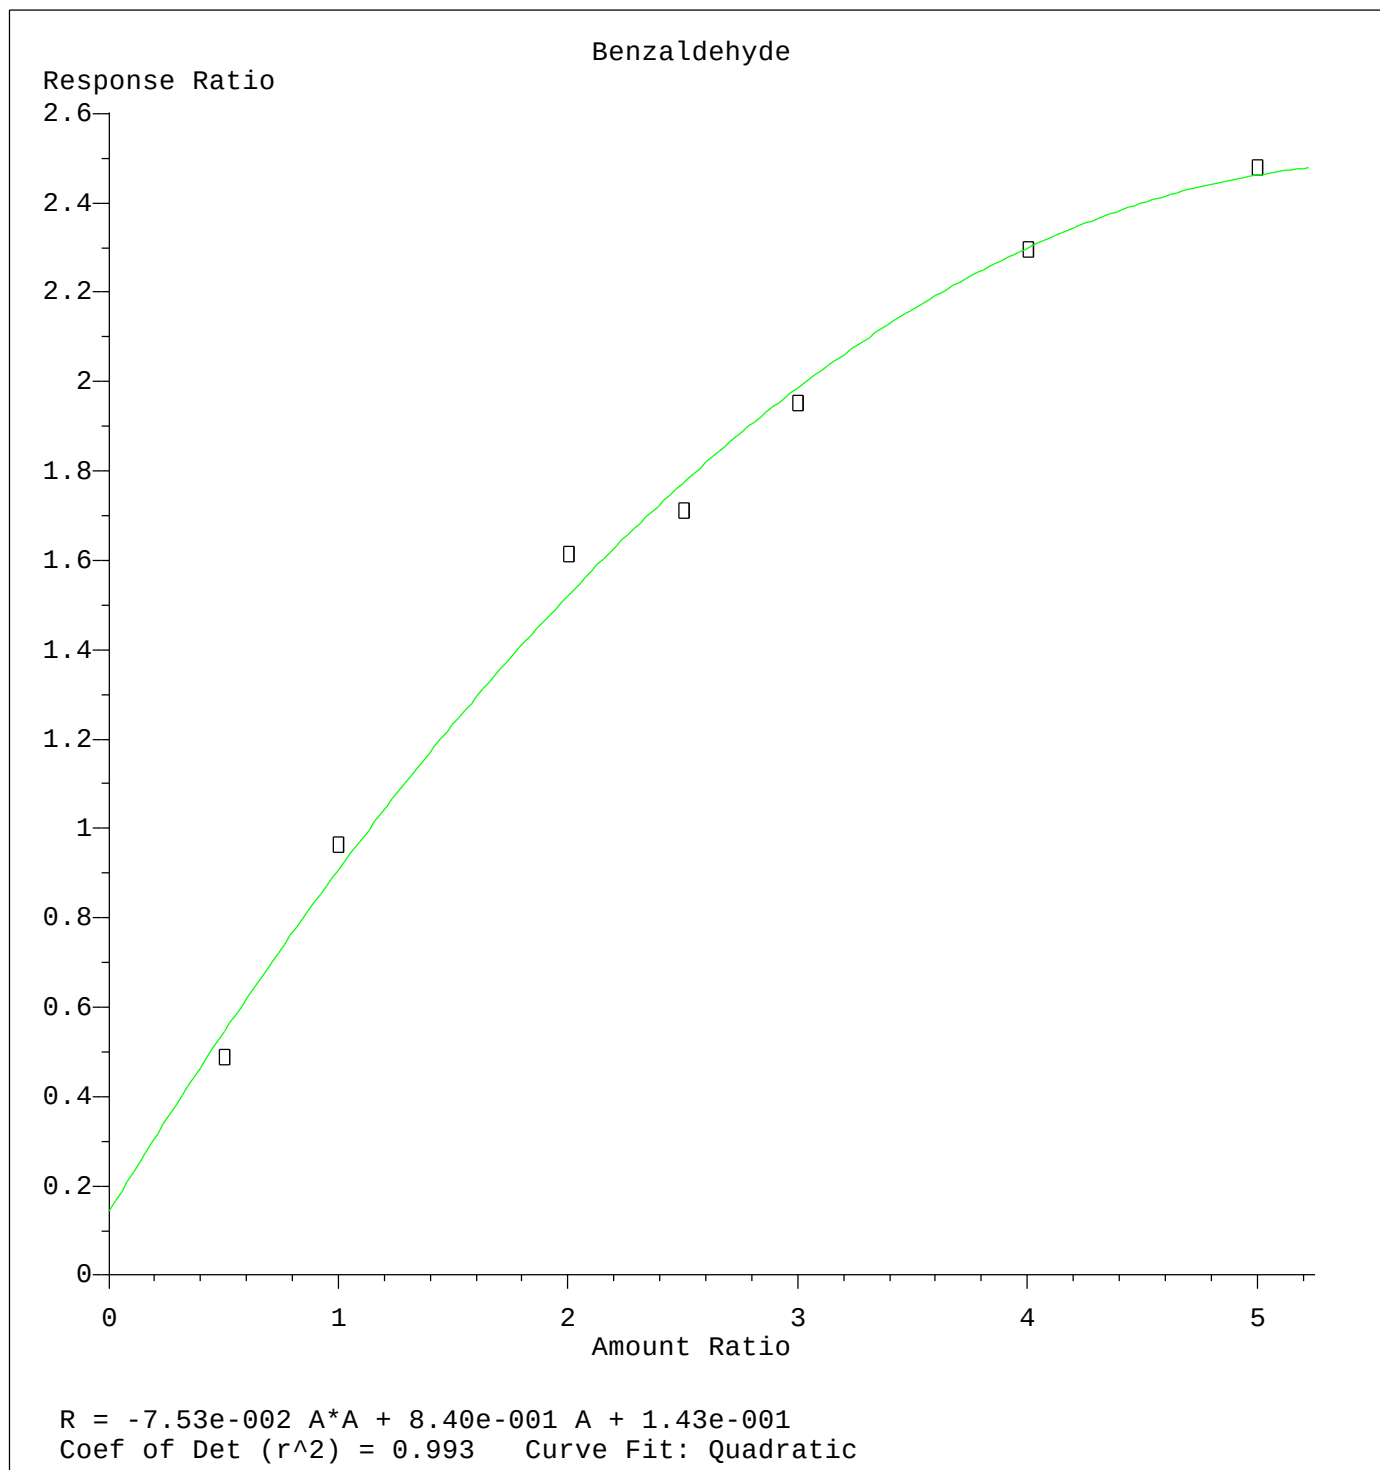


Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Calibration Table Last Updated: Fri Jun 05 15:08:53 2020

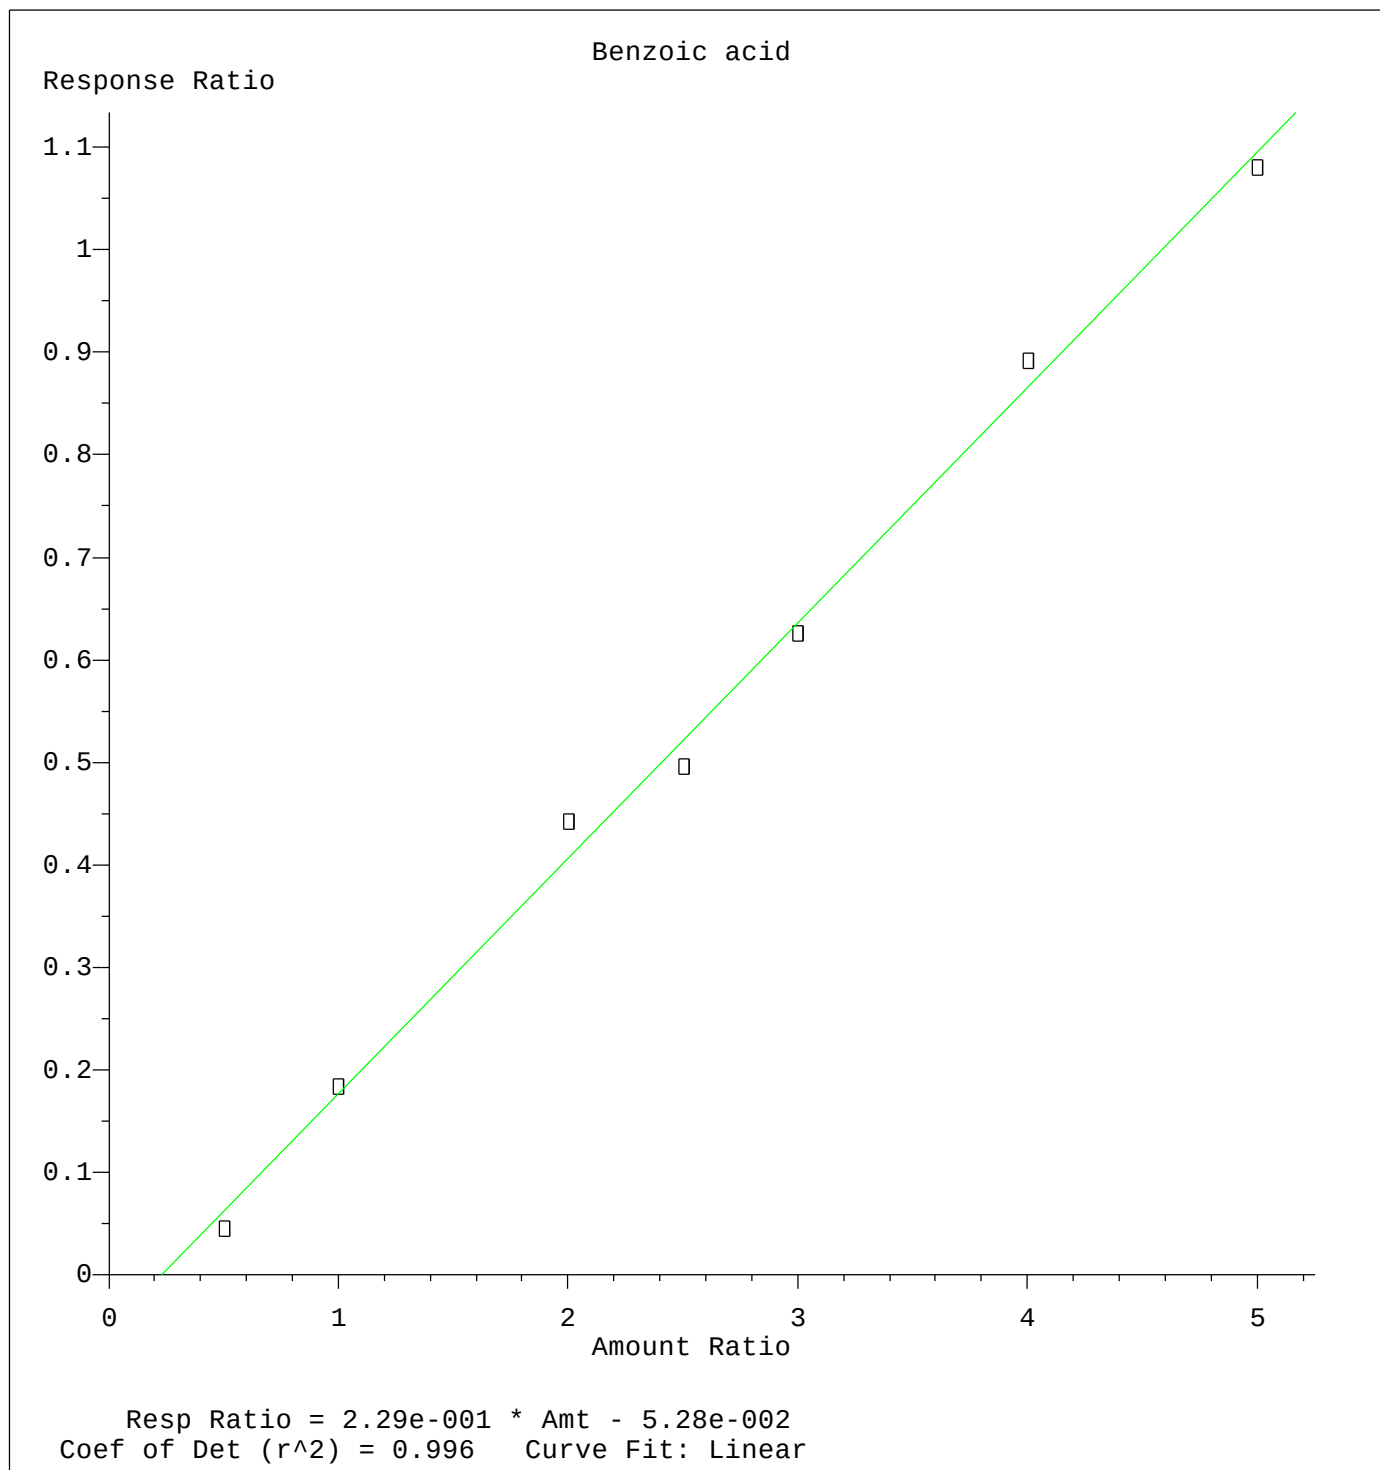

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Calibration Table Last Updated: Fri Jun 05 15:08:53 2020

2,4-Dinitrophenol

Response Ratio

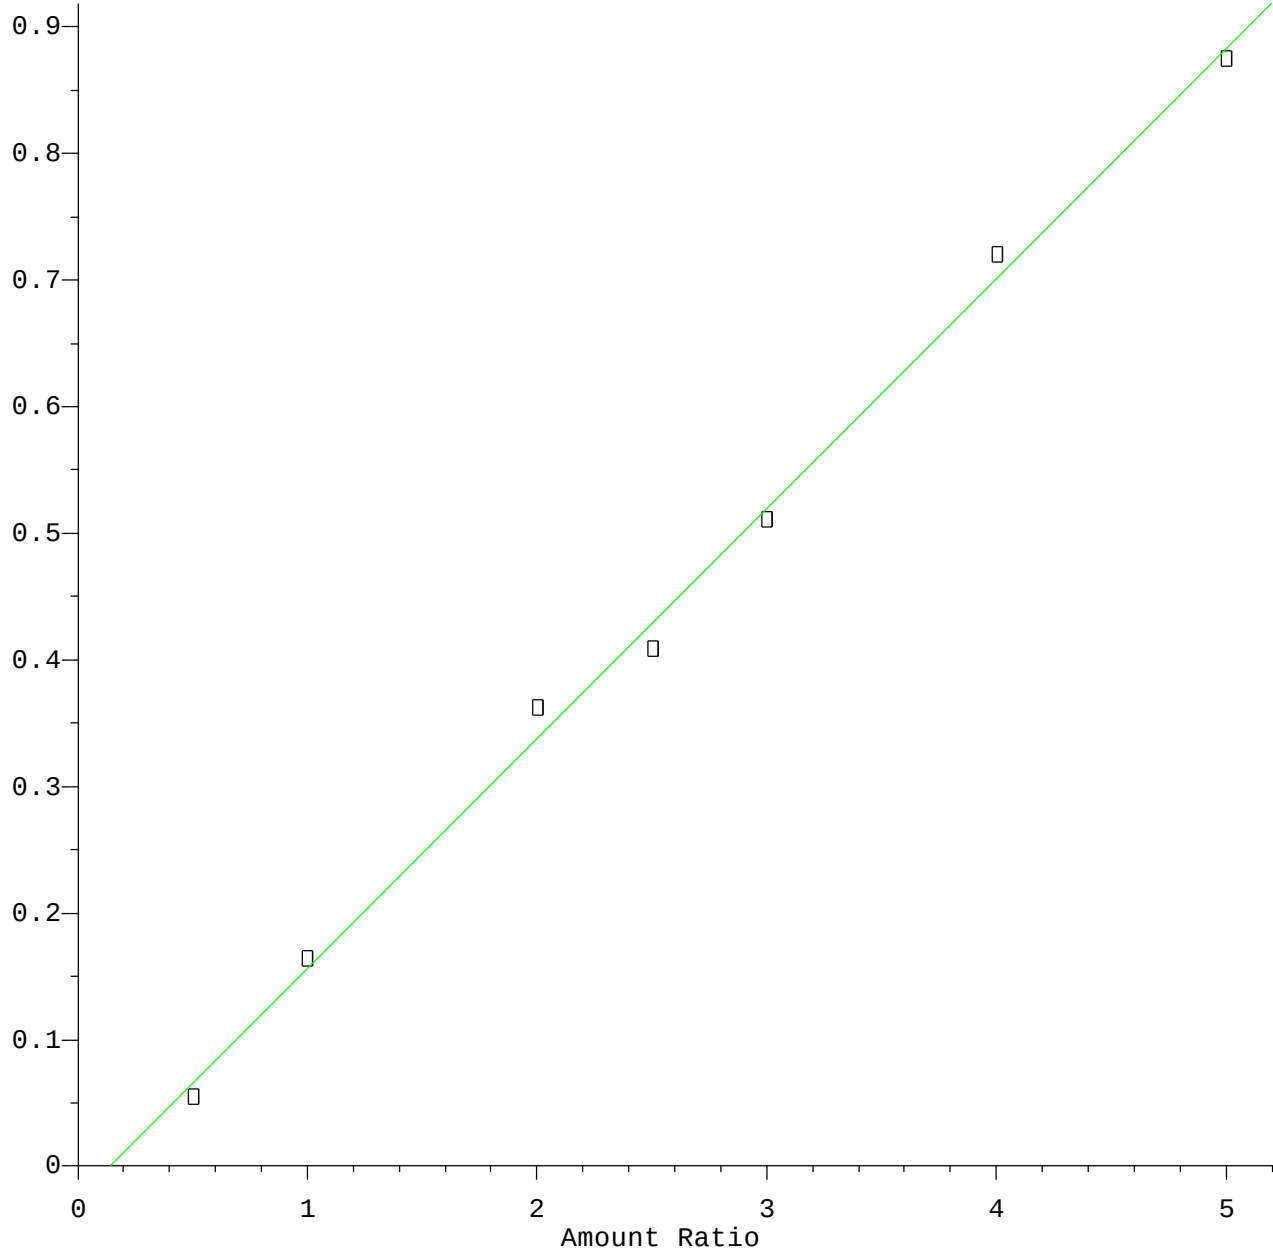


Resp Ratio = $1.82 \times 10^{-1} \times \text{Amt} - 2.53 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Calibration Table Last Updated: Fri Jun 05 15:08:53 2020


4-Chlorophenyl-phenylether

Response Ratio

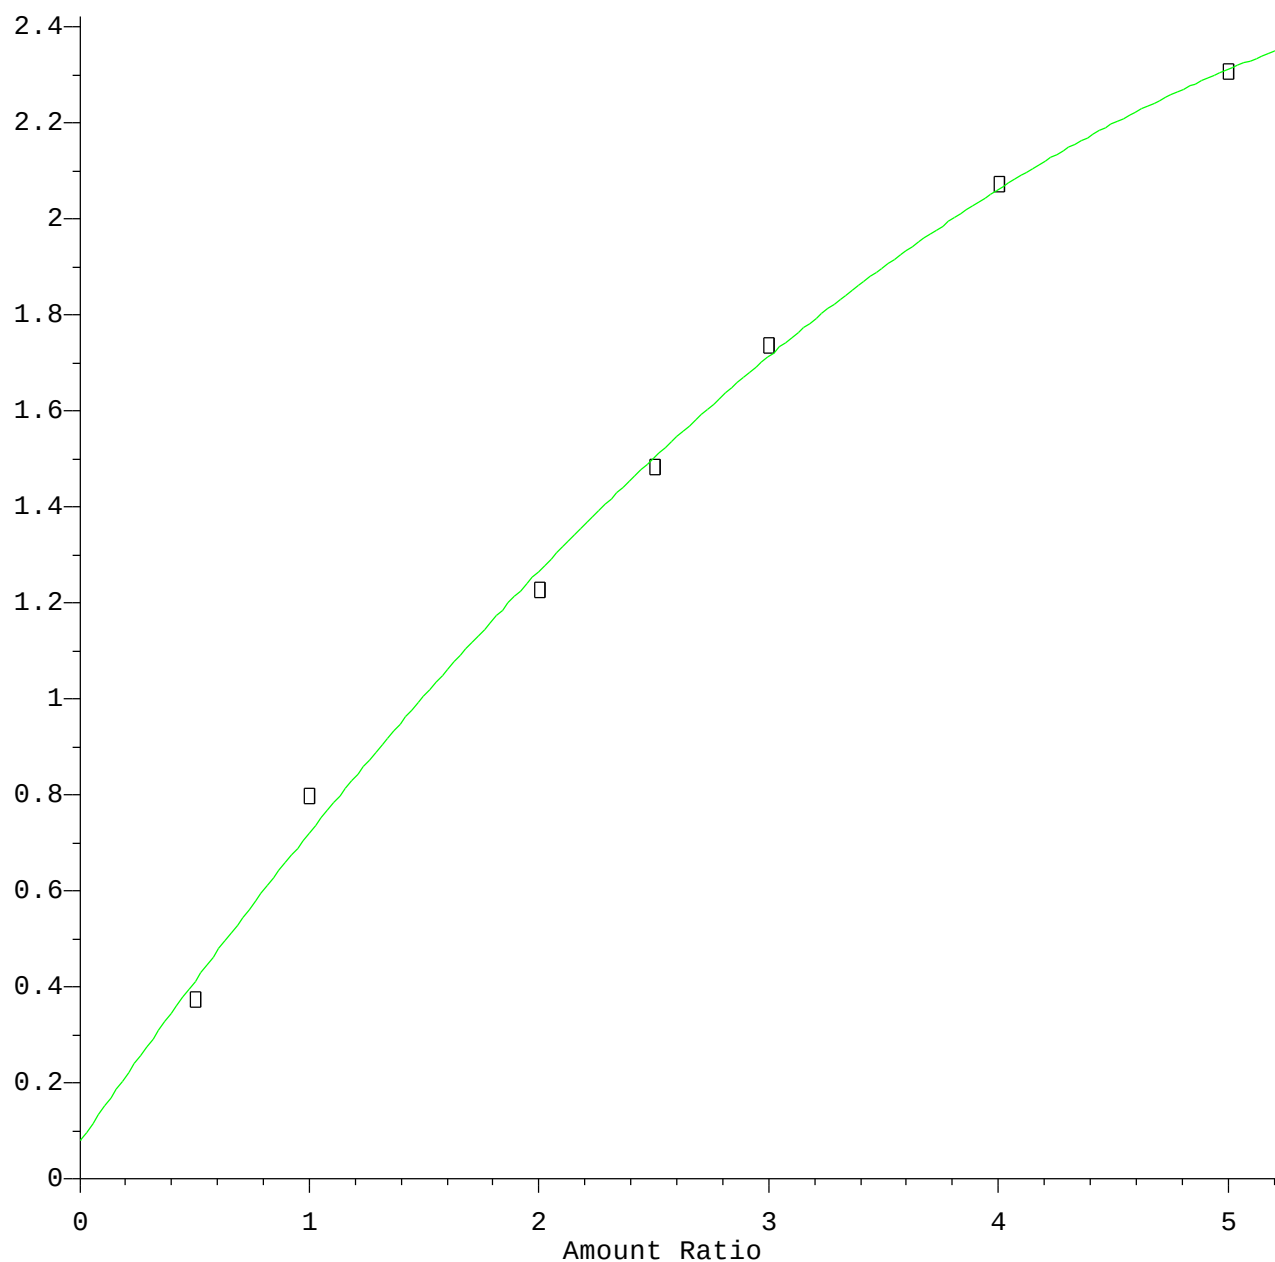

$R = -4.93e-002 A^2 + 6.93e-001 A + 7.87e-002$
Coef of Det (r^2) = 0.996 Curve Fit: Quadratic

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Calibration Table Last Updated: Fri Jun 05 15:08:53 2020

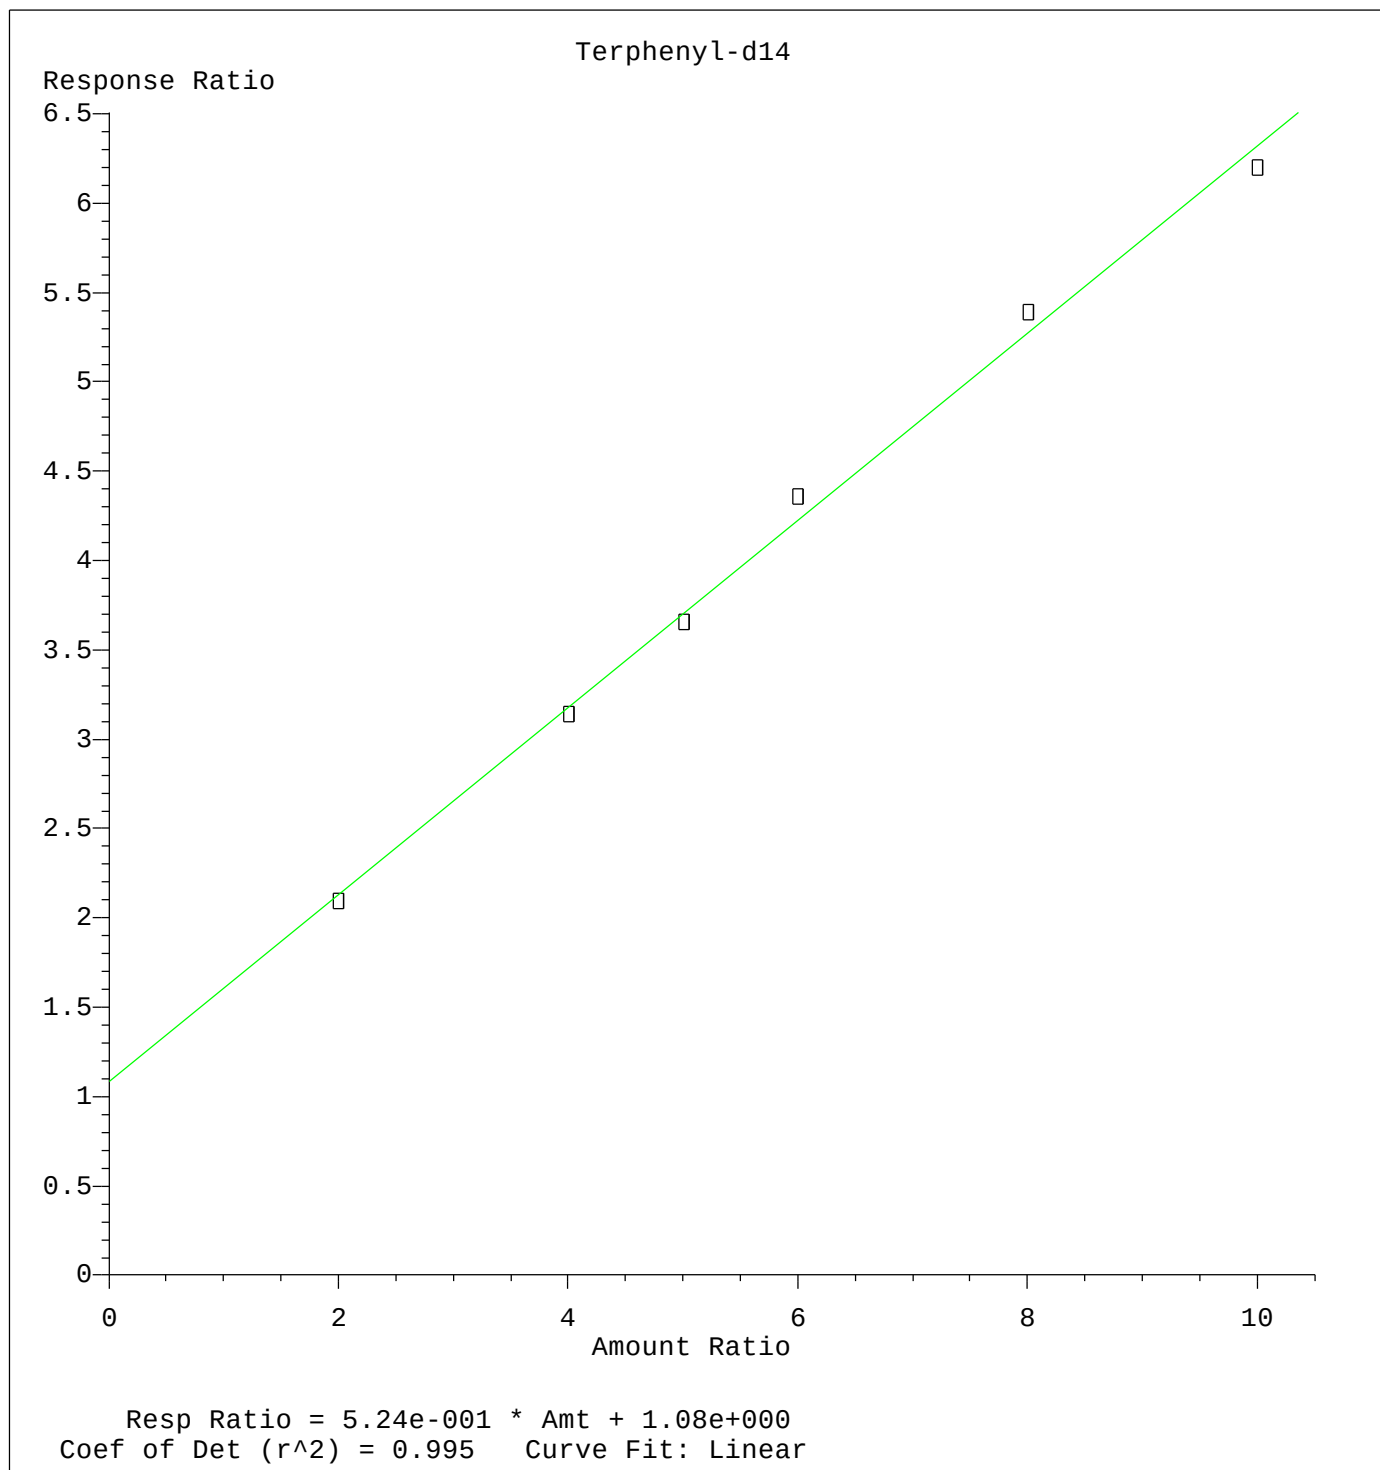

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Calibration Table Last Updated: Fri Jun 05 15:08:53 2020