
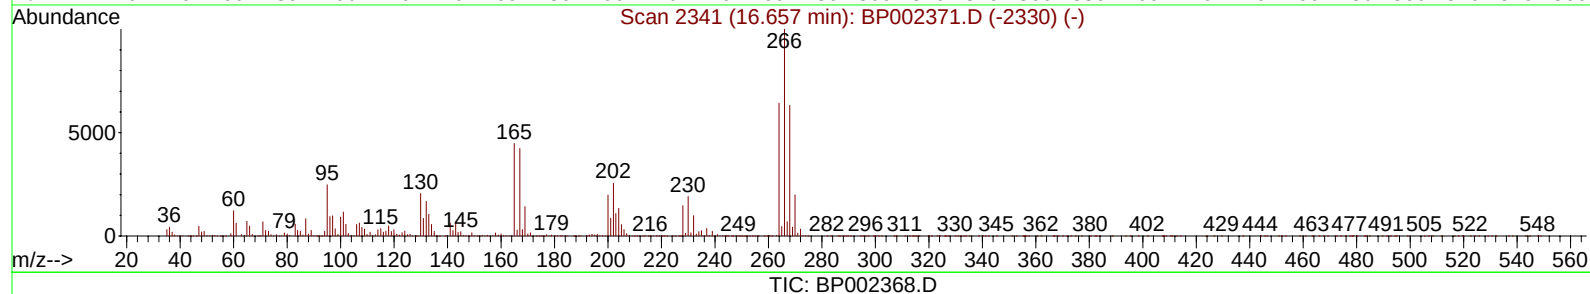
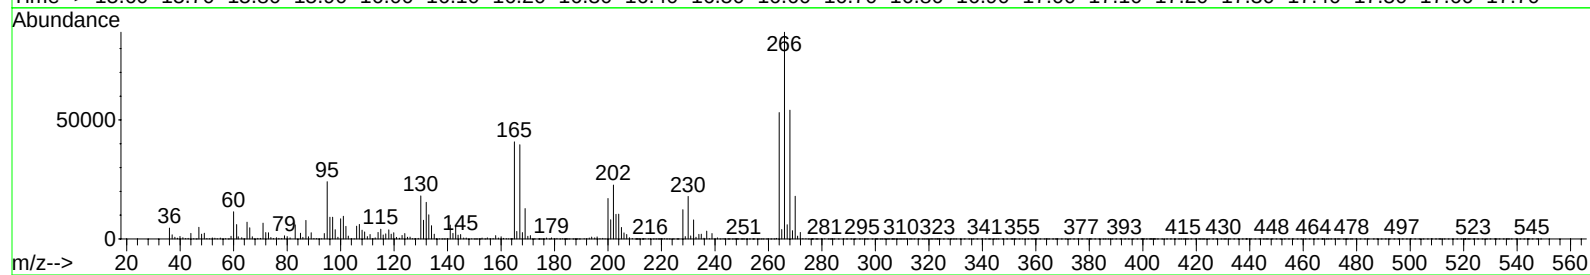


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP060520\
 Data File : BP002368.D
 Acq On : 05 Jun 2020 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 16:42:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

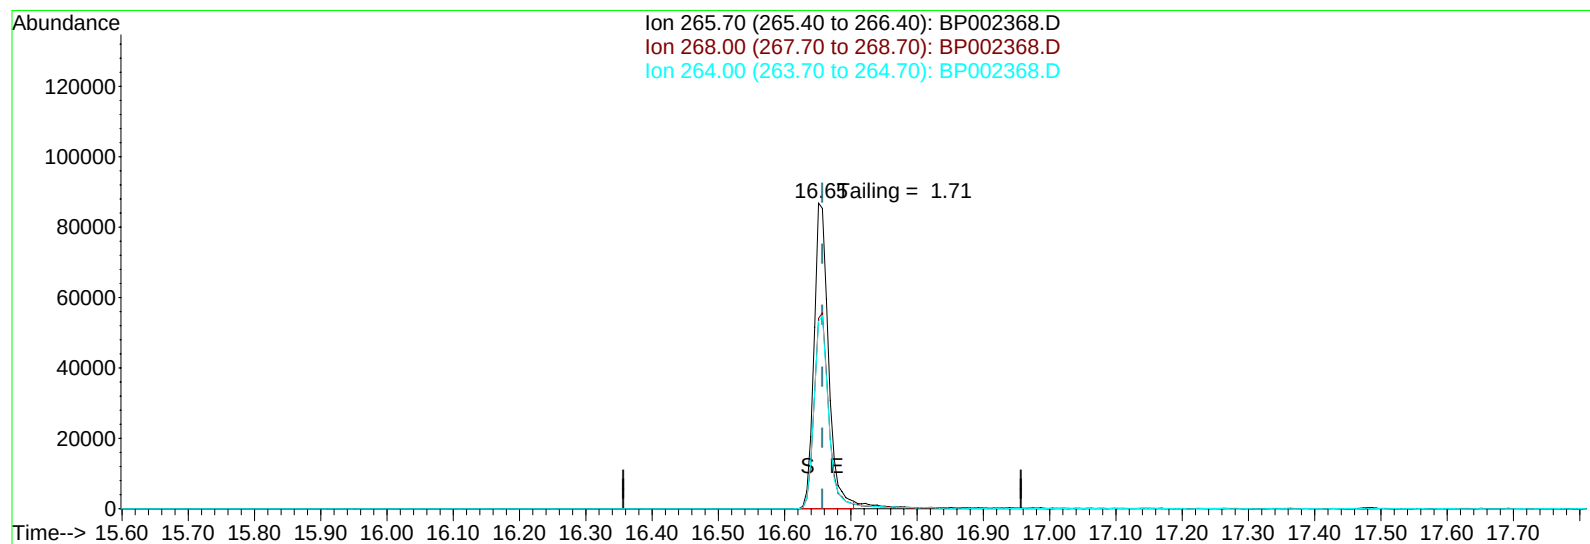

(70) Pentachlorophenol (C)




16.651min (-0.005) 631559.85ng

response 136737

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	62.27
264.00	64.20	61.15
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP060520\
 Data File : BP002368.D
 Acq On : 05 Jun 2020 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 16:42:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

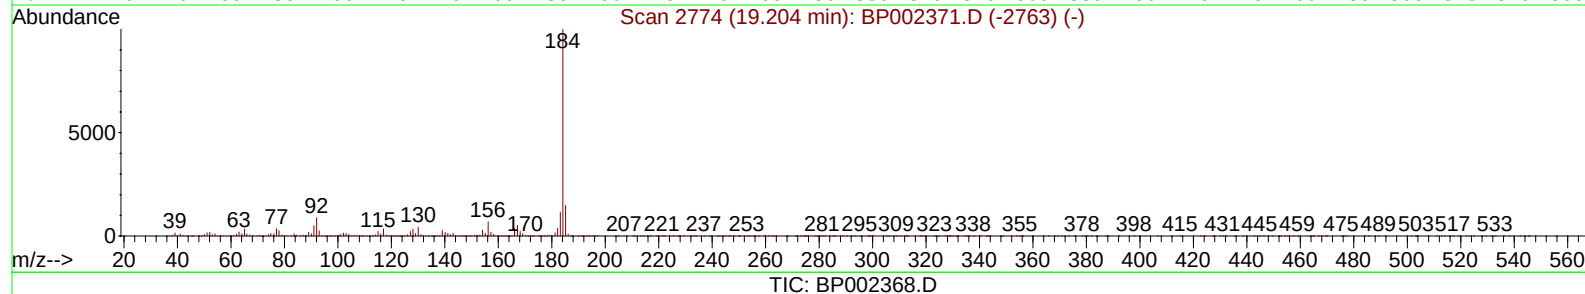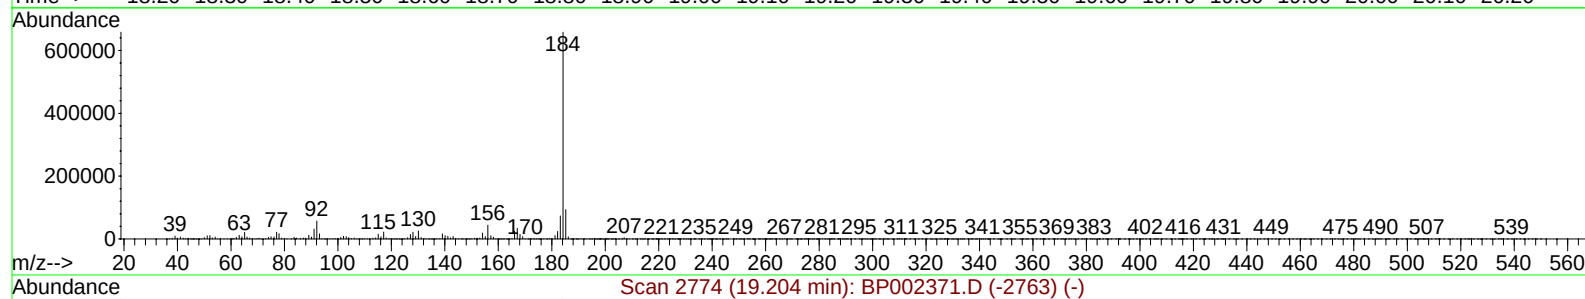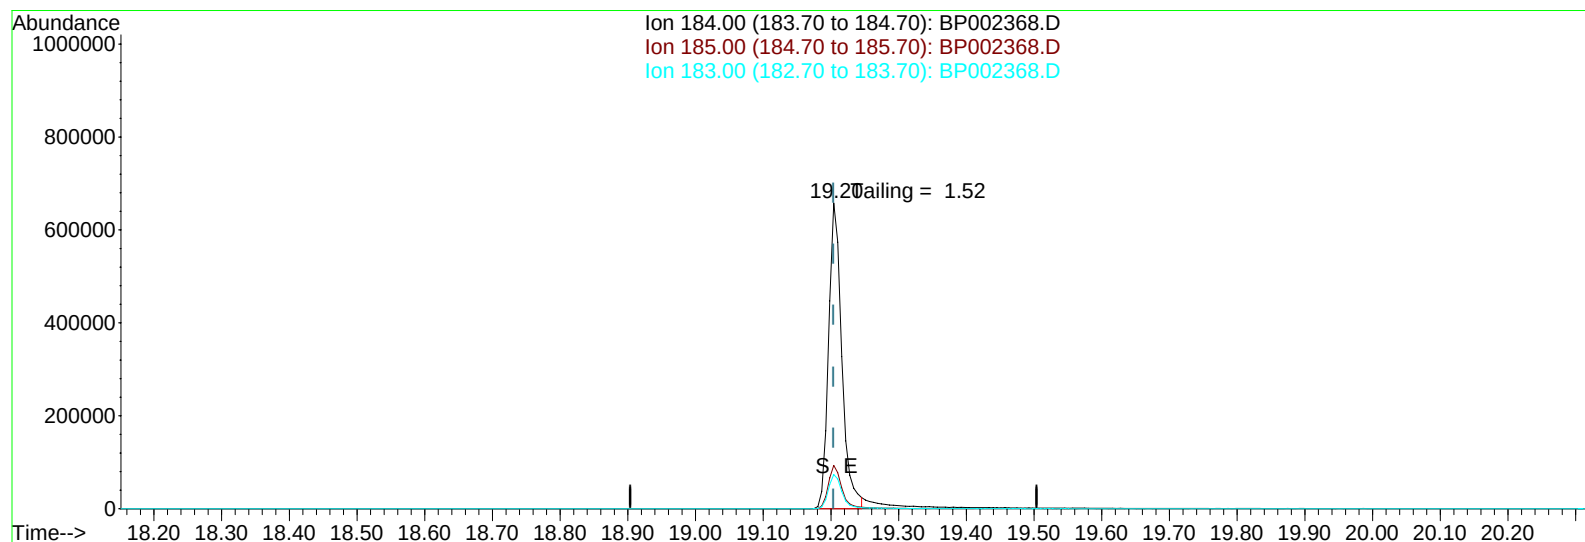

(77) Benzidine

19.204min (+0.000) 1445409.98ng

response 936634

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.18
183.00	11.50	11.18
0.00	0.00	0.00