


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060520\
 Data File : BP002368.D
 Acq On : 05 Jun 2020 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 15:08:53 2020

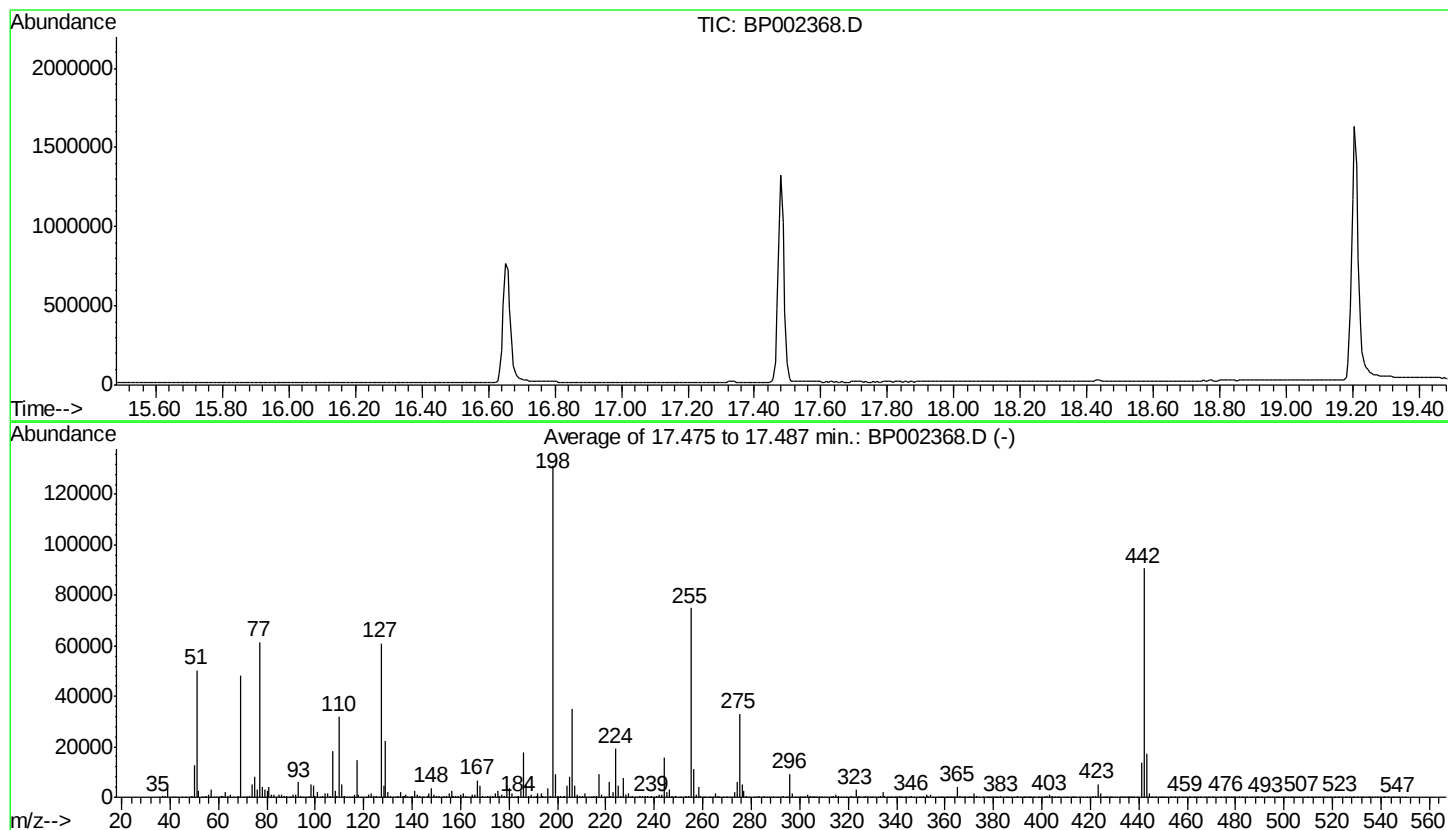

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	50228	PASS
68	69	0.00	2	1.6	753	PASS
69	198	0.00	100	36.6	48075	PASS
70	69	0.00	2	0.5	250	PASS
127	198	10	80	46.4	60960	PASS
197	198	0.00	2	0.4	472	PASS
198	198	100	100	100.0	131388	PASS
199	198	5	9	6.9	9086	PASS
275	198	10	60	25.2	33064	PASS
365	198	1	100	3.2	4191	PASS
441	198	0.01	100	10.5	13861	PASS
442	198	50	100	69.1	90781	PASS
443	442	15	24	19.2	17425	PASS