
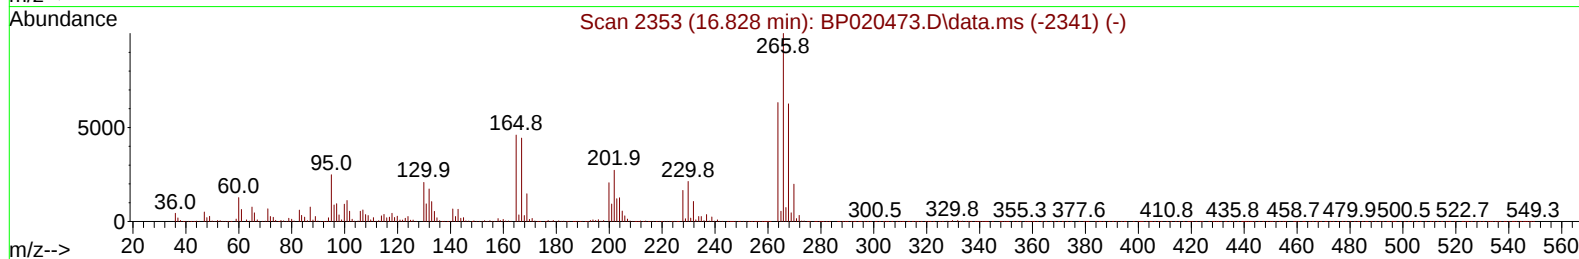
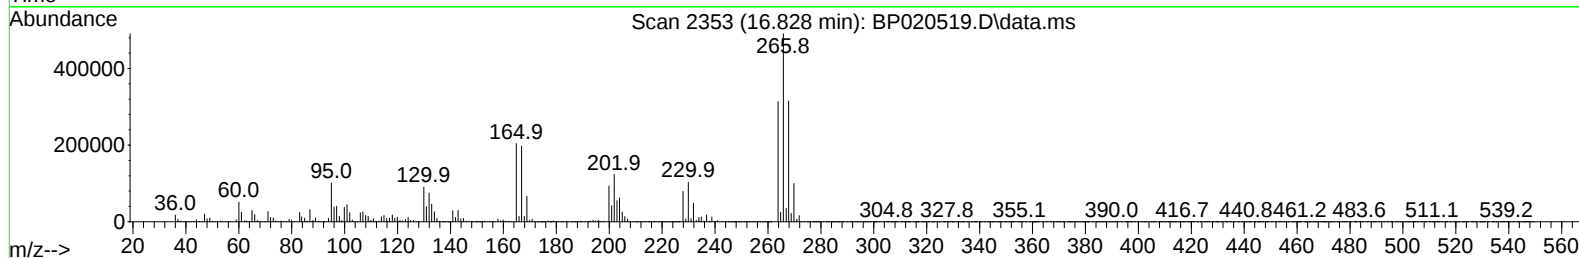


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060524\  
Data File : BP020519.D  
Acq On : 05 Jun 2024 15:57  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 16:33:20 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 30 03:41:03 2024  
Response via : Initial Calibration

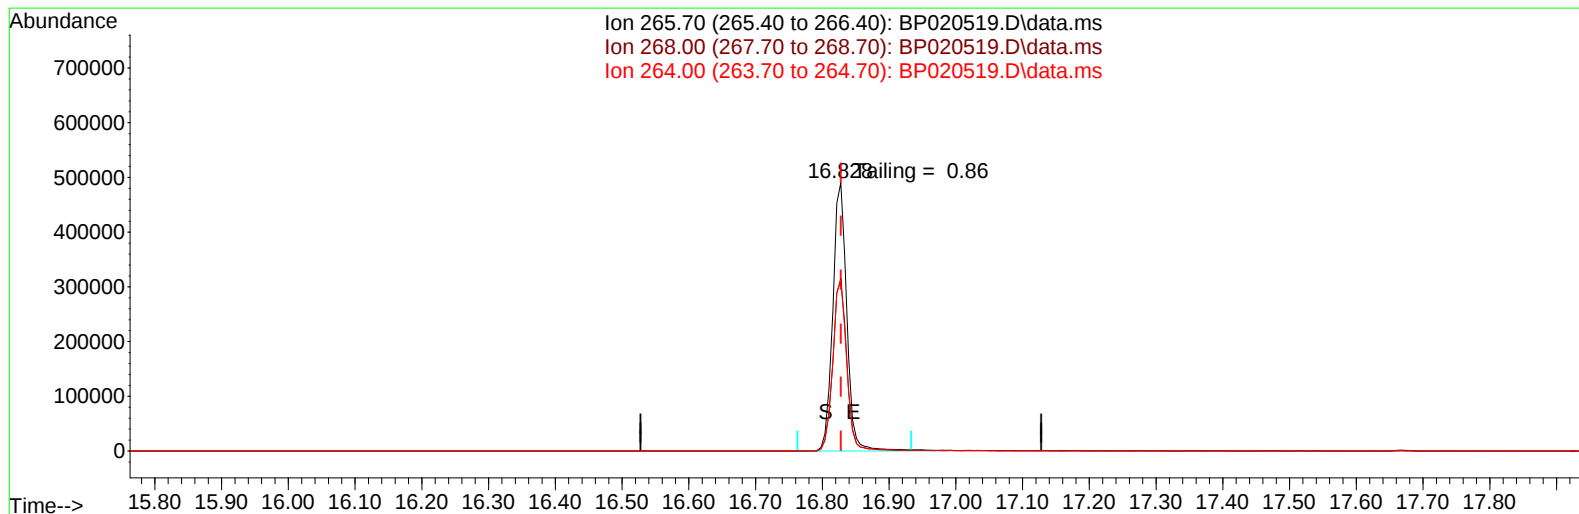

TIC: BP020519.D\data.ms

**(70) Pentachlorophenol (C)**




**16.828min (-0.000) 4896353.71 ng**

**response 716116**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.60  | 64.14  |
| 264.00 | 63.30  | 63.81  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060524\  
Data File : BP020519.D  
Acq On : 05 Jun 2024 15:57  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 16:33:20 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 30 03:41:03 2024  
Response via : Initial Calibration

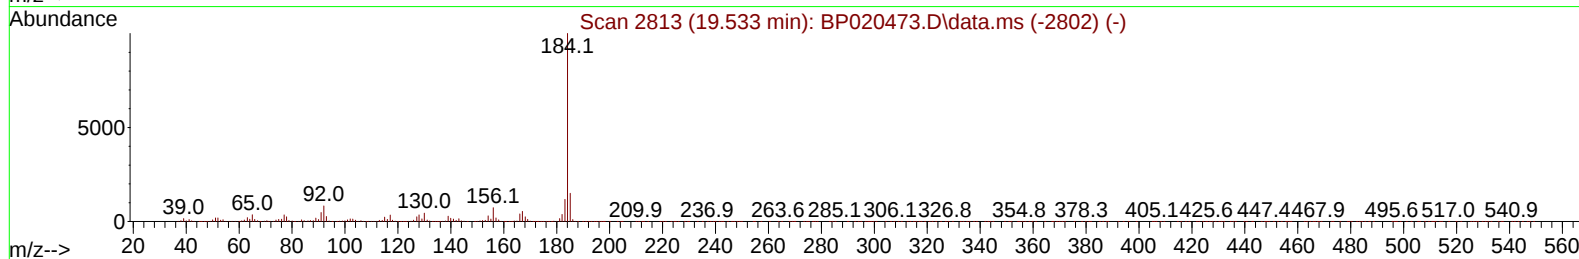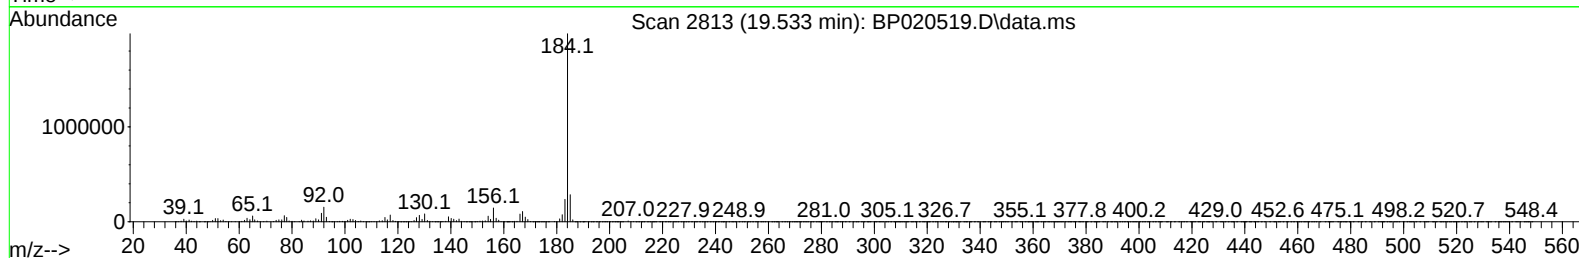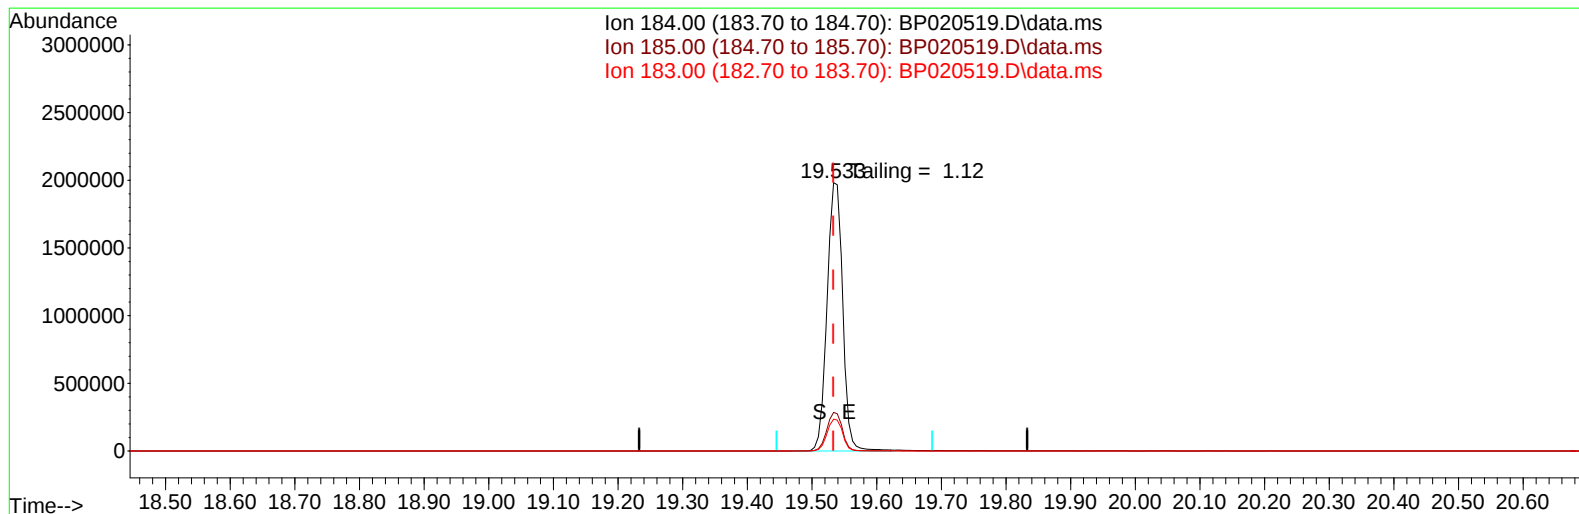

TIC: BP020519.D\data.ms

**(77) Benzidine****19.533min (+ 0.000) 1211169.00 ng****response 3343978**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 14.40  |
| 183.00 | 11.70  | 11.89  |
| 0.00   | 0.00   | 0.00   |