

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020512.D
Acq On : 05 Jun 2024 10:43
Operator : MA/JU
Sample : PB161311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB161311BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP020512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	5	10	14	rBV	145968	193884	1.53%	0.309%
2	5.381	400	407	421	rBV	5050142	7322313	57.70%	11.655%
3	6.934	663	671	683	rBV	4337614	7128873	56.17%	11.347%
4	7.769	805	813	820	rBV	996277	1533179	12.08%	2.440%
5	8.911	998	1007	1018	rBV	3064493	4698203	37.02%	7.478%
6	10.540	1276	1284	1292	rBV	1183023	1974265	15.56%	3.142%
7	13.004	1694	1703	1711	rBV	6209504	9738841	76.74%	15.501%
8	14.387	1929	1938	1946	rBV	1471319	2270720	17.89%	3.614%
9	15.898	2180	2195	2220	rVB	3647769	5825203	45.90%	9.272%
10	17.204	2409	2417	2423	rBV	1535795	2504383	19.73%	3.986%
11	19.933	2875	2881	2888	rBV	10150242	12691321	100.00%	20.200%
12	21.145	3084	3087	3098	rVB2	68109	137074	1.08%	0.218%
13	21.645	3166	3172	3182	rVB	1878842	3094495	24.38%	4.925%
14	25.010	3733	3744	3758	rVB	1335441	3714573	29.27%	5.912%




Sum of corrected areas: 62827327

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020512.D
Acq On : 05 Jun 2024 10:43
Operator : MA/JU
Sample : PB161311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB161311BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

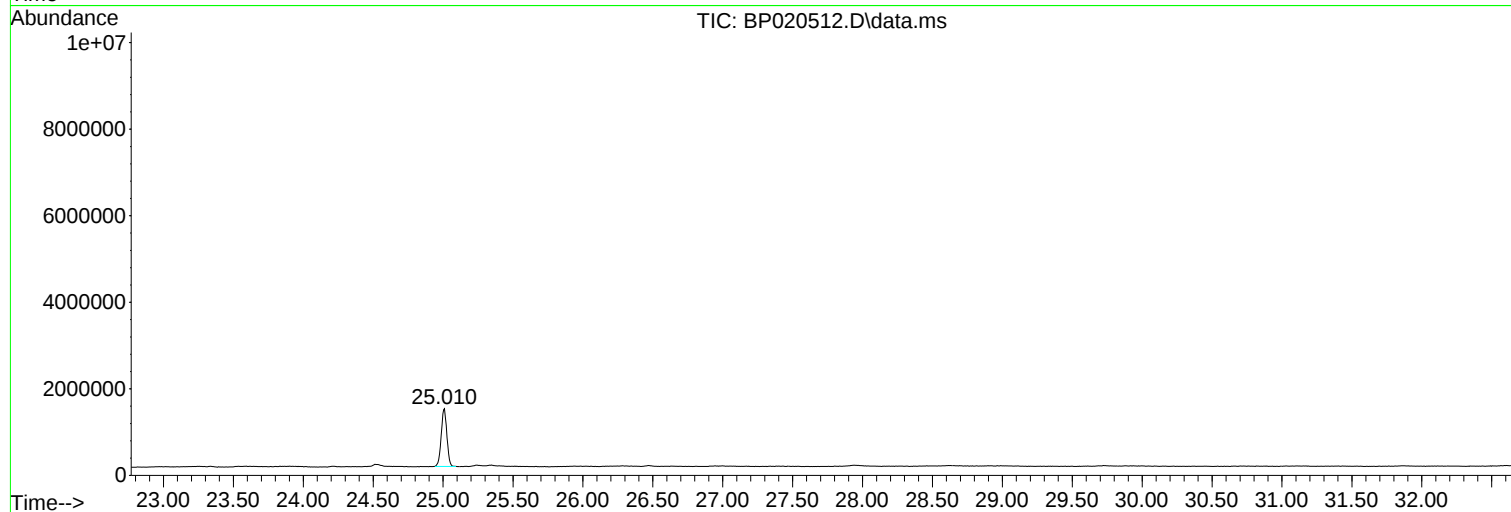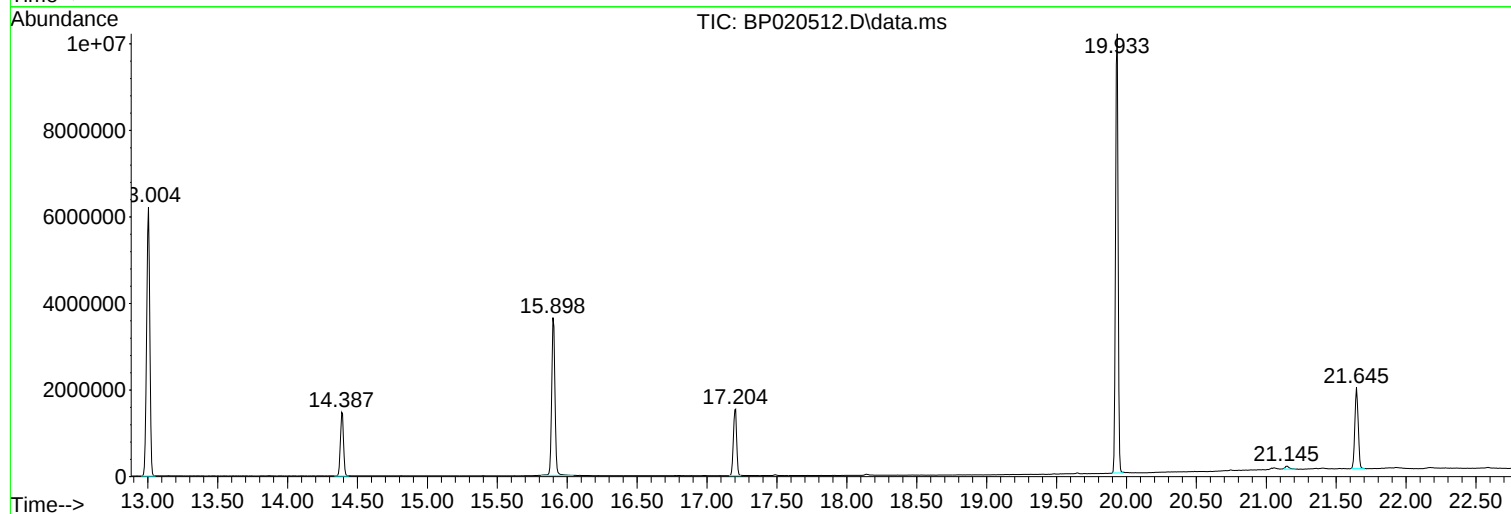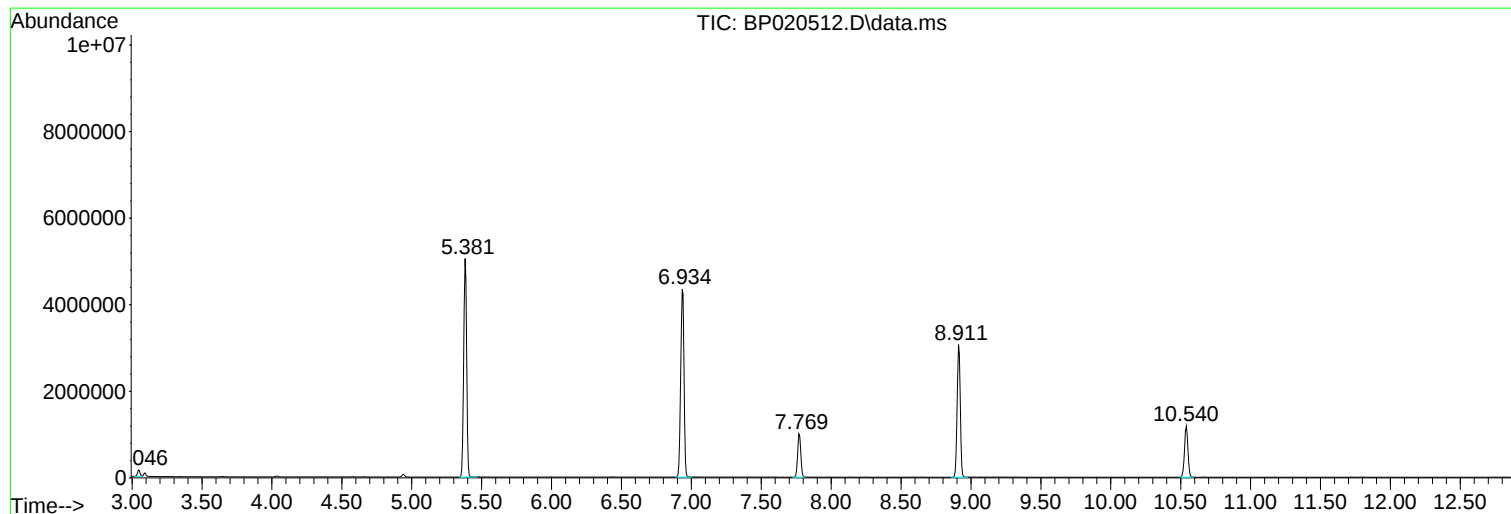

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020512.D
Acq On : 05 Jun 2024 10:43
Operator : MA/JU
Sample : PB161311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB161311BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.046	2.53 ng	193884	1,4-Dichlorobenzene-d4	7.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	17
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

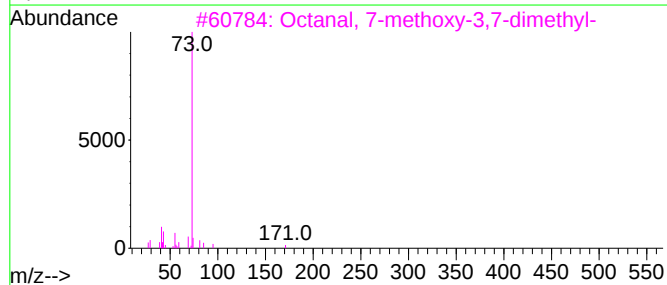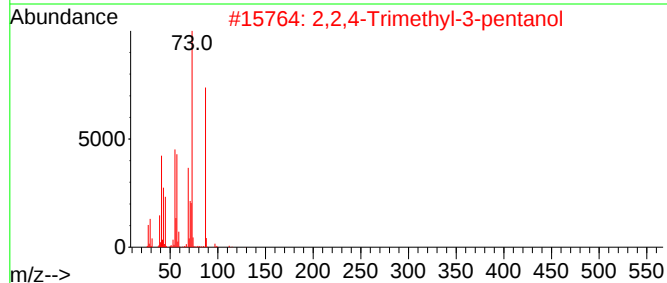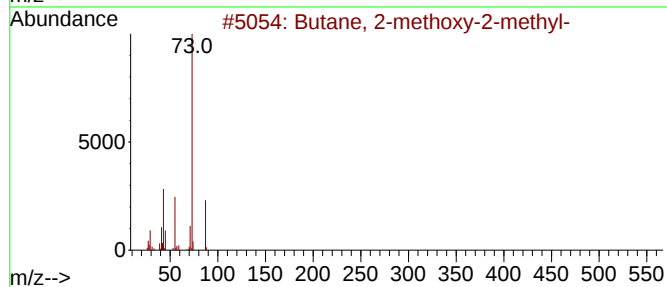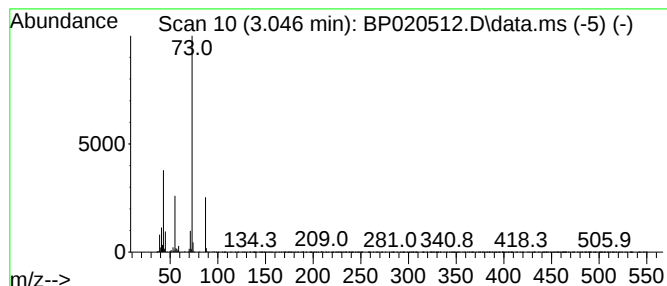

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020512.D
Acq On : 05 Jun 2024 10:43
Operator : MA/JU
Sample : PB161311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB161311BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.046	2.5	ng	193884	1	7.769	1533180	20.0