

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
 Data File : BP020521.D
 Acq On : 05 Jun 2024 17:26
 Operator : MA/JU
 Sample : PB161290BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB161290BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP020521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	5	10	14	rVB	172843	214546	1.79%	0.333%
2	5.381	399	407	425	rVB	5283520	7738954	64.59%	12.017%
3	6.934	663	671	683	rBV	4585250	7481798	62.44%	11.617%
4	7.769	805	813	820	rBV	1129053	1791512	14.95%	2.782%
5	8.910	999	1007	1023	rBV	2941133	4999164	41.72%	7.762%
6	10.534	1275	1283	1293	rBV	1385585	2237323	18.67%	3.474%
7	13.004	1696	1703	1709	rBV	7047311	9921638	82.80%	15.406%
8	14.387	1931	1938	1948	rBV	1655627	2513521	20.98%	3.903%
9	15.904	2173	2196	2215	rBV	3651616	5791441	48.33%	8.993%
10	17.192	2408	2415	2428	rBV	1694105	2546703	21.25%	3.954%
11	19.939	2875	2882	2891	rBV	8854986	11982126	100.00%	18.605%
12	21.645	3166	3172	3180	rBV	2135382	3184788	26.58%	4.945%
13	24.998	3732	3742	3761	rVB	1420330	3998060	33.37%	6.208%




Sum of corrected areas: 64401574

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020521.D
Acq On : 05 Jun 2024 17:26
Operator : MA/JU
Sample : PB161290BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB161290BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

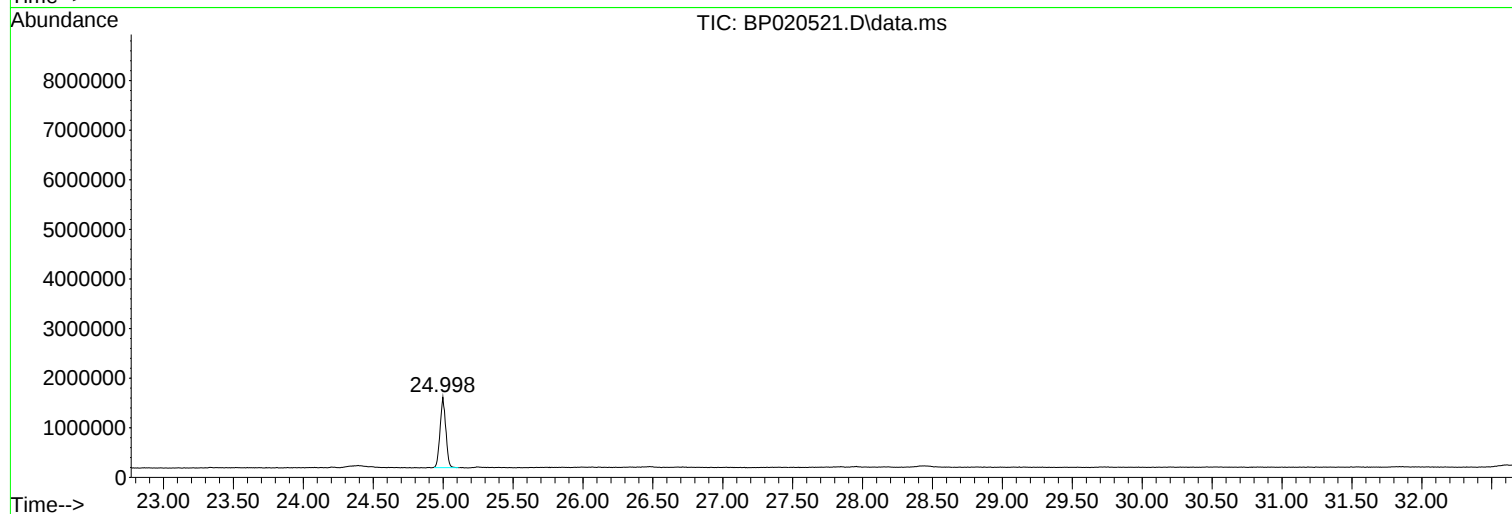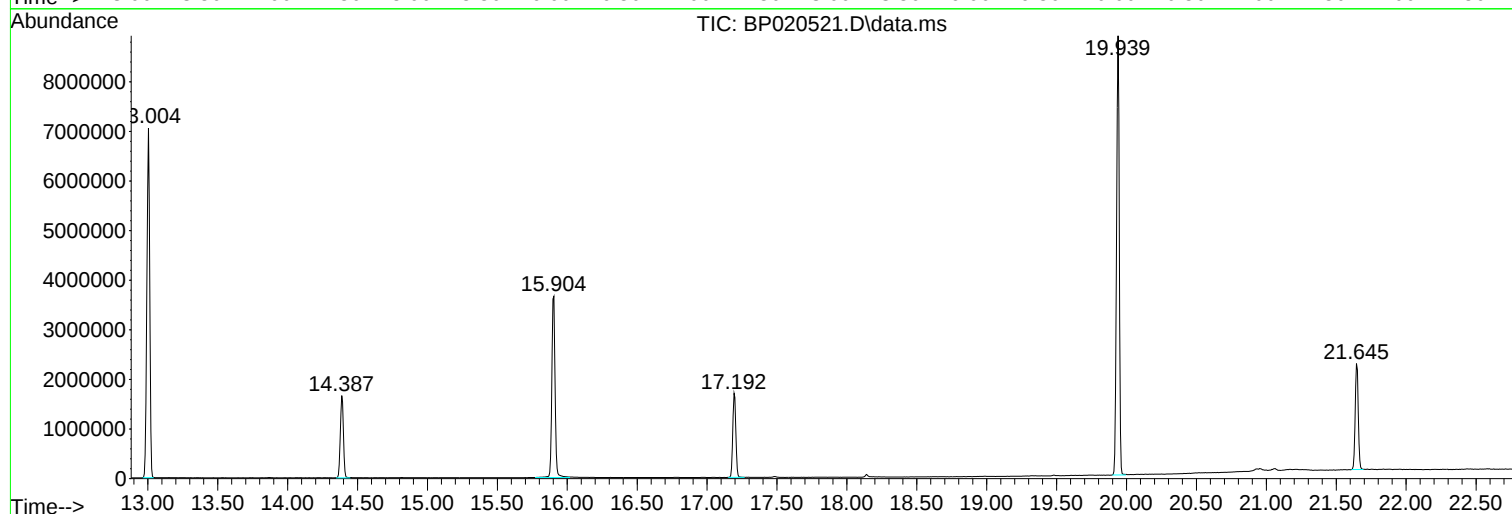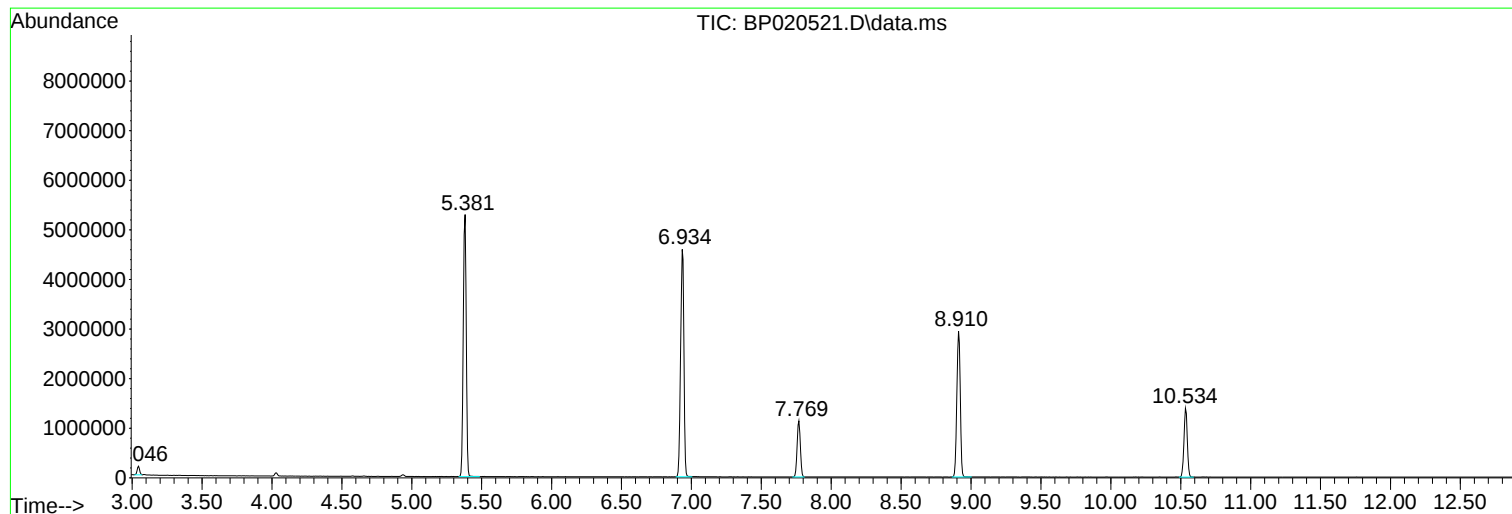

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020521.D
Acq On : 05 Jun 2024 17:26
Operator : MA/JU
Sample : PB161290BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB161290BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.046	2.40 ng	214546	1,4-Dichlorobenzene-d4	7.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	23
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

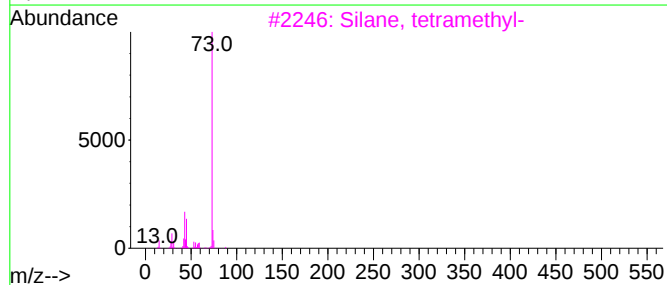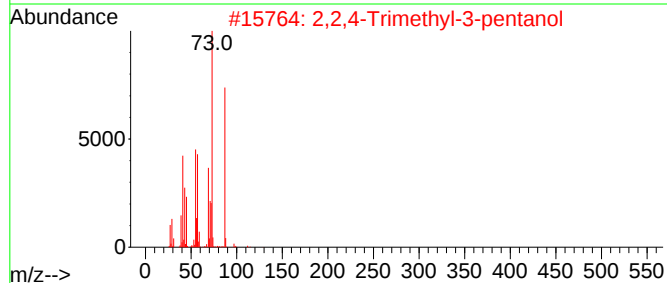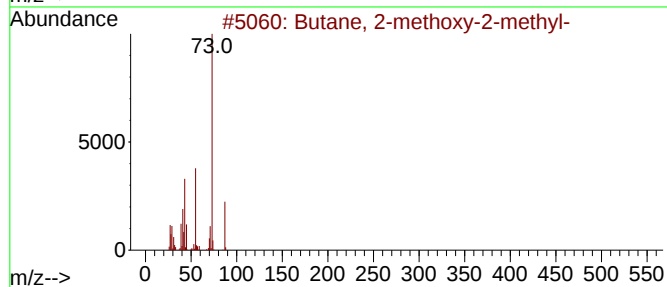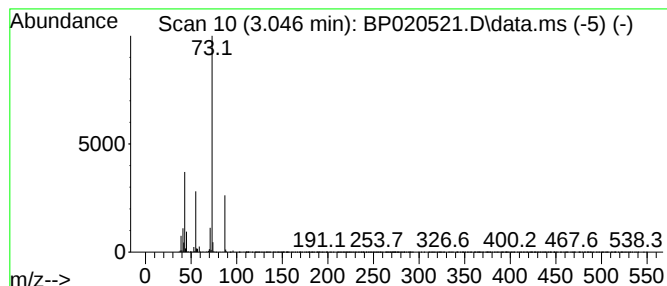

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020521.D
Acq On : 05 Jun 2024 17:26
Operator : MA/JU
Sample : PB161290BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB161290BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.046	2.4	ng	214546	1	7.769	1791510	20.0