
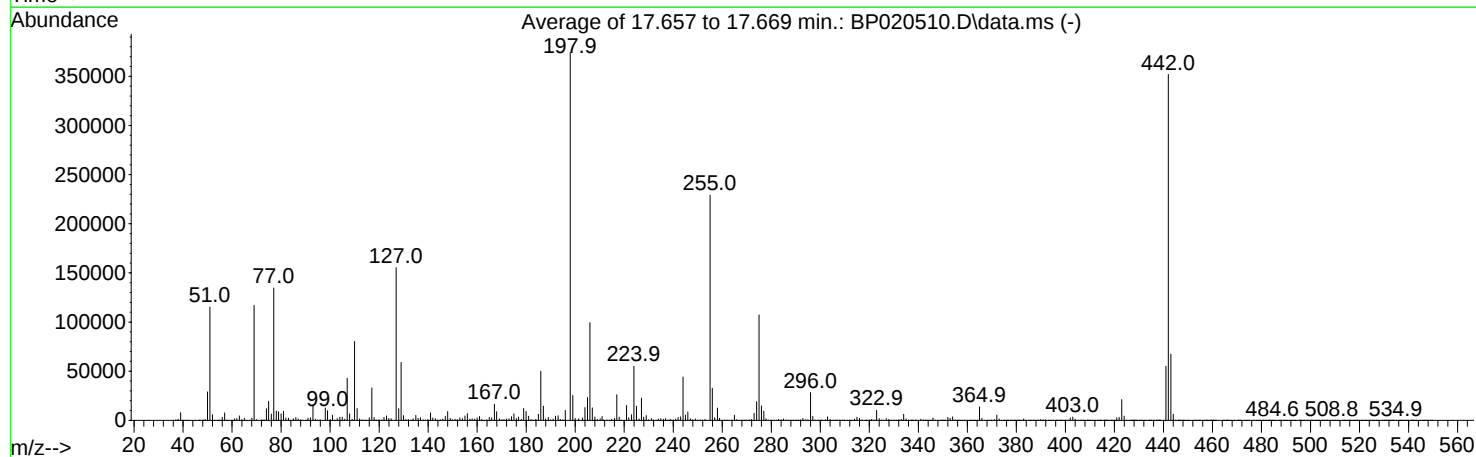


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020510.D
Acq On : 05 Jun 2024 09:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

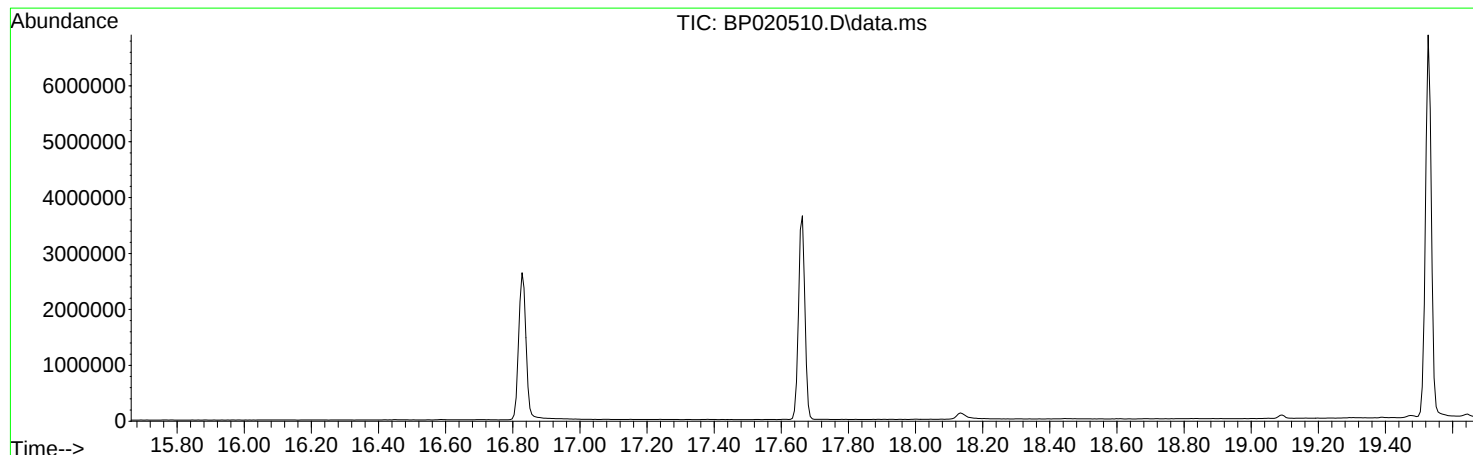




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	115287	PASS
68	69	0.00	2	1.8	2162	PASS
69	198	0.00	100	31.3	117016	PASS
70	69	0.00	2	0.6	656	PASS
127	198	10	80	41.5	155388	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	374223	PASS
199	198	5	9	6.8	25483	PASS
275	198	10	60	28.7	107323	PASS
365	198	1	100	3.6	13630	PASS
441	198	0.01	100	14.7	55077	PASS
442	442	100	100	100.0	351871	PASS
443	442	15	24	19.2	67465	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020510.D
Acq On : 05 Jun 2024 09:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 05 19:21:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

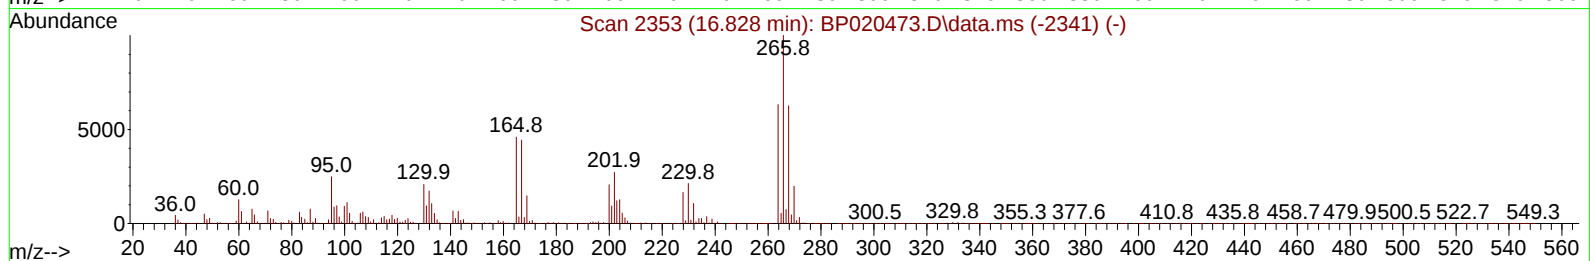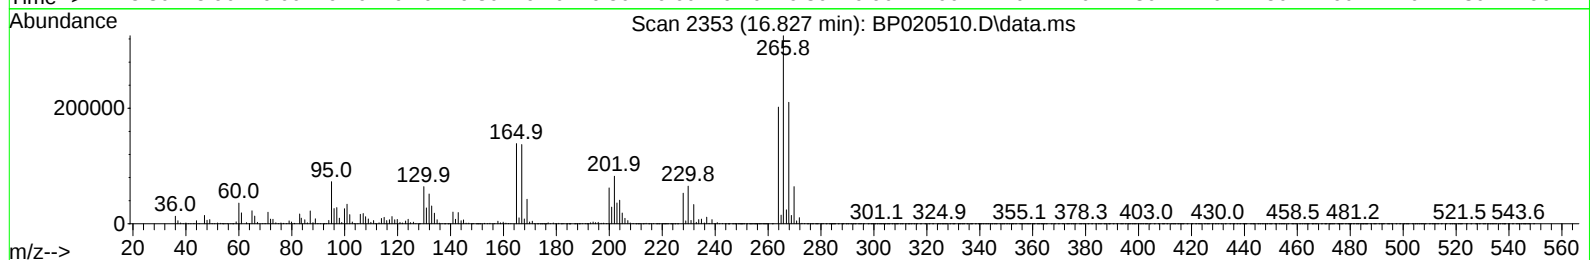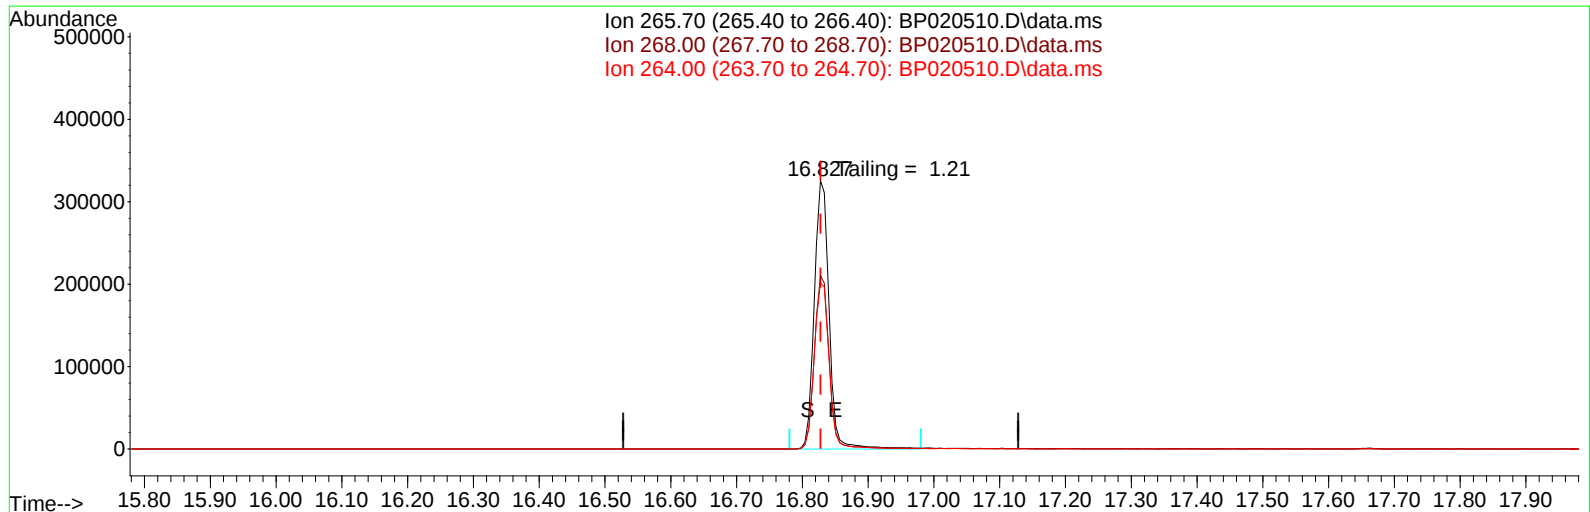

TIC: BP020510.D\data.ms

(70) Pentachlorophenol (C)

16.827min (-0.001) 388630.29 ng




response 508710

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.56
264.00	63.30	62.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020510.D
Acq On : 05 Jun 2024 09:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 05 19:21:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

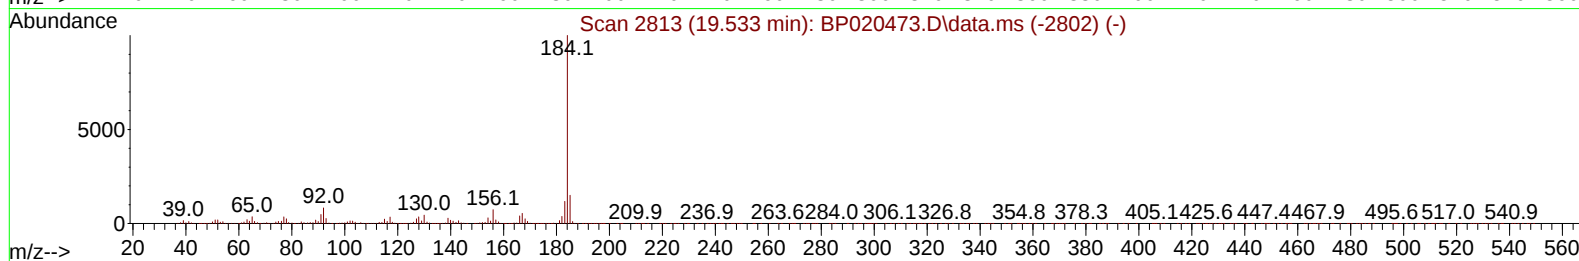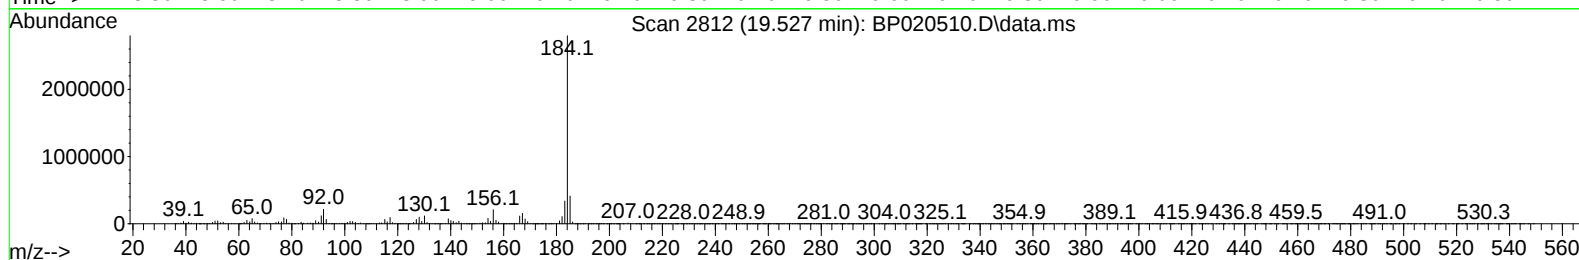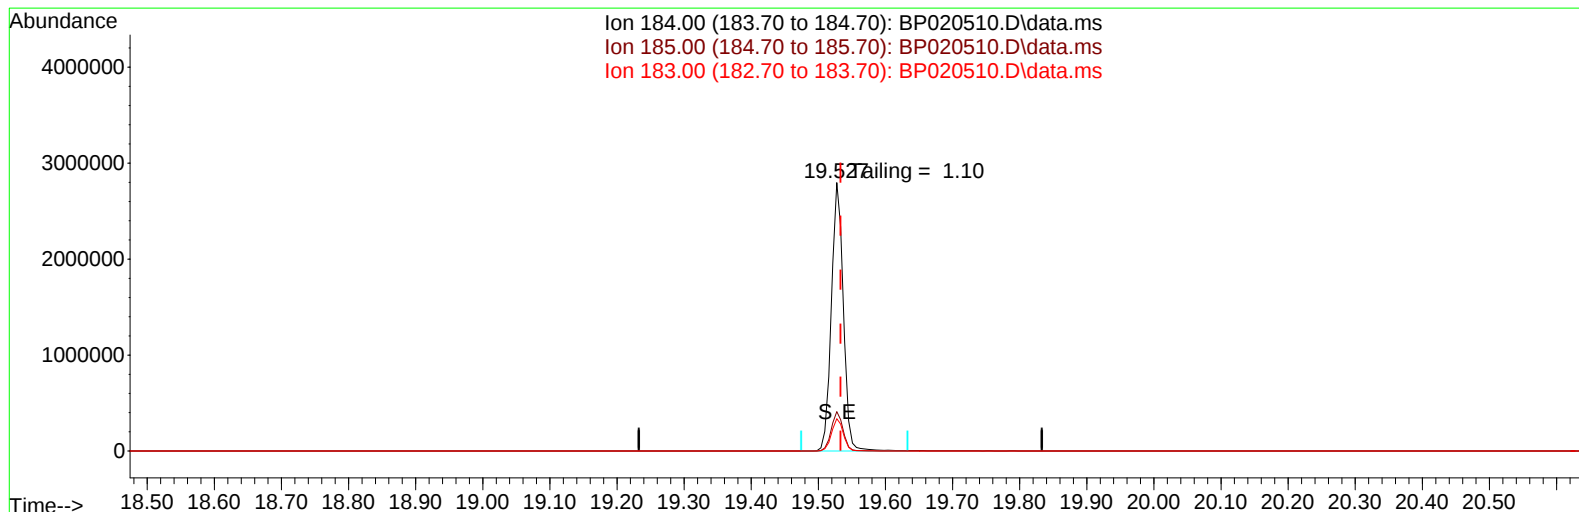

TIC: BP020510.D\data.ms

(77) Benzidine

19.527min (-0.006) 1334174.52 ng

response 3466910

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.71
183.00	11.70	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/5/2024	BNA_P	<u>BP020510.D</u>
Compound Name	Response	Retention Time
DDT	1575061	20.827
DDD	28237	20.363
DDE	2627	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30864	1605925	1.92

Instrument :
BNA_P
ClientSampleId :
DFTPP