
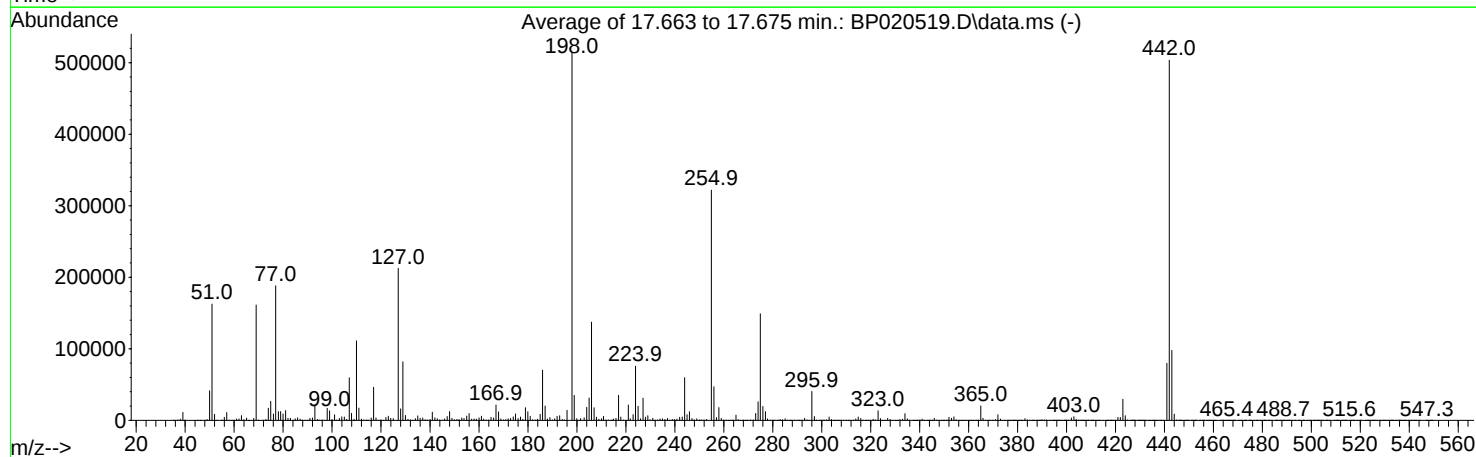


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020519.D
Acq On : 05 Jun 2024 15:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

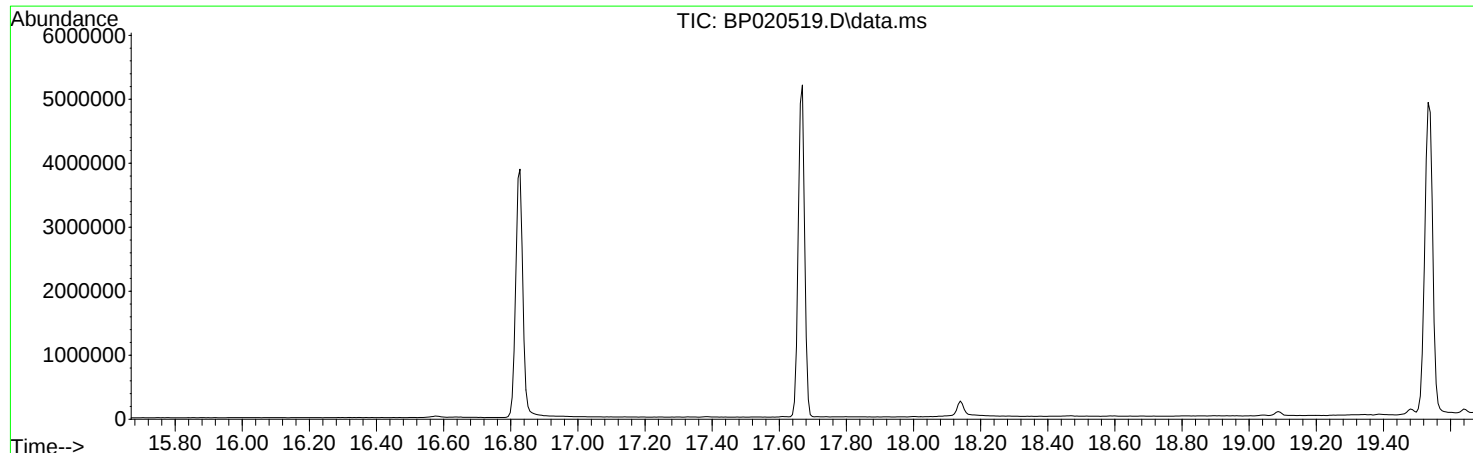




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	162616	PASS
68	69	0.00	2	1.7	2696	PASS
69	198	0.00	100	31.4	161391	PASS
70	69	0.00	2	0.3	486	PASS
127	198	10	80	41.3	212508	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	514283	PASS
199	198	5	9	6.8	34861	PASS
275	198	10	60	29.0	149081	PASS
365	198	1	100	3.9	20219	PASS
441	198	0.01	100	15.5	79859	PASS
442	442	100	100	100.0	503548	PASS
443	442	15	24	19.4	97831	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020519.D
Acq On : 05 Jun 2024 15:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 05 16:33:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

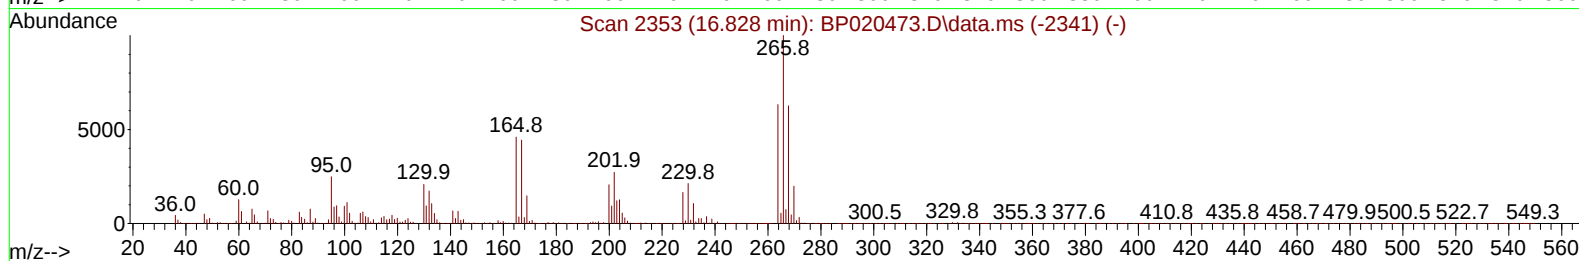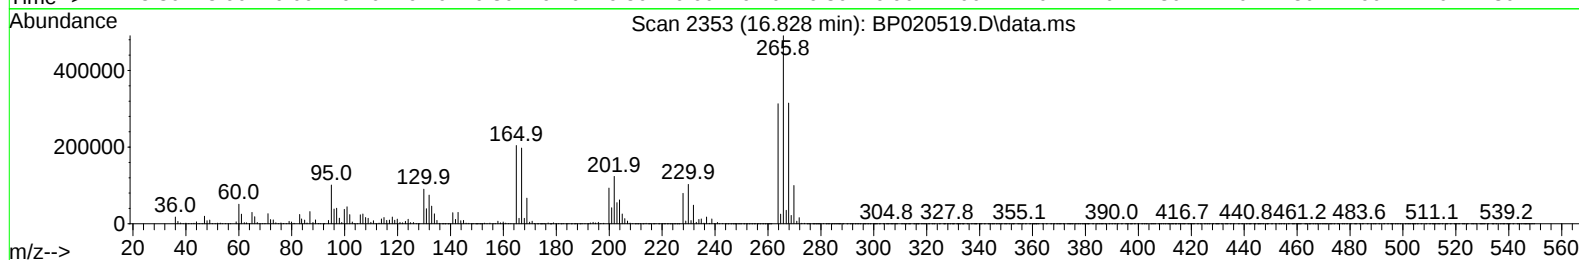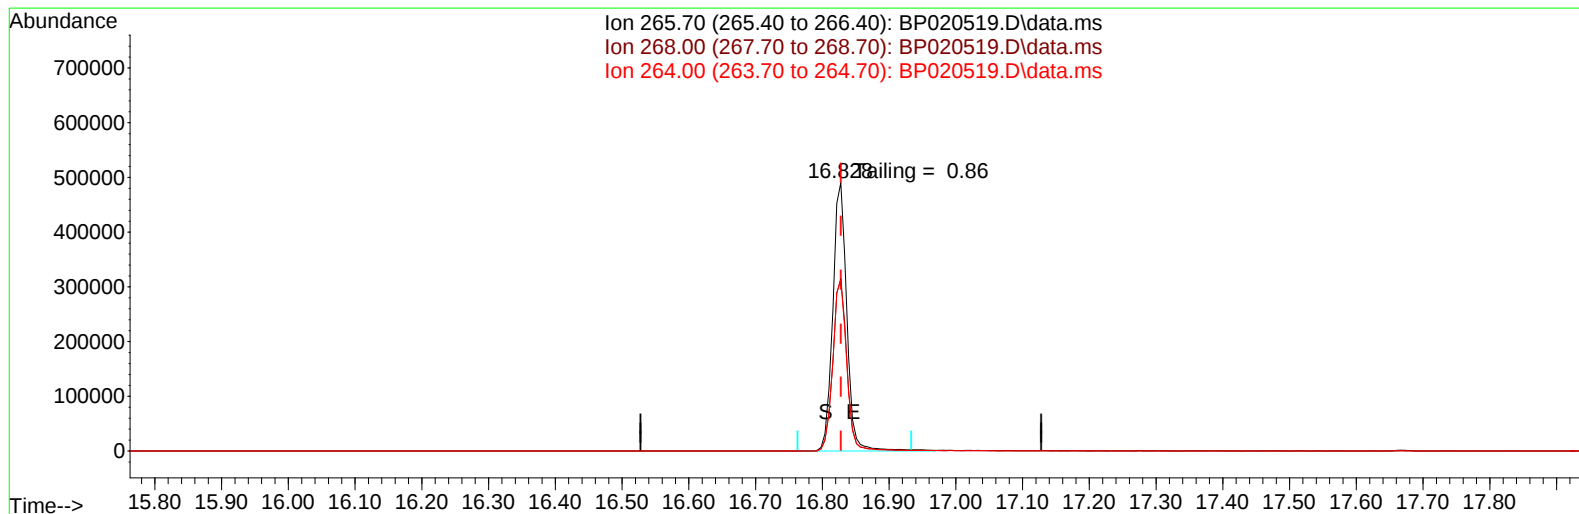

TIC: BP020519.D\data.ms

(70) Pentachlorophenol (C)

16.828min (-0.000) 4896353.71 ng




response 716116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.14
264.00	63.30	63.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060524\
Data File : BP020519.D
Acq On : 05 Jun 2024 15:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 05 16:33:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

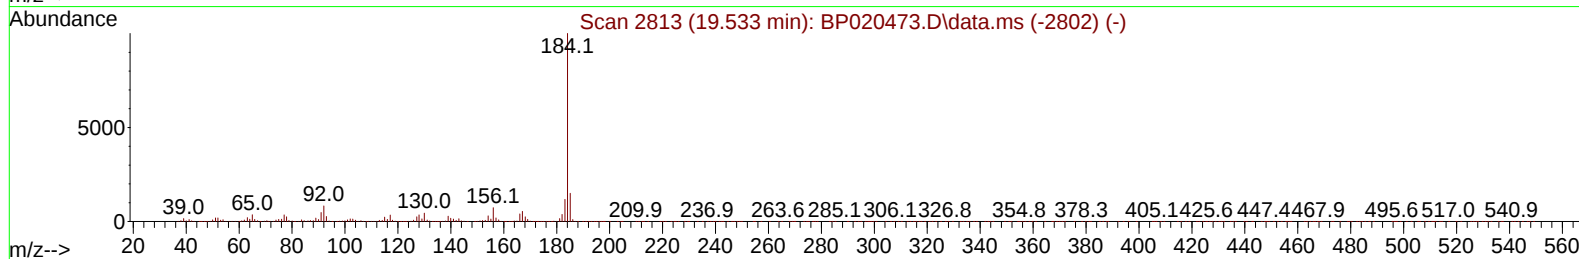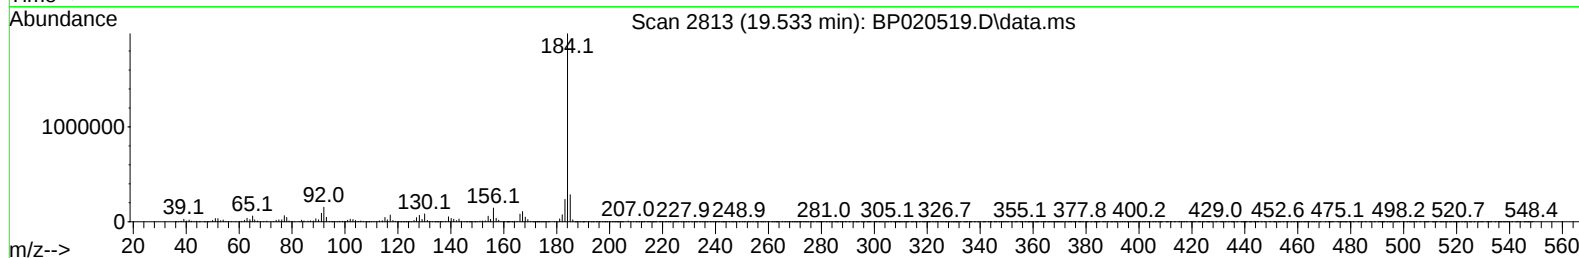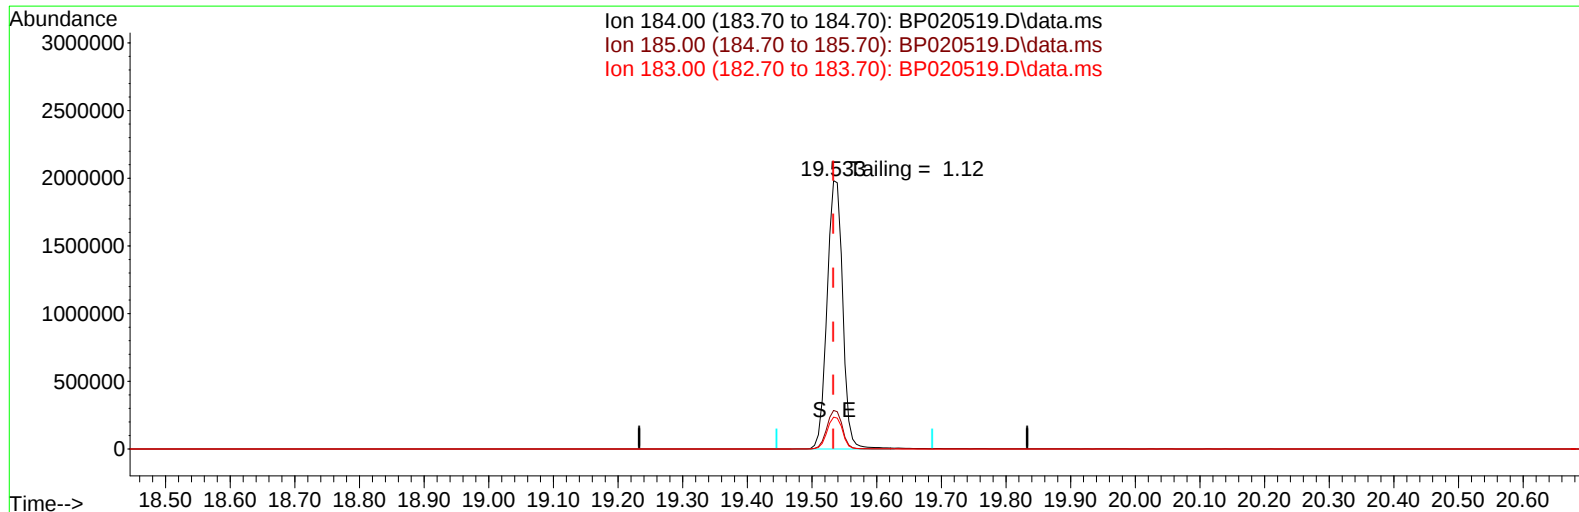

TIC: BP020519.D\data.ms

(77) Benzidine

19.533min (+ 0.000) 1211169.00 ng

response 3343978

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.40
183.00	11.70	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/5/2024	BNA_P	<u>BP020516.D</u>
Compound Name	Response	Retention Time
DDT	1641028	20.827
DDD	29340	20.369
DDE	2682	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32022	1673050	1.91

Instrument :
BNA_P
ClientSampleId :
DFTPP