

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060622\
Data File : BP010702.D
Acq On : 06 Jun 2022 13:57
Operator : CG/JU
Sample : PB145261BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145261BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	392	399	417	rBV	2111367	3190722	31.40%	8.727%
2	7.028	662	670	685	rBV	2171381	3572506	35.15%	9.771%
3	7.846	799	809	820	rBV	302877	515397	5.07%	1.410%
4	9.011	992	1007	1026	rBV	1285200	2283263	22.47%	6.245%
5	10.652	1279	1286	1300	rBV	409260	776202	7.64%	2.123%
6	13.110	1696	1704	1722	rBV	3481785	5237191	51.53%	14.324%
7	14.487	1930	1938	1954	rBV	718143	1131877	11.14%	3.096%
8	15.981	2184	2192	2214	rBV	3128285	4660025	45.85%	12.745%
9	17.245	2400	2407	2418	rBV	950380	1479139	14.55%	4.045%
10	19.804	2836	2842	2847	rBV	8938265	10162656	100.00%	27.795%
11	21.333	3097	3102	3111	rBV	1379455	1793980	17.65%	4.907%
12	23.739	3505	3511	3524	rVB2	826144	1759708	17.32%	4.813%




Sum of corrected areas: 36562666

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060622\
Data File : BP010702.D
Acq On : 06 Jun 2022 13:57
Operator : CG/JU
Sample : PB145261BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145261BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

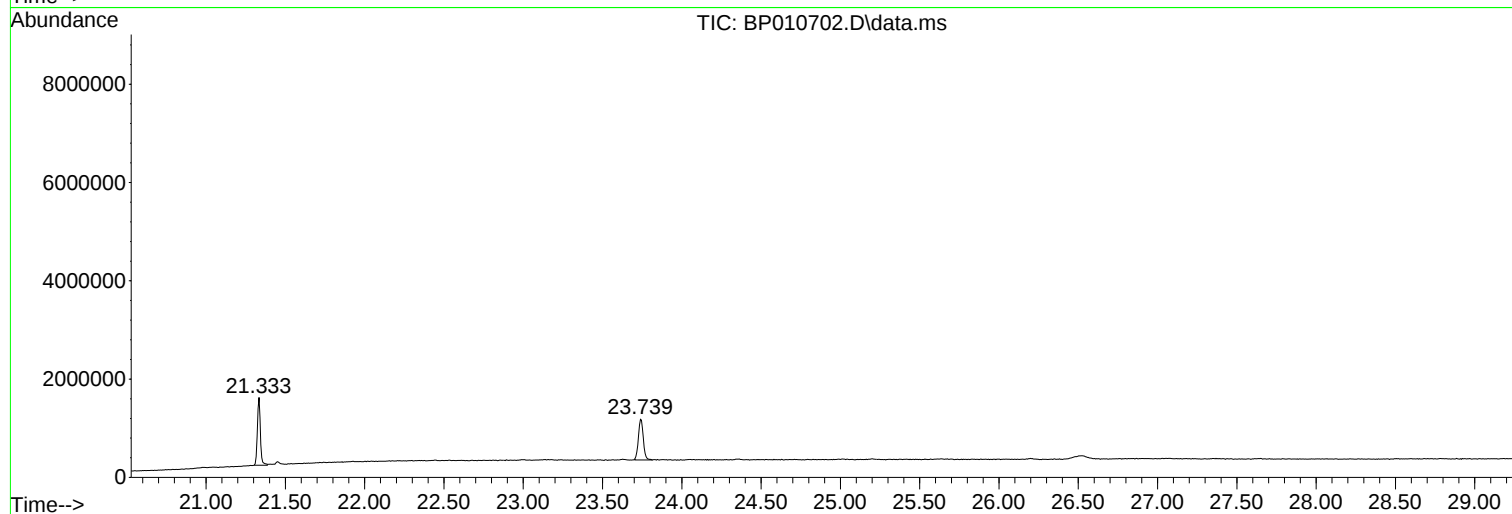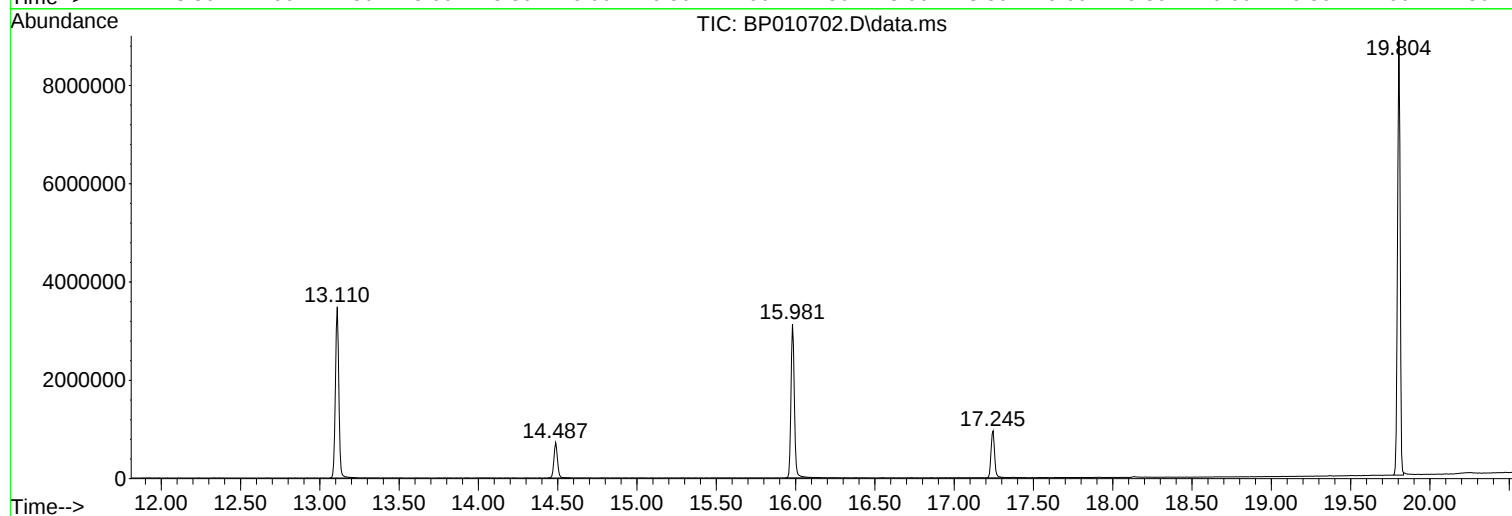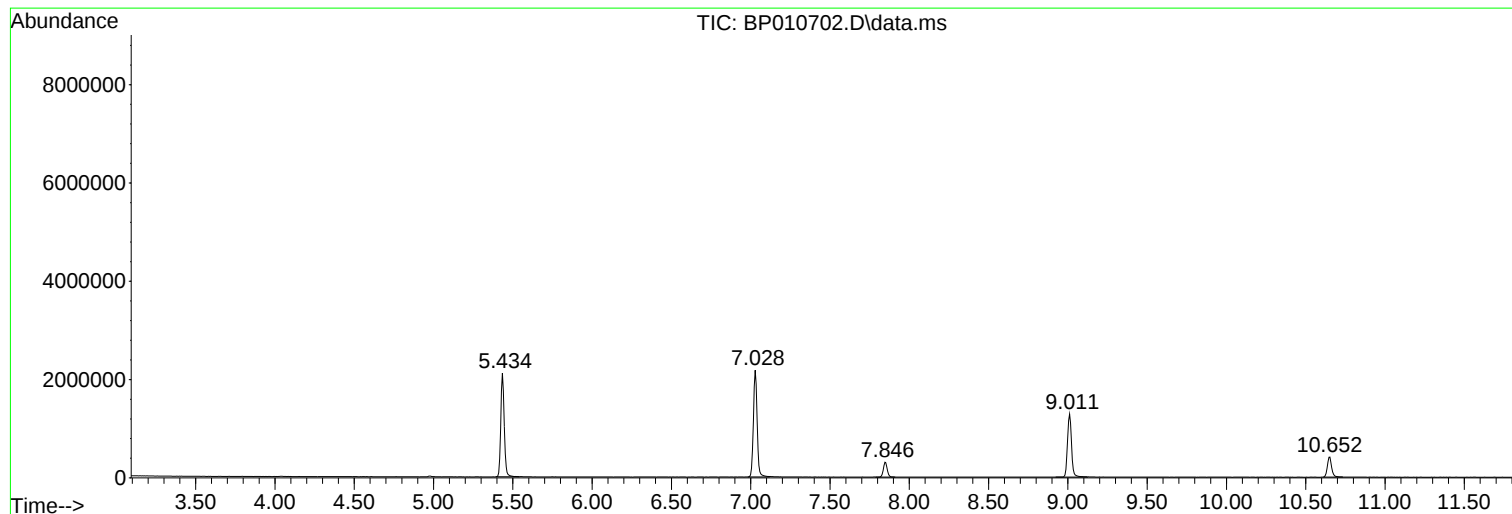

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060622\
Data File : BP010702.D
Acq On : 06 Jun 2022 13:57
Operator : CG/JU
Sample : PB145261BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145261BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060622\
Data File : BP010702.D
Acq On : 06 Jun 2022 13:57
Operator : CG/JU
Sample : PB145261BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145261BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------