


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060622\
Data File : BP010700.D
Acq On : 06 Jun 2022 12:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 06 15:39:44 2022

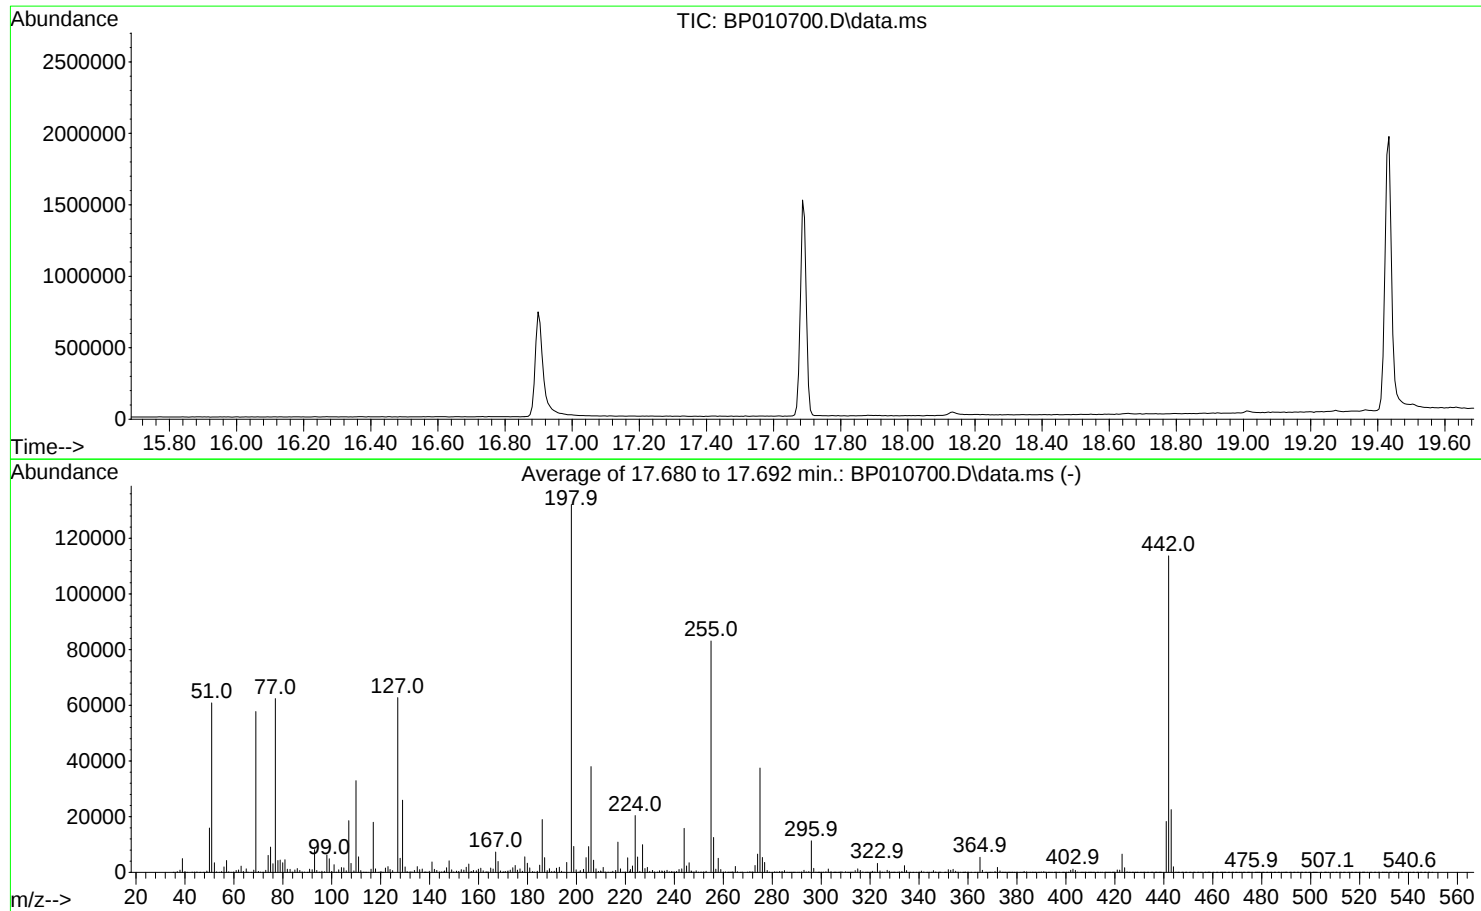


AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	60867	PASS
68	69	0.00	2	1.4	785	PASS
69	198	0.00	100	43.7	57785	PASS
70	69	0.00	2	0.6	349	PASS
127	198	10	80	47.5	62741	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	132130	PASS
199	198	5	9	7.1	9339	PASS
275	198	10	60	28.4	37474	PASS
365	198	1	100	4.1	5431	PASS
441	198	0.01	100	13.8	18295	PASS
442	442	100	100	100.0	113692	PASS
443	442	15	24	19.8	22507	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060622\
 Data File : BP010700.D
 Acq On : 06 Jun 2022 12:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 06 15:32:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 04 01:56:43 2022
 Response via : Initial Calibration

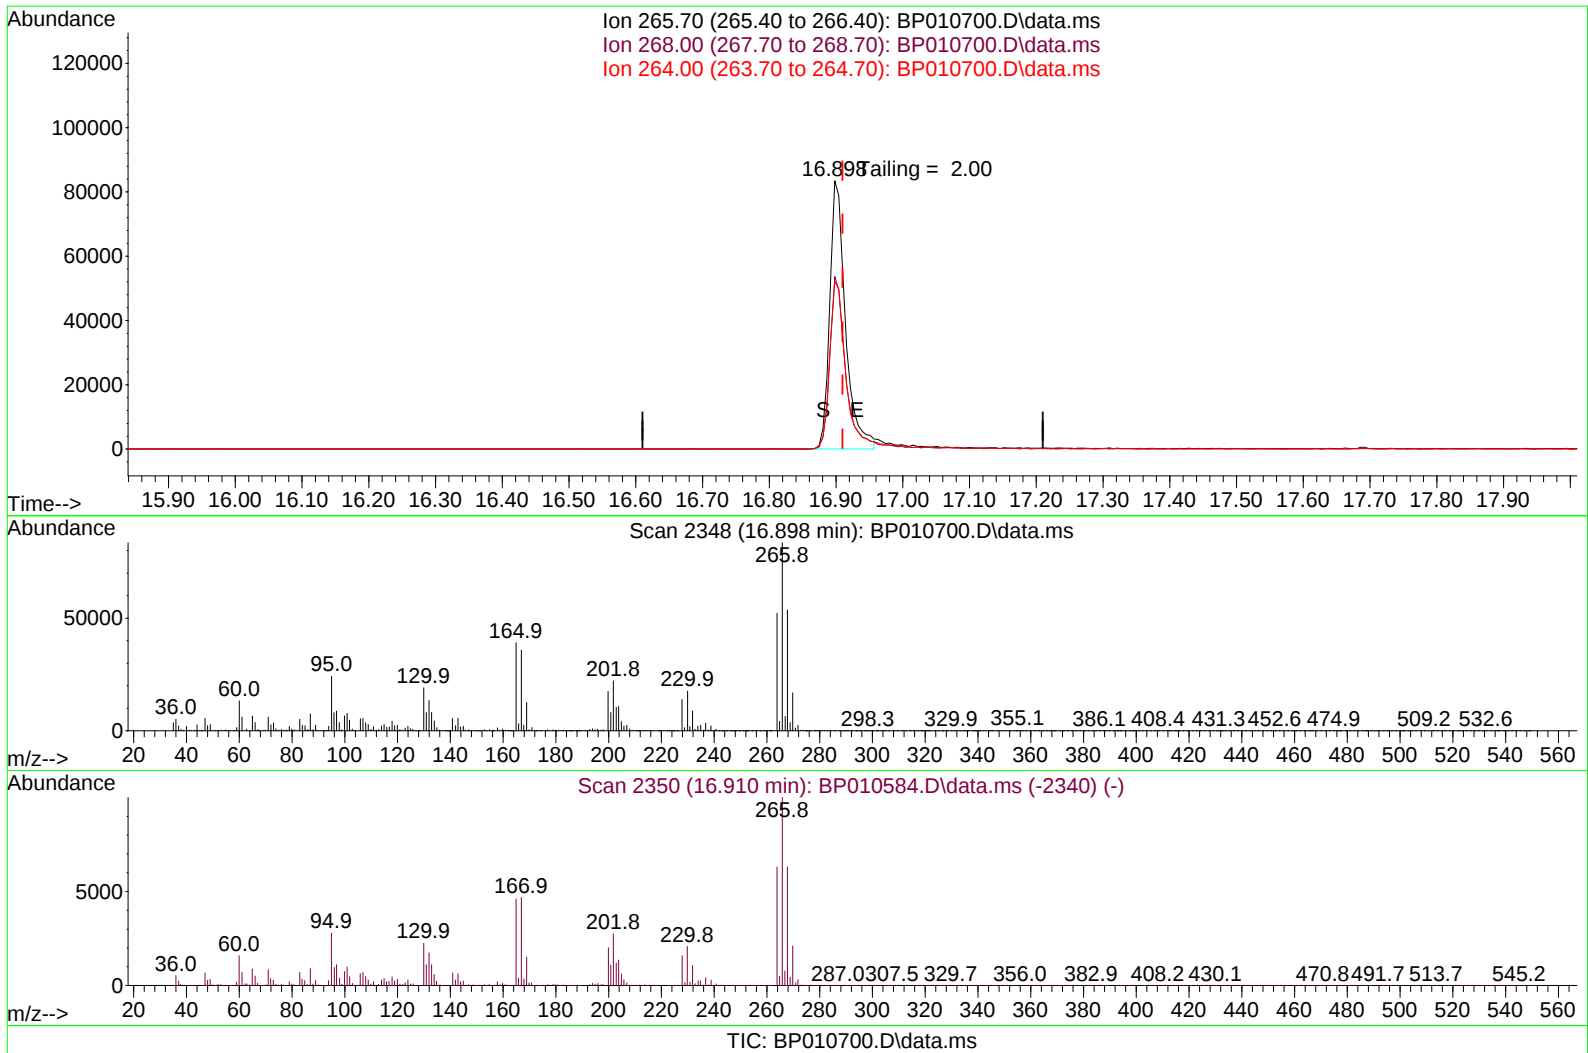

(70) Pentachlorophenol (C)

16.898min (-0.012) 899207.70 ng




response 142659

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.30
264.00	63.00	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060622\
Data File : BP010700.D
Acq On : 06 Jun 2022 12:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 06 15:32:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 01:56:43 2022
Response via : Initial Calibration

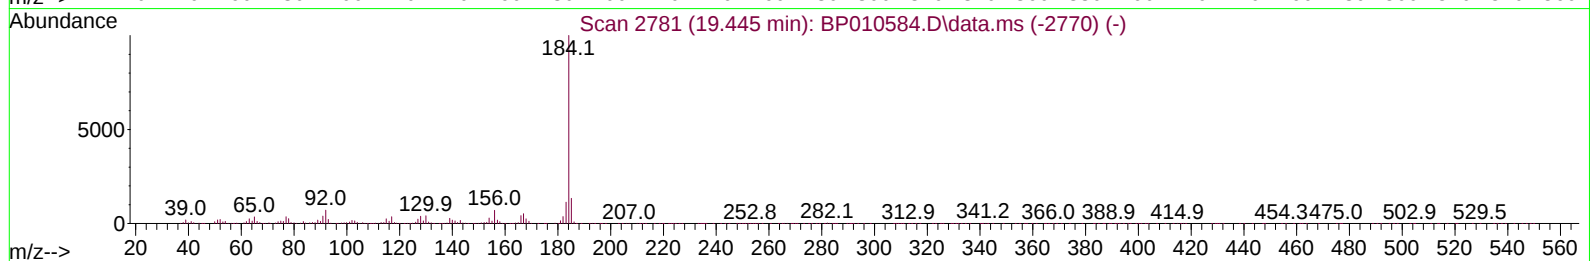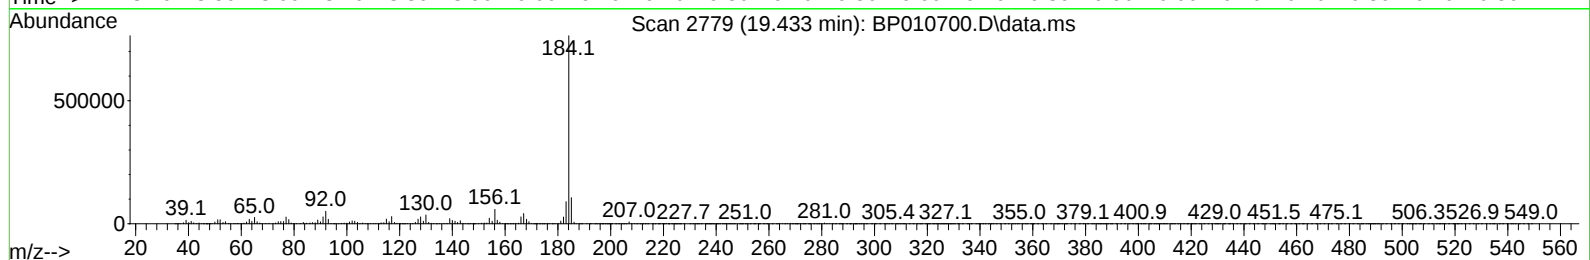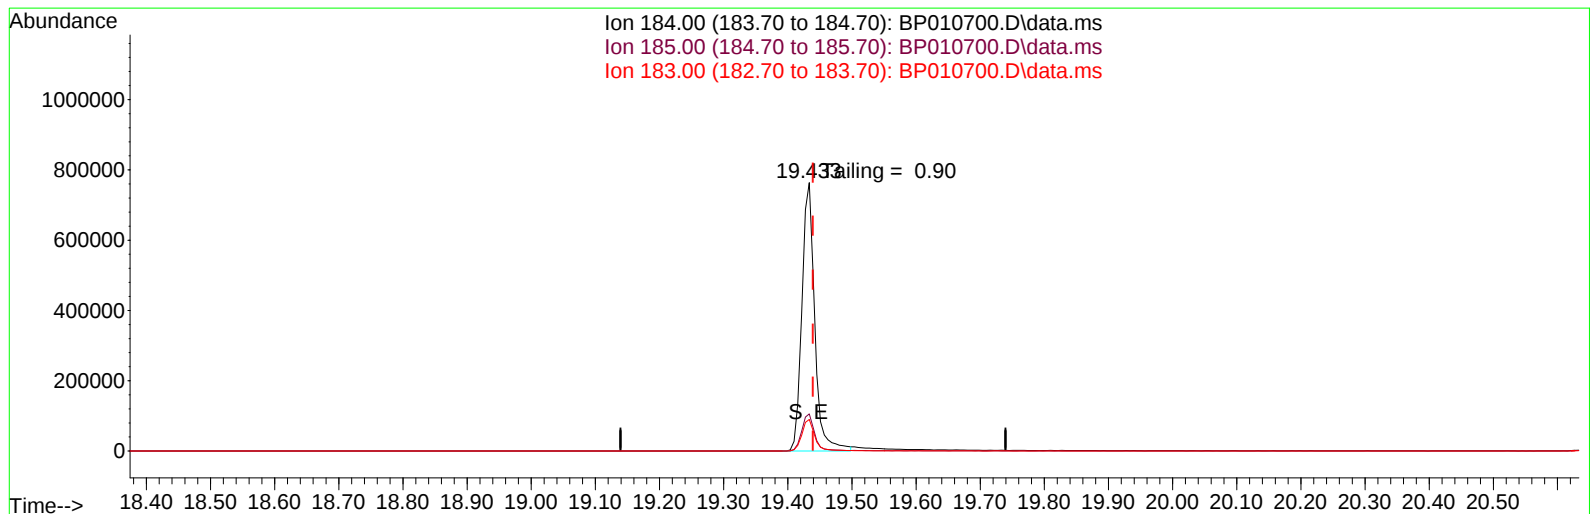

TIC: BP010700.D\data.ms

(77) Benzidine

19.433min (-0.006) 342921.65 ng

response 1106667

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.84
183.00	11.30	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/7/2022	BNA_P	<u>BP010700.D</u>
Compound Name	Response	Retention Time
DDT	536445	20.63
DDD	12070	20.2
DDE	2066	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14136	550581	2.57

Instrument :
BNA_P
ClientSampleId :
DFTPP