

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060624\
Data File : BP020538.D
Acq On : 06 Jun 2024 12:14
Operator : MA/JU
Sample : PB161260BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB161260BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP020538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	4	9	14	rVB	186264	224467	1.52%	0.285%
2	5.381	400	407	423	rBV	6157821	8923738	60.48%	11.321%
3	6.940	664	672	684	rBV	5433997	8923764	60.48%	11.321%
4	7.769	805	813	822	rBV	1193317	1938514	13.14%	2.459%
5	8.916	1000	1008	1025	rBV	3288047	5851391	39.65%	7.423%
6	10.534	1275	1283	1298	rBV	1460019	2620056	17.76%	3.324%
7	12.993	1694	1701	1718	rBV	7811686	12819339	86.88%	16.263%
8	14.387	1931	1938	1948	rBV	2246134	3364130	22.80%	4.268%
9	15.904	2188	2196	2215	rBV	5634373	8943534	60.61%	11.346%
10	17.198	2408	2416	2428	rBV	2638997	3802439	25.77%	4.824%
11	19.939	2876	2882	2893	rBV	11455072	14755746	100.00%	18.720%
12	21.645	3166	3172	3179	rBV2	1927224	3179051	21.54%	4.033%
13	25.010	3736	3744	3761	rVB	1290469	3477031	23.56%	4.411%




Sum of corrected areas: 78823200

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060624\
Data File : BP020538.D
Acq On : 06 Jun 2024 12:14
Operator : MA/JU
Sample : PB161260BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB161260BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

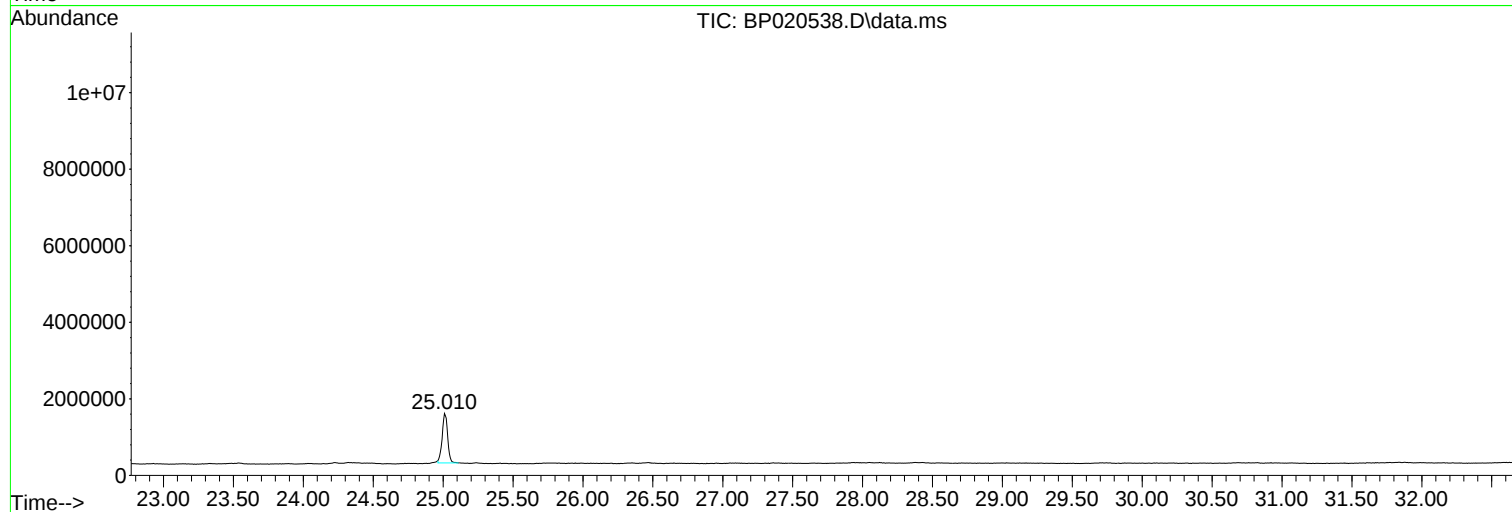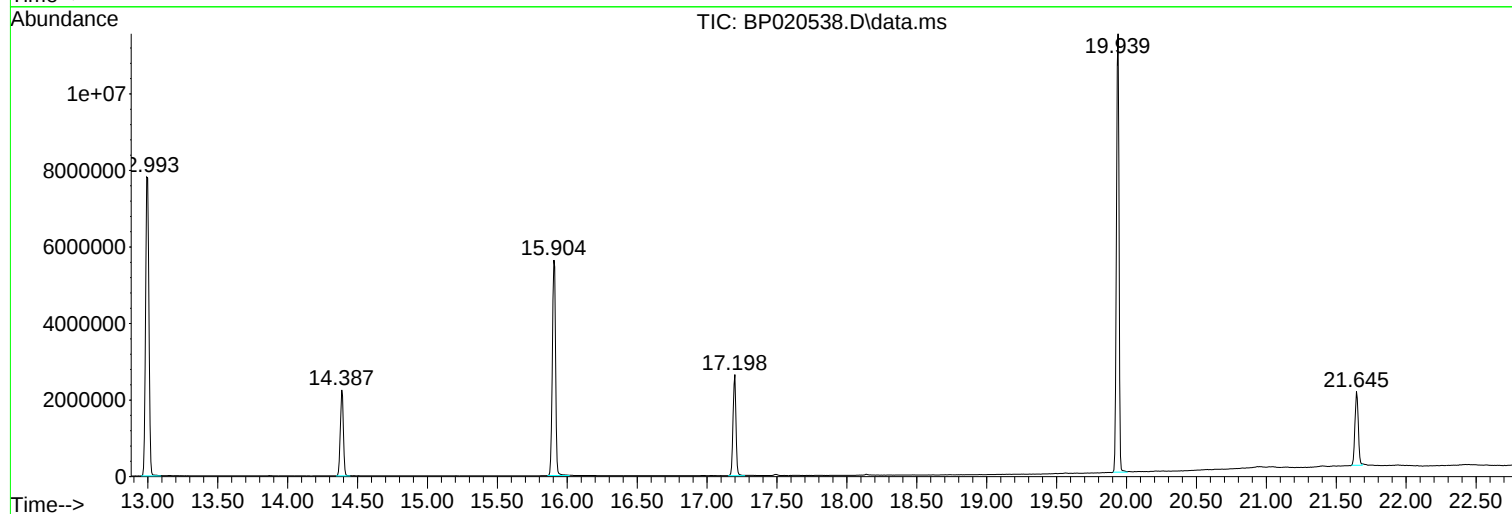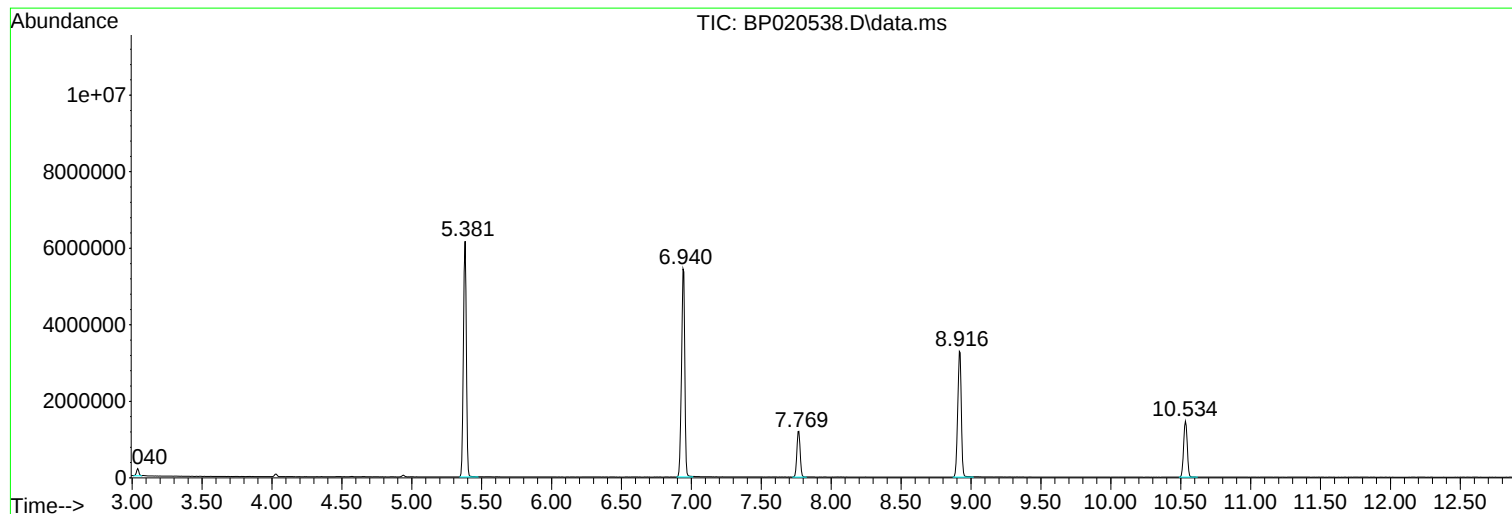

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060624\
Data File : BP020538.D
Acq On : 06 Jun 2024 12:14
Operator : MA/JU
Sample : PB161260BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB161260BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.040	2.32 ng	224467	1,4-Dichlorobenzene-d4	7.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Butanoic acid, 2-hydroxy-2-methyl...	132	C6H12O3	032793-34-3	23
4			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	17
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	14

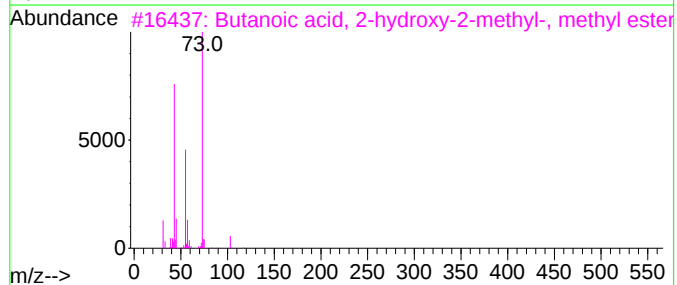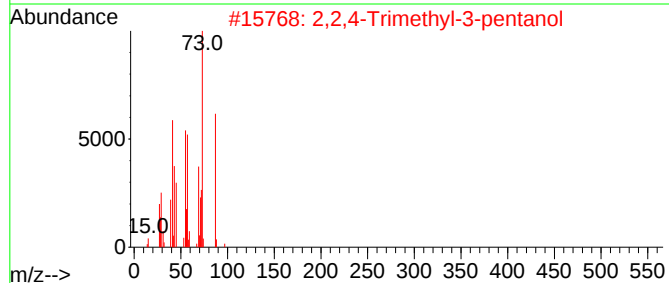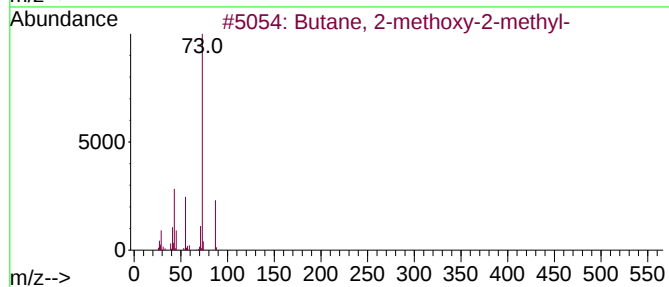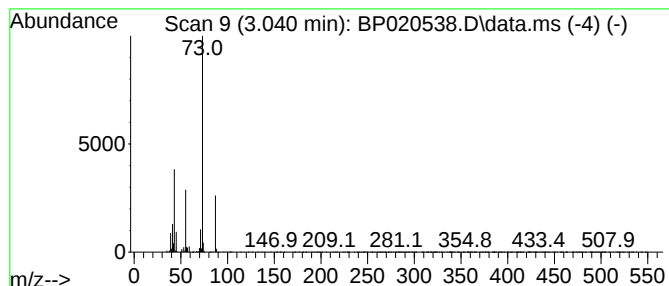

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060624\
Data File : BP020538.D
Acq On : 06 Jun 2024 12:14
Operator : MA/JU
Sample : PB161260BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB161260BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.040	2.3	ng	224467	1	7.769	1938510	20.0