
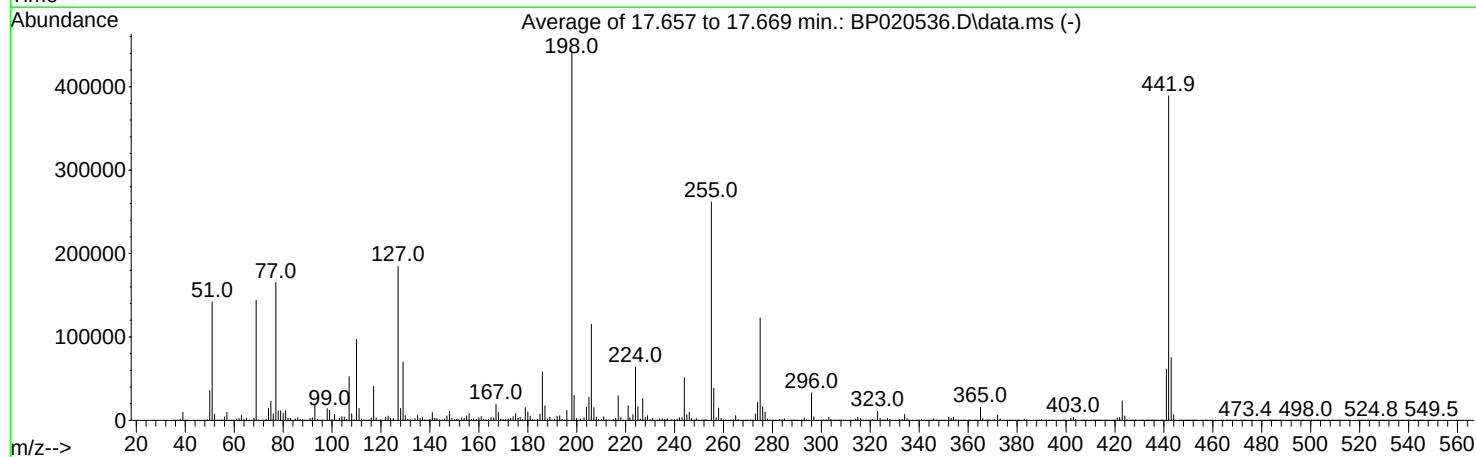


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060624\
Data File : BP020536.D
Acq On : 06 Jun 2024 10:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

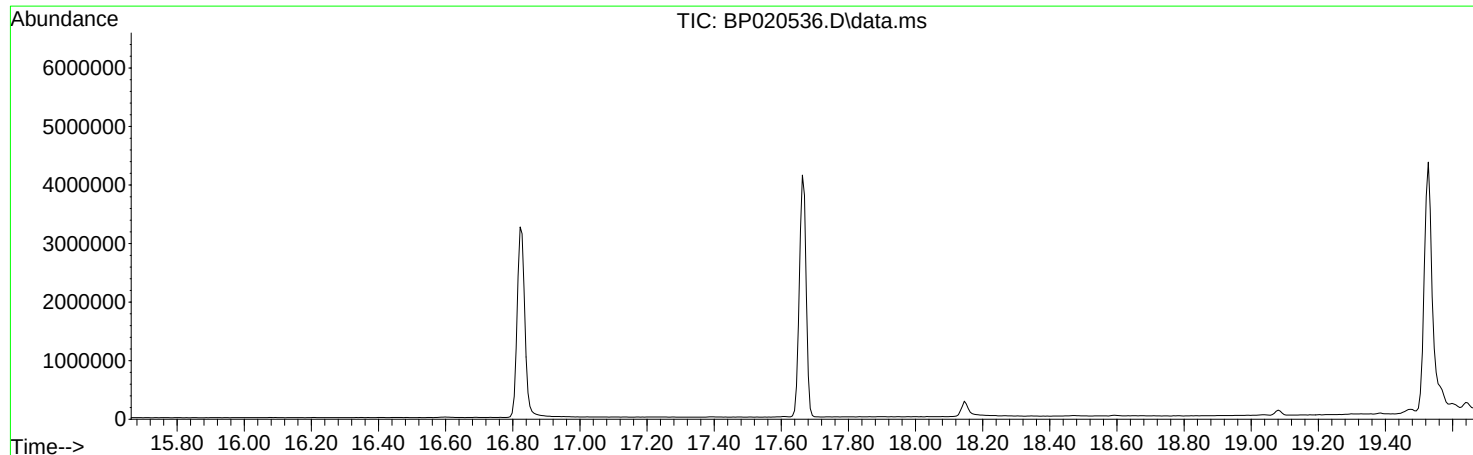

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	142192	PASS
68	69	0.00	2	1.8	2662	PASS
69	198	0.00	100	32.7	144107	PASS
70	69	0.00	2	0.5	674	PASS
127	198	10	80	41.8	184562	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	441010	PASS
199	198	5	9	6.8	29869	PASS
275	198	10	60	27.8	122699	PASS
365	198	1	100	3.6	15821	PASS
441	198	0.01	100	14.0	61675	PASS
442	442	100	100	100.0	389111	PASS
443	442	15	24	19.3	75197	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
6/6/2024	BNA_P	<u>BP020536.D</u>
Compound Name	Response	Retention Time
DDT	1657814	20.822
DDD	30225	20.422
DDE	1374	19.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31599	1689413	1.87

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060624\
Data File : BP020536.D
Acq On : 06 Jun 2024 10:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 06 11:41:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

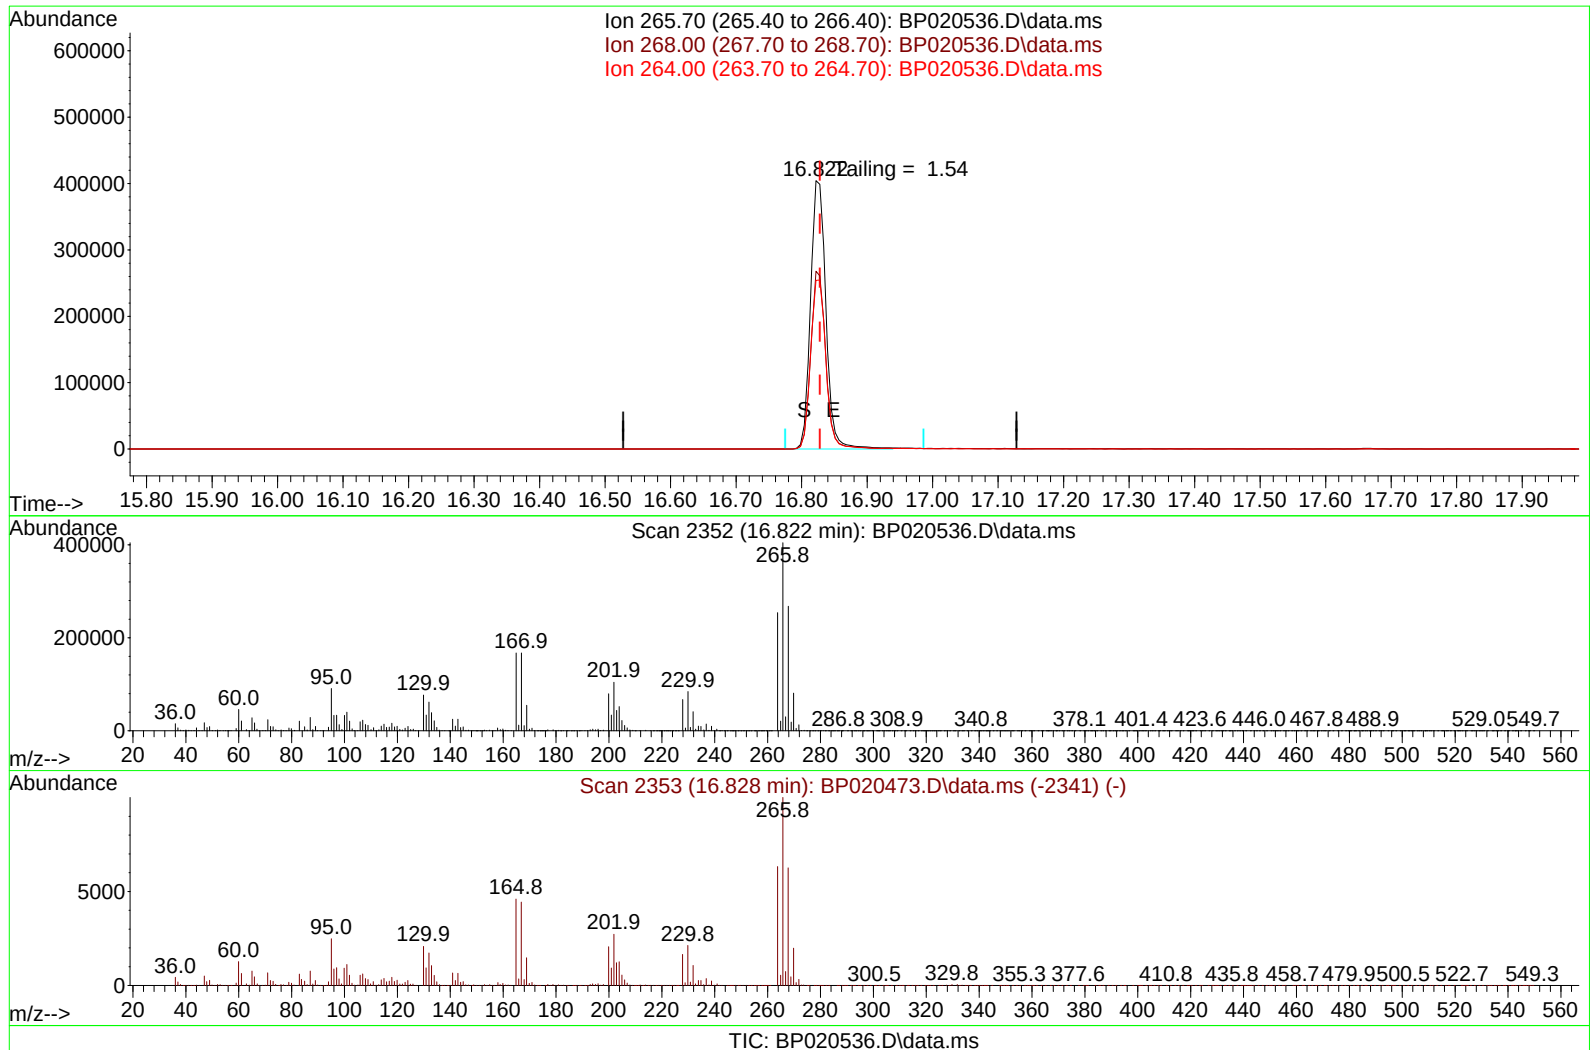

TIC: BP020536.D\data.ms

(70) Pentachlorophenol (C)

16.822min (-0.006) 158330.50 ng m




response 657648

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.24
264.00	63.30	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060624\
Data File : BP020536.D
Acq On : 06 Jun 2024 10:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 06 11:41:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

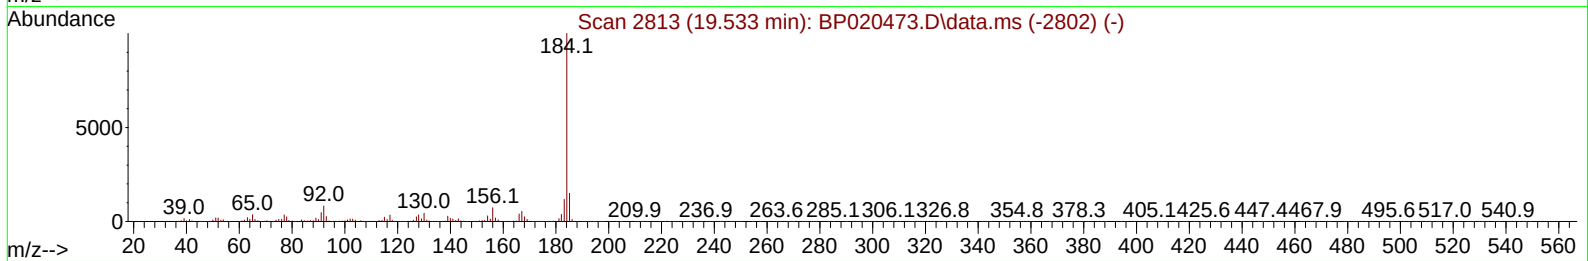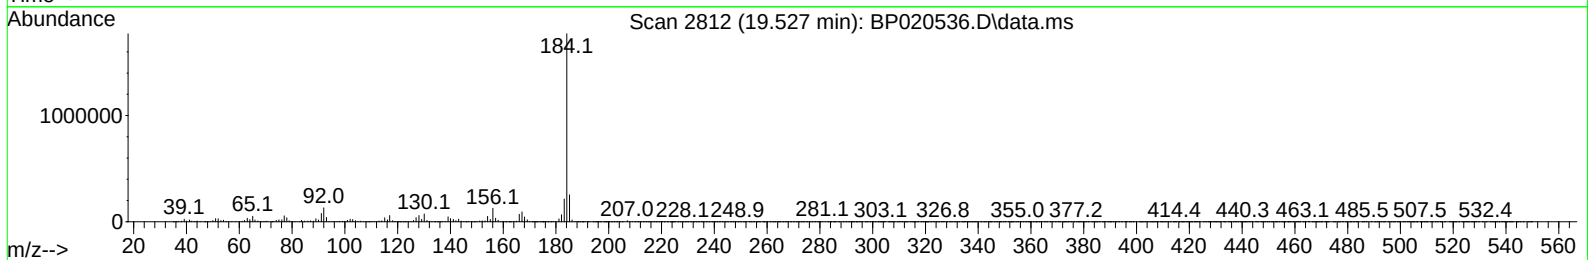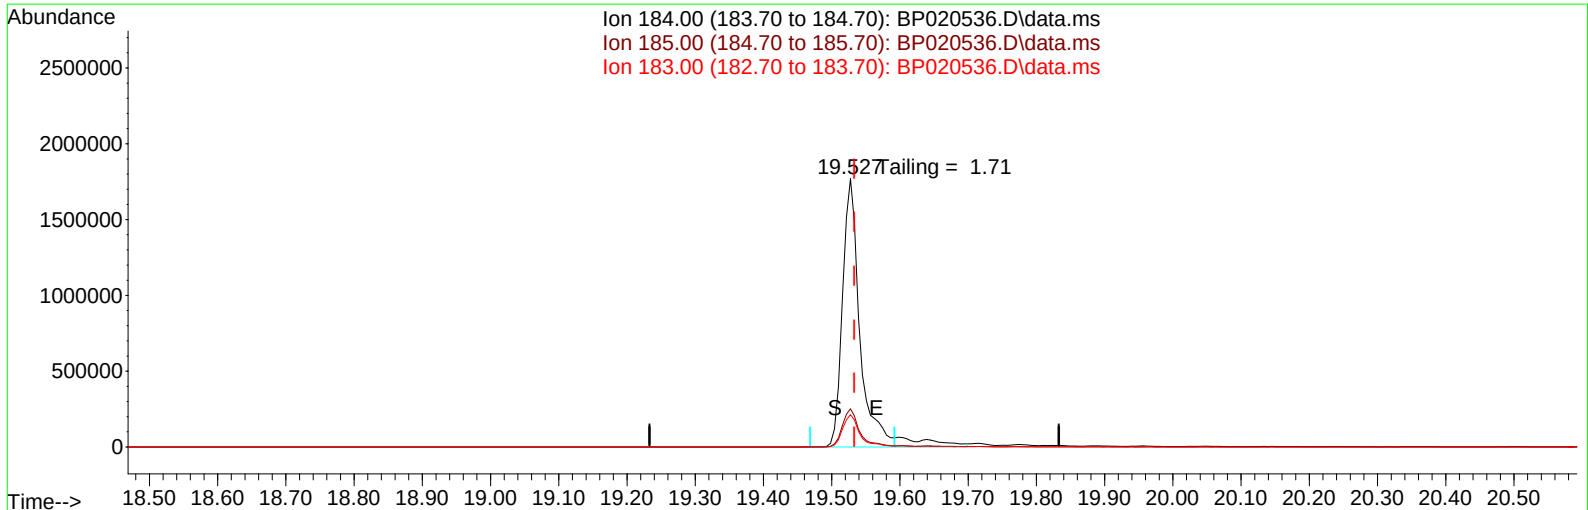

TIC: BP020536.D\data.ms

(77) Benzidine

19.527min (-0.006) 45025.72 ng

response 3112932

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.27
183.00	11.70	12.07
0.00	0.00	0.00