
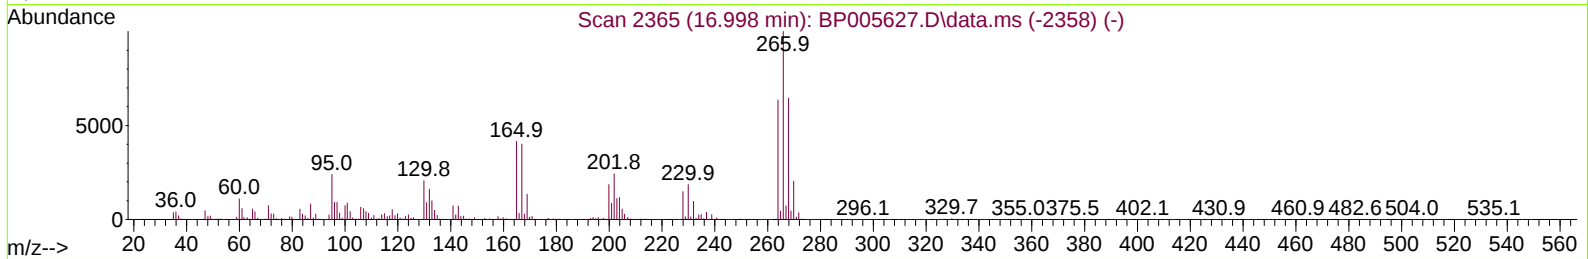
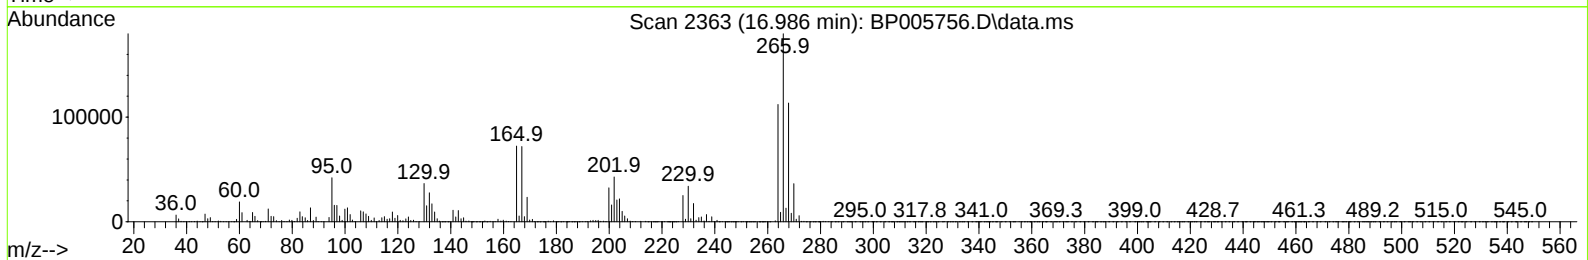


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060721\
 Data File : BP005756.D
 Acq On : 08 Jun 2021 00:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 02:44:57 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 07 12:13:53 2021
 Response via : Initial Calibration

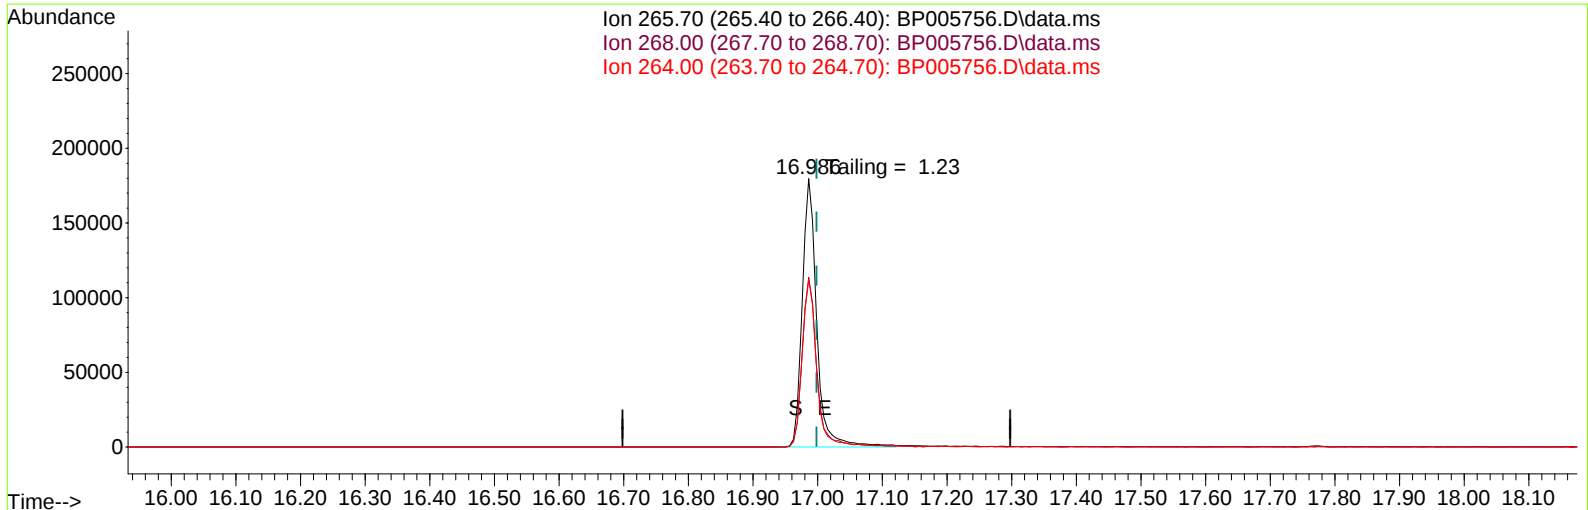

TIC: BP005756.D\data.ms

(70) Pentachlorophenol (C)




16.986min (-0.012) 65845.63 ng

response 283271

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.19
264.00	67.10	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060721\
 Data File : BP005756.D
 Acq On : 08 Jun 2021 00:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 02:44:57 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 07 12:13:53 2021
 Response via : Initial Calibration

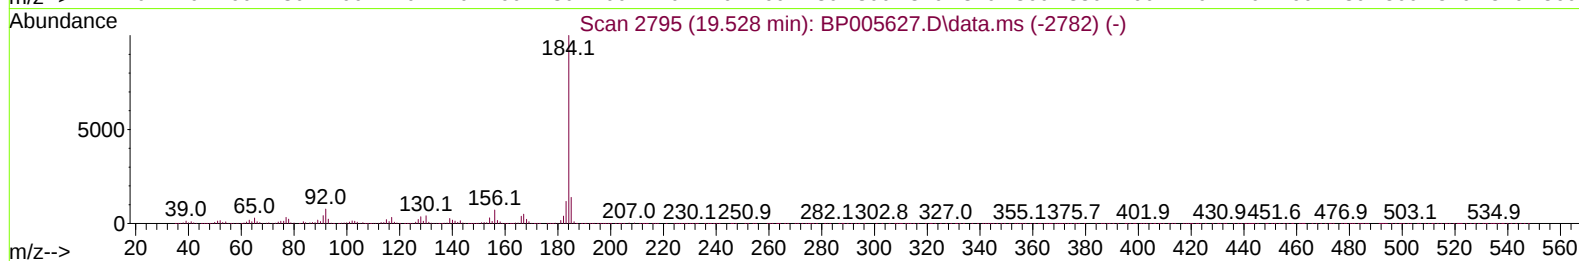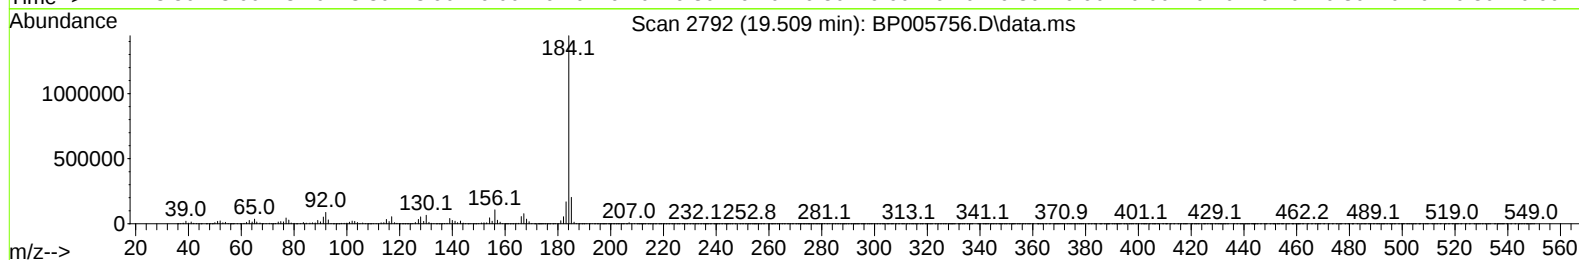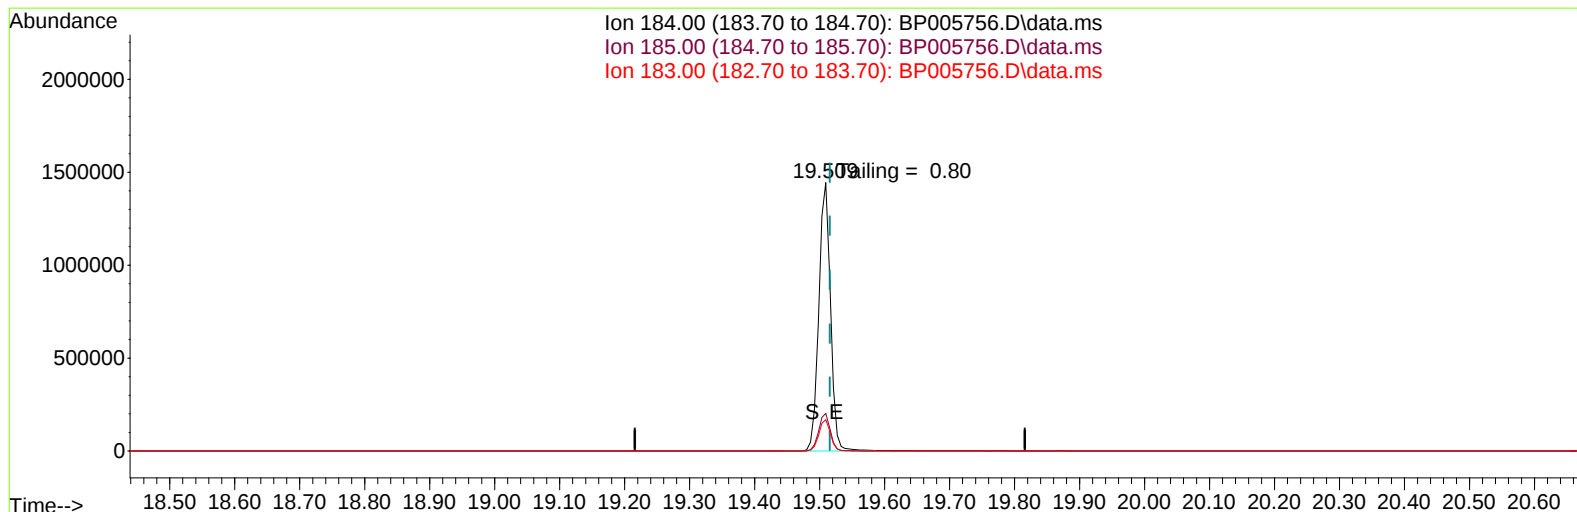

TIC: BP005756.D\data.ms

(77) Benzidine**19.509min (-0.006) 516802.72 ng****response 1815730**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.02
183.00	12.30	11.70
0.00	0.00	0.00