

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060721\
 Data File : BP005758.D
 Acq On : 08 Jun 2021 01:54
 Operator : CG/JU
 Sample : PB136884BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB136884BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.534	406	416	432	rBV	2579334	3872043	40.10%	9.410%
2	7.134	680	688	700	rBV	2409039	3911356	40.51%	9.506%
3	7.969	822	830	838	rBV	524767	846489	8.77%	2.057%
4	9.134	1018	1028	1040	rBV	1539552	2594093	26.86%	6.304%
5	10.775	1298	1307	1317	rBV	691021	1157275	11.98%	2.813%
6	13.222	1715	1723	1737	rBV	4013198	6099430	63.17%	14.823%
7	14.592	1949	1956	1970	rBV	1060178	1562966	16.19%	3.798%
8	16.081	2201	2209	2233	rBV	3246531	4944983	51.21%	12.018%
9	17.333	2415	2422	2434	rBV	1325274	1946598	20.16%	4.731%
10	19.880	2849	2855	2860	rBV	7441009	9656176	100.00%	23.467%
11	21.398	3108	3113	3122	rBV	1774663	2288326	23.70%	5.561%
12	23.827	3519	3526	3537	rVB2	1078883	2267335	23.48%	5.510%




Sum of corrected areas: 41147070

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060721\
Data File : BP005758.D
Acq On : 08 Jun 2021 01:54
Operator : CG/JU
Sample : PB136884BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136884BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

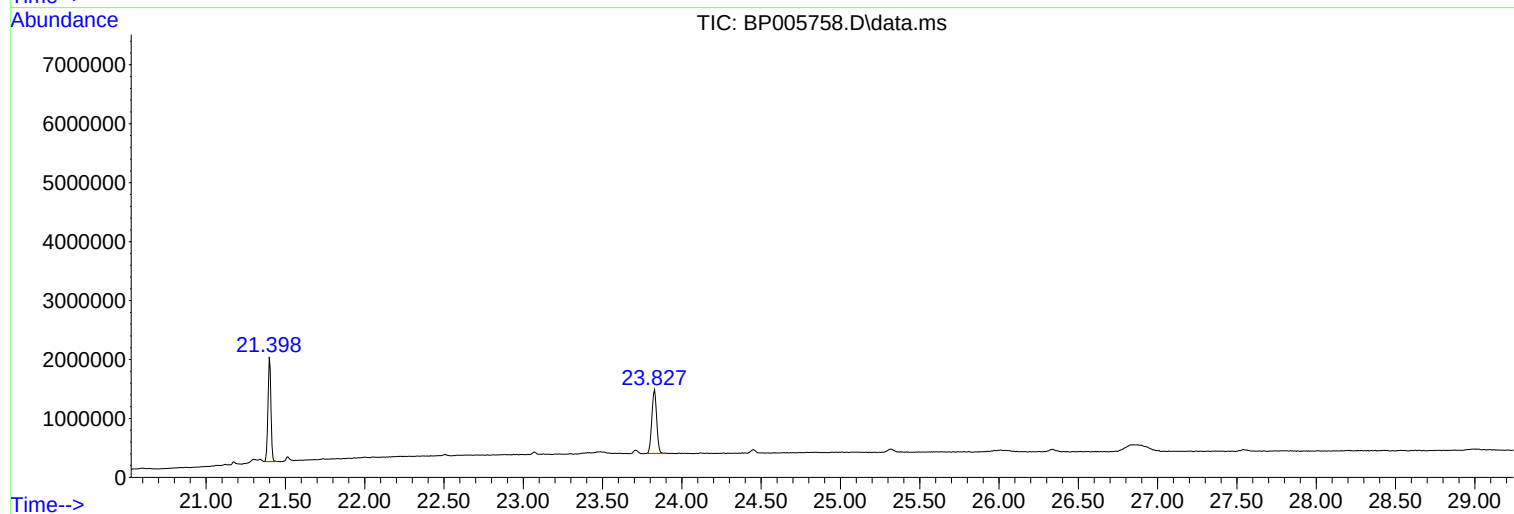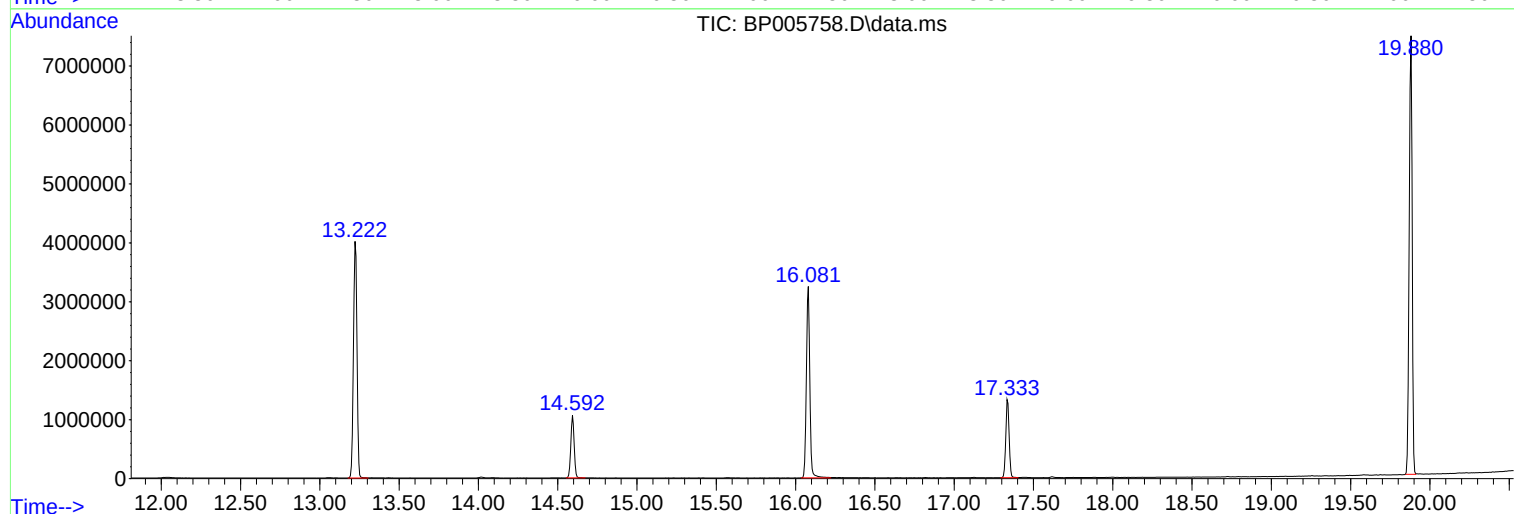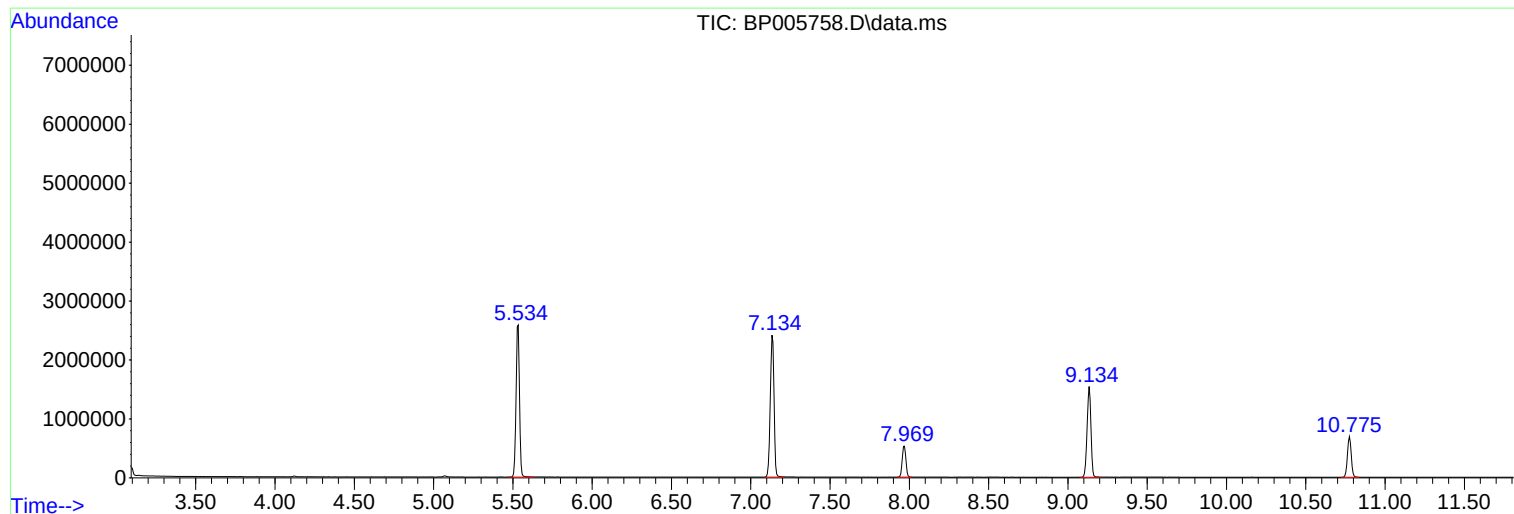

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060721\
Data File : BP005758.D
Acq On : 08 Jun 2021 01:54
Operator : CG/JU
Sample : PB136884BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136884BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060721\
Data File : BP005758.D
Acq On : 08 Jun 2021 01:54
Operator : CG/JU
Sample : PB136884BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136884BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------