
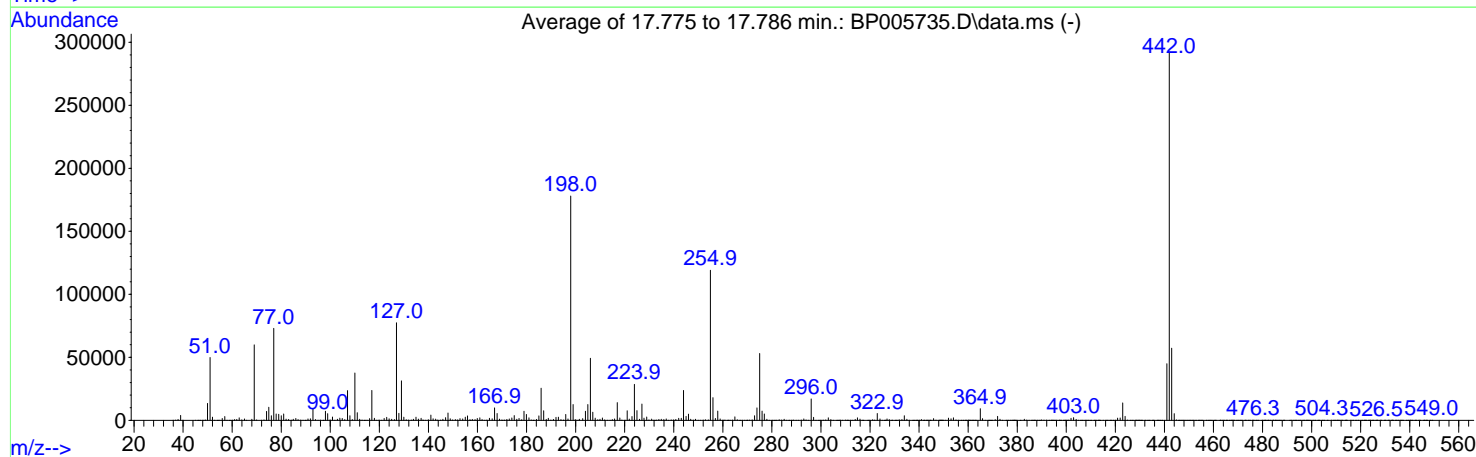


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060721\  
 Data File : BP005735.D  
 Acq On : 07 Jun 2021 10:26  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052721.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jun 07 12:13:53 2021

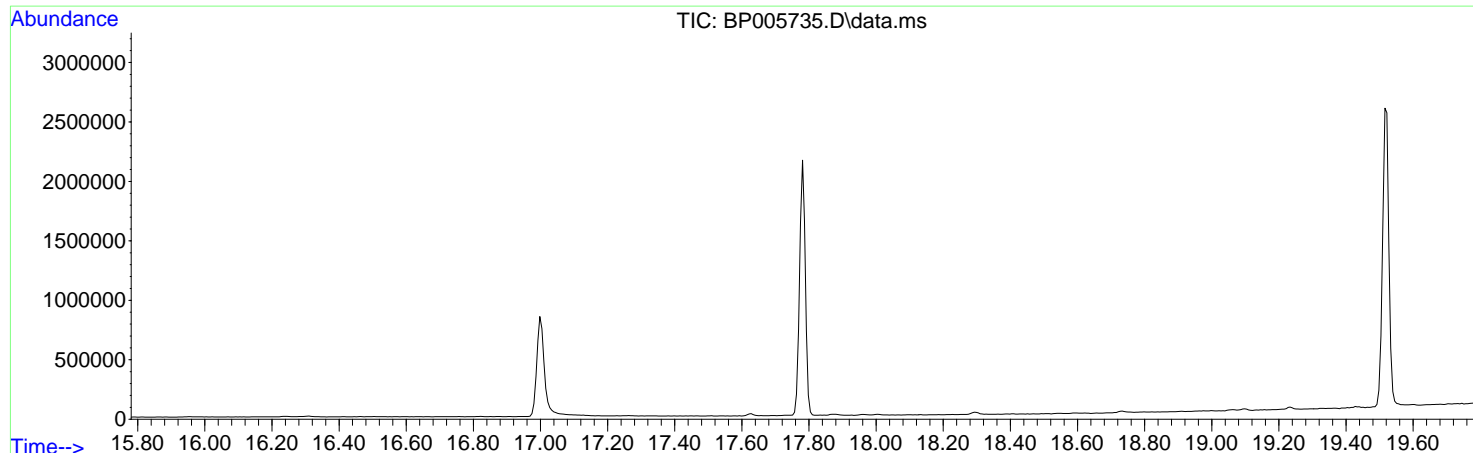




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	49885	PASS
68	69	0.00	2	1.5	917	PASS
69	198	0.00	100	33.7	59947	PASS
70	69	0.00	2	0.6	369	PASS
127	198	10	80	43.5	77420	PASS
197	198	0.00	2	0.6	1117	PASS
198	198	100	100	100.0	177973	PASS
199	198	5	9	7.1	12580	PASS
275	198	10	60	29.8	53072	PASS
365	198	1	100	5.2	9335	PASS
441	198	0.01	100	25.3	44968	PASS
442	442	100	100	100.0	291861	PASS
443	442	15	24	19.6	57311	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060721\  
 Data File : BP005735.D  
 Acq On : 07 Jun 2021 10:26  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_P  
**ClientSampleId :**  
 DFTPP

Quant Time: Jun 07 12:05:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052721.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu May 27 16:11:11 2021  
 Response via : Initial Calibration

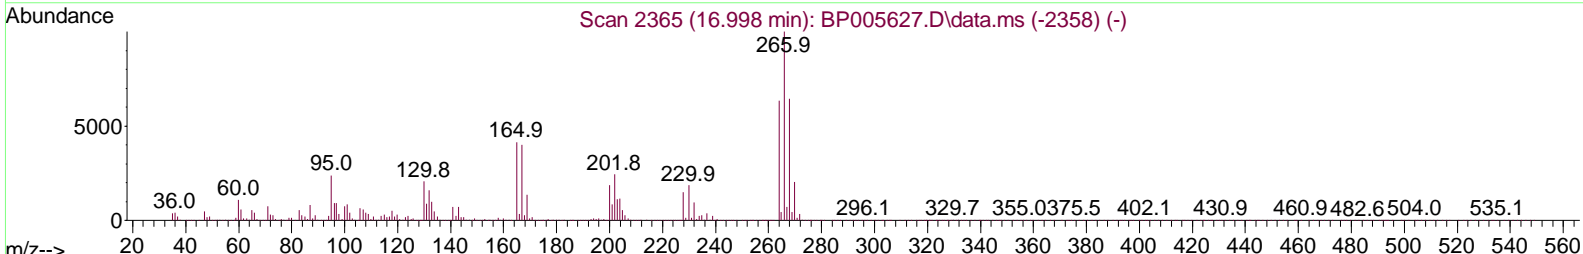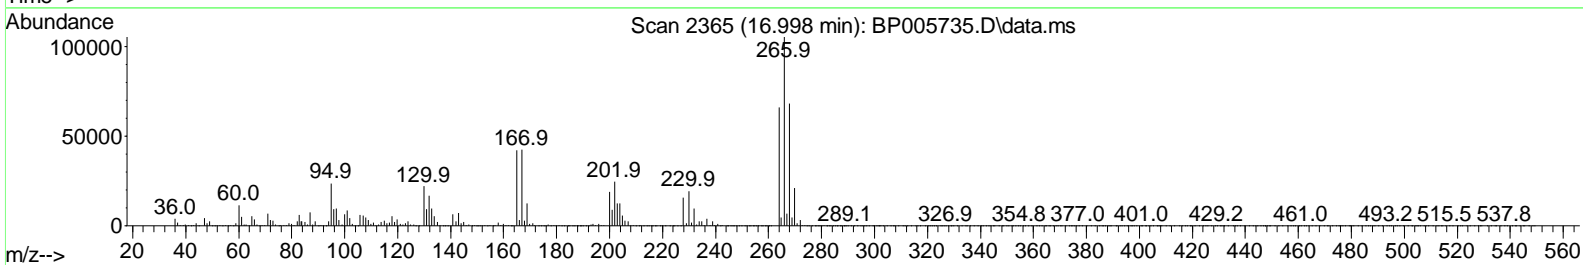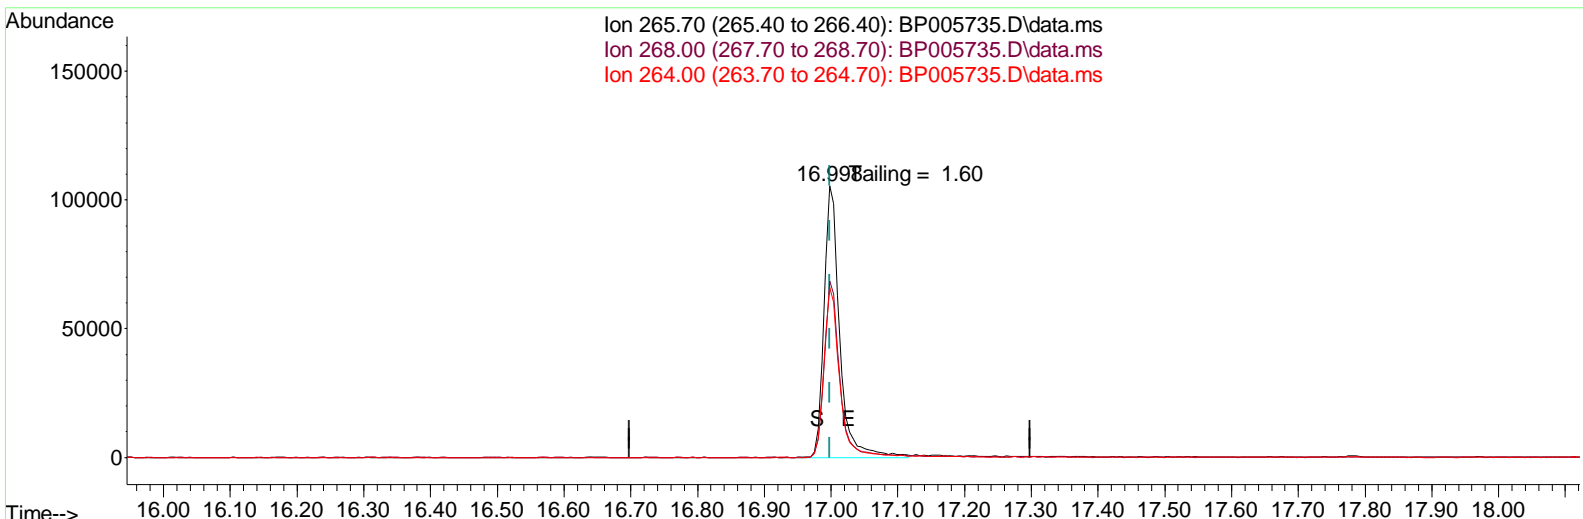

TIC: BP005735.D\data.ms

(70) Pentachlorophenol (C)

16.998min (-0.000) 890868.85 ng




response 173042

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	64.85
264.00	67.10	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060721\  
 Data File : BP005735.D  
 Acq On : 07 Jun 2021 10:26  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_P  
**ClientSampleId :**  
 DFTPP

Quant Time: Jun 07 12:05:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052721.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu May 27 16:11:11 2021  
 Response via : Initial Calibration

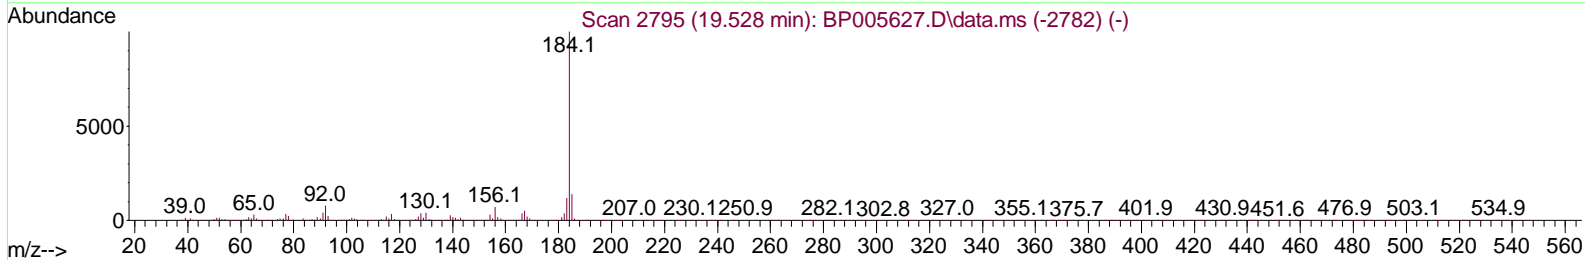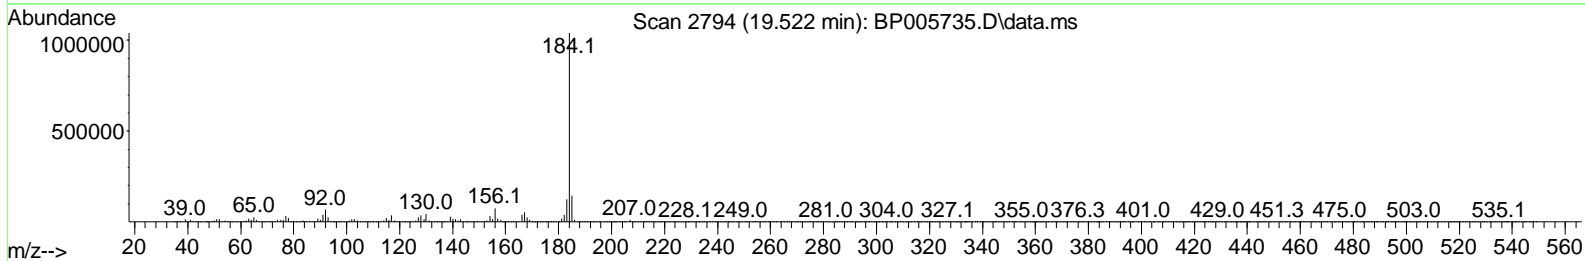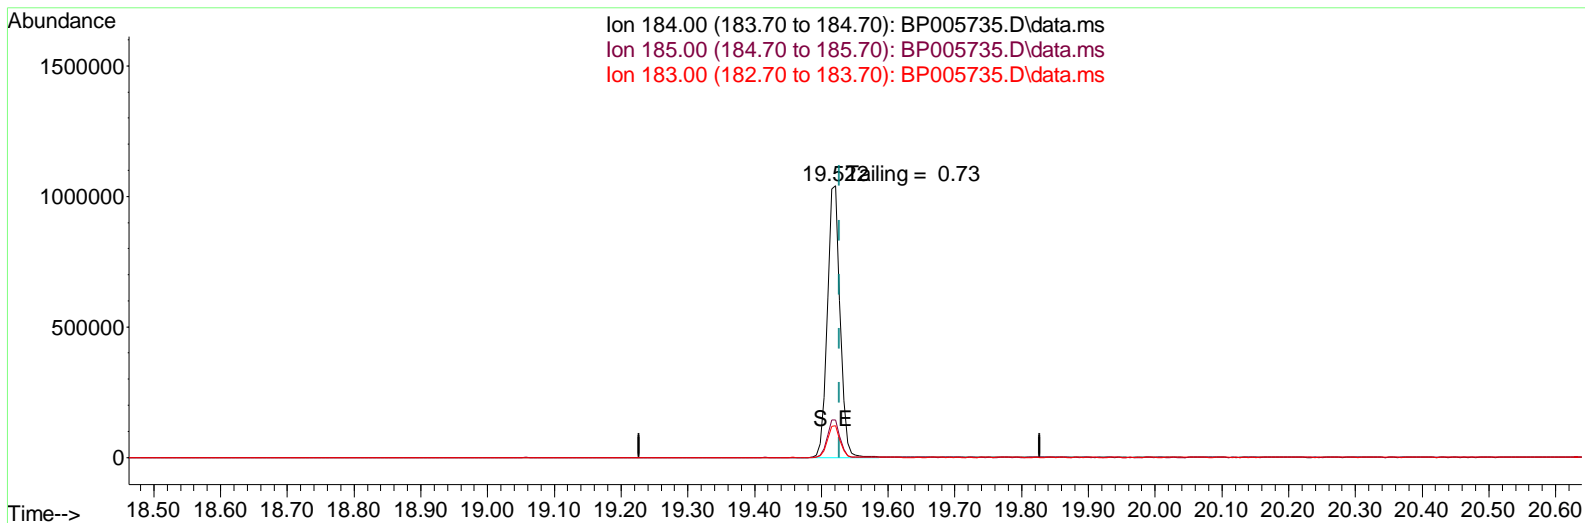

TIC: BP005735.D\data.ms

(77) Benzidine

19.522min (-0.006) 330243.28 ng

response 1379785

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.88
183.00	12.30	11.80
0.00	0.00	0.00

### DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/7/2021	BNA_P	BP005735.D
Compound Name	Response	Retention Time
DDT	665839	20.716
DDD	1551	20.292
DDE	1673	19.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3224	669063	0.48

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP