
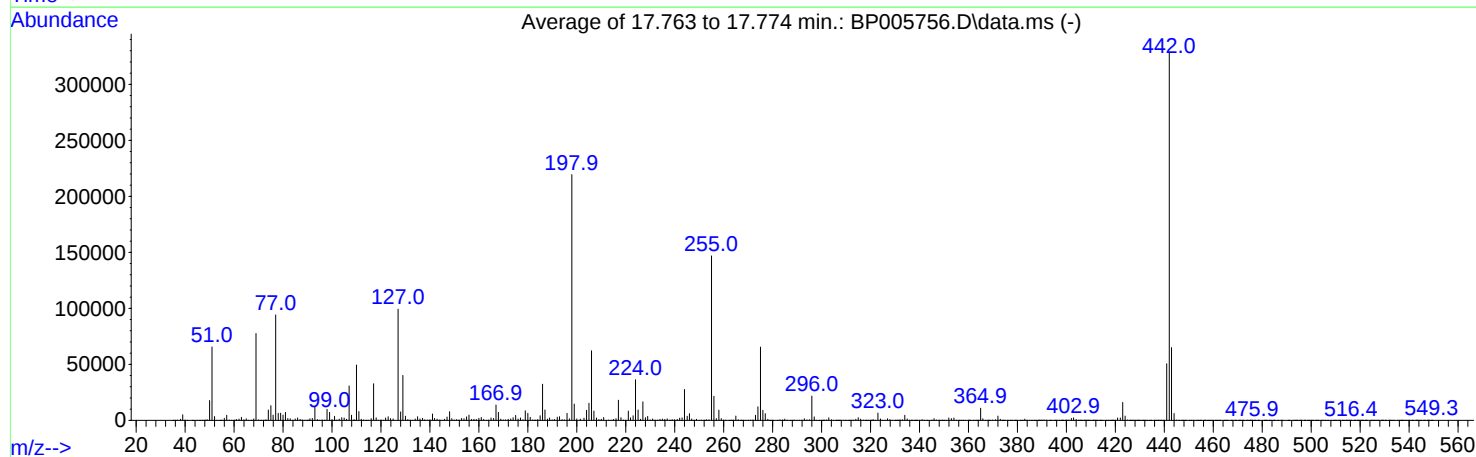


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060721\
 Data File : BP005756.D
 Acq On : 08 Jun 2021 00:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 07 12:13:53 2021

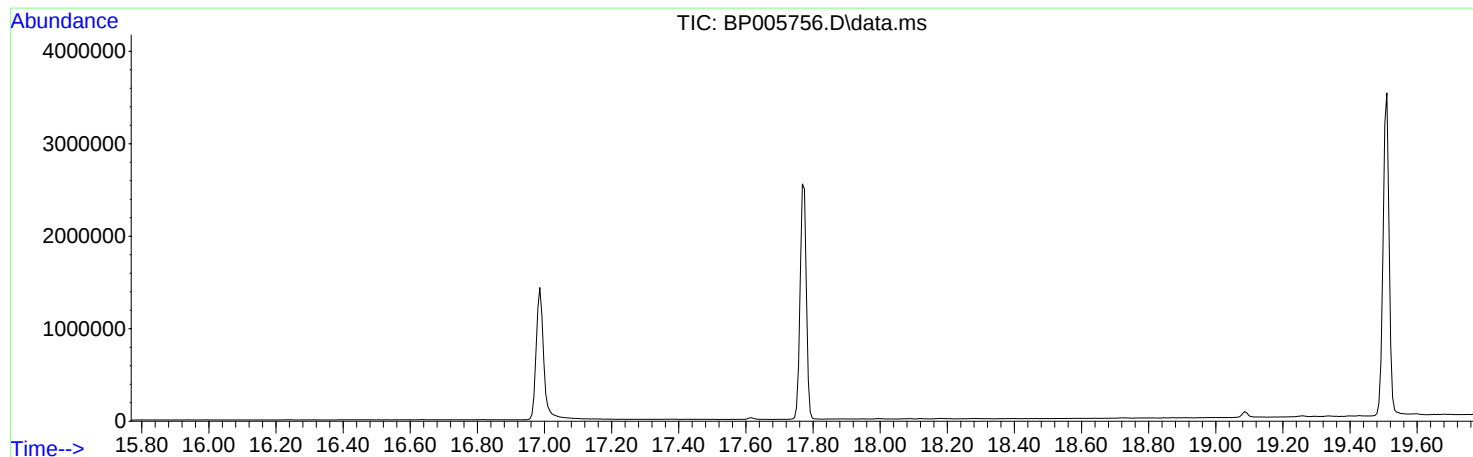




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	65644	PASS
68	69	0.00	2	1.8	1374	PASS
69	198	0.00	100	35.4	77641	PASS
70	69	0.00	2	0.5	420	PASS
127	198	10	80	45.3	99368	PASS
197	198	0.00	2	0.7	1480	PASS
198	198	100	100	100.0	219418	PASS
199	198	5	9	6.7	14629	PASS
275	198	10	60	29.9	65515	PASS
365	198	1	100	5.0	10932	PASS
441	198	0.01	100	23.1	50595	PASS
442	442	100	100	100.0	328469	PASS
443	442	15	24	19.8	64969	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060721\
Data File : BP005756.D
Acq On : 08 Jun 2021 00:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 08 02:44:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 07 12:13:53 2021
Response via : Initial Calibration

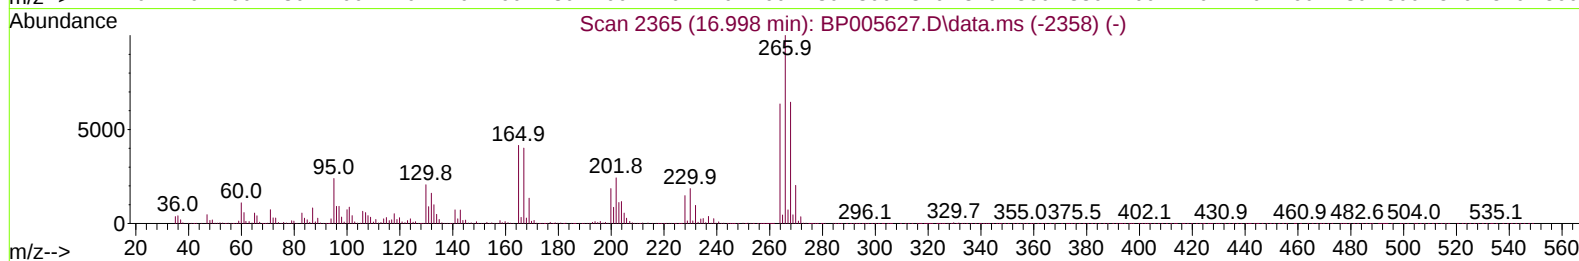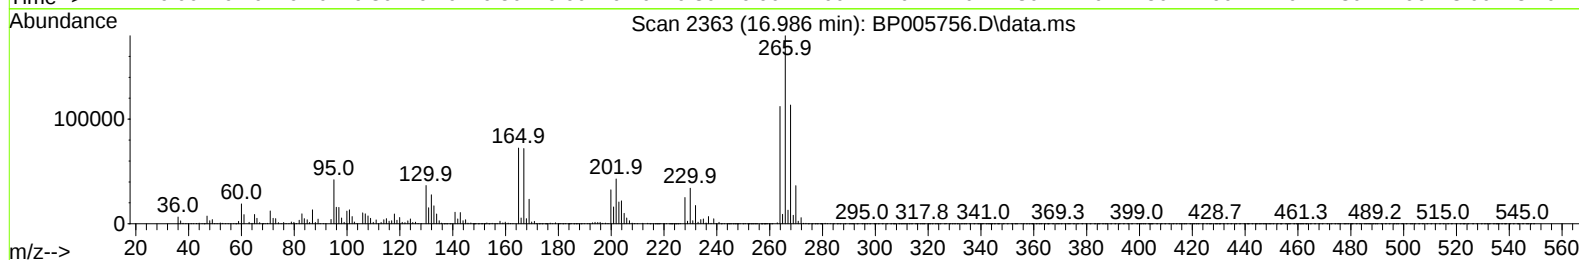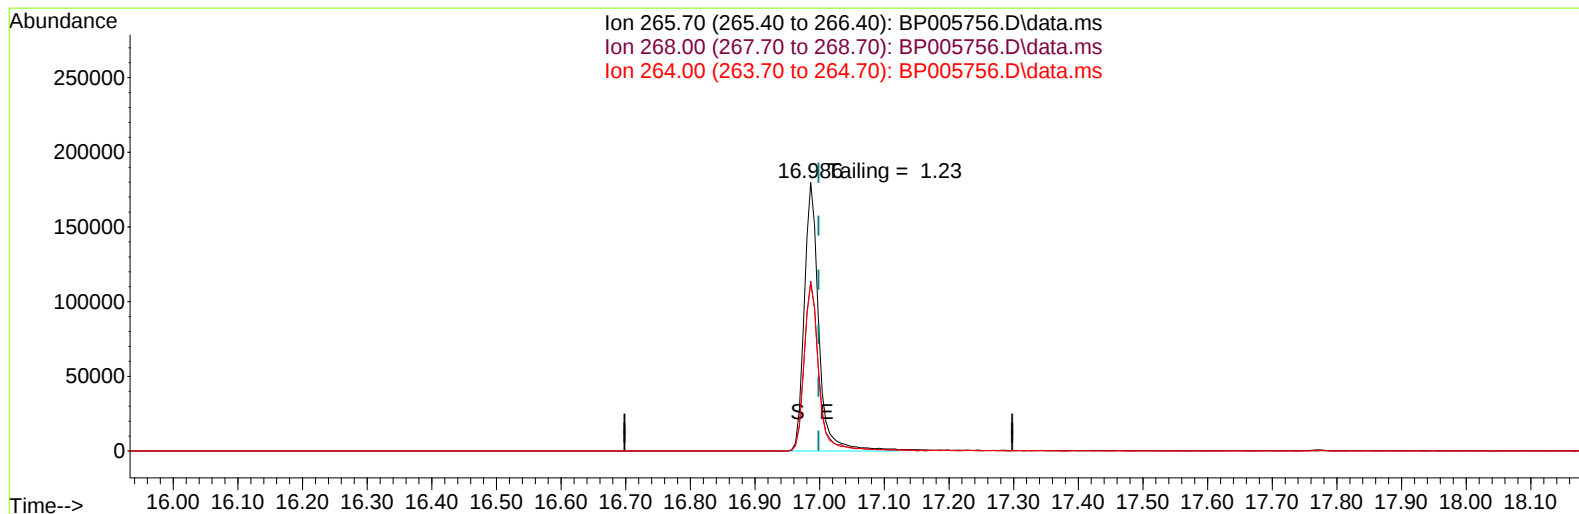

TIC: BP005756.D\data.ms

(70) Pentachlorophenol (C)

16.986min (-0.012) 65845.63 ng




response 283271

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.19
264.00	67.10	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060721\
 Data File : BP005756.D
 Acq On : 08 Jun 2021 00:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 08 02:44:57 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 07 12:13:53 2021
 Response via : Initial Calibration

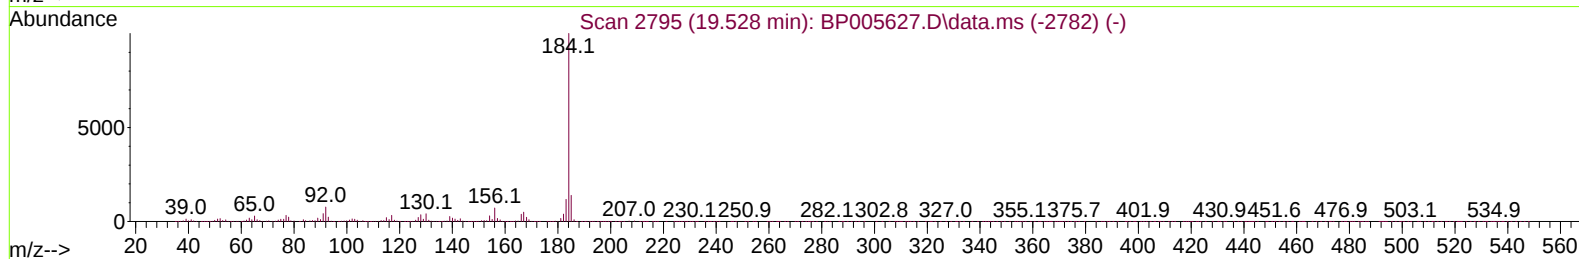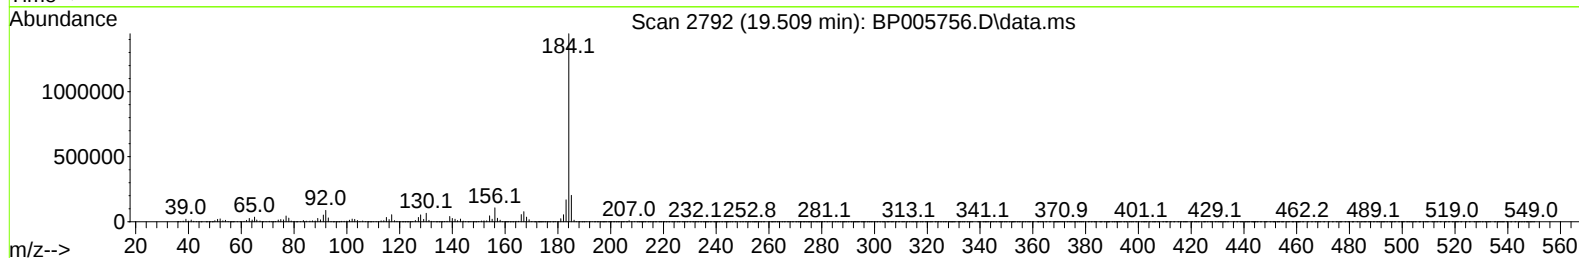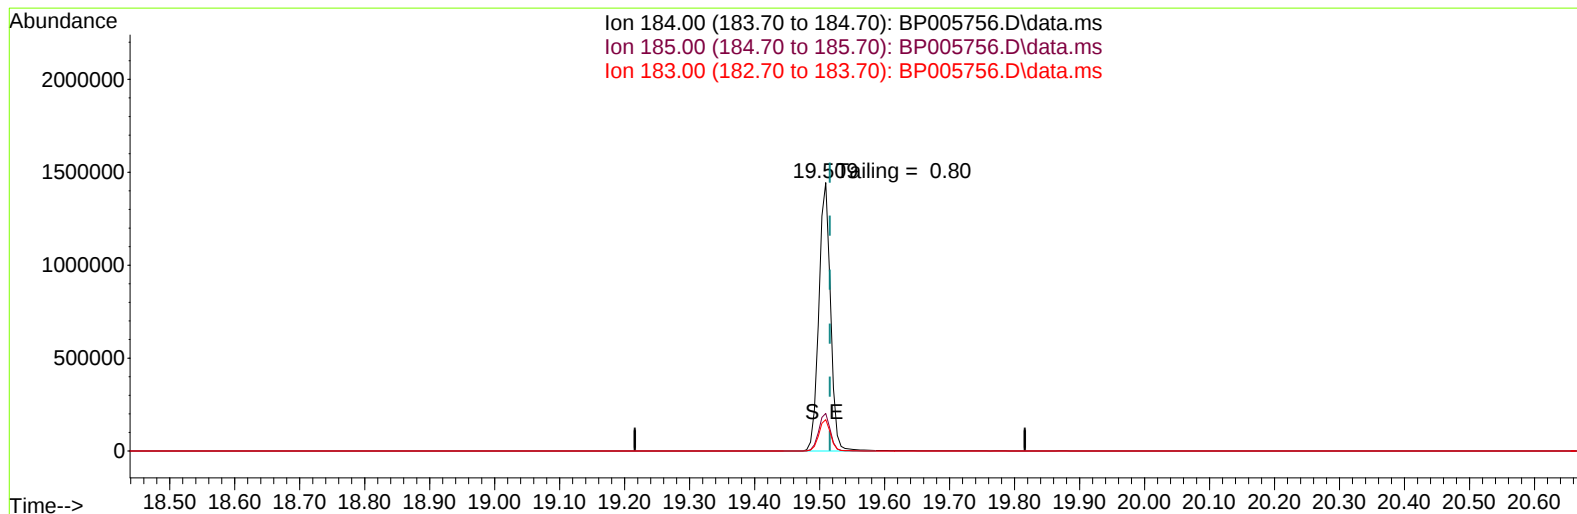

TIC: BP005756.D\data.ms

(77) Benzidine

19.509min (-0.006) 516802.72 ng

response 1815730

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.02
183.00	12.30	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/7/2021	BNA_P	BP005756.D
Compound Name	Response	Retention Time
DDT	889237	20.704
DDD	27734	20.274
DDE	4467	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32201	921438	3.49