
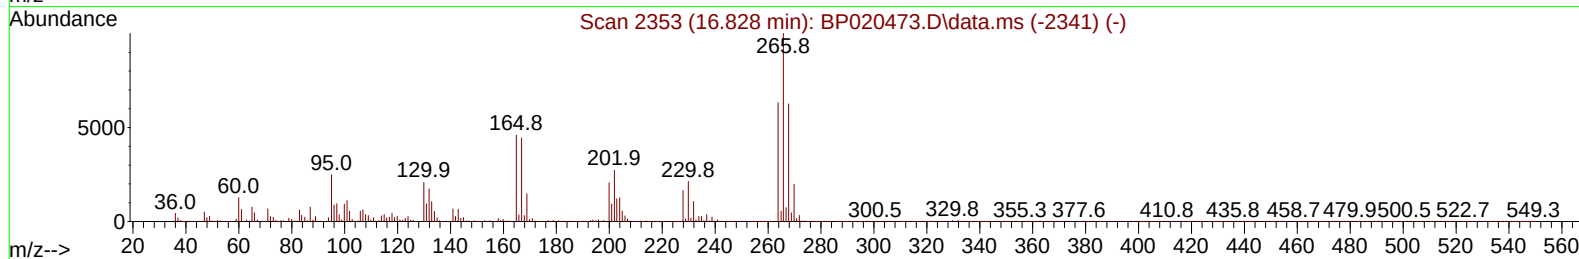
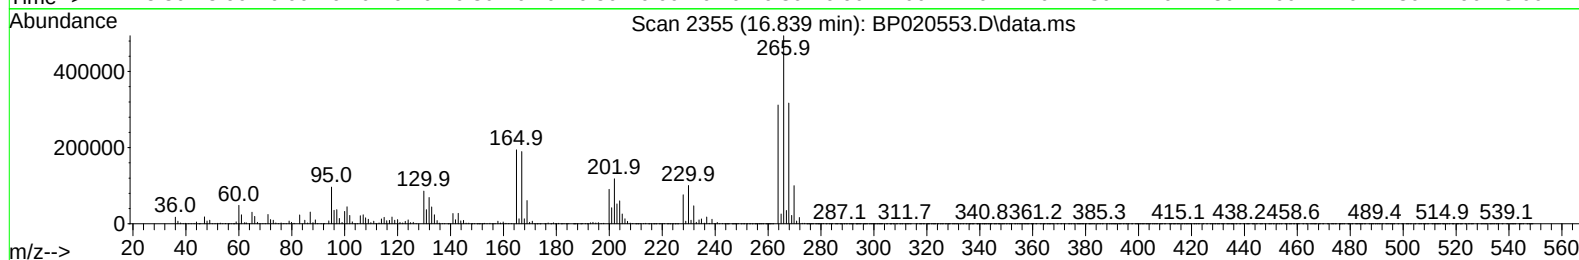


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060724\
Data File : BP020553.D
Acq On : 07 Jun 2024 09:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 20:03:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

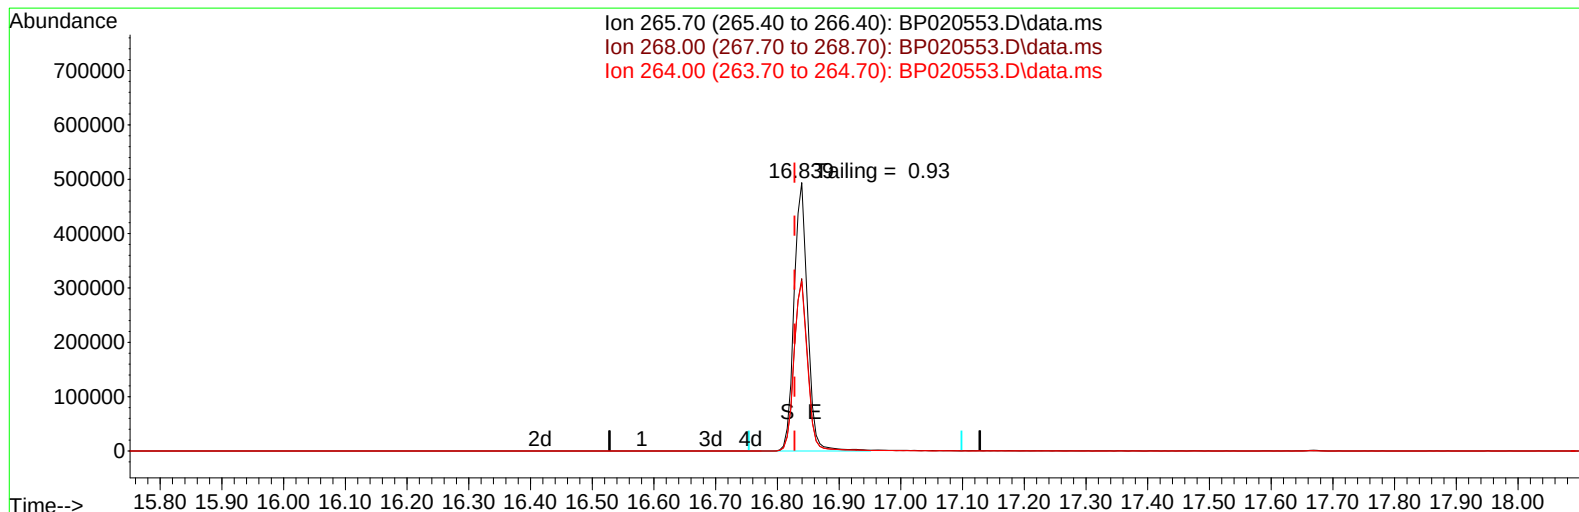

TIC: BP020553.D\data.ms

(70) Pentachlorophenol (C)




16.839min (+ 0.011) 4559738.44 ng m

response 766917

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.19
264.00	63.30	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060724\
 Data File : BP020553.D
 Acq On : 07 Jun 2024 09:32
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 20:03:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 30 03:41:03 2024
 Response via : Initial Calibration

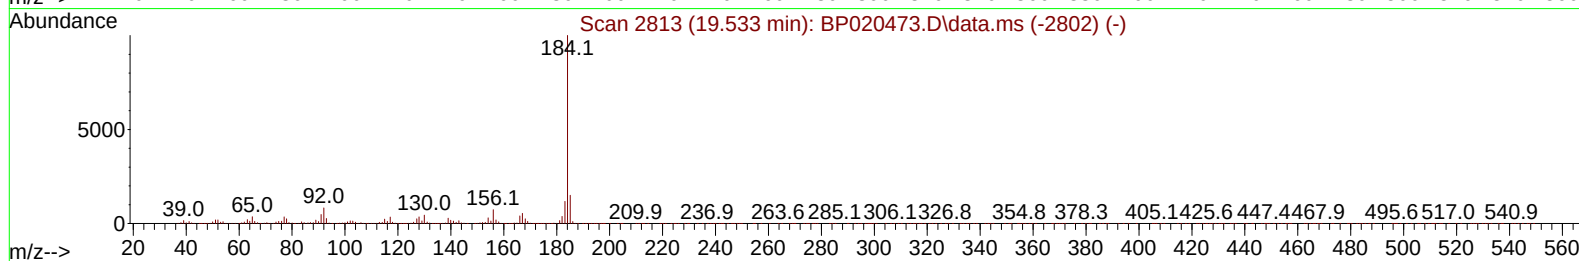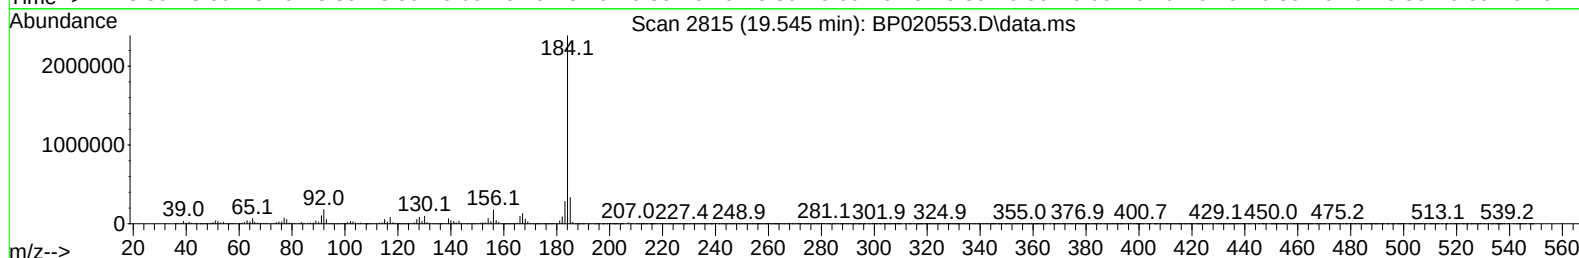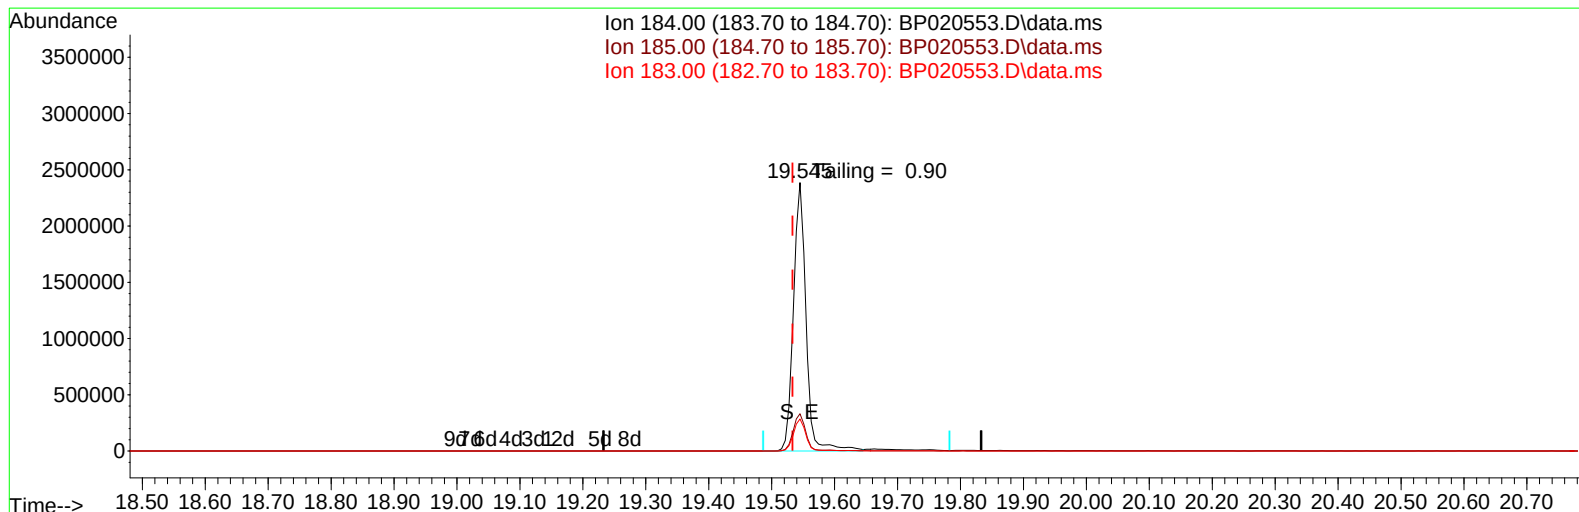

TIC: BP020553.D\data.ms

(77) Benzidine

19.545min (+ 0.012) 202707.78 ng m

response 3407296

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.92
183.00	11.70	11.95
0.00	0.00	0.00