

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060724\
 Data File : BP020566.D
 Acq On : 07 Jun 2024 19:14
 Operator : MA/JU
 Sample : P2756-01 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OR-02-06062024

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP020566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	24	rVB	783867	1159373	22.38%	2.870%
2	4.922	323	329	335	rBV2	64030	101819	1.97%	0.252%
3	5.369	398	405	414	rBV	1063847	1554222	30.00%	3.847%
4	6.928	663	670	682	rVB	952914	1561335	30.14%	3.865%
5	7.758	803	811	820	rBV	1326679	2012773	38.85%	4.982%
6	8.899	998	1005	1016	rBV	588833	1004926	19.40%	2.487%
7	10.534	1272	1283	1290	rBV	1665129	2752239	53.12%	6.812%
8	12.998	1692	1702	1713	rBV	1613987	2497804	48.21%	6.182%
9	14.110	1886	1891	1897	rBV2	33243	62712	1.21%	0.155%
10	14.381	1928	1937	1944	rBV	2369764	3718270	71.77%	9.203%
11	15.263	2083	2087	2093	rVB	50415	67157	1.30%	0.166%
12	15.687	2153	2159	2163	rBV	34148	63510	1.23%	0.157%
13	15.792	2174	2177	2186	rVB	49525	80983	1.56%	0.200%
14	15.898	2188	2195	2206	rBV	1165560	1938719	37.42%	4.799%
15	16.139	2232	2236	2246	rVB	101188	195477	3.77%	0.484%
16	16.963	2372	2376	2380	rBV2	94702	120618	2.33%	0.299%
17	17.010	2381	2384	2390	rVB4	45800	76437	1.48%	0.189%
18	17.198	2409	2416	2420	rBV	3204463	4370686	84.36%	10.818%
19	17.234	2420	2422	2427	rVB	166548	217802	4.20%	0.539%
20	17.322	2434	2437	2443	rVB	70173	100120	1.93%	0.248%
21	17.728	2502	2506	2510	rVB	104620	125283	2.42%	0.310%
22	18.139	2571	2576	2583	rVB4	193581	382666	7.39%	0.947%
23	18.304	2600	2604	2608	rBV2	60696	91841	1.77%	0.227%
24	18.445	2625	2628	2636	rVB	98681	133252	2.57%	0.330%
25	19.057	2729	2732	2736	rVB2	67755	86380	1.67%	0.214%
26	19.116	2739	2742	2748	rVV3	119496	165984	3.20%	0.411%
27	19.328	2773	2778	2785	rVB	571507	816072	15.75%	2.020%
28	19.475	2800	2803	2811	rBV5	129620	298297	5.76%	0.738%
29	19.704	2838	2842	2852	rVB	610329	1057095	20.40%	2.616%
30	19.928	2876	2880	2885	rBV	2928174	3426305	66.13%	8.481%
31	21.645	3165	3172	3179	rBV2	2433550	4980673	96.14%	12.328%
32	25.016	3739	3745	3758	rVB	1840318	5180873	100.00%	12.823%




Sum of corrected areas: 40401703

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060724\
Data File : BP020566.D
Acq On : 07 Jun 2024 19:14
Operator : MA/JU
Sample : P2756-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-02-06062024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

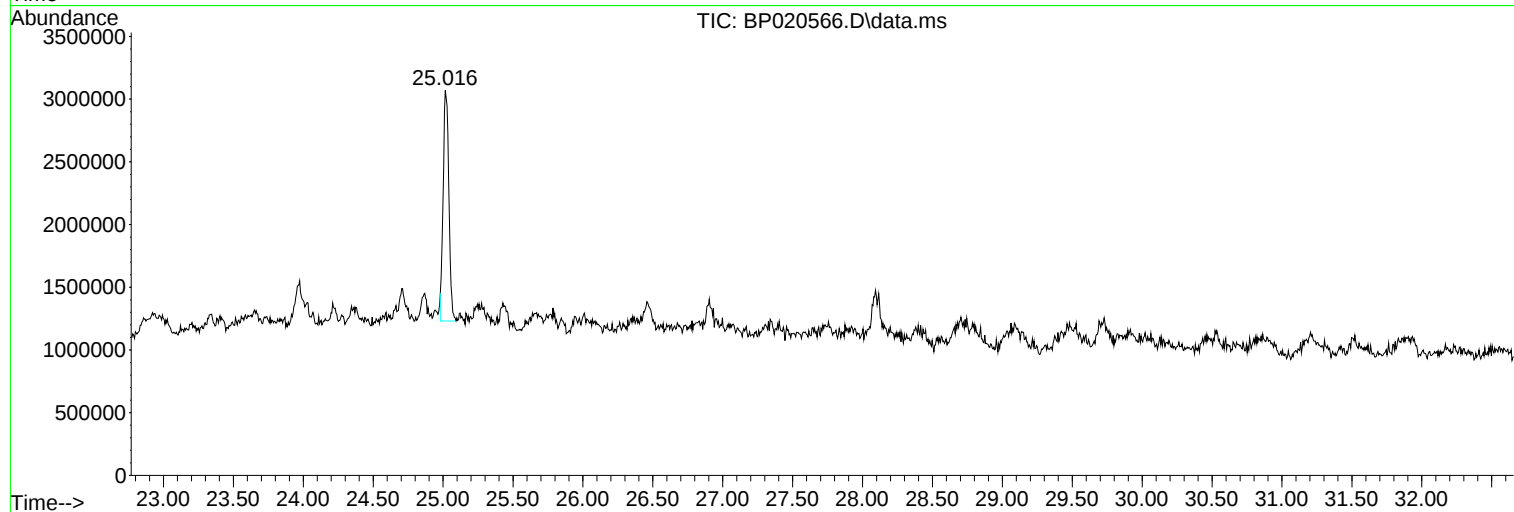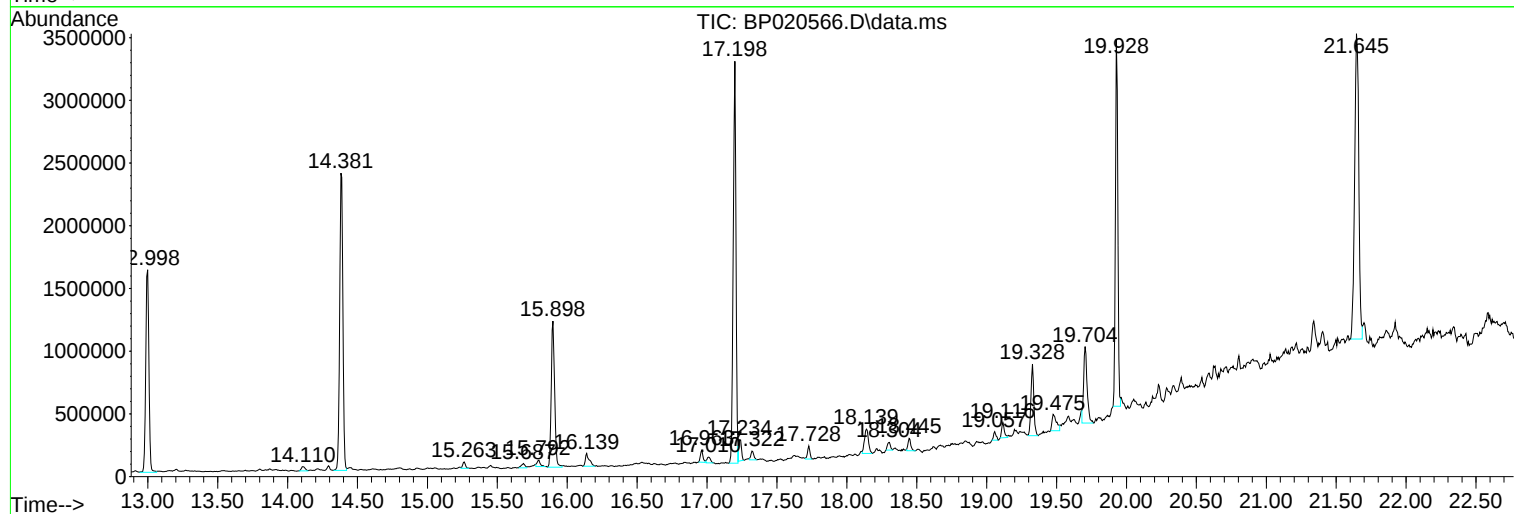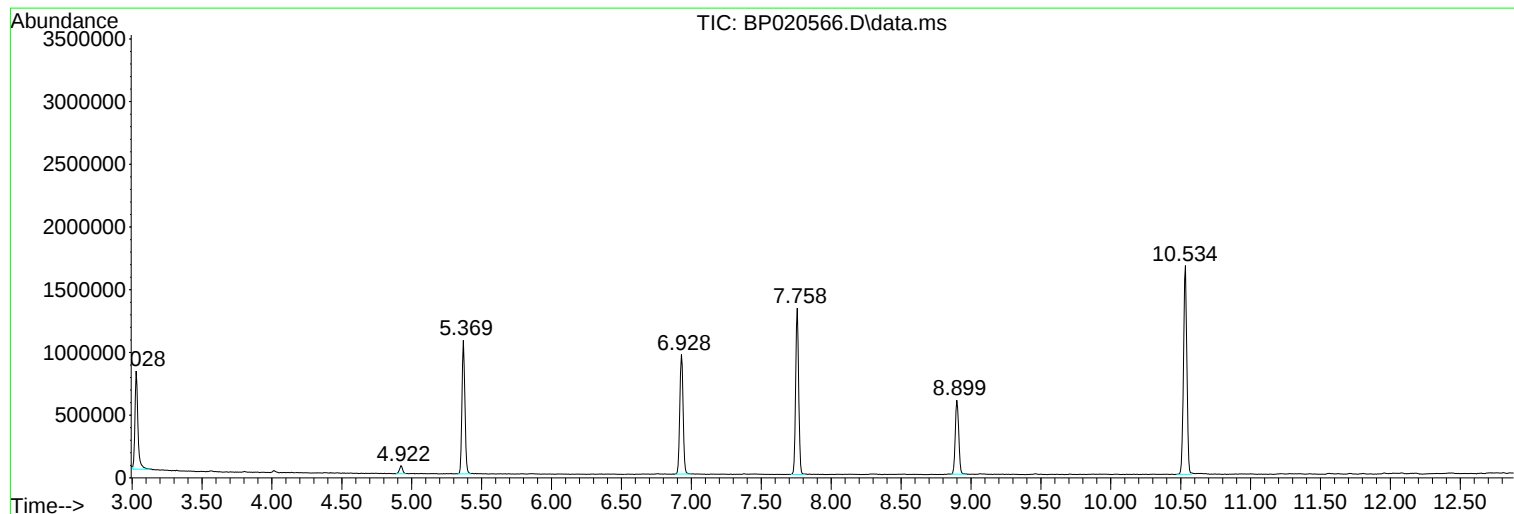

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060724\
Data File : BP020566.D
Acq On : 07 Jun 2024 19:14
Operator : MA/JU
Sample : P2756-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-02-06062024










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.028	11.52 ng	1159370	1,4-Dichlorobenzene-d4	7.758

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	23
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	12

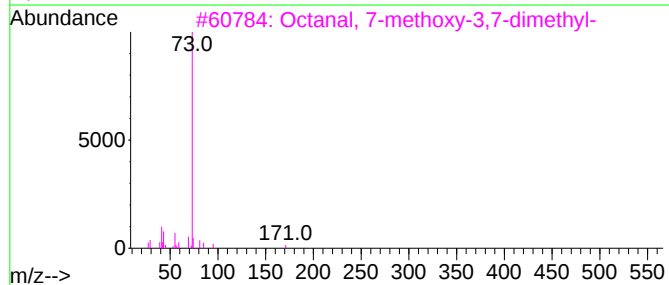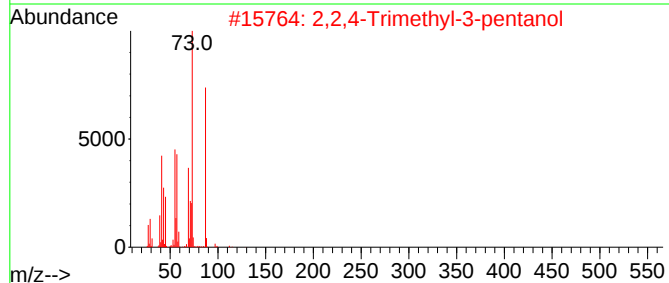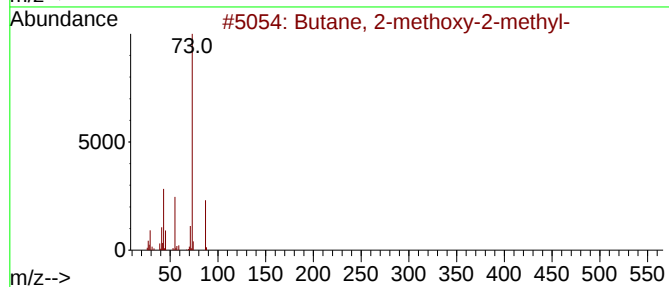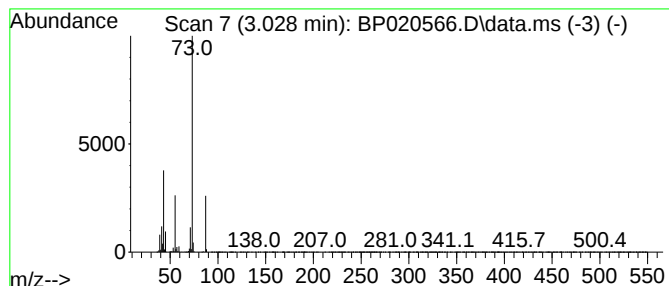

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060724\
Data File : BP020566.D
Acq On : 07 Jun 2024 19:14
Operator : MA/JU
Sample : P2756-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-02-06062024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.028	11.5	ng	1159370	1	7.758	2012770	20.0