
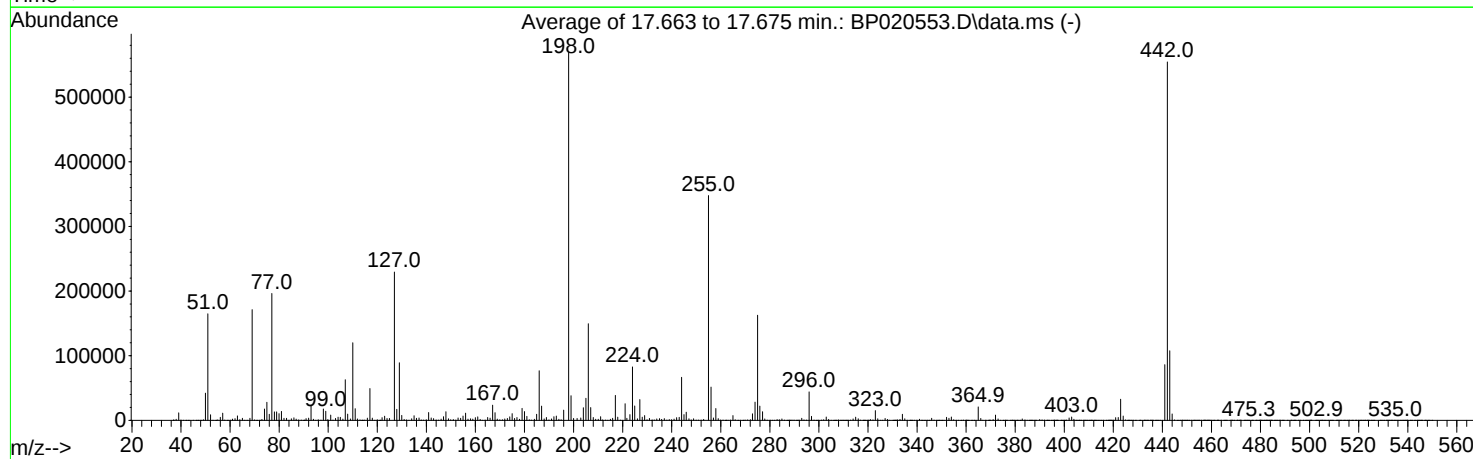


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060724\
Data File : BP020553.D
Acq On : 07 Jun 2024 09:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

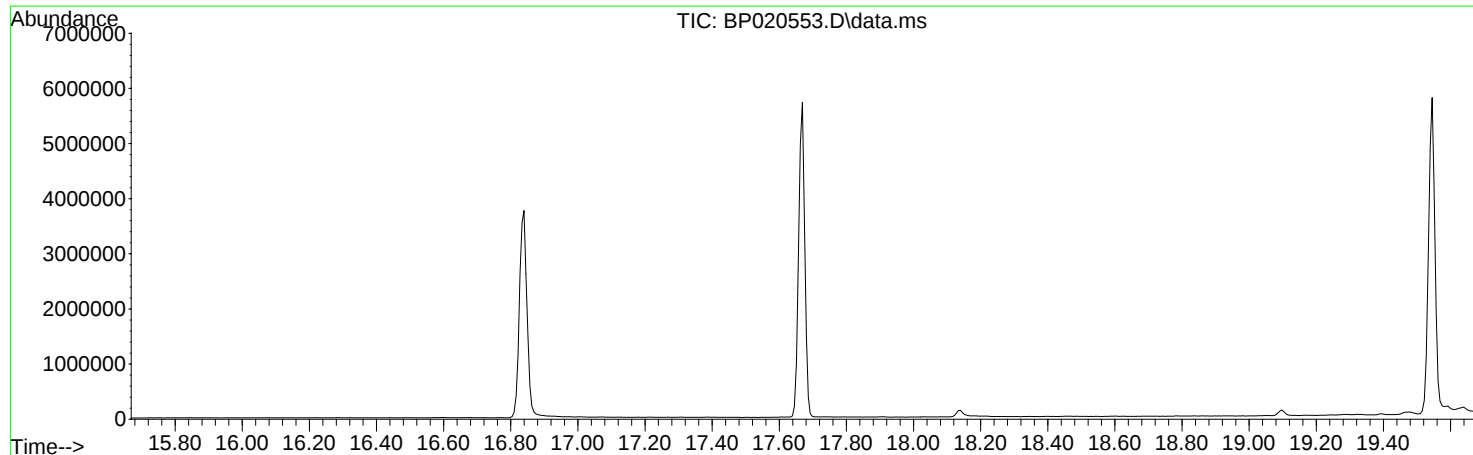


AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	164934	PASS
68	69	0.00	2	2.0	3353	PASS
69	198	0.00	100	30.1	171367	PASS
70	69	0.00	2	0.4	699	PASS
127	198	10	80	40.3	229316	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	568942	PASS
199	198	5	9	6.7	38123	PASS
275	198	10	60	28.6	162641	PASS
365	198	1	100	3.7	20842	PASS
441	198	0.01	100	15.1	86192	PASS
442	442	100	100	100.0	554314	PASS
443	442	15	24	19.4	107595	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060724\
Data File : BP020553.D
Acq On : 07 Jun 2024 09:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 07 20:03:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

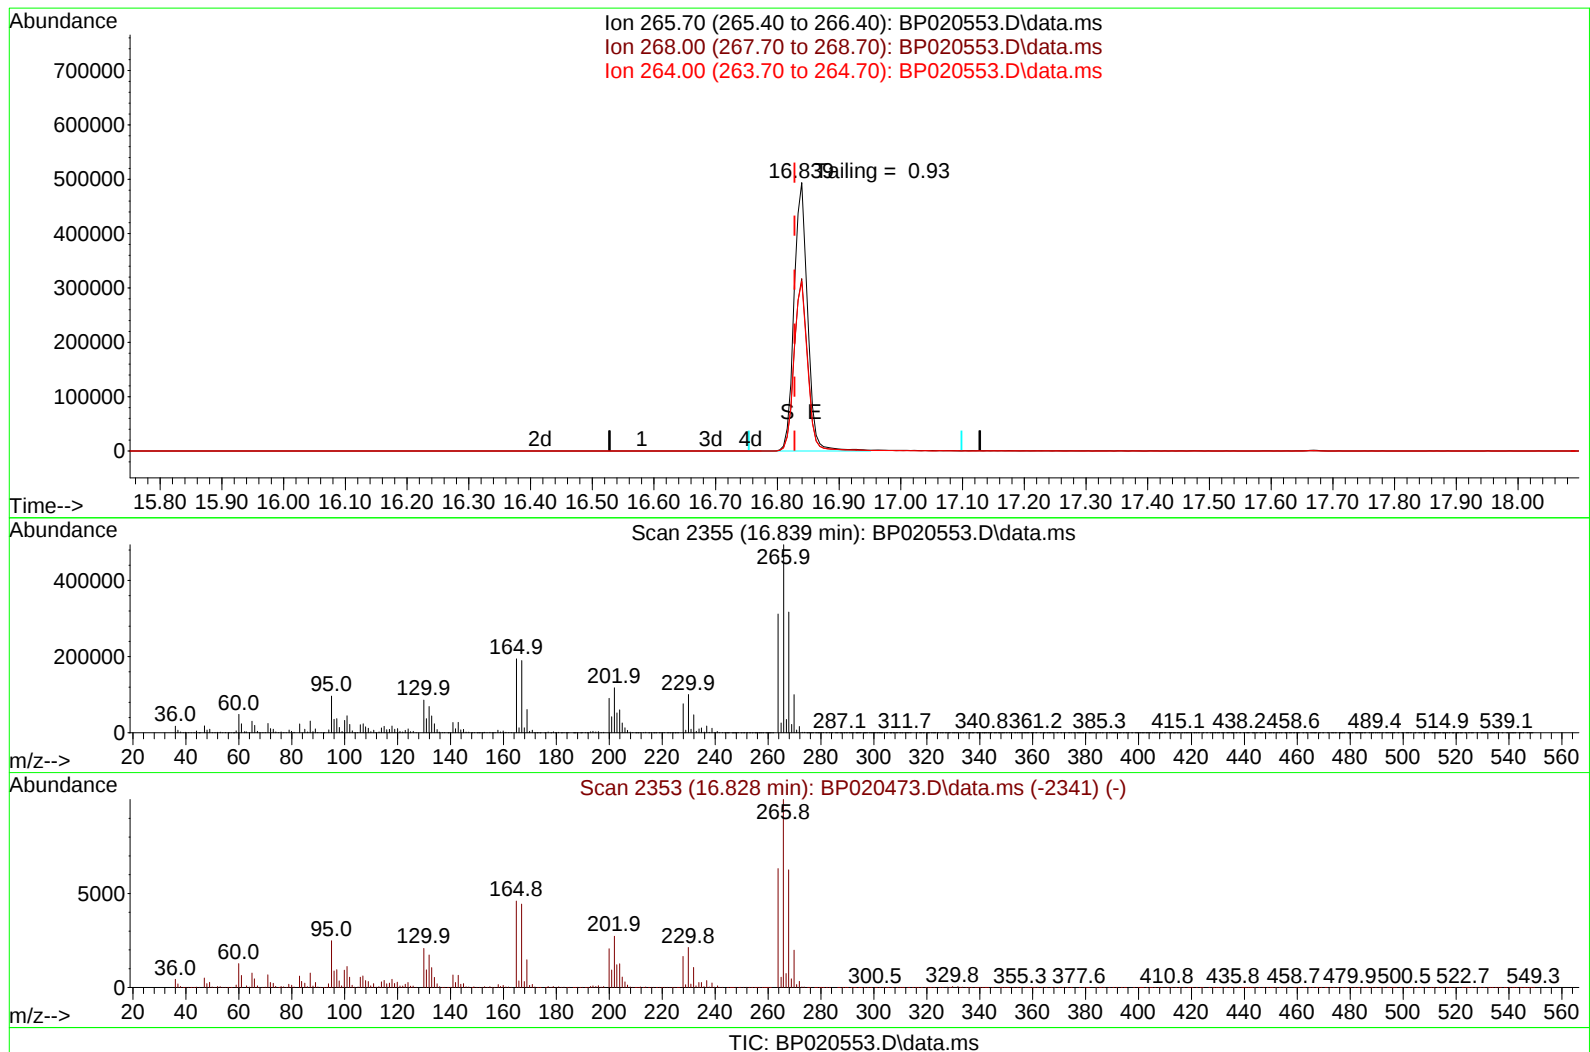

TIC: BP020553.D\data.ms

(70) Pentachlorophenol (C)

16.839min (+ 0.011) 4559738.44 ng m




response 766917

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.19
264.00	63.30	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060724\
Data File : BP020553.D
Acq On : 07 Jun 2024 09:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 07 20:03:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

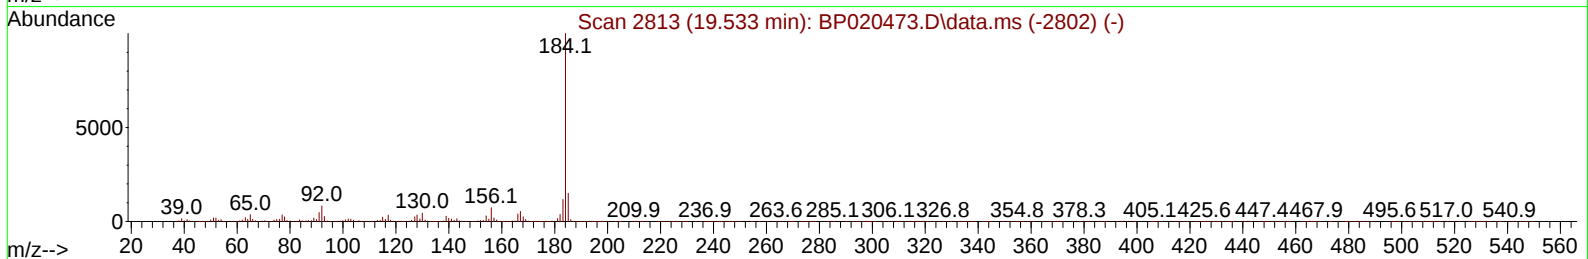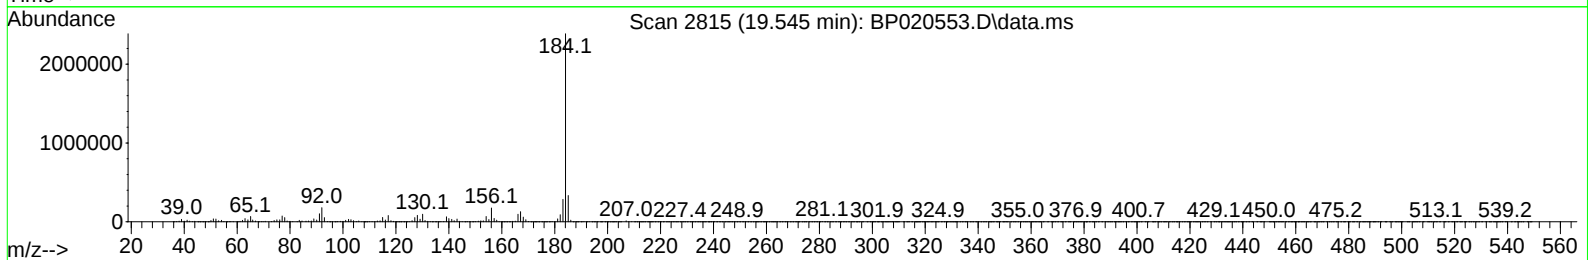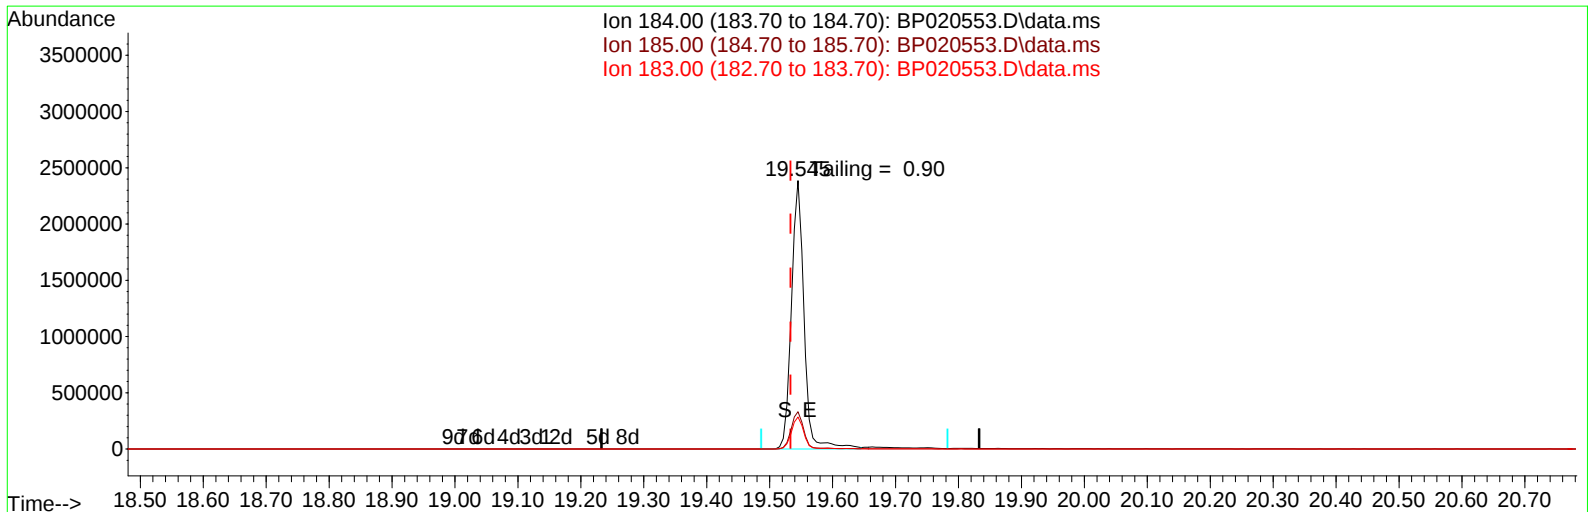

TIC: BP020553.D\data.ms

(77) Benzidine

19.545min (+ 0.012) 202707.78 ng m

response 3407296

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.92
183.00	11.70	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/7/2024	BNA_P	<u>BP020553.D</u>
Compound Name	Response	Retention Time
DDT	1728322	20.833
DDD	37802	20.369
DDE	3979	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41781	1770103	2.36

Instrument :
BNA_P
ClientSampleId :
DFTPP