
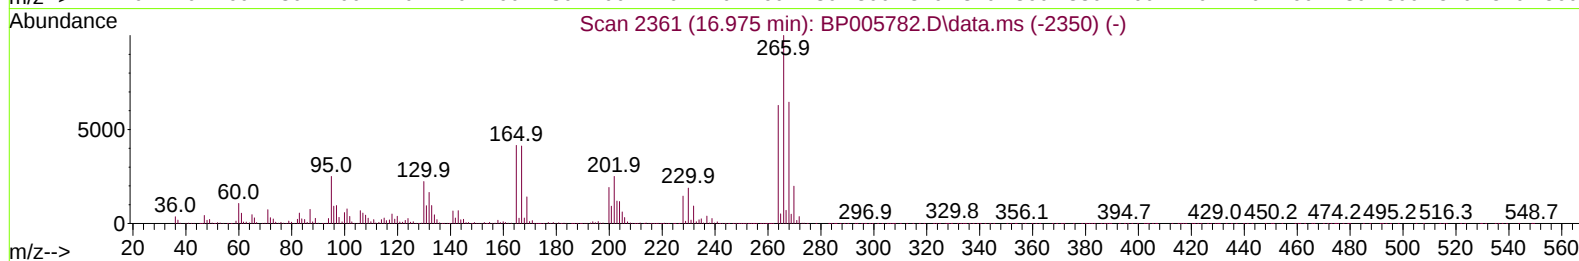
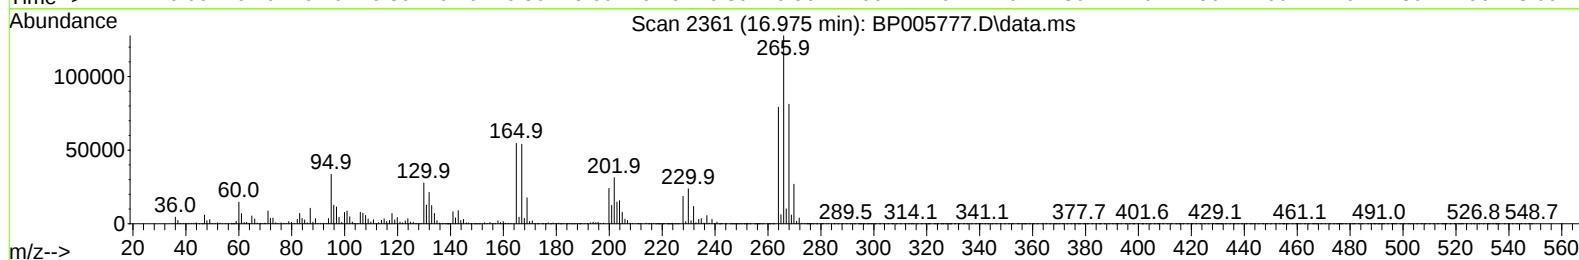


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060821\
 Data File : BP005777.D
 Acq On : 08 Jun 2021 16:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 03:09:33 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 02:47:38 2021
 Response via : Initial Calibration

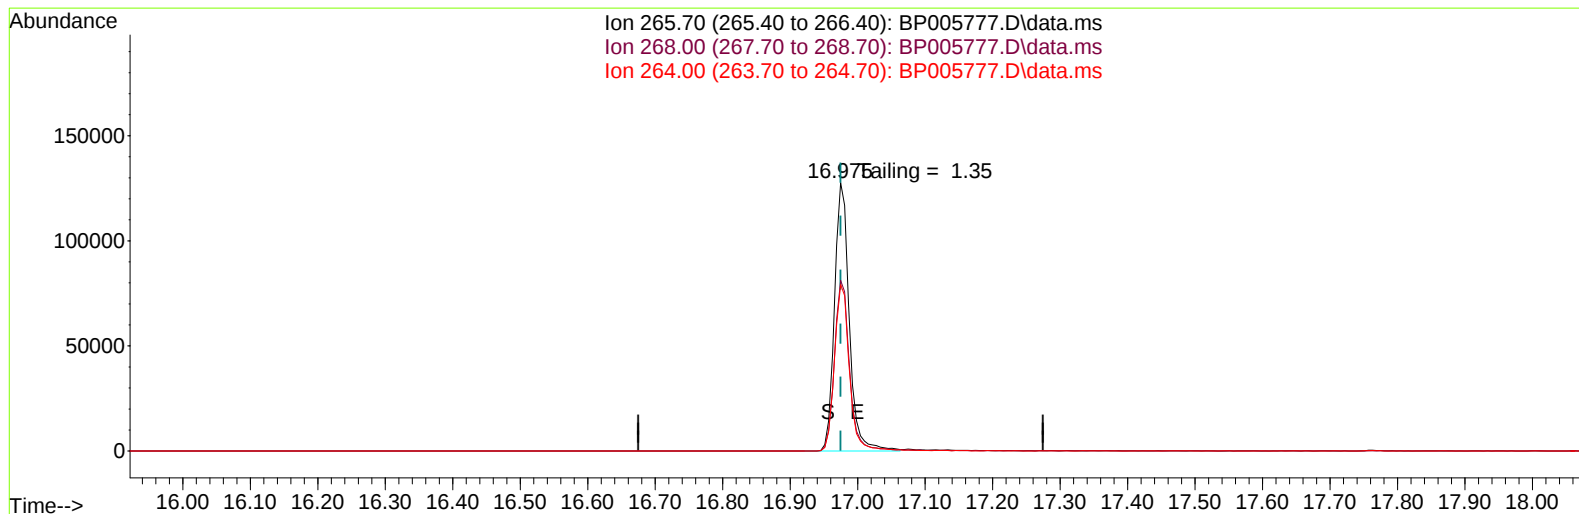

TIC: BP005777.D\data.ms




(70) Pentachlorophenol (C)

16.975min (-0.000) 1340493.53 ng

response 194941

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.57
264.00	62.90	62.01
0.00	0.00	0.00

Quant Time: Jun 09 03:09:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 09 02:47:38 2021
Response via : Initial Calibration

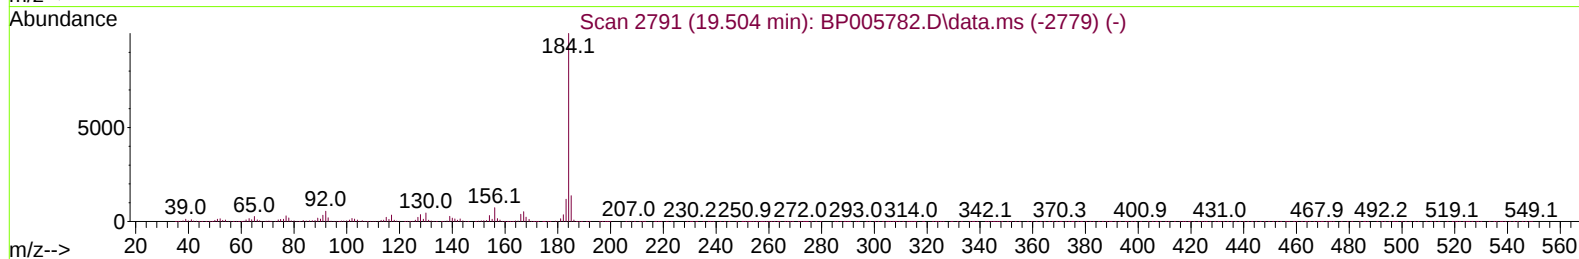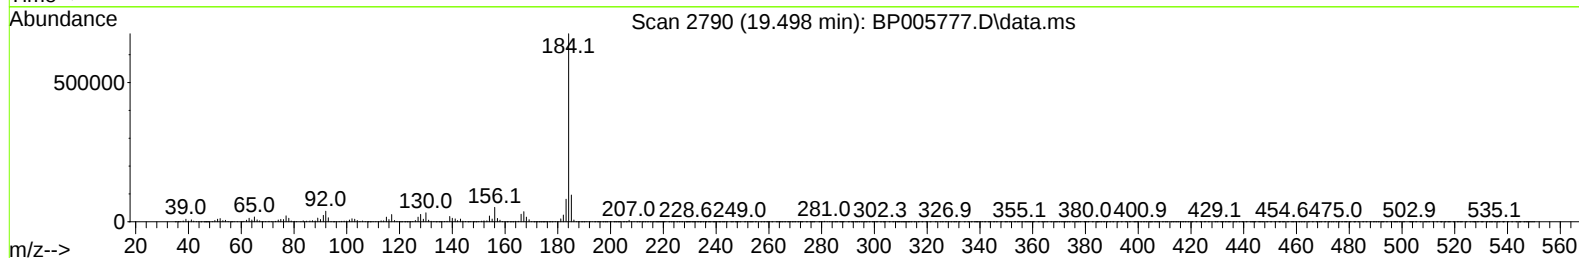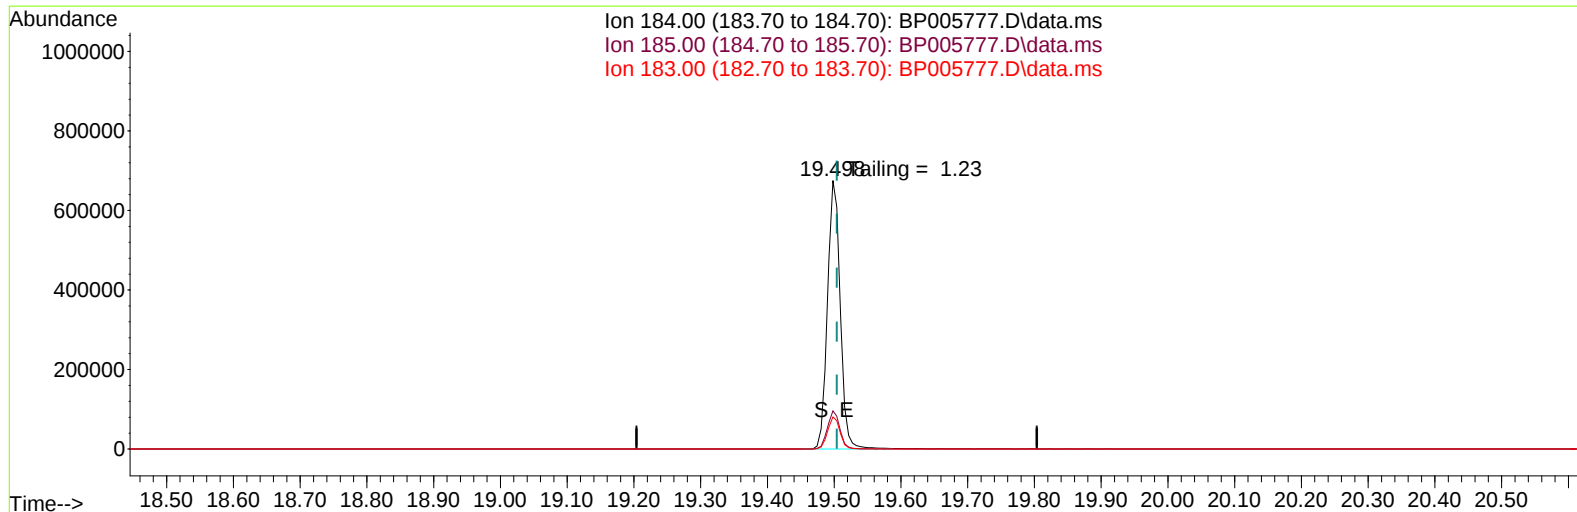

TIC: BP005777.D\data.ms

(77) Benzidine

19.498min (-0.006) 374238.56 ng

response **895523**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	13.70	14.25
--------	-------	-------

183.00	11.90	11.98
--------	-------	-------

0.00 0.00 0.00