
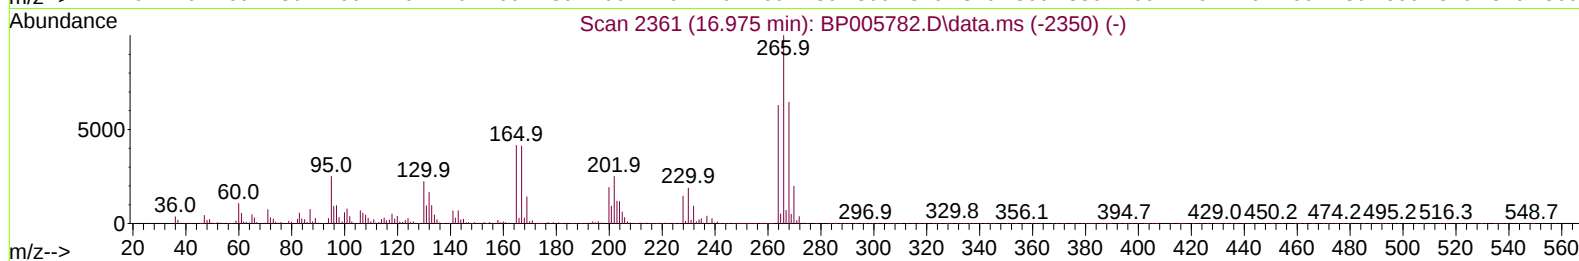
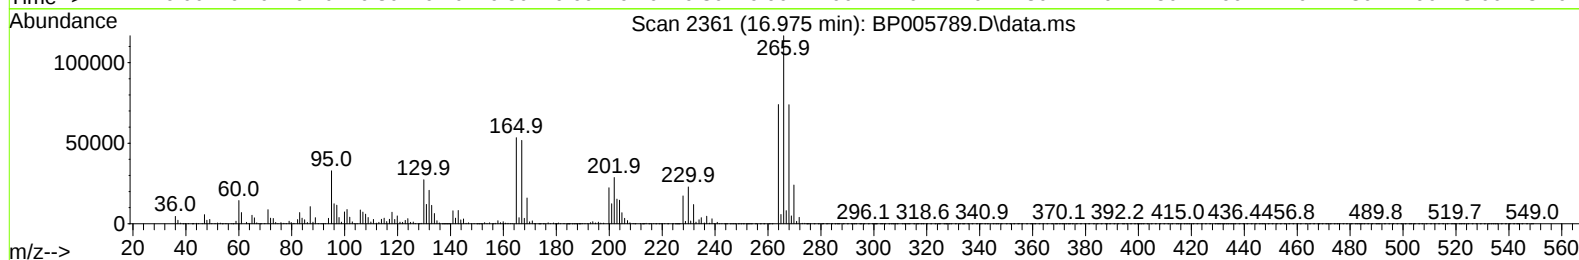


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060821\
Data File : BP005789.D
Acq On : 09 Jun 2021 00:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 07:16:41 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 09 02:47:38 2021
Response via : Initial Calibration

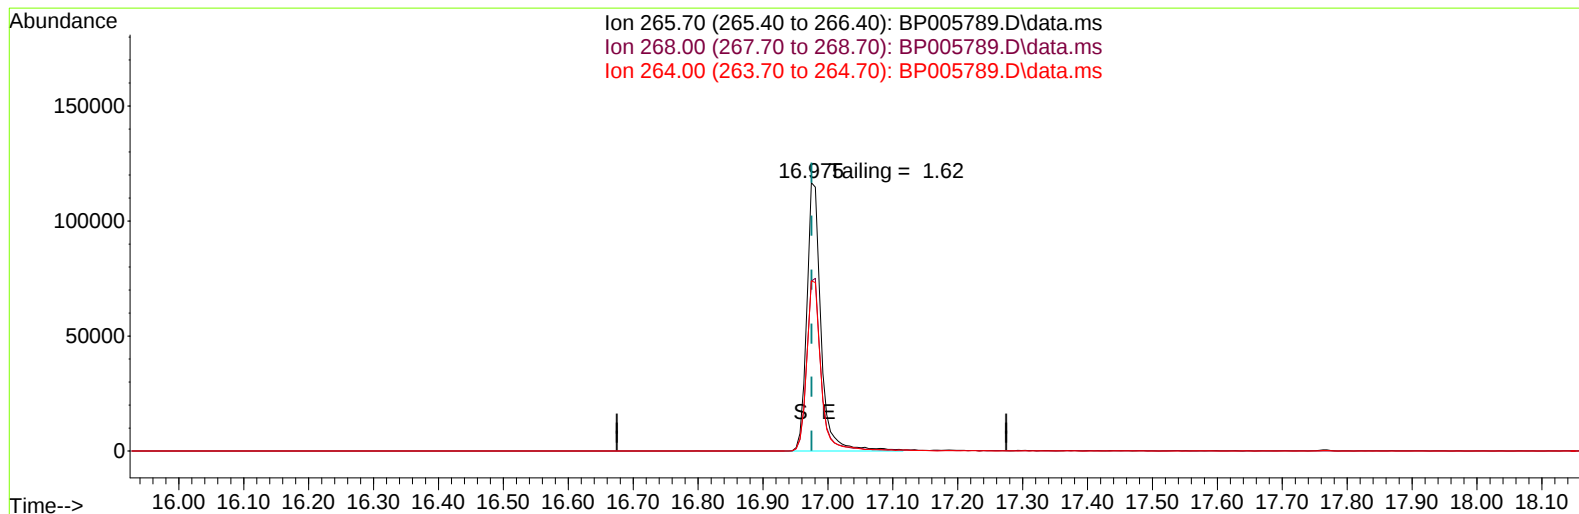

TIC: BP005789.D\data.ms

(70) Pentachlorophenol (C)




16.975min (-0.000) 116107.24 ng

response 178781

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.32
264.00	62.90	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060821\
 Data File : BP005789.D
 Acq On : 09 Jun 2021 00:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 07:16:41 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 02:47:38 2021
 Response via : Initial Calibration

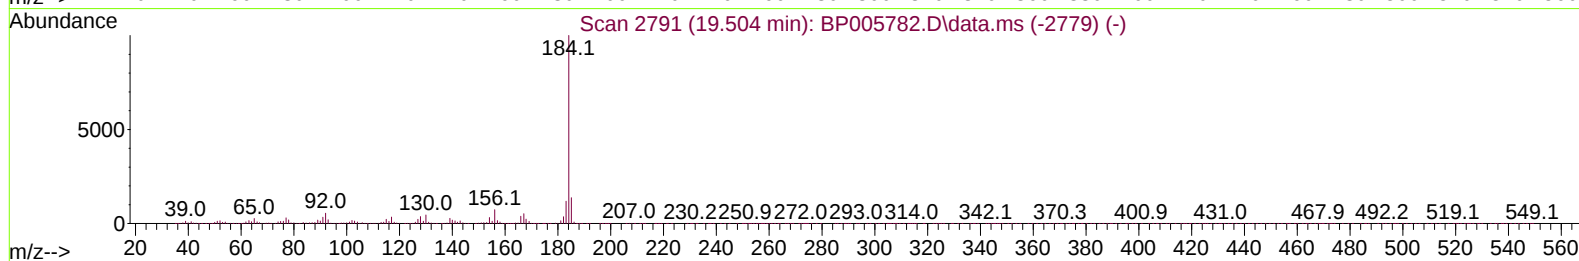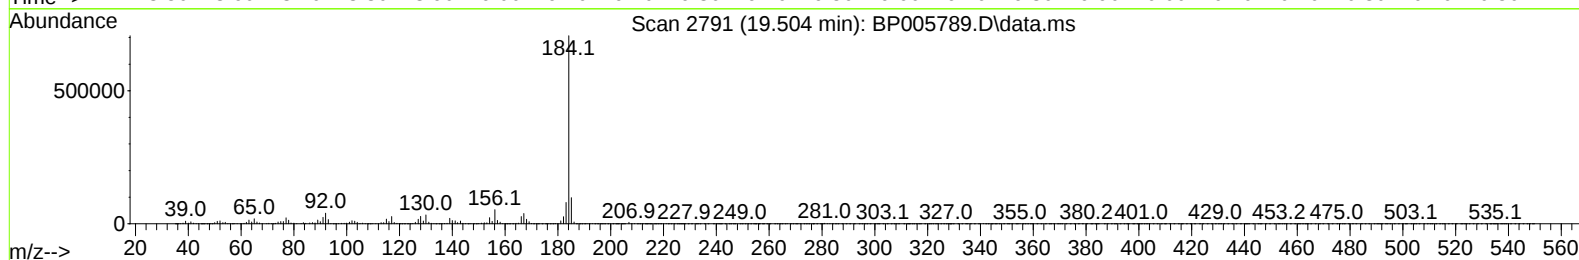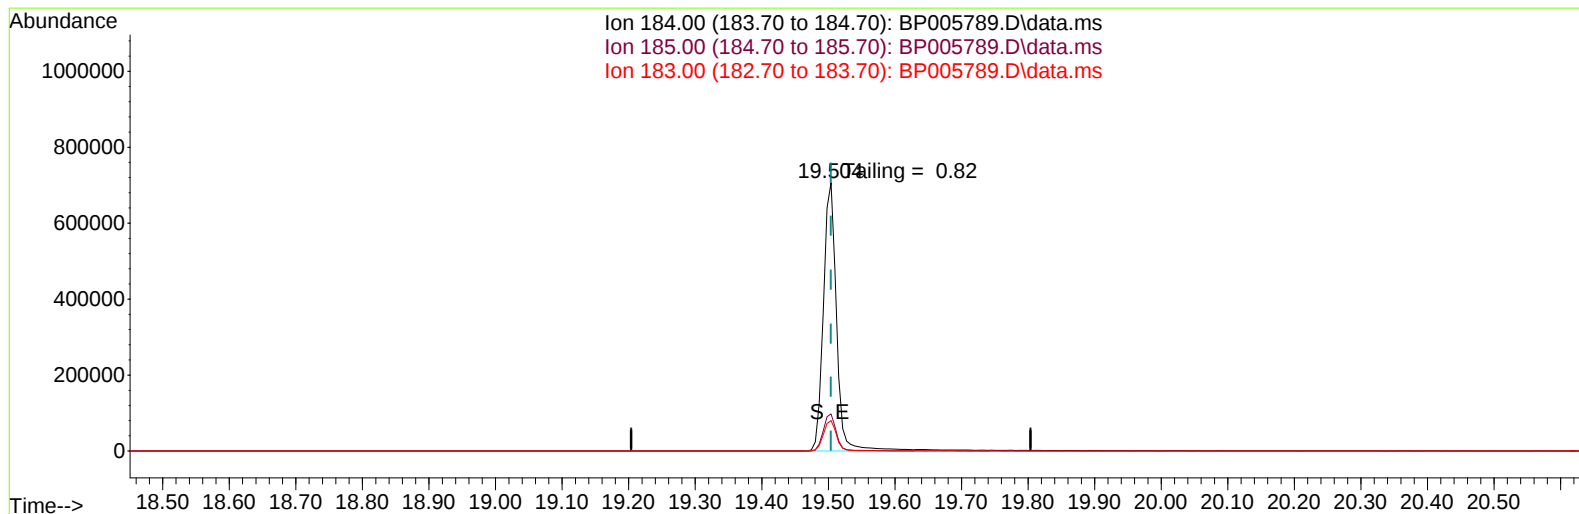

TIC: BP005789.D\data.ms

(77) Benzidine**19.504min (-0.000) 104754.00 ng****response 969976**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.86
183.00	11.90	11.37
0.00	0.00	0.00