
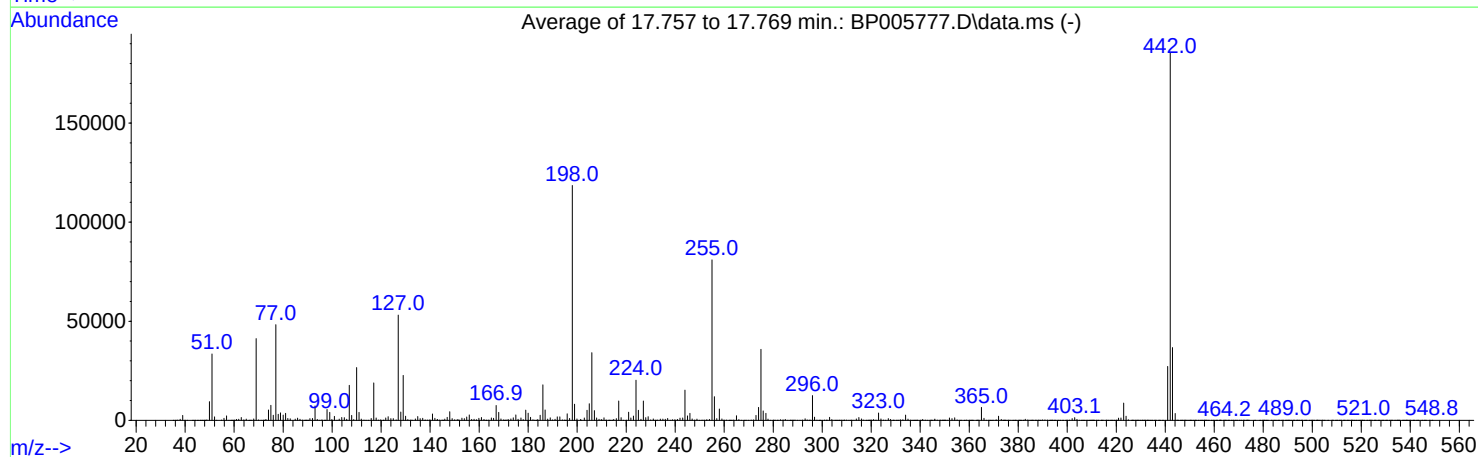


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060821\
 Data File : BP005777.D
 Acq On : 08 Jun 2021 16:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 09 11:54:55 2021

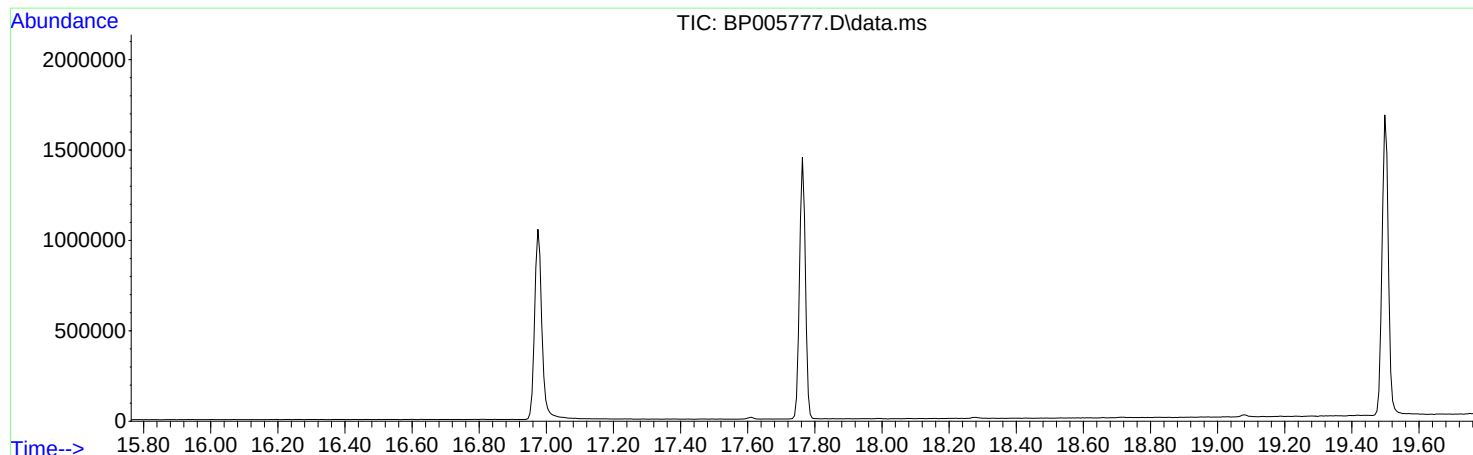




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	33494	PASS
68	69	0.00	2	1.8	729	PASS
69	198	0.00	100	34.8	41216	PASS
70	69	0.00	2	0.5	212	PASS
127	198	10	80	44.8	53116	PASS
197	198	0.00	2	0.9	1008	PASS
198	198	100	100	100.0	118485	PASS
199	198	5	9	6.9	8129	PASS
275	198	10	60	30.3	35883	PASS
365	198	1	100	5.5	6531	PASS
441	198	0.01	100	23.0	27240	PASS
442	442	100	100	100.0	185579	PASS
443	442	15	24	19.8	36735	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060821\
Data File : BP005777.D
Acq On : 08 Jun 2021 16:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 09 03:09:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 09 02:47:38 2021
Response via : Initial Calibration

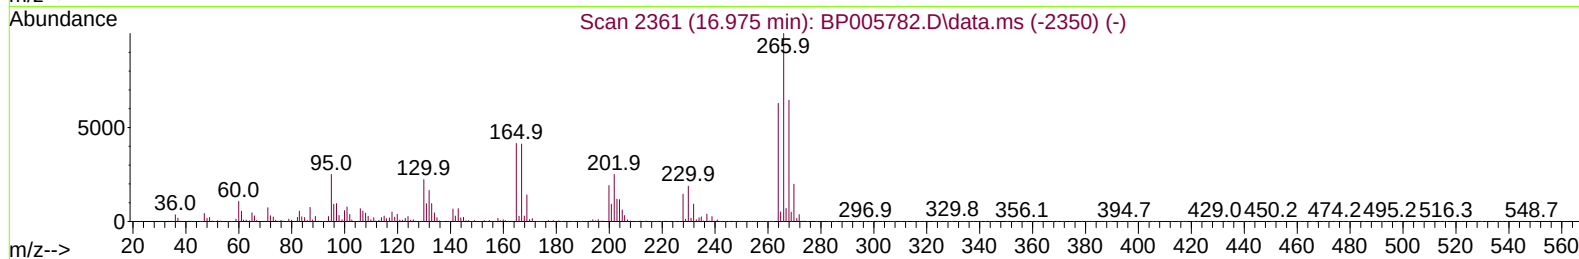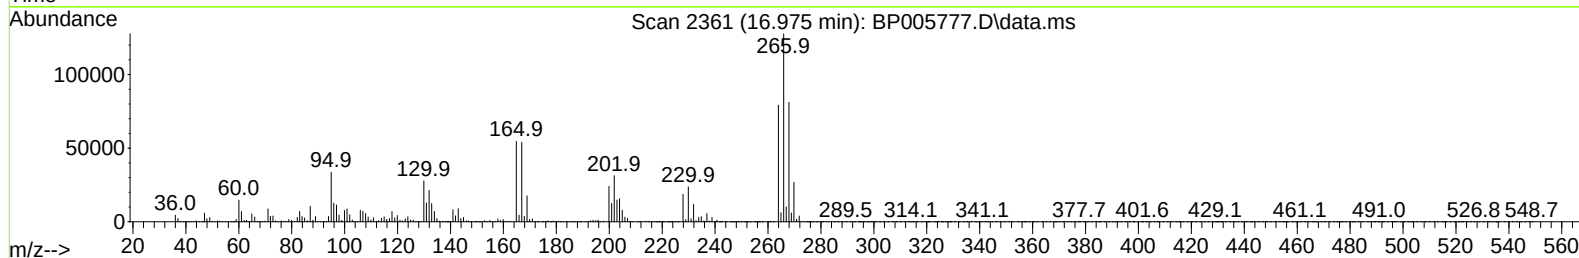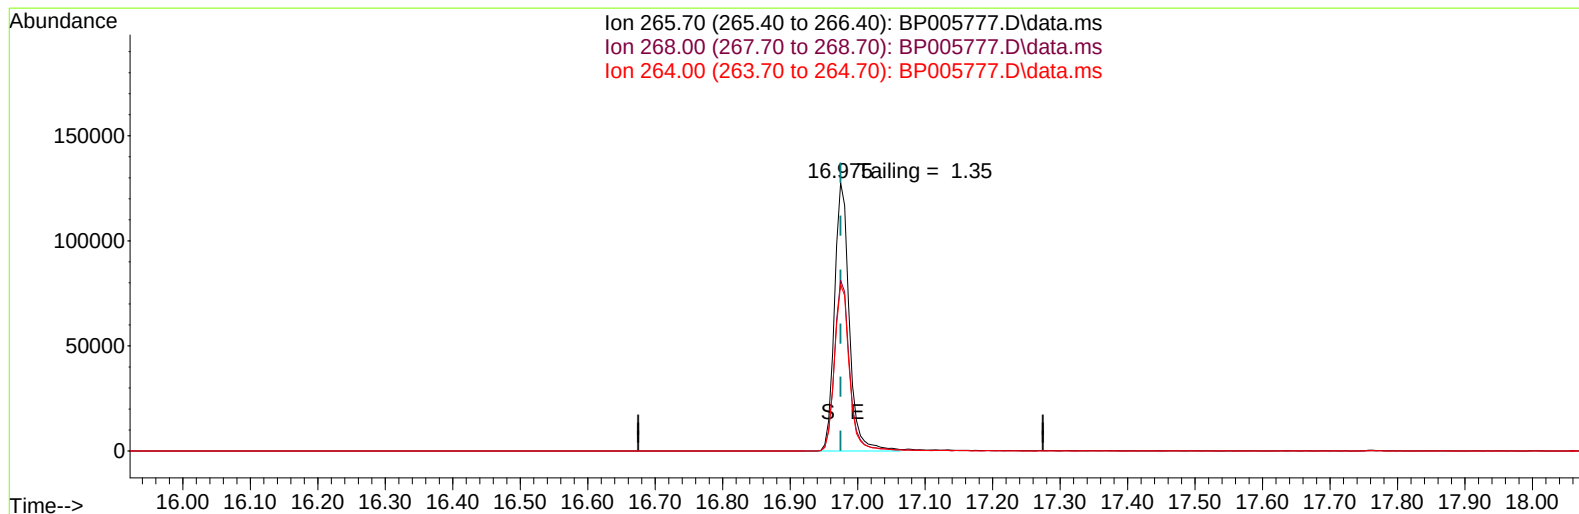

TIC: BP005777.D\data.ms

(70) Pentachlorophenol (C)

16.975min (-0.000) 1340493.53 ng




response 194941

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.57
264.00	62.90	62.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060821\
Data File : BP005777.D
Acq On : 08 Jun 2021 16:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 09 03:09:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 09 02:47:38 2021
Response via : Initial Calibration

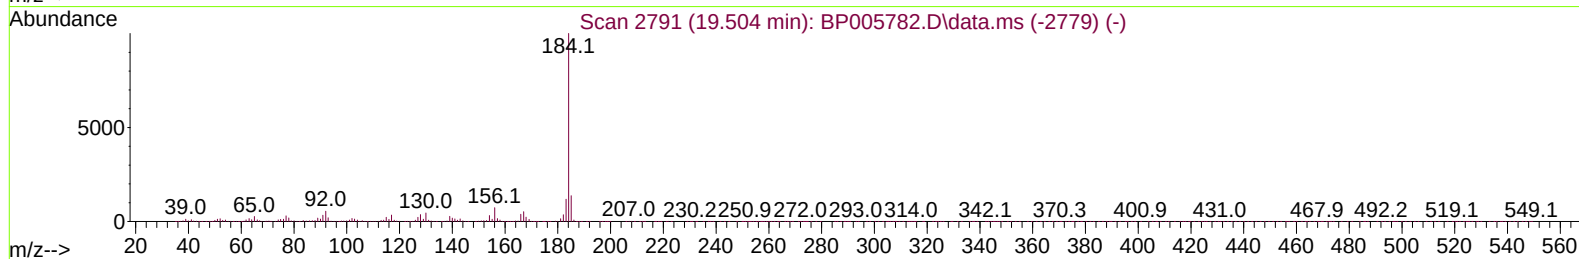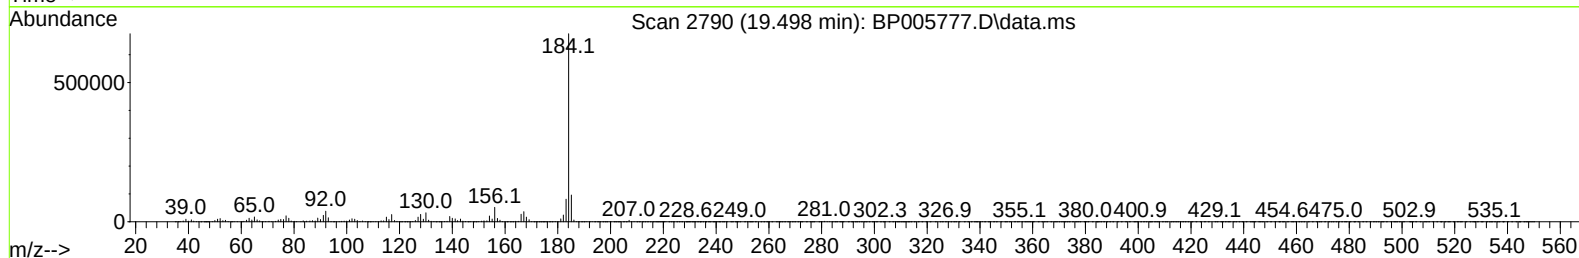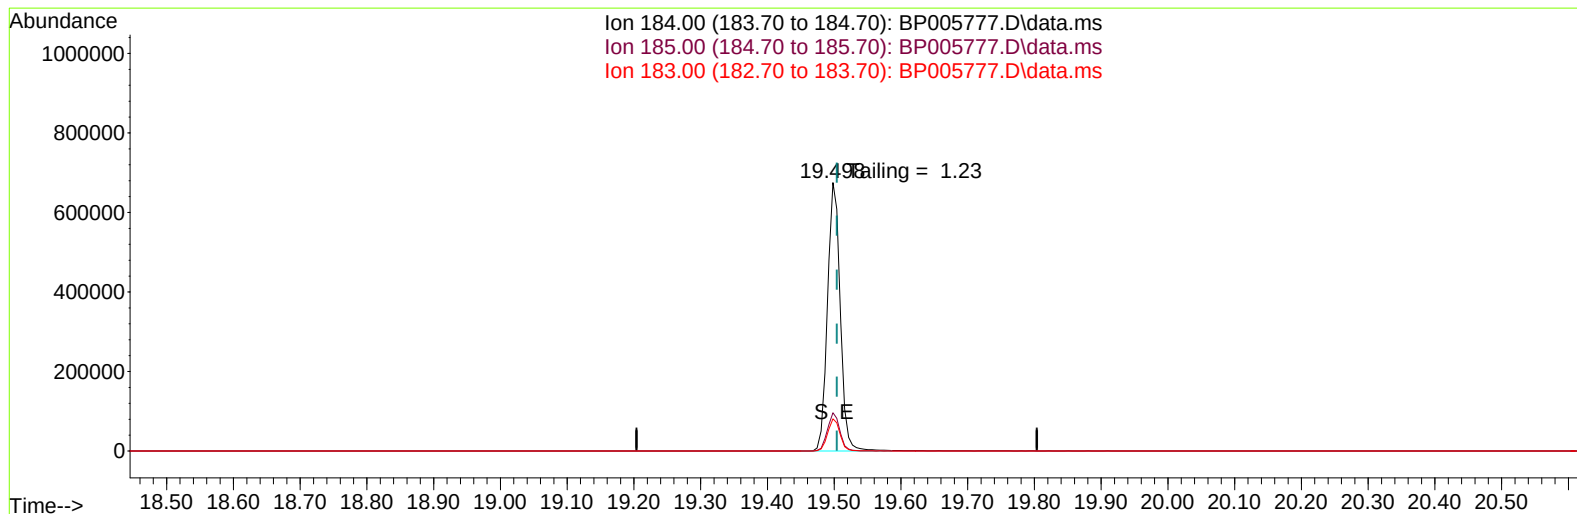

TIC: BP005777.D\data.ms

(77) Benzidine

19.498min (-0.006) 374238.56 ng

response 895523

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.25
183.00	11.90	11.98
0.00	0.00	0.00

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/8/2021	BNA_P	<u>BP005777.D</u>
Compound Name	Response	Retention Time
DDT	459444	20.698
DDD	3301	20.322
DDE	867	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4168	463612	0.90